

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030524\
 Data File : BN030268.D
 Acq On : 05 Mar 2024 12:46
 Operator : MA/JU
 Sample : SSTDICC0.1
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Quant Time: Mar 05 17:43:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN030524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 05 17:02:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.811	152	1527	0.400	ng	0.00
7) Naphthalene-d8	10.605	136	3924	0.400	ng	0.00
13) Acenaphthene-d10	14.457	164	1963	0.400	ng	0.00
19) Phenanthrene-d10	17.218	188	4048	0.400	ng	0.00
29) Chrysene-d12	21.438	240	3491	0.400	ng	0.00
35) Perylene-d12	23.803	264	3912	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.384	112	421	0.105	ng	0.00
5) Phenol-d6	6.980	99	369	0.088	ng	0.00
8) Nitrobenzene-d5	8.982	82	306	0.085	ng	0.01
11) 2-Methylnaphthalene-d10	12.208	152	486	0.085	ng	0.00
14) 2,4,6-Tribromophenol	15.964	330	95	0.094	ng	0.00
15) 2-Fluorobiphenyl	13.089	172	758	0.093	ng	0.00
27) Fluoranthene-d10	19.266	212	1067	0.096	ng	0.00
31) Terphenyl-d14	19.879	244	937	0.103	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.326	88	254	0.128	ng	# 85
3) n-Nitrosodimethylamine	3.665	42	206	0.099	ng	# 96
6) bis(2-Chloroethyl)ether	7.255	93	286	0.086	ng	# 97
9) Naphthalene	10.658	128	1072	0.098	ng	# 85
10) Hexachlorobutadiene	10.925	225	255	0.102	ng	# 99
12) 2-Methylnaphthalene	12.284	142	624	0.092	ng	93
16) Acenaphthylene	14.180	152	896	0.095	ng	99
17) Acenaphthene	14.522	154	596	0.097	ng	98
18) Fluorene	15.518	166	713	0.097	ng	99
20) 4,6-Dinitro-2-methylph...	15.629	198	60	0.068	ng	# 22
21) 4-Bromophenyl-phenylether	16.424	248	229	0.093	ng	# 75
22) Hexachlorobenzene	16.523	284	282	0.099	ng	95
23) Atrazine	16.709	200	204	0.093	ng	# 78
24) Pentachlorophenol	16.871	266	119	0.080	ng	96
25) Phenanthrene	17.268	178	1083	0.094	ng	96
26) Anthracene	17.355	178	957	0.090	ng	96
28) Fluoranthene	19.299	202	1366	0.097	ng	# 96
30) Pyrene	19.661	202	1481	0.101	ng	98
32) Benzo(a)anthracene	21.429	228	1163	0.095	ng	93
33) Chrysene	21.483	228	1330	0.100	ng	95
34) Bis(2-ethylhexyl)phtha...	21.375	149	1196	0.123	ng	99
36) Indeno(1,2,3-cd)pyrene	26.232	276	1549	0.095	ng	# 85
37) Benzo(b)fluoranthene	23.090	252	1275	0.093	ng	# 60
38) Benzo(k)fluoranthene	23.136	252	1324	0.095	ng	# 57
39) Benzo(a)pyrene	23.698	252	1146	0.095	ng	# 45
40) Dibenzo(a,h)anthracene	26.262	278	1153	0.090	ng	# 55
41) Benzo(g,h,i)perylene	26.963	276	1444	0.097	ng	# 78

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030524\
Data File : BN030268.D
Acq On : 05 Mar 2024 12:46
Operator : MA/JU
Sample : SSTDICC0.1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Quant Time: Mar 05 17:43:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN030524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 05 17:02:24 2024
Response via : Initial Calibration








#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.811 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN030268.D
 Acq: 05 Mar 2024 12:46

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1



Tgt Ion: 152 Resp: 1527




Ion	Ratio	Lower	Upper
152	100		
150	150.2	119.4	179.0
115	67.4	56.9	85.3




#2
 1,4-Dioxane
 Concen: 0.128 ng
 RT: 3.326 min Scan# 34
 Delta R.T. 0.007 min
 Lab File: BN030268.D
 Acq: 05 Mar 2024 12:46

Tgt Ion: 88 Resp: 254

Ion	Ratio	Lower	Upper
88	100		
43	44.9	23.8	35.8
58	51.2	46.2	69.4







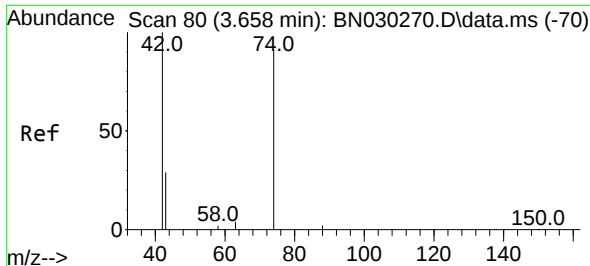

#3
n-Nitrosodimethylamine
Concen: 0.099 ng
RT: 3.665 min Scan# 81
Delta R.T. 0.007 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion: 42 Resp: 206
Ion Ratio Lower Upper
42 100
74 95.1 79.4 119.0
44 21.8 0.0 0.0#



#4
2-Fluorophenol
Concen: 0.105 ng
RT: 5.384 min Scan# 319
Delta R.T. -0.000 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46

Tgt Ion: 112 Resp: 421
Ion Ratio Lower Upper
112 100
64 55.6 41.8 62.8
63 33.0 27.1 40.7









#5
Phenol-d6
Concen: 0.088 ng
RT: 6.980 min Scan# 540
Delta R.T. -0.000 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	99	Resp:	369
Ion	Ratio	Lower	Upper
99	100		
42	27.4	19.0	28.6
71	50.9	36.0	54.0



#6
bis(2-Chloroethyl)ether
Concen: 0.086 ng
RT: 7.255 min Scan# 578
Delta R.T. -0.000 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46

Tgt Ion:	93	Resp:	286
Ion	Ratio	Lower	Upper
93	100		
63	75.9	57.7	86.5
95	35.3	28.6	43.0









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.605 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	136	Resp:	3924
Ion	Ratio	Lower	Upper
136	100		
137	13.5	10.5	15.7
54	9.1	6.4	9.6
68	7.0	5.4	8.2



#8
Nitrobenzene-d5
Concen: 0.085 ng
RT: 8.982 min Scan# 787
Delta R.T. 0.011 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46

Tgt Ion:	82	Resp:	306
Ion	Ratio	Lower	Upper
82	100		
128	57.5	32.2	48.2#
54	63.8	47.3	70.9









#9
Naphthalene
Concen: 0.098 ng
RT: 10.658 min Scan# 944
Delta R.T. -0.000 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:128 Resp: 1072
Ion Ratio Lower Upper
128 100
129 18.8 10.8 16.2#
127 21.2 11.7 17.5#



#10
Hexachlorobutadiene
Concen: 0.102 ng
RT: 10.925 min Scan# 969
Delta R.T. -0.000 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46

Tgt Ion:225 Resp: 255
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 62.7 50.6 76.0









#11
2-Methylnaphthalene-d10
Concen: 0.085 ng
RT: 12.208 min Scan# 11
Delta R.T. 0.004 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:152 Resp: 486
Ion Ratio Lower Upper
152 100
151 23.5 16.7 25.1



#12
2-Methylnaphthalene
Concen: 0.092 ng
RT: 12.284 min Scan# 1228
Delta R.T. 0.004 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46

Tgt Ion:142 Resp: 624
Ion Ratio Lower Upper
142 100
141 89.3 74.2 111.4
115 60.2 40.7 61.1





#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.457 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN030268.D

Acq: 05 Mar 2024 12:46

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:164 Resp: 1963

Ion Ratio Lower Upper

164 100

162 105.9 83.4 125.2

160 52.5 41.7 62.5



#14

2,4,6-Tribromophenol

Concen: 0.094 ng

RT: 15.964 min Scan# 1673

Delta R.T. -0.000 min

Lab File: BN030268.D

Acq: 05 Mar 2024 12:46




Tgt Ion:330 Resp: 95


Ion Ratio Lower Upper

330 100

332 107.4 72.6 108.8

141 63.2 41.3 61.9#







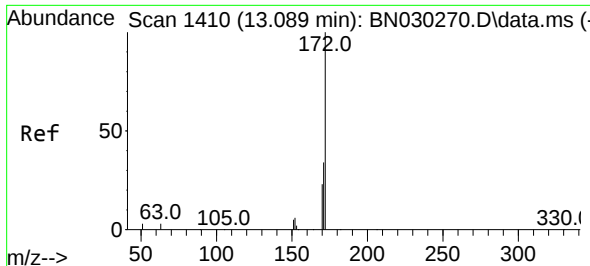

#15
2-Fluorobiphenyl
Concen: 0.093 ng
RT: 13.089 min Scan# 1410
Delta R.T. -0.000 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	172	Resp:	758
Ion Ratio	Lower	Upper	
172	100		
171	41.1	29.0	43.4
170	32.0	20.2	30.2

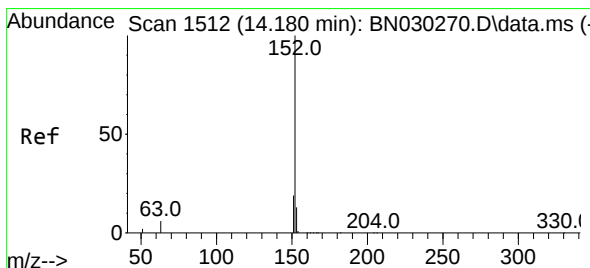

#16
Acenaphthylene
Concen: 0.095 ng
RT: 14.180 min Scan# 1512
Delta R.T. -0.000 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46

Tgt Ion:	152	Resp:	896
Ion Ratio	Lower	Upper	
152	100		
151	19.6	16.1	24.1
153	12.1	10.3	15.5





#17

Acenaphthene

Concen: 0.097 ng

RT: 14.522 min Scan# 11

Delta R.T. -0.000 min

Lab File: BN030268.D

Acq: 05 Mar 2024 12:46

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:154 Resp: 596

Ion Ratio Lower Upper

154 100

153 114.1 92.9 139.3

152 56.9 47.3 70.9



#18

Fluorene

Concen: 0.097 ng

RT: 15.518 min Scan# 1637

Delta R.T. -0.000 min

Lab File: BN030268.D

Acq: 05 Mar 2024 12:46




Tgt Ion:166 Resp: 713


Ion Ratio Lower Upper

166 100

165 98.9 79.9 119.9

167 14.6 11.0 16.4





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.218 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN030268.D

Acq: 05 Mar 2024 12:46

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:188 Resp: 4048

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 10.9 7.8 11.6



#20

4,6-Dinitro-2-methylphenol

Concen: 0.068 ng

RT: 15.629 min Scan# 1646

Delta R.T. 0.012 min

Lab File: BN030268.D

Acq: 05 Mar 2024 12:46




Tgt Ion:198 Resp: 60


Ion Ratio Lower Upper

198 100

51 170.3 67.4 101.2#

105 107.8 50.8 76.2#









#21
4-Bromophenyl-phenylether
Concen: 0.093 ng
RT: 16.424 min Scan# 1710
Delta R.T. 0.012 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:248 Resp: 229
Ion Ratio Lower Upper
248 100
250 103.4 71.3 106.9
141 75.4 88.0 132.0#



#22
Hexachlorobenzene
Concen: 0.099 ng
RT: 16.523 min Scan# 1718
Delta R.T. 0.012 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46

Tgt Ion:284 Resp: 282
Ion Ratio Lower Upper
284 100
142 49.3 41.0 61.6
249 38.3 27.4 41.2





#23

Atrazine

Concen: 0.093 ng

RT: 16.709 min Scan# 1733

Delta R.T. 0.012 min

Lab File: BN030268.D

Acq: 05 Mar 2024 12:46

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:200 Resp: 204

Ion Ratio Lower Upper

200 100

173 51.3 30.8 46.2#

215 63.8 38.7 58.1#



#24

Pentachlorophenol

Concen: 0.080 ng

RT: 16.871 min Scan# 1746

Delta R.T. -0.000 min

Lab File: BN030268.D

Acq: 05 Mar 2024 12:46




Tgt Ion:266 Resp: 119


Ion Ratio Lower Upper

266 100

264 57.1 49.1 73.7

268 59.7 49.2 73.8





#25

Phenanthrene

Concen: 0.094 ng

RT: 17.268 min Scan# 1778

Delta R.T. 0.012 min

Lab File: BN030268.D

Acq: 05 Mar 2024 12:46

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:178 Resp: 1083

Ion Ratio Lower Upper

178 100

176 19.3 16.0 24.0

179 18.5 12.4 18.6



#26

Anthracene

Concen: 0.090 ng

RT: 17.355 min Scan# 1785

Delta R.T. -0.000 min

Lab File: BN030268.D

Acq: 05 Mar 2024 12:46




Tgt Ion:178 Resp: 957


Ion Ratio Lower Upper

178 100

176 20.1 15.3 22.9

179 18.7 12.5 18.7









#27
Fluoranthene-d10
Concen: 0.096 ng
RT: 19.266 min Scan# 2041
Delta R.T. 0.005 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:212 Resp: 1067
Ion Ratio Lower Upper
212 100
106 11.4 8.2 12.4
104 7.8 4.7 7.1#



#28
Fluoranthene
Concen: 0.097 ng
RT: 19.299 min Scan# 2048
Delta R.T. 0.005 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46

Tgt Ion:202 Resp: 1366
Ion Ratio Lower Upper
202 100
101 10.0 6.3 9.5#
203 18.0 13.4 20.0









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.438 min Scan# 2464
Delta R.T. -0.000 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:240 Resp: 3491
Ion Ratio Lower Upper
240 100
120 16.6 12.2 18.2
236 30.8 25.2 37.8



#30
Pyrene
Concen: 0.101 ng
RT: 19.661 min Scan# 2126
Delta R.T. -0.000 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46

Tgt Ion:202 Resp: 1481
Ion Ratio Lower Upper
202 100
200 20.5 16.9 25.3
203 16.6 14.1 21.1









#31
 Terphenyl-d14
 Concen: 0.103 ng
 RT: 19.879 min Scan# 2173
 Delta R.T. -0.000 min
 Lab File: BN030268.D
 Acq: 05 Mar 2024 12:46




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion:244 Resp: 937
 Ion Ratio Lower Upper
 244 100
 212 16.7 9.5 14.3#
 122 20.2 11.8 17.6#



#32
 Benzo(a)anthracene
 Concen: 0.095 ng
 RT: 21.429 min Scan# 2463
 Delta R.T. -0.000 min
 Lab File: BN030268.D
 Acq: 05 Mar 2024 12:46

Tgt Ion:228 Resp: 1163
 Ion Ratio Lower Upper
 228 100
 226 32.6 23.1 34.7
 229 24.6 17.0 25.4







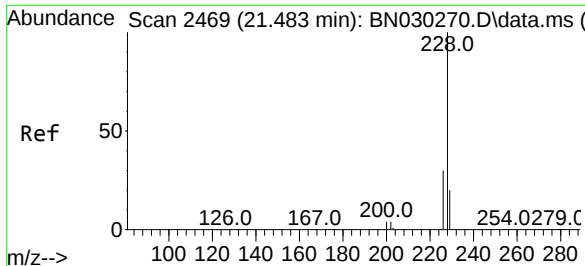

#33
Chrysene
Concen: 0.100 ng
RT: 21.483 min Scan# 2469
Delta R.T. -0.000 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:228 Resp: 1330
Ion Ratio Lower Upper
228 100
226 33.6 24.6 37.0
229 24.0 17.3 25.9

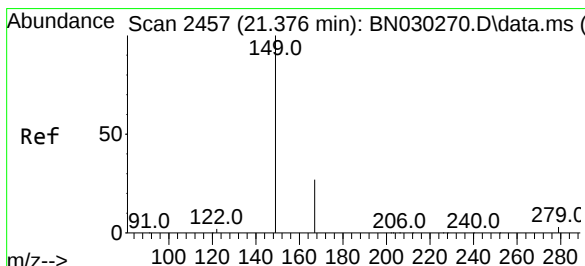

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.123 ng
RT: 21.375 min Scan# 2457
Delta R.T. -0.000 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46

Tgt Ion:149 Resp: 1196
Ion Ratio Lower Upper
149 100
167 26.0 20.6 30.8
279 5.5 4.0 6.0









#35
Perylene-d12
Concen: 0.400 ng
RT: 23.803 min Scan# 3050
Delta R.T. -0.000 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:264 Resp: 3912




Ion	Ratio	Lower	Upper
264	100		
260	26.1	21.7	32.5
265	64.2	50.8	76.2




#36
Indeno(1,2,3-cd)pyrene
Concen: 0.095 ng
RT: 26.232 min Scan# 3881
Delta R.T. 0.006 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46

Tgt Ion:276 Resp: 1549


Ion	Ratio	Lower	Upper
276	100		
138	8.2	17.4	26.2#
277	24.7	18.9	28.3








#37
Benzo(b)fluoranthene
Concen: 0.093 ng
RT: 23.090 min Scan# 21
Delta R.T. 0.003 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1







Tgt Ion:252 Resp: 1275
Ion Ratio Lower Upper
252 100
253 56.9 25.4 38.0#
125 23.1 10.0 15.0#



#38
Benzo(k)fluoranthene
Concen: 0.095 ng
RT: 23.136 min Scan# 2822
Delta R.T. 0.006 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46

Tgt Ion:252 Resp: 1324
Ion Ratio Lower Upper
252 100
253 58.6 25.7 38.5#
125 27.4 11.5 17.3#









#39
Benzo(a)pyrene
Concen: 0.095 ng
RT: 23.698 min Scan# 3014
Delta R.T. -0.000 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:252 Resp: 1146
Ion Ratio Lower Upper
252 100
253 75.1 30.8 46.2#
125 32.7 12.5 18.7#



#40
Dibenzo(a,h)anthracene
Concen: 0.090 ng
RT: 26.262 min Scan# 3891
Delta R.T. 0.003 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46


Tgt Ion:278 Resp: 1153
Ion Ratio Lower Upper
278 100
139 34.6 15.5 23.3#
279 63.9 27.3 40.9#





#41
Benzo(g,h,i)perylene
Concen: 0.097 ng
RT: 26.963 min Scan# 41
Delta R.T. -0.000 min
Lab File: BN030268.D
Acq: 05 Mar 2024 12:46

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1



Tgt Ion:276 Resp: 1444
Ion Ratio Lower Upper
276 100
277 36.5 20.6 30.8#
138 33.3 18.2 27.4#

