

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030524\
 Data File : BN030272.D
 Acq On : 05 Mar 2024 15:11
 Operator : MA/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: Mar 05 16:55:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN030524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 05 16:52:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.811	152	1486	0.400	ng	0.00
7) Naphthalene-d8	10.605	136	3794	0.400	ng	0.00
13) Acenaphthene-d10	14.458	164	1906	0.400	ng	0.00
19) Phenanthrene-d10	17.218	188	4054	0.400	ng	0.00
29) Chrysene-d12	21.438	240	3687	0.400	ng	0.00
35) Perylene-d12	23.800	264	3900	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.384	112	6216	1.593	ng	0.00
5) Phenol-d6	6.973	99	6964	1.697	ng	0.00
8) Nitrobenzene-d5	8.971	82	5907	1.706	ng	0.00
11) 2-Methylnaphthalene-d10	12.200	152	9365	1.701	ng	0.00
14) 2,4,6-Tribromophenol	15.952	330	1695	1.729	ng	-0.01
15) 2-Fluorobiphenyl	13.078	172	13476	1.702	ng	-0.01
27) Fluoranthene-d10	19.262	212	18719	1.682	ng	0.00
31) Terphenyl-d14	19.875	244	15468	1.618	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.319	88	2843	1.475	ng	95
3) n-Nitrosodimethylamine	3.644	42	3307	1.638	ng	# 96
6) bis(2-Chloroethyl)ether	7.248	93	5544	1.704	ng	97
9) Naphthalene	10.648	128	17368	1.639	ng	96
10) Hexachlorobutadiene	10.925	225	3921	1.621	ng	# 100
12) 2-Methylnaphthalene	12.272	142	11001	1.683	ng	98
16) Acenaphthylene	14.180	152	15596	1.695	ng	99
17) Acenaphthene	14.522	154	9989	1.683	ng	99
18) Fluorene	15.505	166	12272	1.718	ng	99
20) 4,6-Dinitro-2-methylph...	15.605	198	1577	1.874	ng	# 60
21) 4-Bromophenyl-phenylether	16.411	248	4195	1.693	ng	90
22) Hexachlorobenzene	16.511	284	4744	1.656	ng	99
23) Atrazine	16.697	200	3728	1.697	ng	# 90
24) Pentachlorophenol	16.871	266	2657	1.780	ng	97
25) Phenanthrene	17.255	178	19792	1.707	ng	99
26) Anthracene	17.355	178	18272	1.715	ng	99
28) Fluoranthene	19.294	202	24121	1.708	ng	99
30) Pyrene	19.656	202	24872	1.607	ng	100
32) Benzo(a)anthracene	21.420	228	21507	1.664	ng	97
33) Chrysene	21.474	228	23097	1.651	ng	98
34) Bis(2-ethylhexyl)phtha...	21.375	149	15246	1.480	ng	# 99
36) Indeno(1,2,3-cd)pyrene	26.218	276	27468	1.681	ng	# 86
37) Benzo(b)fluoranthene	23.081	252	23420	1.719	ng	# 87
38) Benzo(k)fluoranthene	23.131	252	23659	1.708	ng	# 87
39) Benzo(a)pyrene	23.692	252	20559	1.708	ng	# 81
40) Dibenzo(a,h)anthracene	26.247	278	22326	1.738	ng	# 88
41) Benzo(g,h,i)perylene	26.961	276	24672	1.666	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030524\
Data File : BN030272.D
Acq On : 05 Mar 2024 15:11
Operator : MA/JU
Sample : SSTDICC1.6
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Quant Time: Mar 05 16:55:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN030524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 05 16:52:50 2024
Response via : Initial Calibration

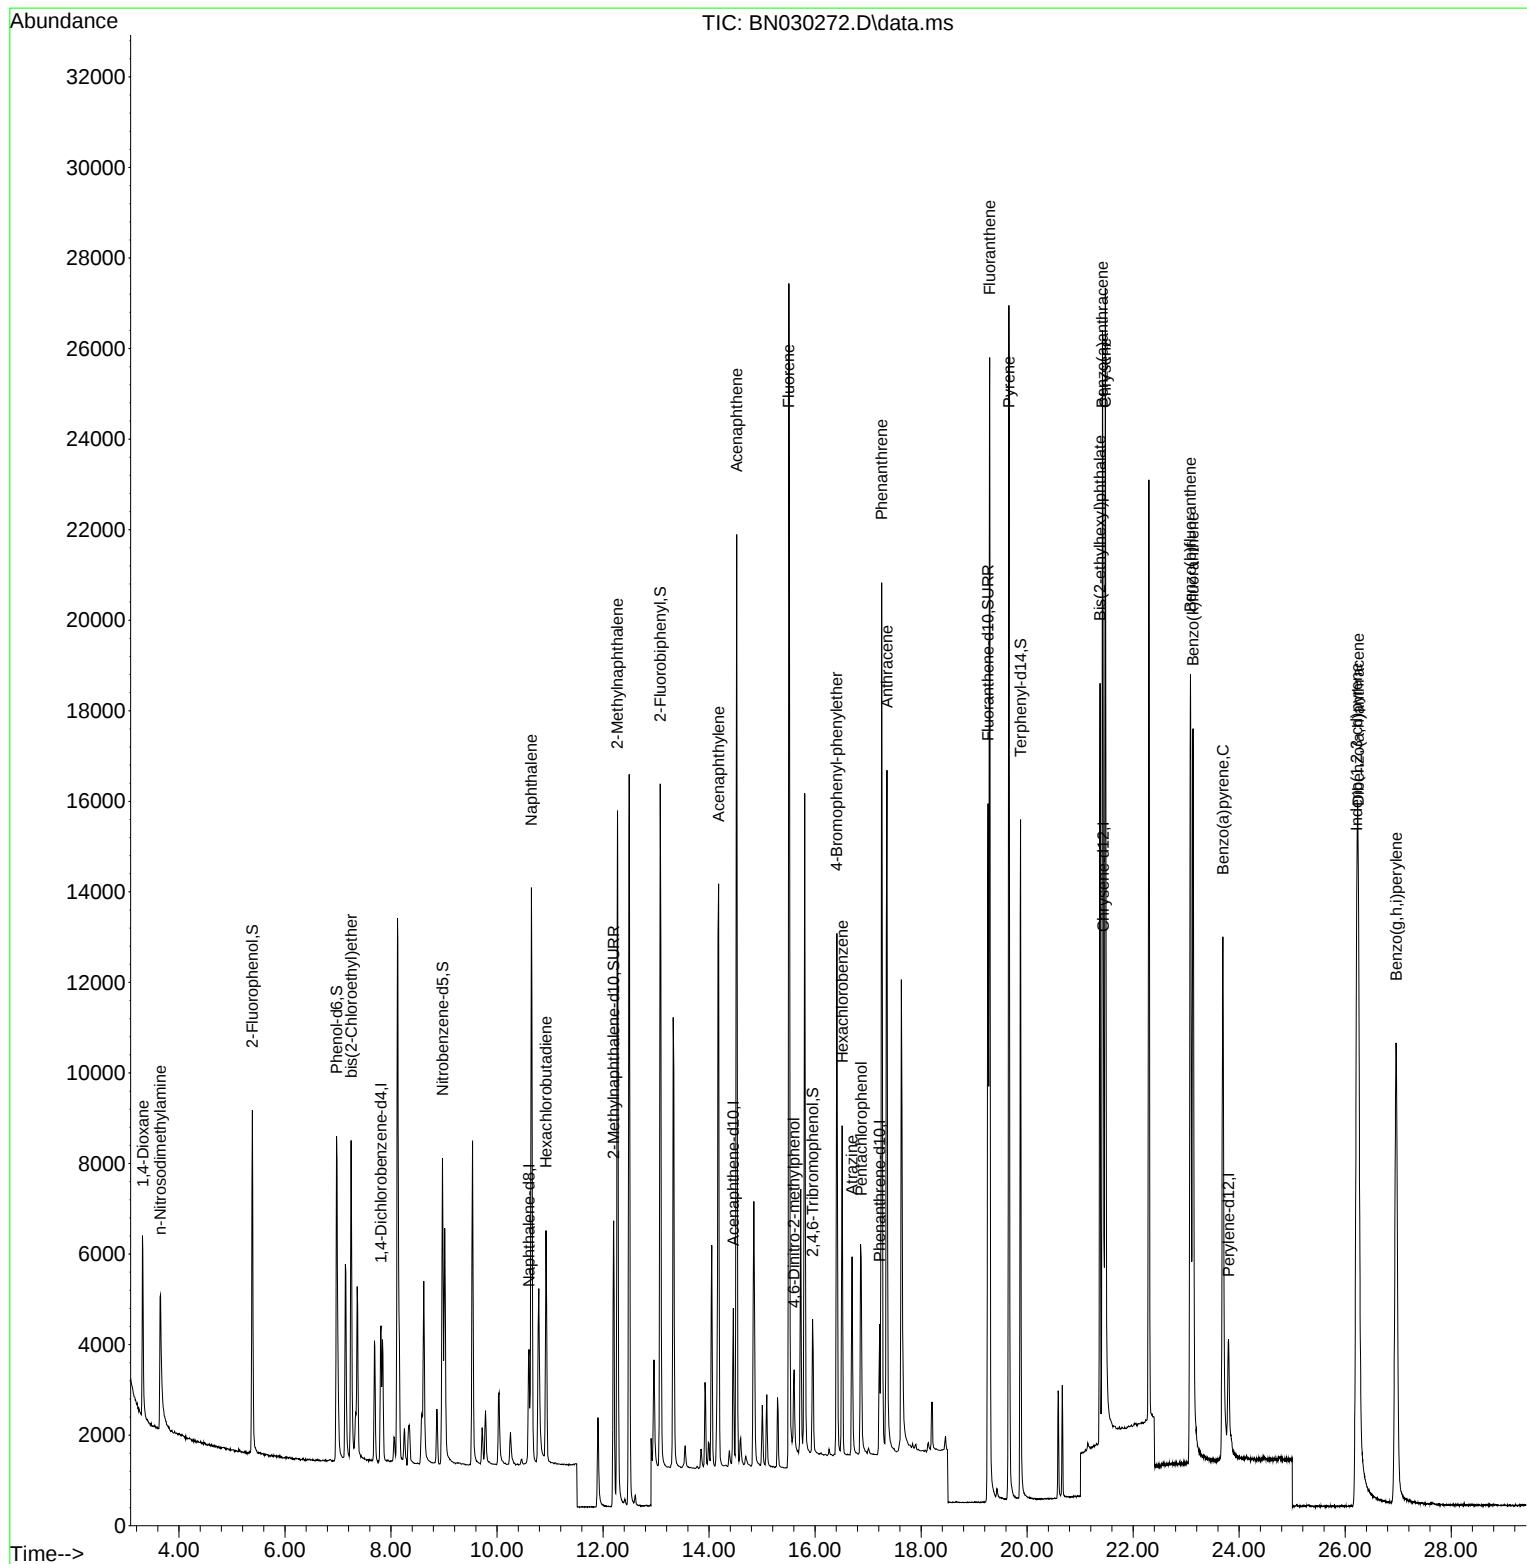






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.811 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN030272.D
 Acq: 05 Mar 2024 15:11

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6



Tgt Ion:152 Resp: 1486




Ion	Ratio	Lower	Upper
152	100		
150	148.4	119.4	179.0
115	68.4	56.9	85.3

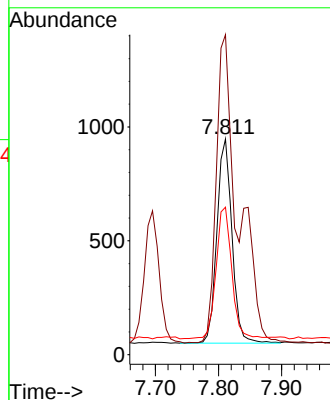


#2
 1,4-Dioxane
 Concen: 1.475 ng
 RT: 3.319 min Scan# 33
 Delta R.T. -0.000 min
 Lab File: BN030272.D
 Acq: 05 Mar 2024 15:11

Tgt Ion: 88 Resp: 2843

Ion	Ratio	Lower	Upper
88	100		
43	32.3	23.8	35.8
58	61.6	46.2	69.4

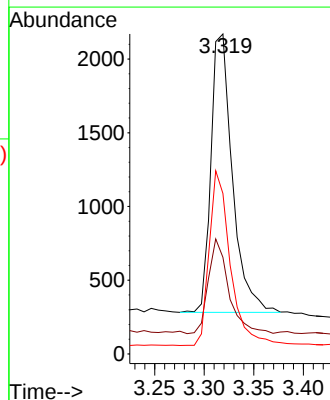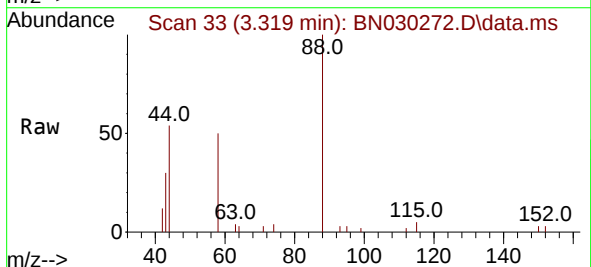

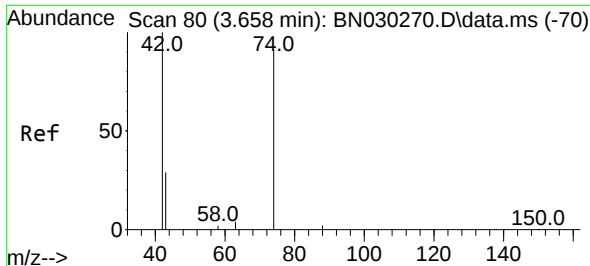

#3

n-Nitrosodimethylamine

Concen: 1.638 ng

RT: 3.644 min Scan# 71

Delta R.T. -0.014 min

Lab File: BN030272.D

Acq: 05 Mar 2024 15:11

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion: 42 Resp: 3307

Ion Ratio Lower Upper

42 100

74 95.4 79.4 119.0

44 3.2 0.0 0.0#

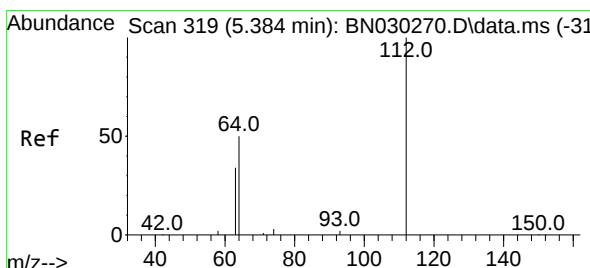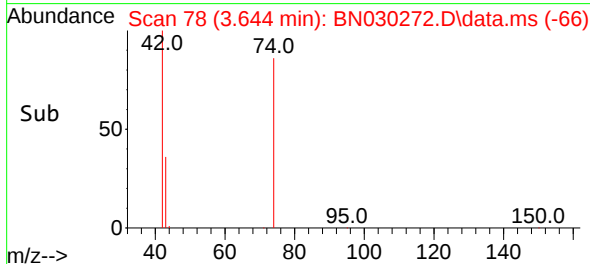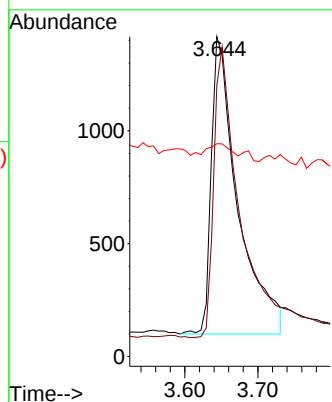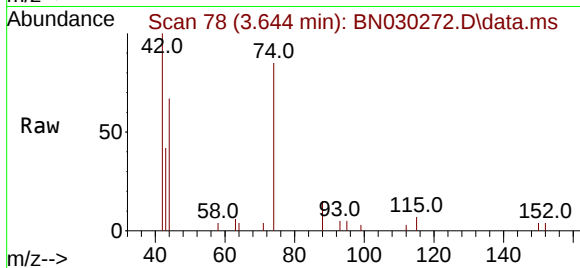

#4

2-Fluorophenol

Concen: 1.593 ng

RT: 5.384 min Scan# 319

Delta R.T. -0.000 min

Lab File: BN030272.D

Acq: 05 Mar 2024 15:11




Tgt Ion: 112 Resp: 6216


Ion Ratio Lower Upper

112 100

64 51.6 41.8 62.8

63 33.6 27.1 40.7


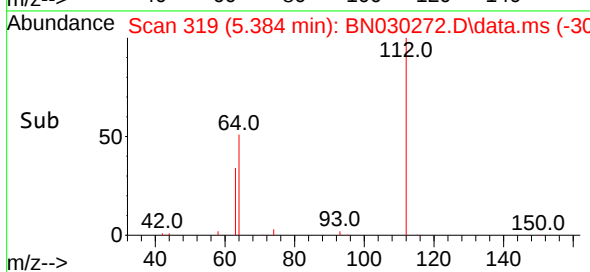
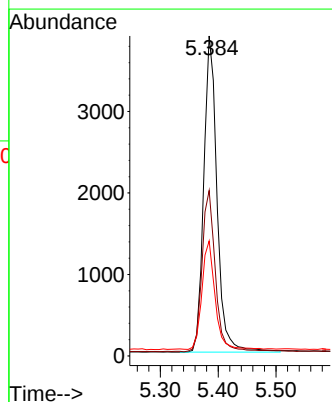
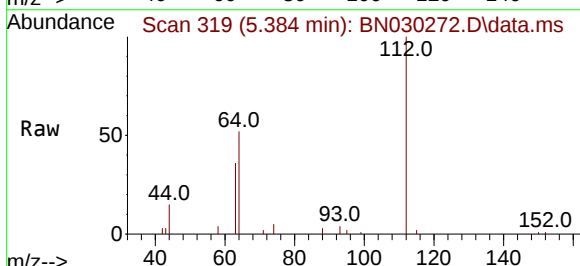




#5
Phenol-d6
Concen: 1.697 ng
RT: 6.973 min Scan# 51
Delta R.T. -0.007 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 99 Resp: 6964
Ion Ratio Lower Upper
99 100
42 23.3 19.0 28.6
71 45.5 36.0 54.0

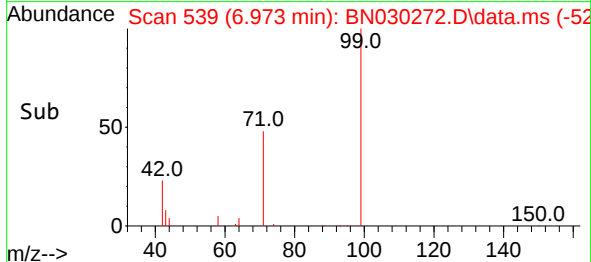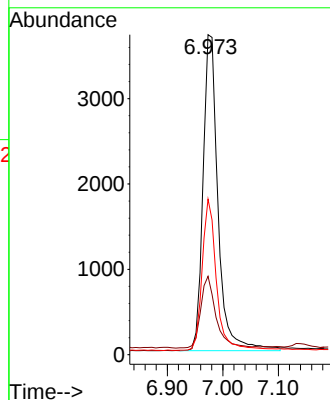

#6
bis(2-Chloroethyl)ether
Concen: 1.704 ng
RT: 7.248 min Scan# 577
Delta R.T. -0.007 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11

Tgt Ion: 93 Resp: 5544
Ion Ratio Lower Upper
93 100
63 69.9 57.7 86.5
95 33.8 28.6 43.0



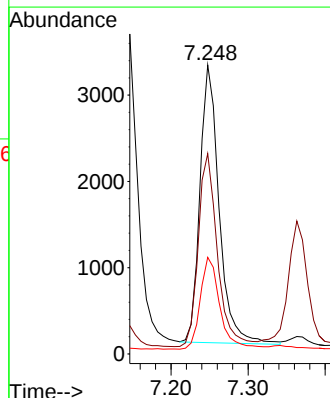





#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.605 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	136	Resp:	3794
Ion	Ratio	Lower	Upper
136	100		
137	13.0	10.5	15.7
54	7.0	6.4	9.6
68	5.7	5.4	8.2

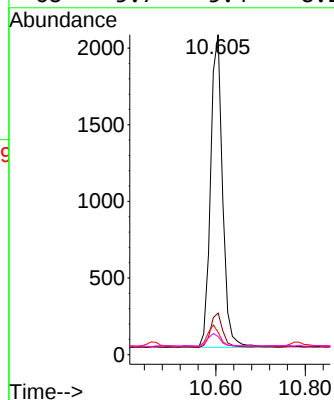

#8
Nitrobenzene-d5
Concen: 1.706 ng
RT: 8.971 min Scan# 786
Delta R.T. -0.000 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11

Tgt Ion:	82	Resp:	5907
Ion	Ratio	Lower	Upper
82	100		
128	39.5	32.2	48.2
54	50.7	47.3	70.9

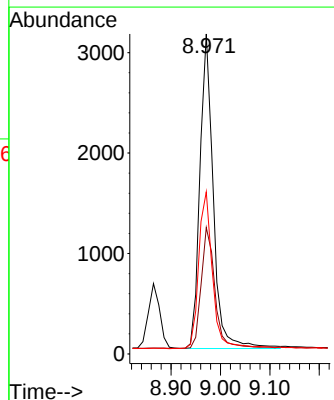

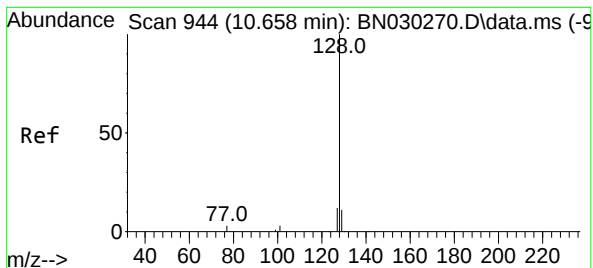

#9

Naphthalene

Concen: 1.639 ng

RT: 10.648 min Scan# 944

Delta R.T. -0.011 min

Lab File: BN030272.D

Acq: 05 Mar 2024 15:11

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:128 Resp: 17368

Ion Ratio Lower Upper

128 100

129 11.4 10.8 16.2

127 13.8 11.7 17.5

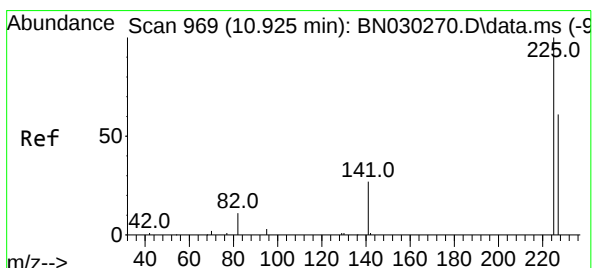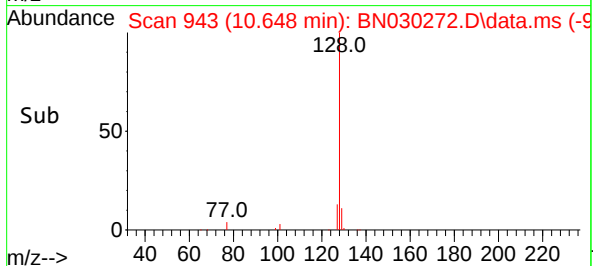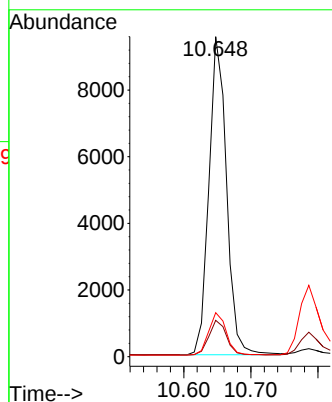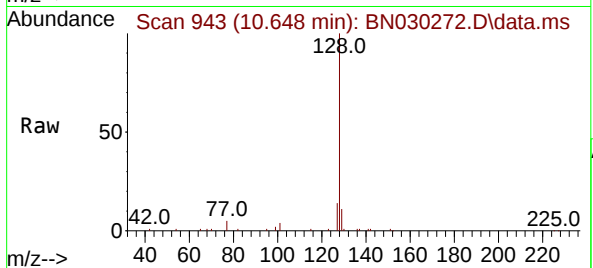

#10

Hexachlorobutadiene

Concen: 1.621 ng

RT: 10.925 min Scan# 969

Delta R.T. -0.000 min

Lab File: BN030272.D

Acq: 05 Mar 2024 15:11




Tgt Ion:225 Resp: 3921


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 63.1 50.6 76.0


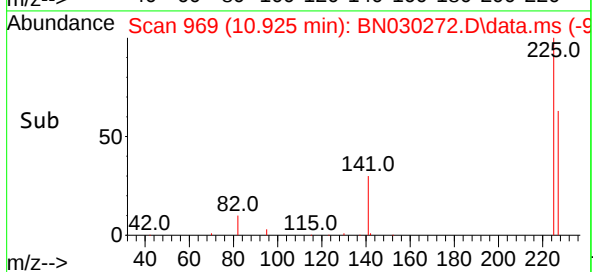
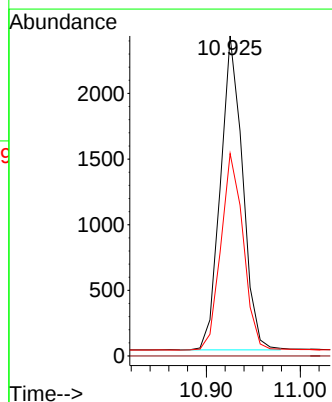
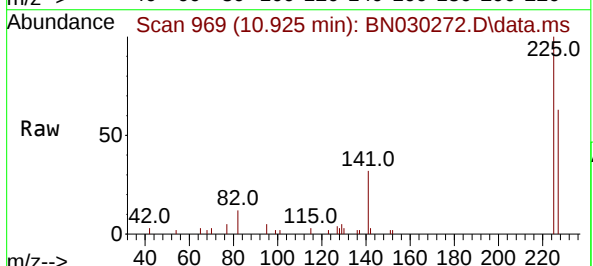




#11
2-Methylnaphthalene-d10
Concen: 1.701 ng
RT: 12.200 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:152 Resp: 9365
Ion Ratio Lower Upper
152 100
151 20.6 16.7 25.1



#12
2-Methylnaphthalene
Concen: 1.683 ng
RT: 12.272 min Scan# 1225
Delta R.T. -0.008 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11

Tgt Ion:142 Resp: 11001
Ion Ratio Lower Upper
142 100
141 90.8 74.2 111.4
115 49.5 40.7 61.1




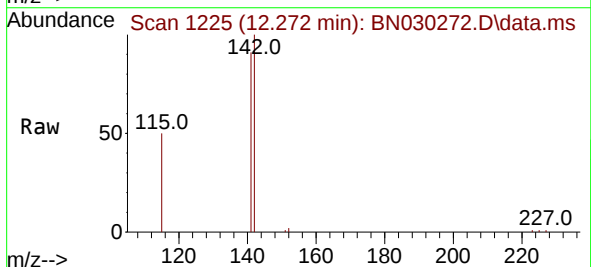




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.458 min Scan# 1538
Delta R.T. -0.000 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:164 Resp: 1906
Ion Ratio Lower Upper
164 100
162 107.1 83.4 125.2
160 50.9 41.7 62.5



#14
2,4,6-Tribromophenol
Concen: 1.729 ng
RT: 15.952 min Scan# 1672
Delta R.T. -0.012 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11

Tgt Ion:330 Resp: 1695
Ion Ratio Lower Upper
330 100
332 95.2 72.6 108.8
141 53.9 41.3 61.9




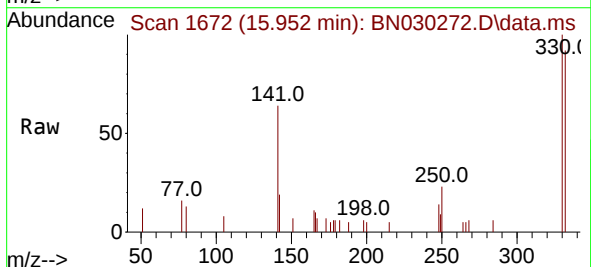


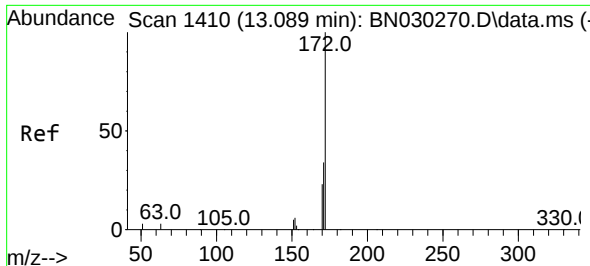

#15
2-Fluorobiphenyl
Concen: 1.702 ng
RT: 13.078 min Scan# 1410
Delta R.T. -0.011 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	172	Resp:	13476
Ion Ratio	Lower	Upper	
172	100		
171	35.6	29.0	43.4
170	25.0	20.2	30.2

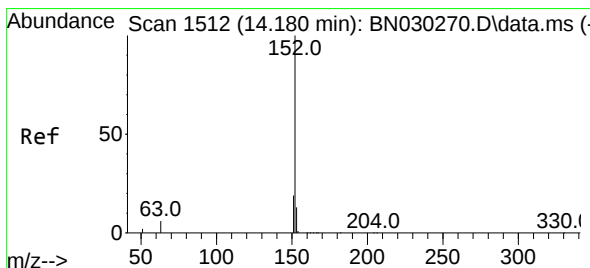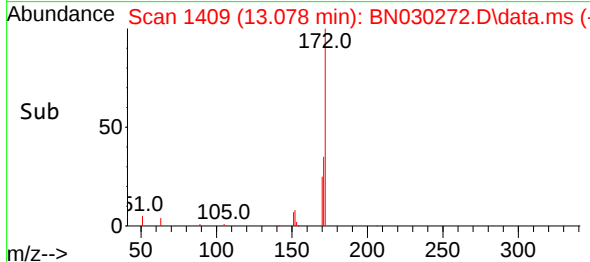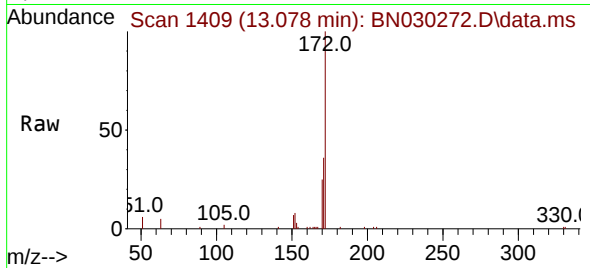

#16
Acenaphthylene
Concen: 1.695 ng
RT: 14.180 min Scan# 1512
Delta R.T. -0.000 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11

Tgt Ion:	152	Resp:	15596
Ion Ratio	Lower	Upper	
152	100		
151	19.7	16.1	24.1
153	13.2	10.3	15.5


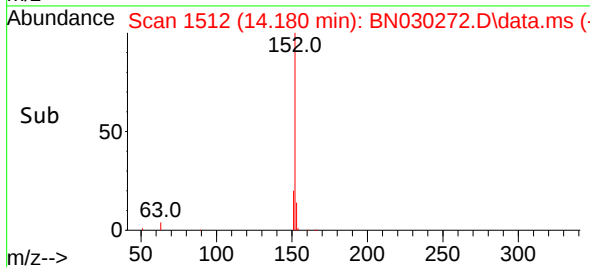

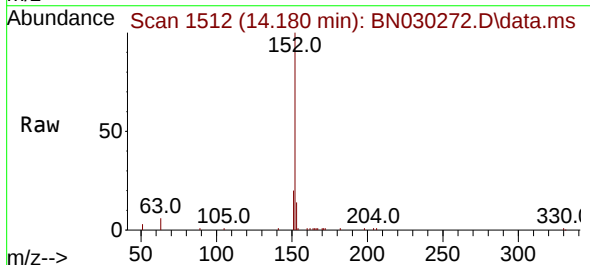




#17
Acenaphthene
Concen: 1.683 ng
RT: 14.522 min Scan# 1544
Delta R.T. -0.000 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:154 Resp: 9989
Ion Ratio Lower Upper
154 100
153 117.0 92.9 139.3
152 59.1 47.3 70.9



#18
Fluorene
Concen: 1.718 ng
RT: 15.505 min Scan# 1636
Delta R.T. -0.012 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11

Tgt Ion:166 Resp: 12272
Ion Ratio Lower Upper
166 100
165 98.5 79.9 119.9
167 13.4 11.0 16.4




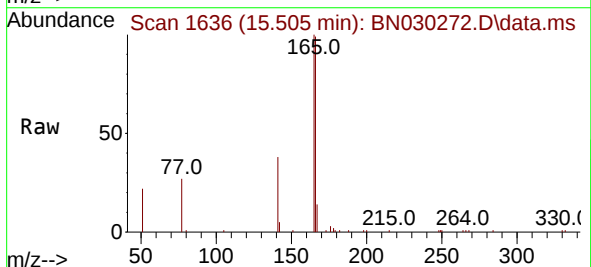


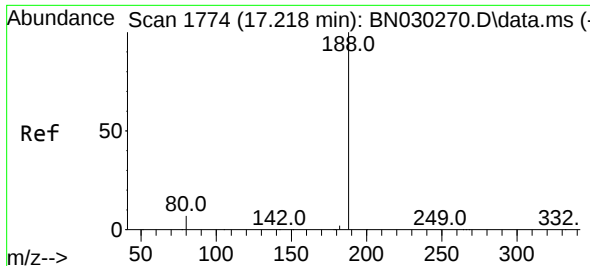

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.218 min Scan# 1774
Delta R.T. -0.000 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:188 Resp: 4054
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.5 7.8 11.6

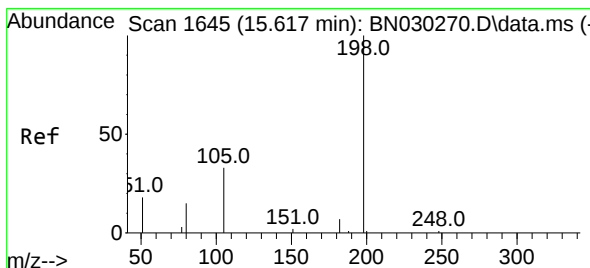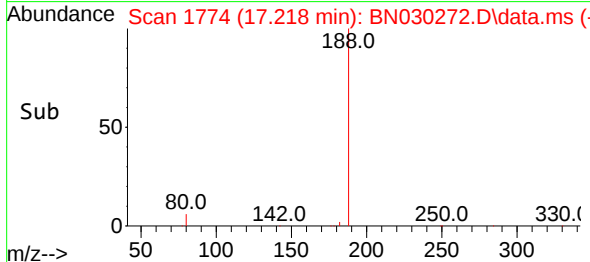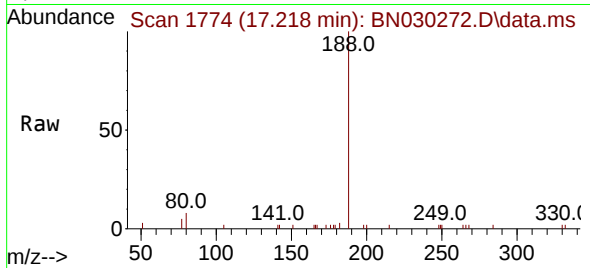

#20
4,6-Dinitro-2-methylphenol
Concen: 1.874 ng
RT: 15.605 min Scan# 1644
Delta R.T. -0.012 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11

Tgt Ion:198 Resp: 1577
Ion Ratio Lower Upper
198 100
51 40.9 67.4 101.2#
105 40.3 50.8 76.2#


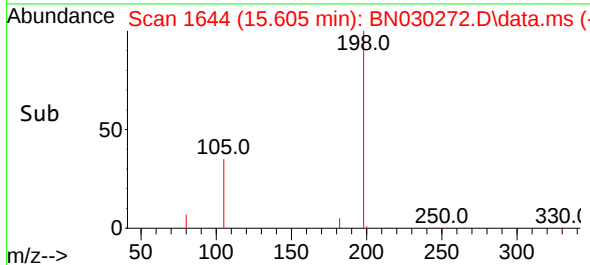

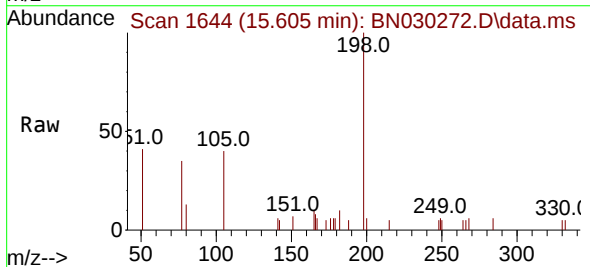




#21
4-Bromophenyl-phenylether
Concen: 1.693 ng
RT: 16.411 min Scan# 1709
Delta R.T. -0.000 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:248 Resp: 4195
Ion Ratio Lower Upper
248 100
250 92.0 71.3 106.9
141 94.1 88.0 132.0

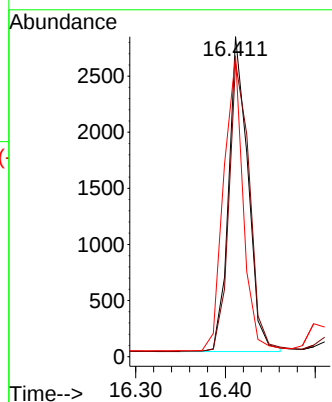

#22
Hexachlorobenzene
Concen: 1.656 ng
RT: 16.511 min Scan# 1717
Delta R.T. -0.000 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11

Tgt Ion:284 Resp: 4744
Ion Ratio Lower Upper
284 100
142 52.2 41.0 61.6
249 33.8 27.4 41.2



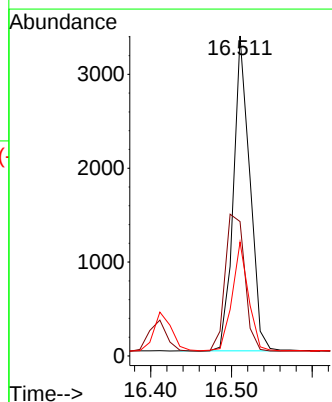
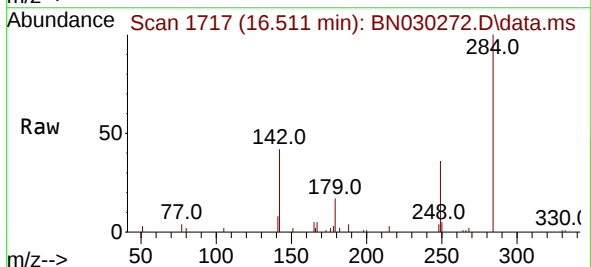




#23
Atrazine
Concen: 1.697 ng
RT: 16.697 min Scan# 1732
Delta R.T. -0.000 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:200 Resp: 3728
Ion Ratio Lower Upper
200 100
173 27.3 30.8 46.2#
215 46.4 38.7 58.1

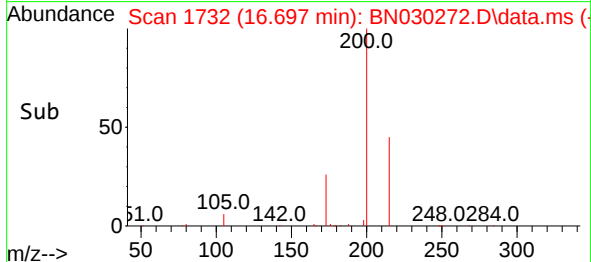

#24
Pentachlorophenol
Concen: 1.780 ng
RT: 16.871 min Scan# 1746
Delta R.T. -0.000 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11

Tgt Ion:266 Resp: 2657
Ion Ratio Lower Upper
266 100
264 62.7 49.1 73.7
268 65.2 49.2 73.8


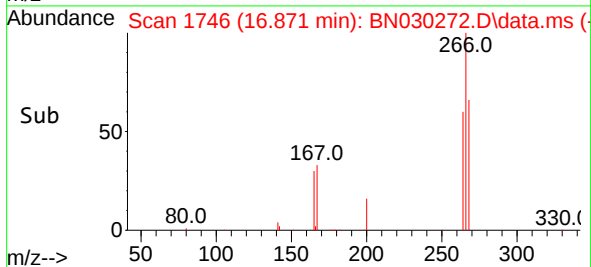

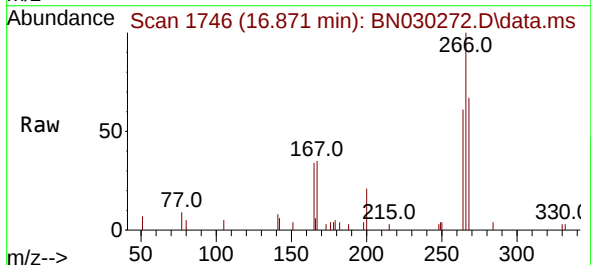


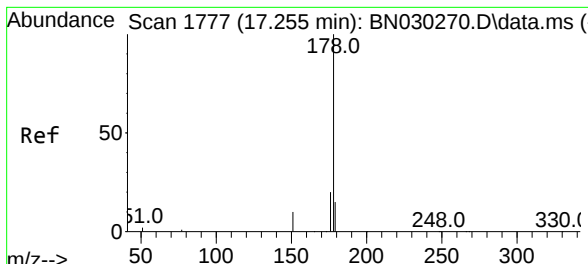

#25
 Phenanthrene
 Concen: 1.707 ng
 RT: 17.255 min Scan# 1777
 Delta R.T. -0.000 min
 Lab File: BN030272.D
 Acq: 05 Mar 2024 15:11




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:	178	Resp:	19792
Ion Ratio	Lower	Upper	
178	100		
176	19.4	16.0	24.0
179	15.2	12.4	18.6

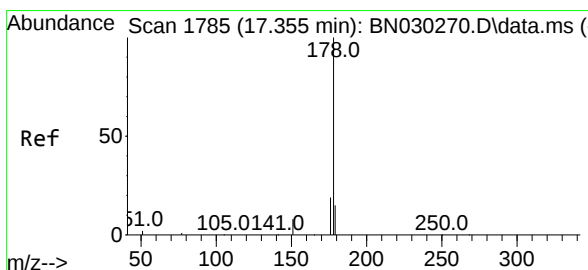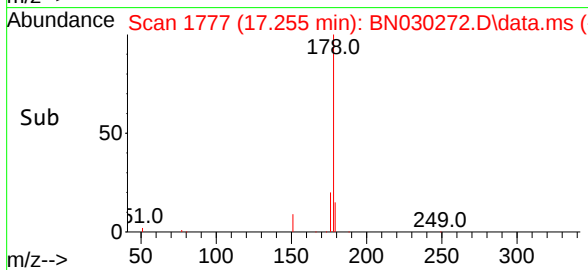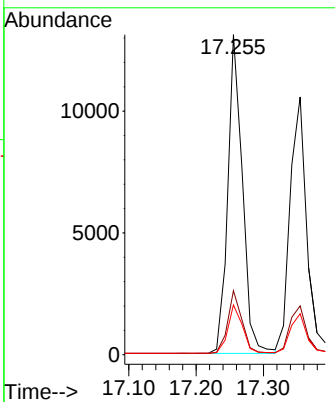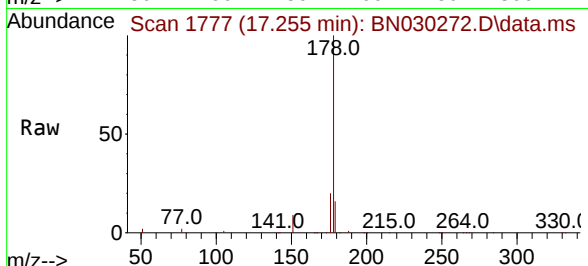

#26
 Anthracene
 Concen: 1.715 ng
 RT: 17.355 min Scan# 1785
 Delta R.T. -0.000 min
 Lab File: BN030272.D
 Acq: 05 Mar 2024 15:11

Tgt Ion:	178	Resp:	18272
Ion Ratio	Lower	Upper	
178	100		
176	18.4	15.3	22.9
179	15.3	12.5	18.7


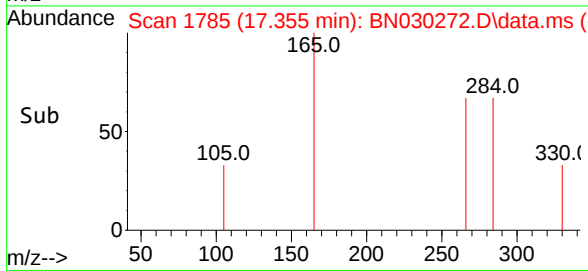
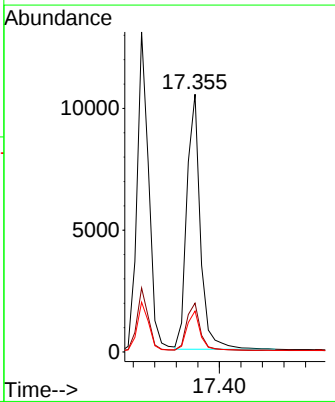
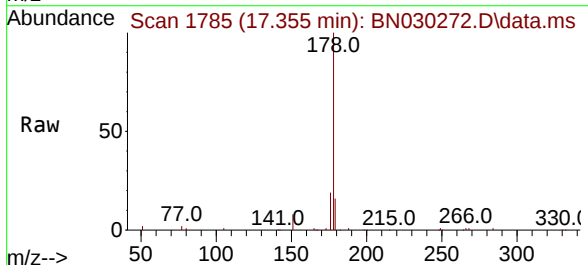




#27
Fluoranthene-d10
Concen: 1.682 ng
RT: 19.262 min Scan# 2040
Delta R.T. -0.000 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:212 Resp: 18719
Ion Ratio Lower Upper
212 100
106 10.4 8.2 12.4
104 6.3 4.7 7.1

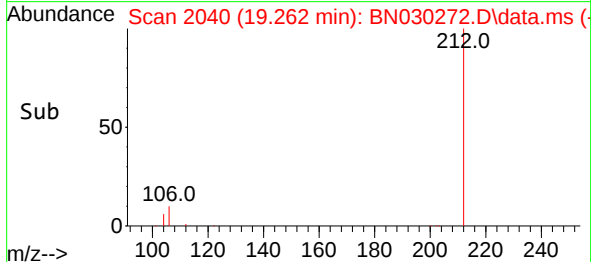

#28
Fluoranthene
Concen: 1.708 ng
RT: 19.294 min Scan# 2047
Delta R.T. -0.000 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11

Tgt Ion:202 Resp: 24121
Ion Ratio Lower Upper
202 100
101 8.6 6.3 9.5
203 17.0 13.4 20.0

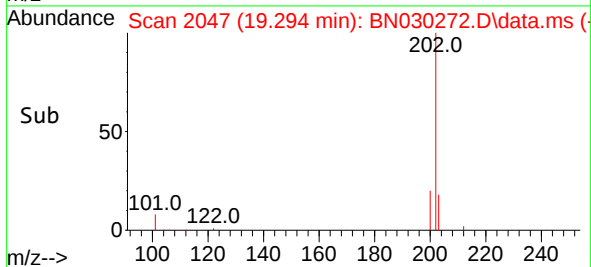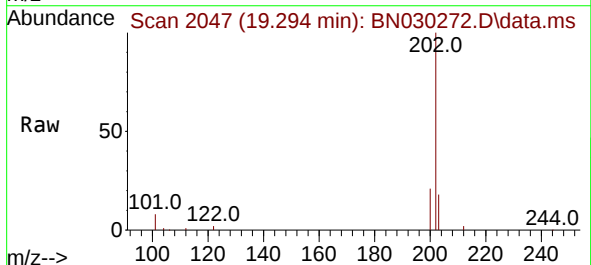

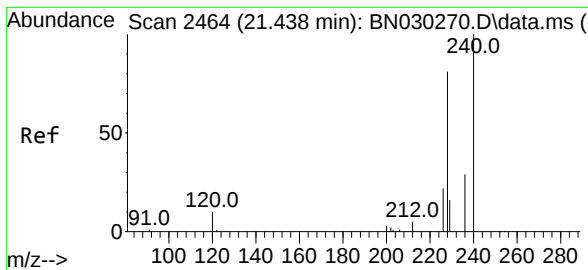

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.438 min Scan# 2464

Delta R.T. -0.000 min

Lab File: BN030272.D

Acq: 05 Mar 2024 15:11

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:240 Resp: 3687

Ion Ratio Lower Upper

240 100

120 12.8 12.2 18.2

236 30.5 25.2 37.8

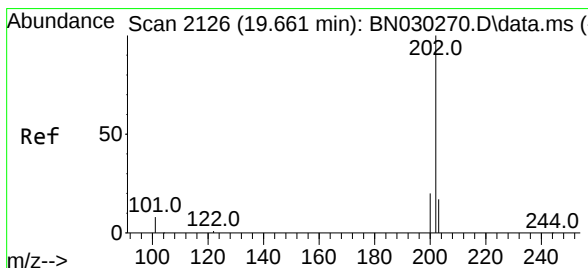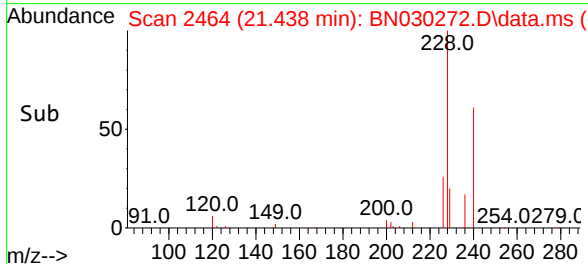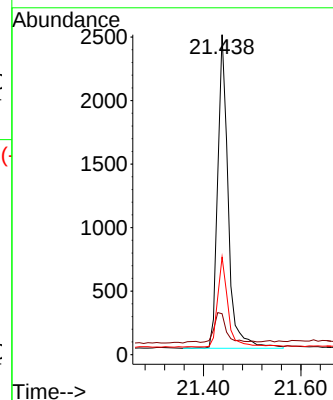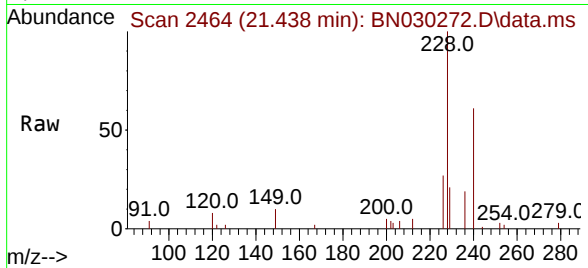

#30

Pyrene

Concen: 1.607 ng

RT: 19.656 min Scan# 2125

Delta R.T. -0.005 min

Lab File: BN030272.D

Acq: 05 Mar 2024 15:11




Tgt Ion:202 Resp: 24872


Ion Ratio Lower Upper

202 100

200 21.3 16.9 25.3

203 17.7 14.1 21.1


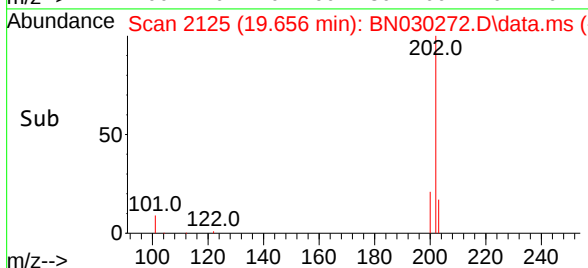
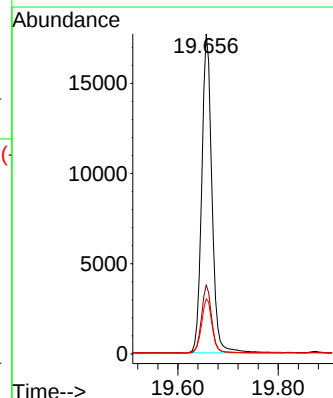
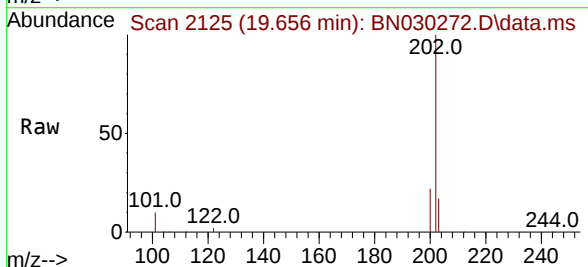




#31
 Terphenyl-d14
 Concen: 1.618 ng
 RT: 19.875 min Scan# 2173
 Delta R.T. -0.005 min
 Lab File: BN030272.D
 Acq: 05 Mar 2024 15:11




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:244 Resp: 15468
 Ion Ratio Lower Upper
 244 100
 212 9.9 9.5 14.3
 122 12.8 11.8 17.6

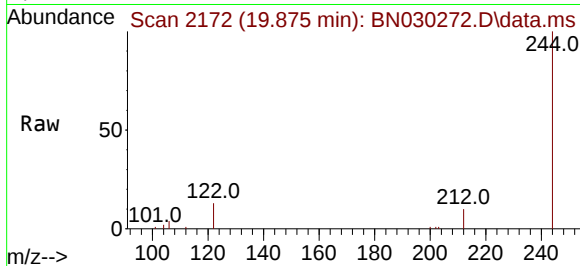

#32
 Benzo(a)anthracene
 Concen: 1.664 ng
 RT: 21.420 min Scan# 2462
 Delta R.T. -0.009 min
 Lab File: BN030272.D
 Acq: 05 Mar 2024 15:11

Tgt Ion:228 Resp: 21507
 Ion Ratio Lower Upper
 228 100
 226 27.6 23.1 34.7
 229 19.3 17.0 25.4




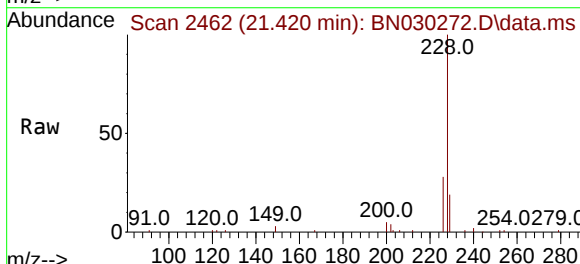


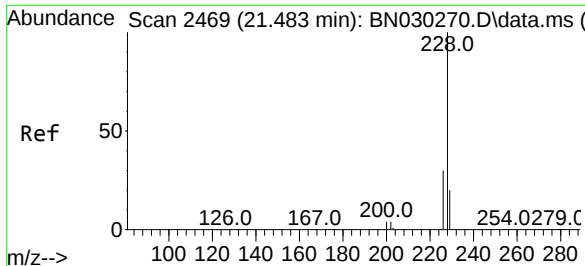

#33
Chrysene
Concen: 1.651 ng
RT: 21.474 min Scan# 2468
Delta R.T. -0.009 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:228 Resp: 23097
Ion Ratio Lower Upper
228 100
226 30.6 24.6 37.0
229 19.4 17.3 25.9

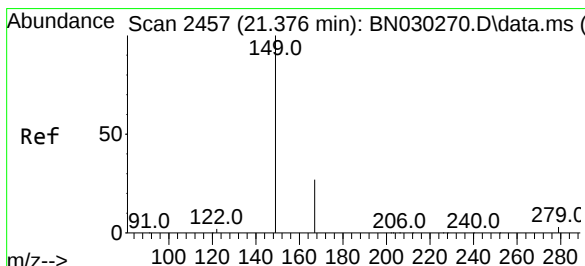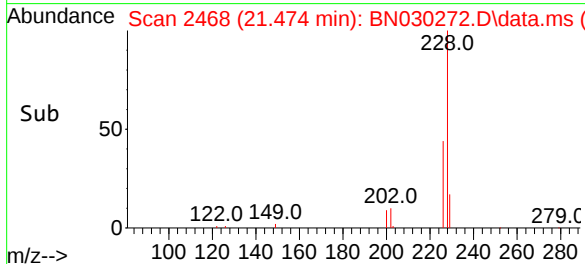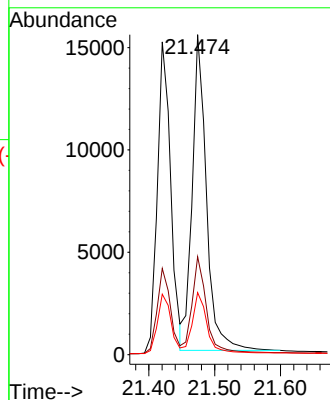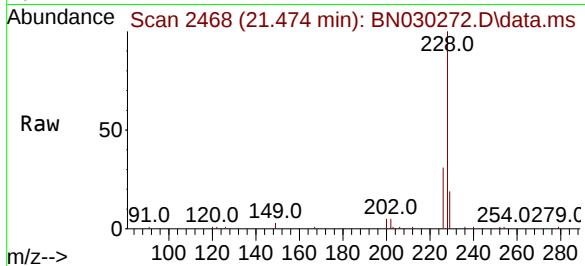

#34
Bis(2-ethylhexyl)phthalate
Concen: 1.480 ng
RT: 21.375 min Scan# 2457
Delta R.T. -0.000 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11

Tgt Ion:149 Resp: 15246
Ion Ratio Lower Upper
149 100
167 25.7 20.6 30.8
279 3.4 4.0 6.0#

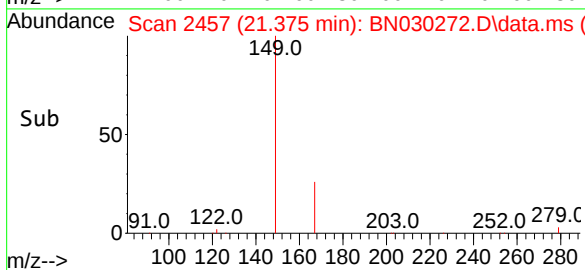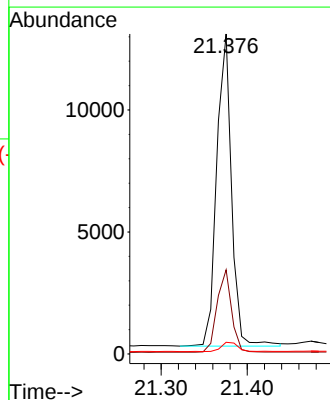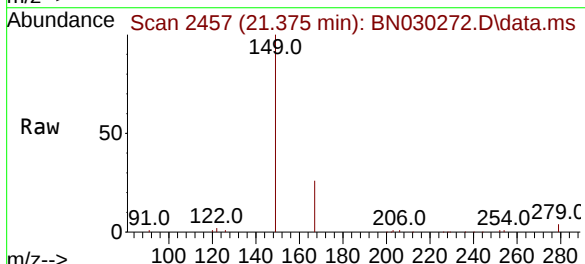



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.800 min Scan# 3049

Delta R.T. -0.003 min

Lab File: BN030272.D


Acq: 05 Mar 2024 15:11

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6






Tgt Ion:264 Resp: 3900

Ion Ratio Lower Upper

264 100

260 26.6 21.7 32.5

265 58.9 50.8 76.2

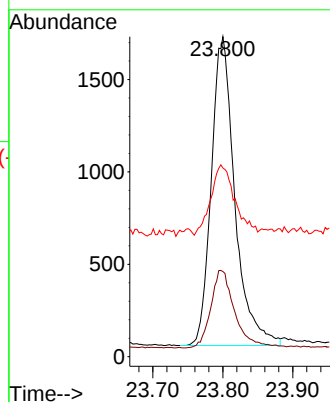

#36

Indeno(1,2,3-cd)pyrene

Concen: 1.681 ng

RT: 26.218 min Scan# 3876

Delta R.T. -0.009 min

Lab File: BN030272.D

Acq: 05 Mar 2024 15:11




Tgt Ion:276 Resp: 27468


Ion Ratio Lower Upper

276 100

138 9.0 17.4 26.2#

277 24.2 18.9 28.3



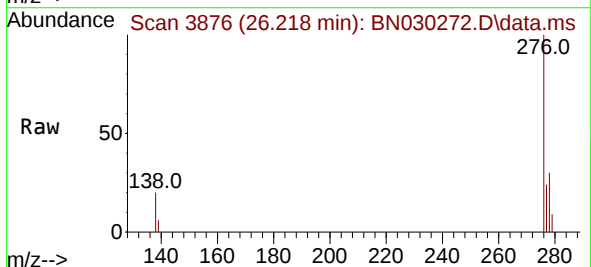
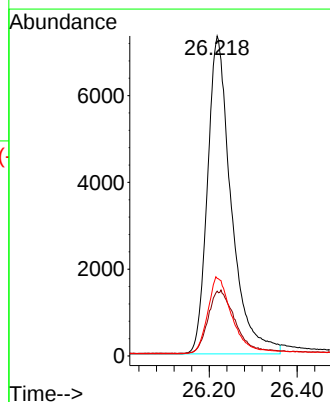


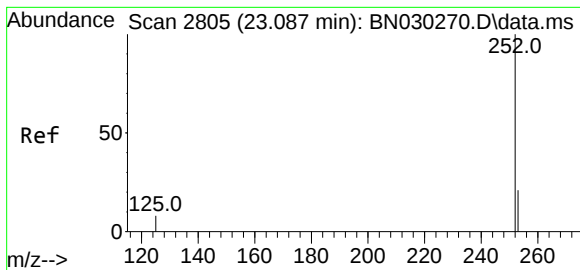

#37
Benzo(b)fluoranthene
Concen: 1.719 ng
RT: 23.081 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 23420
Ion Ratio Lower Upper
252 100
253 23.4 25.4 38.0#
125 9.4 10.0 15.0#

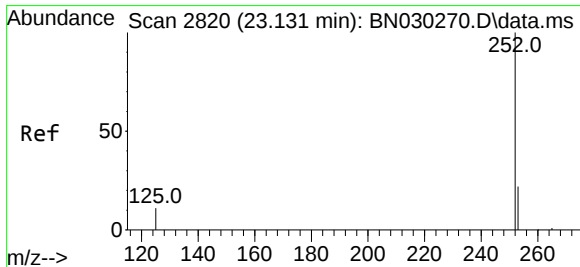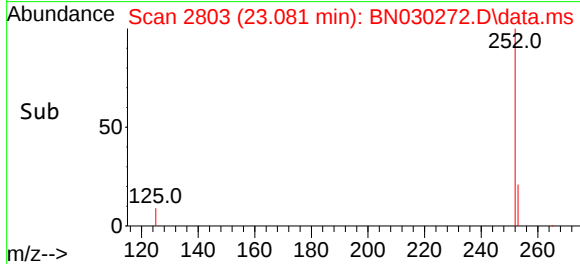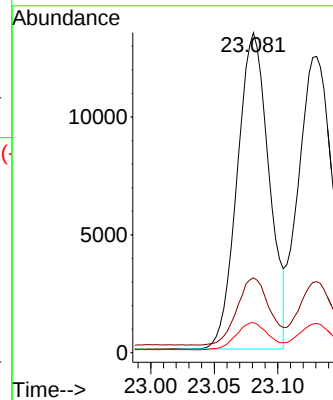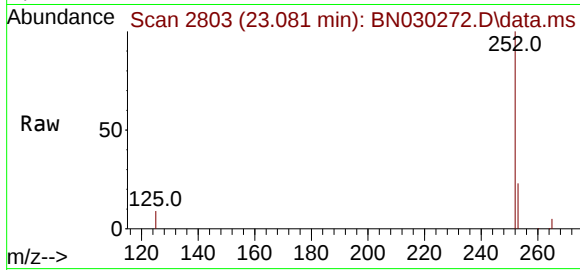

#38
Benzo(k)fluoranthene
Concen: 1.708 ng
RT: 23.131 min Scan# 2820
Delta R.T. -0.000 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11


Tgt Ion:252 Resp: 23659
Ion Ratio Lower Upper
252 100
253 24.0 25.7 38.5#
125 9.9 11.5 17.3#

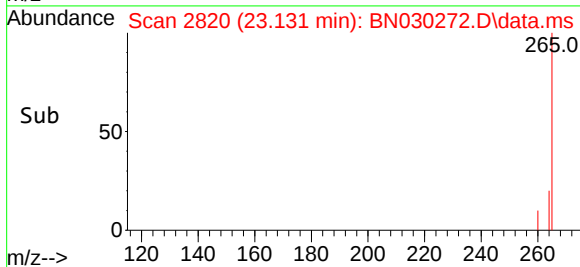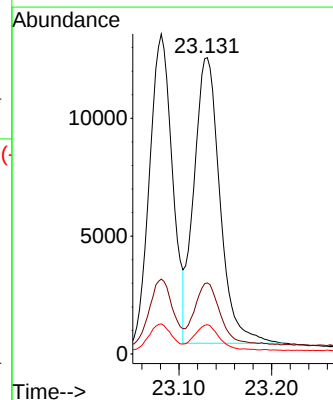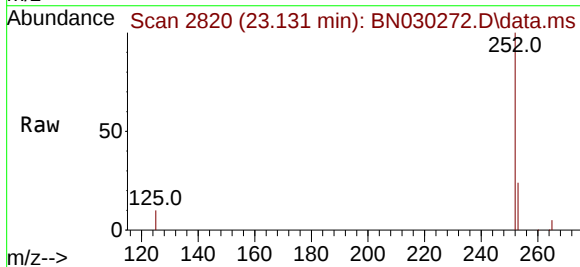






#39
Benzo(a)pyrene
Concen: 1.708 ng
RT: 23.692 min Scan# 3012
Delta R.T. -0.006 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6







Tgt Ion:252 Resp: 20559
Ion Ratio Lower Upper
252 100
253 25.4 30.8 46.2#
125 10.7 12.5 18.7#



#40
Dibenzo(a,h)anthracene
Concen: 1.738 ng
RT: 26.247 min Scan# 3886
Delta R.T. -0.012 min
Lab File: BN030272.D
Acq: 05 Mar 2024 15:11

Tgt Ion:278 Resp: 22326
Ion Ratio Lower Upper
278 100
139 15.7 15.5 23.3
279 26.0 27.3 40.9#

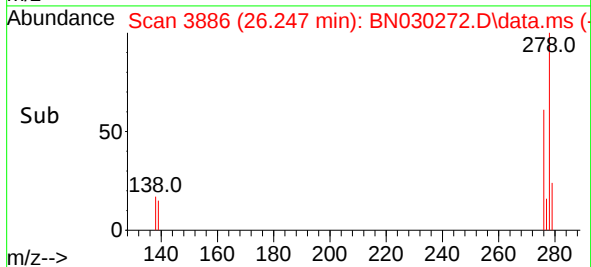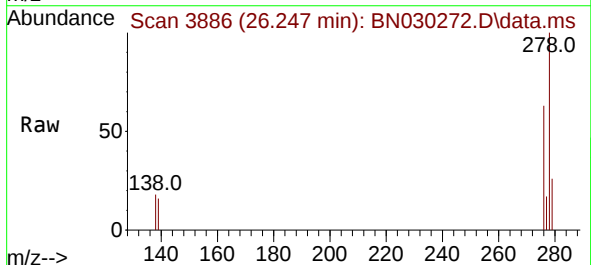

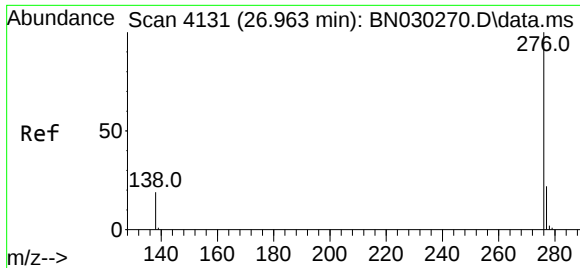

#41
 Benzo(g,h,i)perylene
 Concen: 1.666 ng
 RT: 26.961 min Scan# 41
 Delta R.T. -0.003 min
 Lab File: BN030272.D
 Acq: 05 Mar 2024 15:11

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Tgt Ion:	276	Resp:	24672
Ion Ratio	Lower	Upper	
276	100		
277	23.6	20.6	30.8
138	20.5	18.2	27.4

