
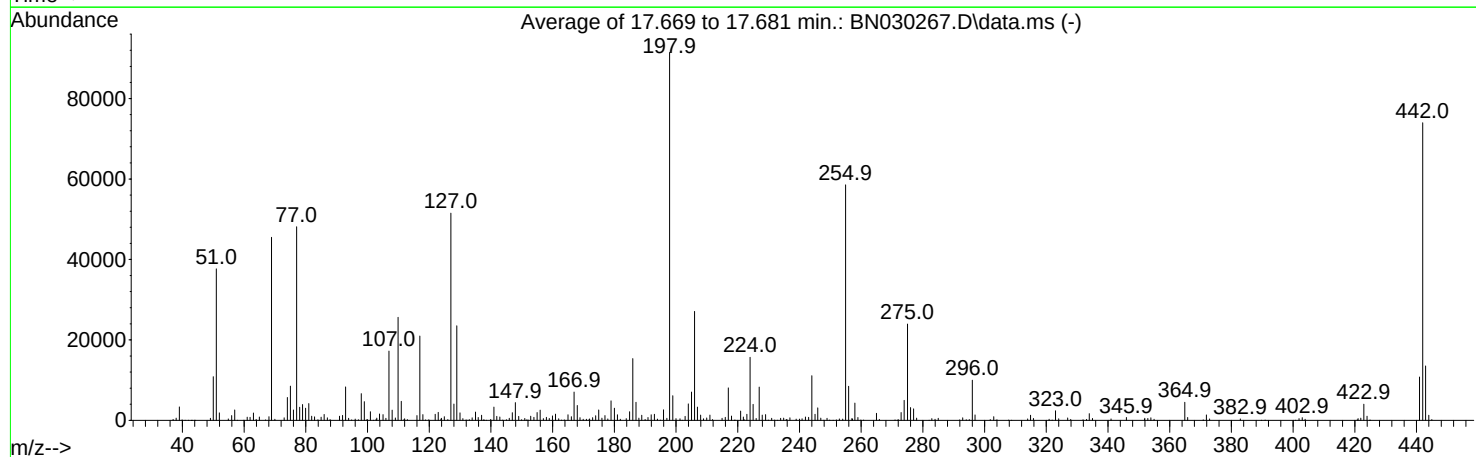


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030524\
Data File : BN030267.D
Acq On : 05 Mar 2024 11:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN030524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 05 17:44:16 2024

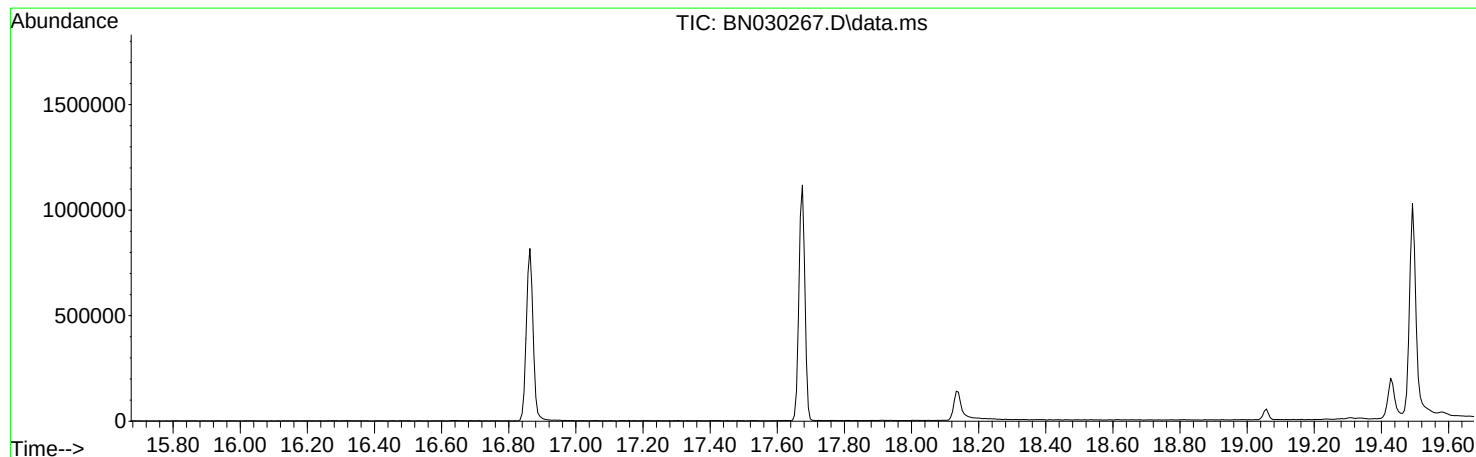




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	37659	PASS
68	69	0.00	2	2.0	929	PASS
69	198	0.00	100	49.8	45509	PASS
70	69	0.00	2	0.6	272	PASS
127	198	10	80	56.3	51504	PASS
197	198	0.00	2	0.6	533	PASS
198	198	100	100	100.0	91445	PASS
199	198	5	9	6.7	6117	PASS
275	198	10	60	26.2	23963	PASS
365	198	1	100	4.9	4498	PASS
441	198	0.01	100	11.8	10798	PASS
442	442	50	100	100.0	73987	PASS
443	442	15	24	18.3	13532	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030524\
Data File : BN030267.D
Acq On : 05 Mar 2024 11:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 06 02:54:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 02:54:35 2024
Response via : Initial Calibration

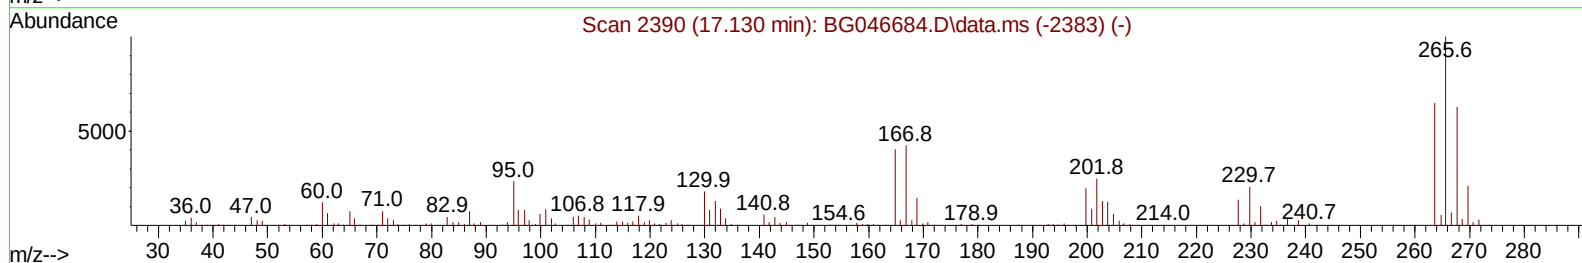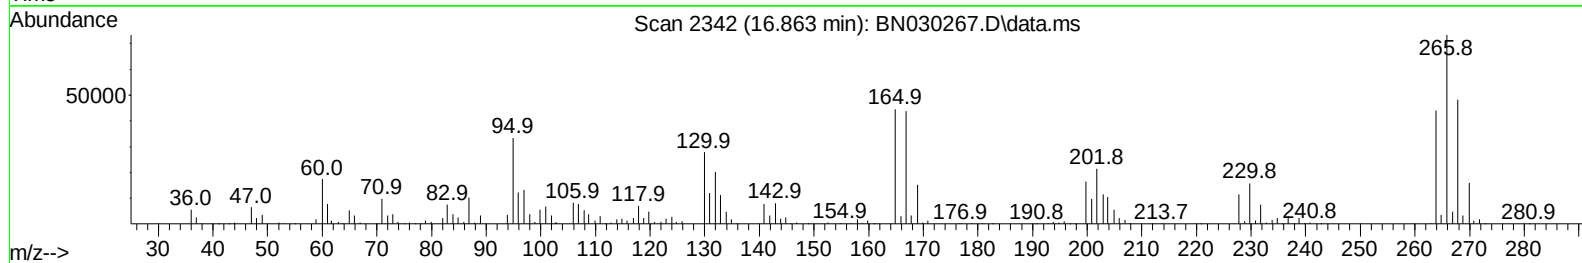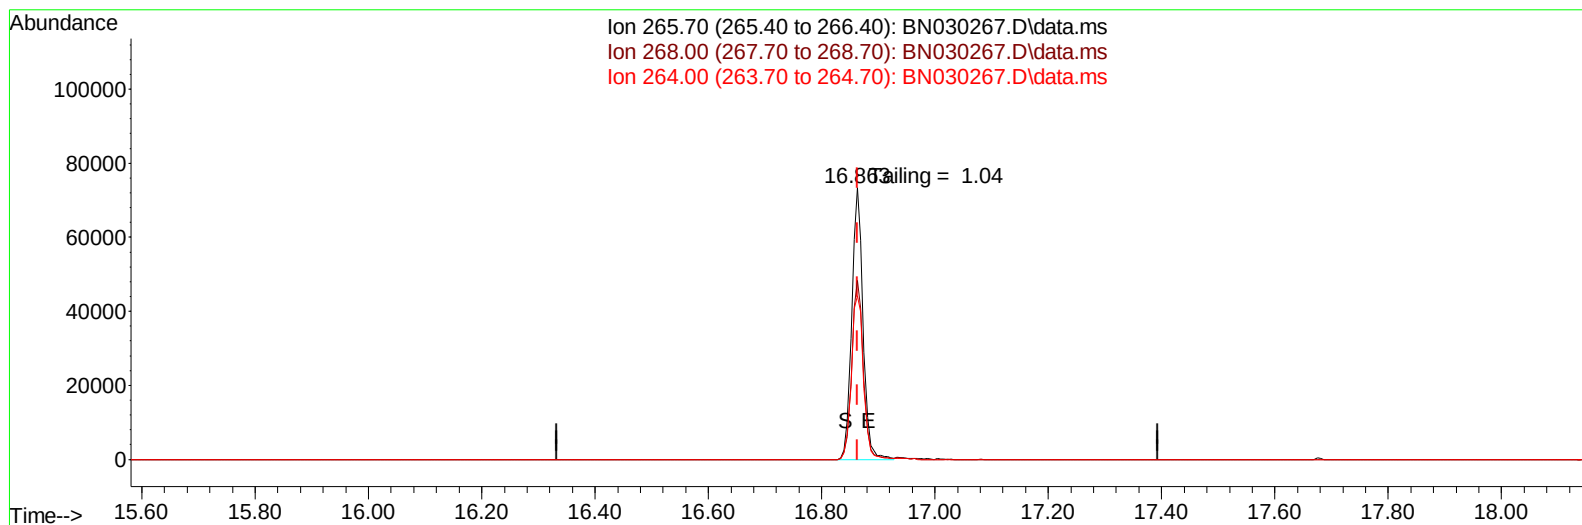

TIC: BN030267.D\data.ms

(70) Pentachlorophenol (C)

16.863min (0.000) 17600.37 ng




response 101935

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.98
264.00	61.60	60.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030524\
Data File : BN030267.D
Acq On : 05 Mar 2024 11:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 06 02:54:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 02:54:35 2024
Response via : Initial Calibration

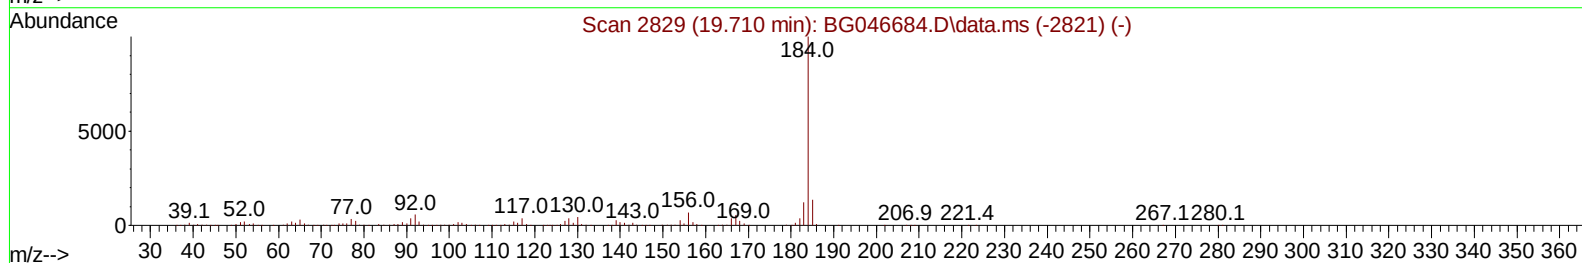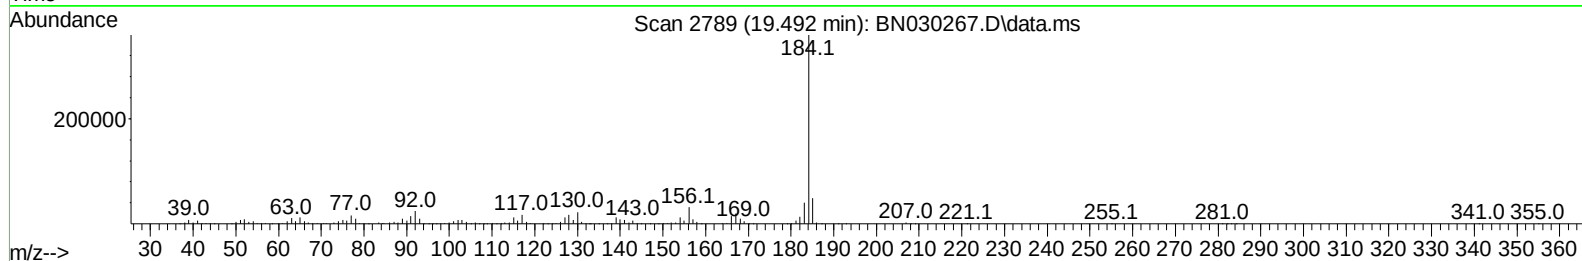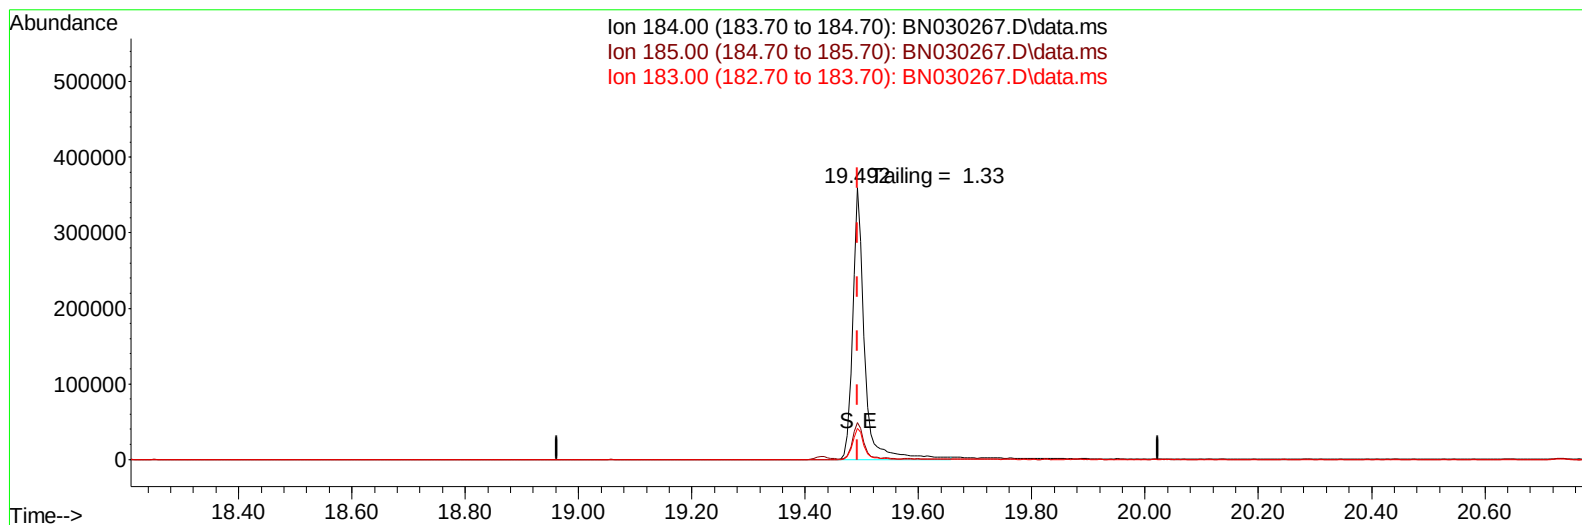

TIC: BN030267.D\data.ms

(77) Benzidine

19.492min (0.000) 0.00 ng

response 520326

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.60
183.00	13.20	11.36
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/5/2024	BNA_N	<u>BN030267.D</u>
Compound Name	Response	Retention Time
DDT	302889	20.733
DDD	9752	20.292
DDE	187	19.725
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9939	312828	3.18

Instrument :
BNA_N
ClientSampleId :
DFTPP