
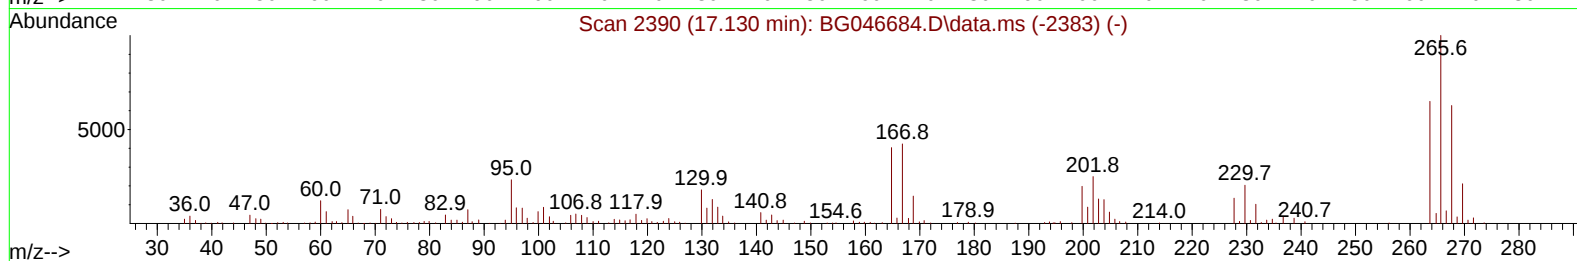
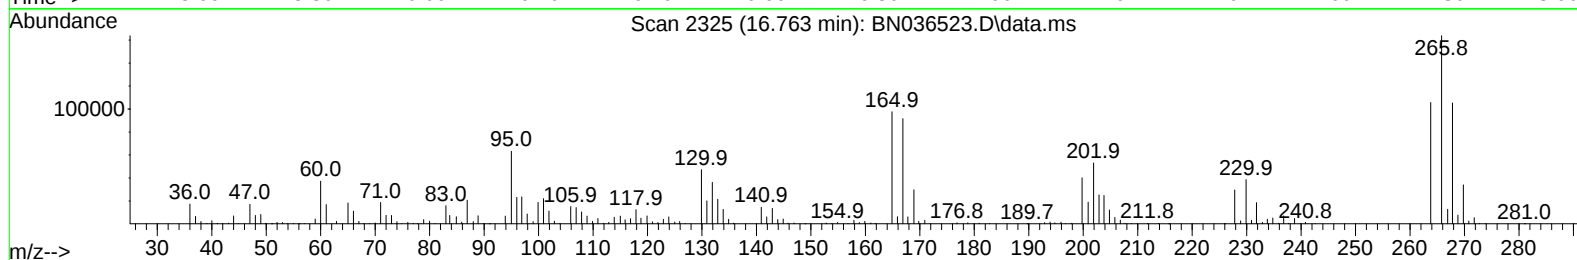


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030525\
Data File : BN036523.D
Acq On : 05 Mar 2025 12:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 16:03:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

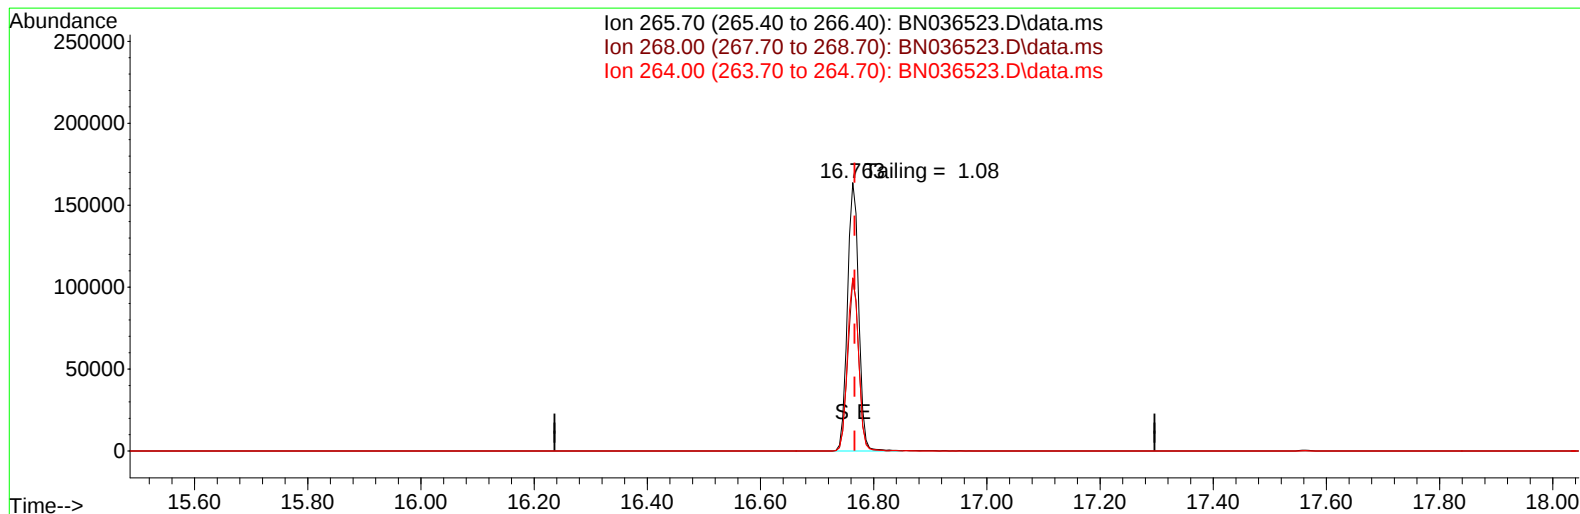

TIC: BN036523.D\data.ms

(70) Pentachlorophenol (C)




16.763min (-0.003) 22410.75 ng

response 227405

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.26
264.00	61.60	64.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030525\
Data File : BN036523.D
Acq On : 05 Mar 2025 12:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 16:03:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

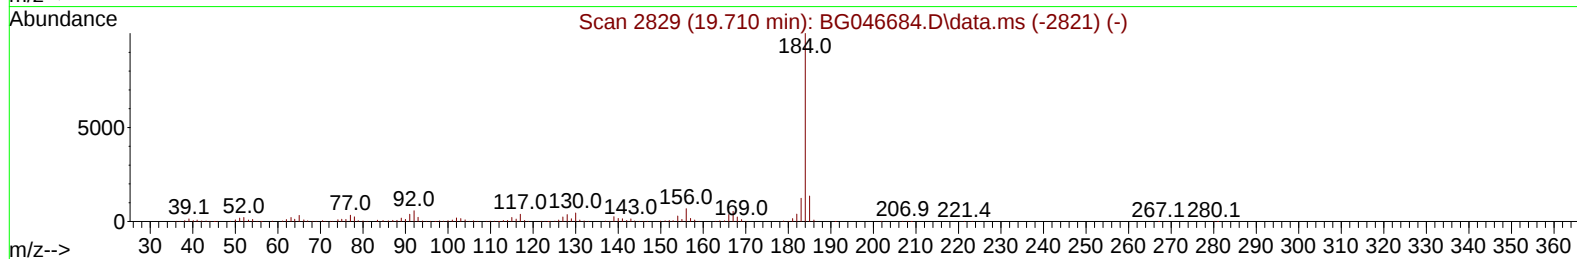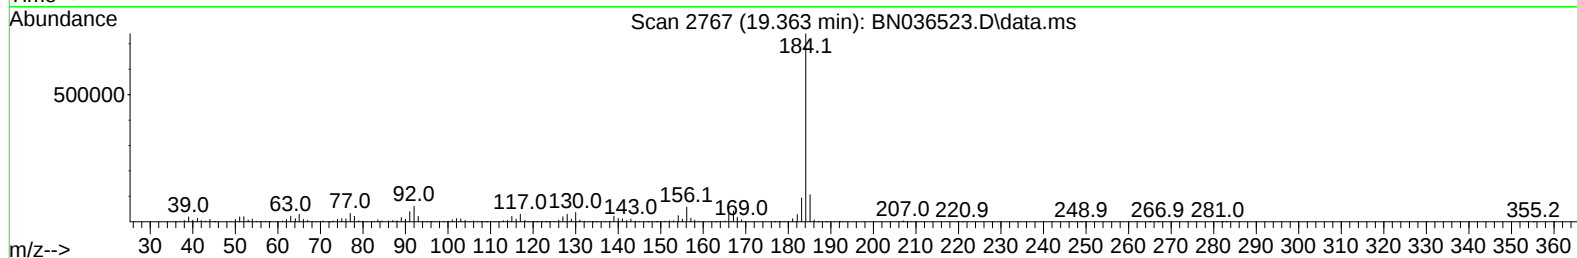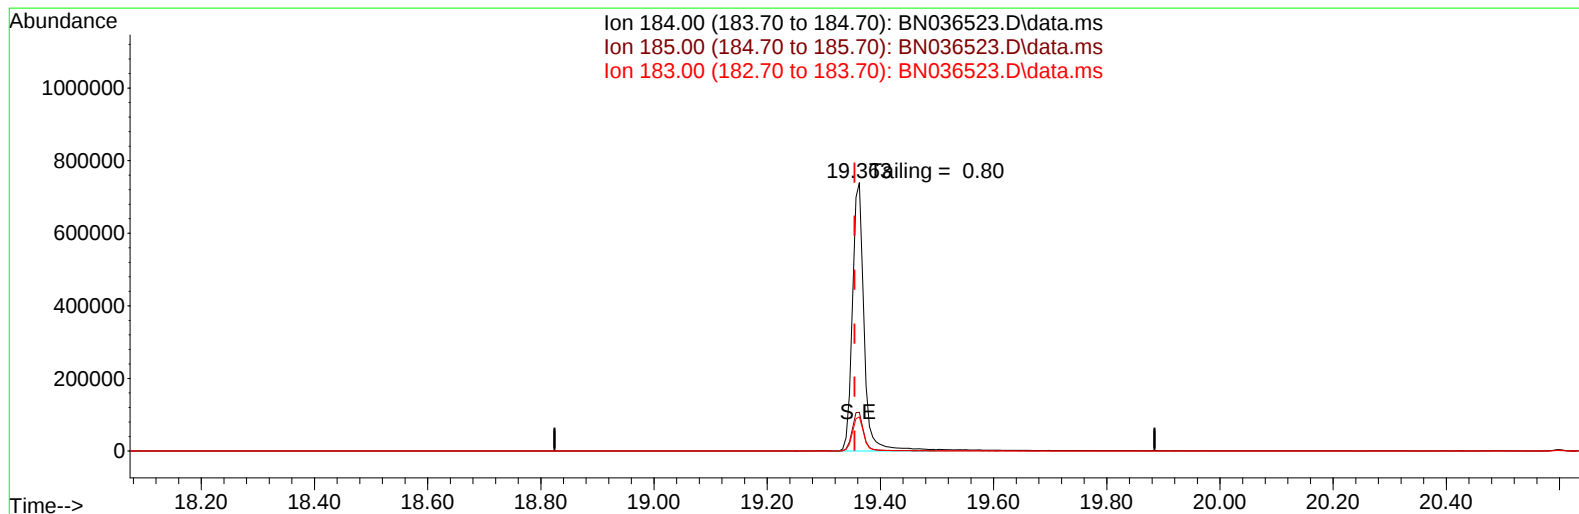

TIC: BN036523.D\data.ms

(77) Benzidine

19.363min (+ 0.009) 0.00 ng

response 1065965

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.43
183.00	13.20	12.74
0.00	0.00	0.00