
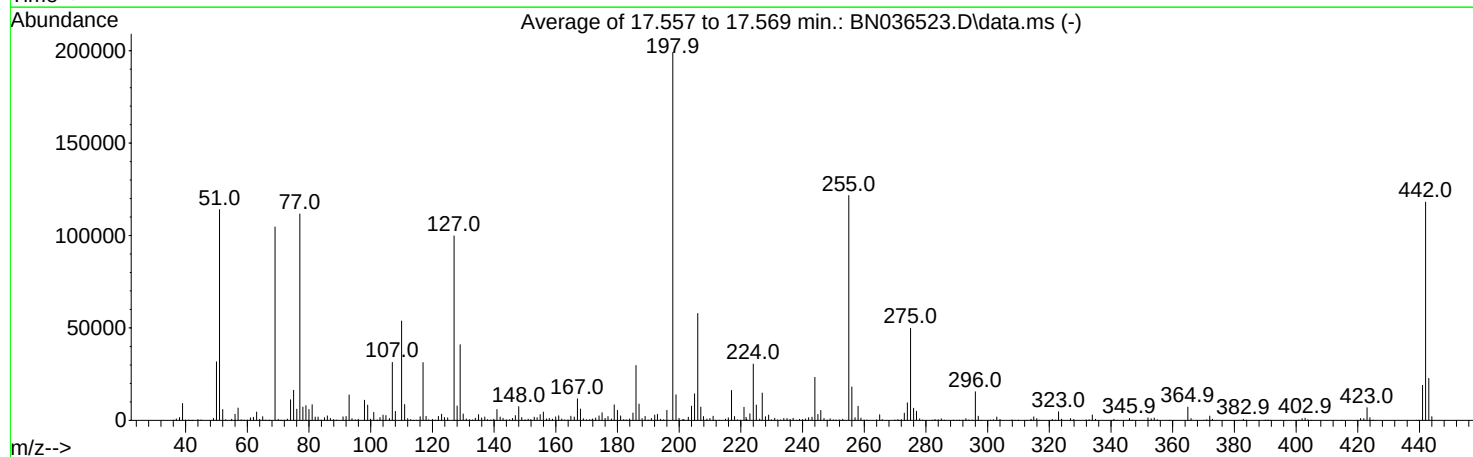


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN030525\  
Data File : BN036523.D  
Acq On : 05 Mar 2025 12:52  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN021025.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Mar 05 16:08:57 2025

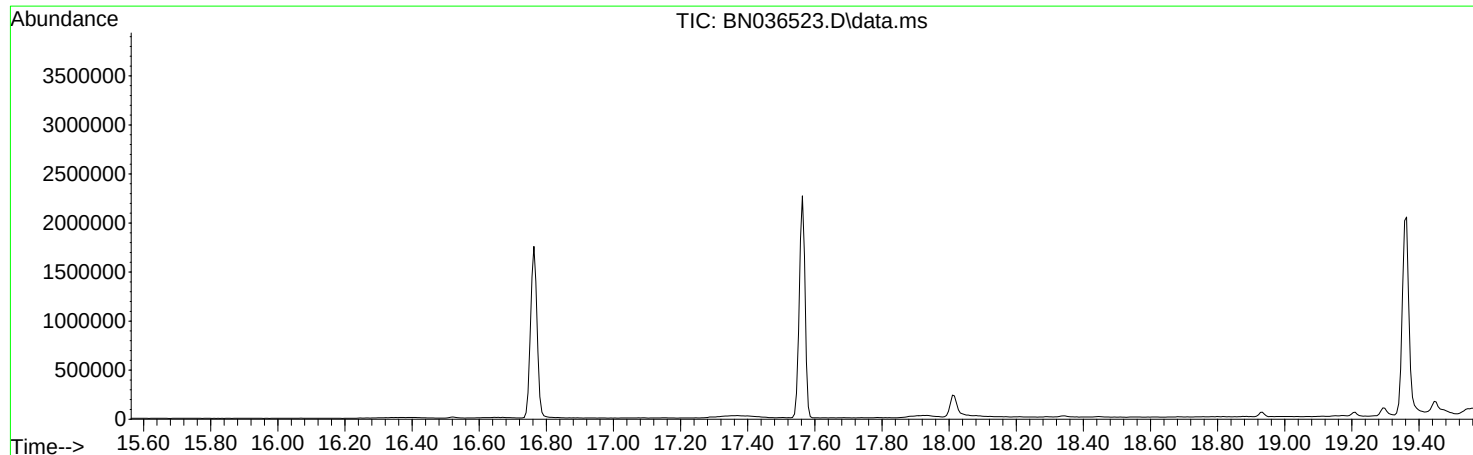

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 57.3         | 113984     | PASS                |
| 68             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 69             | 198             | 0.00            | 100             | 52.6         | 104689     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 639        | PASS                |
| 127            | 198             | 10              | 80              | 50.2         | 99840      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 199040     | PASS                |
| 199            | 198             | 5               | 9               | 7.0          | 13866      | PASS                |
| 275            | 198             | 10              | 60              | 25.0         | 49821      | PASS                |
| 365            | 198             | 1               | 100             | 3.6          | 7186       | PASS                |
| 441            | 198             | 0.01            | 100             | 9.5          | 18995      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 118091     | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 22664      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 3/5/2025      | BNA_N            | <u>BN036523.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 725032           | 20.598             |
| DDD           | 9634             | 20.21              |
| DDE           | 159              | 19.651             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 9793          | 734825           | 1.33               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN030525\  
Data File : BN036523.D  
Acq On : 05 Mar 2025 12:52  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Mar 05 16:03:48 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 25 04:23:53 2024  
Response via : Initial Calibration

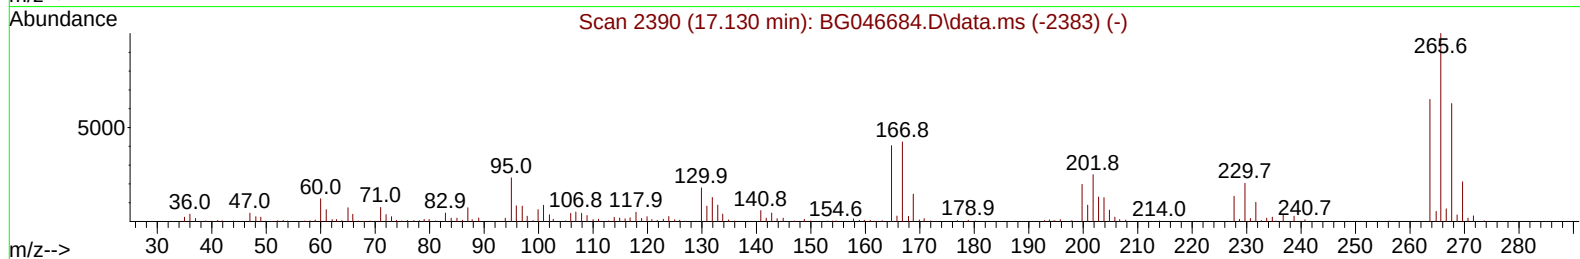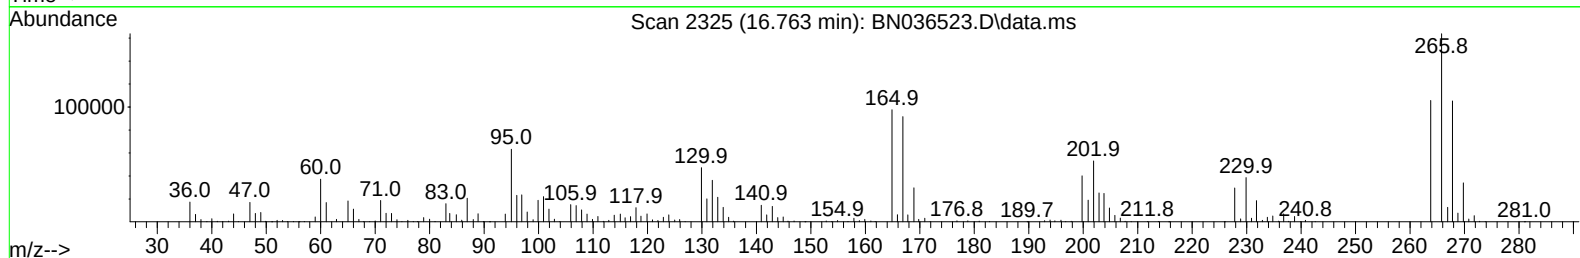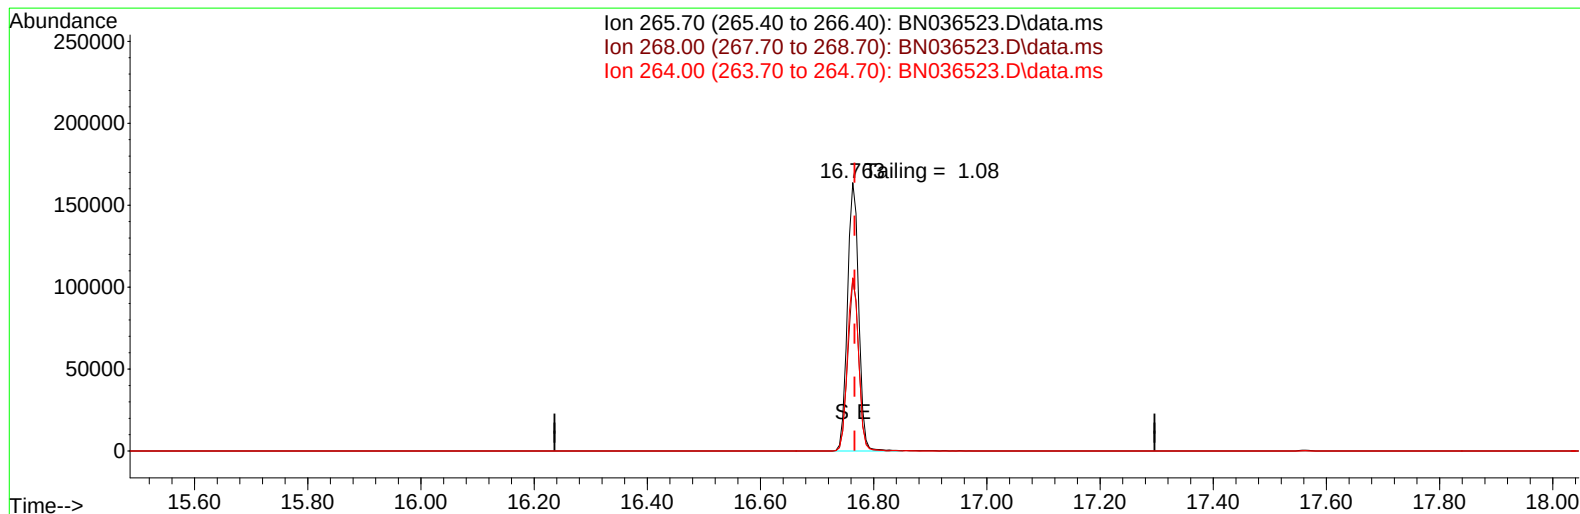

TIC: BN036523.D\data.ms

**(70) Pentachlorophenol (C)**

**16.763min (-0.003) 22410.75 ng**




**response 227405**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 64.26  |
| 264.00 | 61.60  | 64.52  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN030525\  
Data File : BN036523.D  
Acq On : 05 Mar 2025 12:52  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Mar 05 16:03:48 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 25 04:23:53 2024  
Response via : Initial Calibration

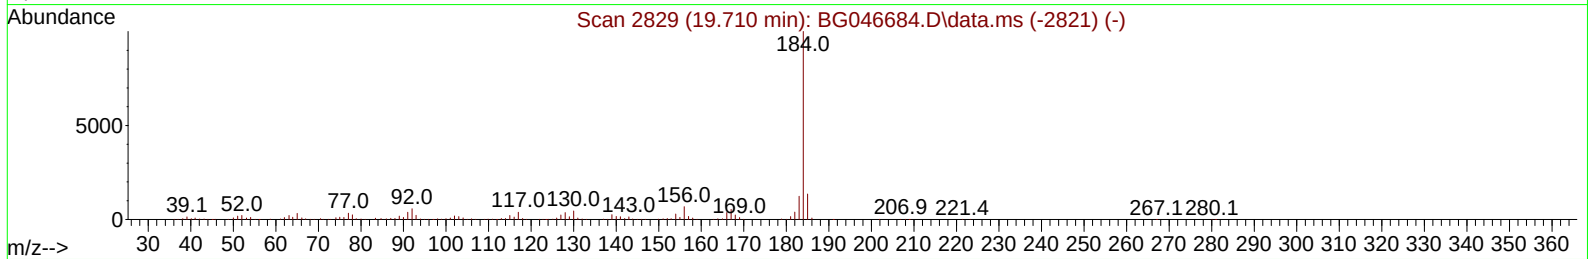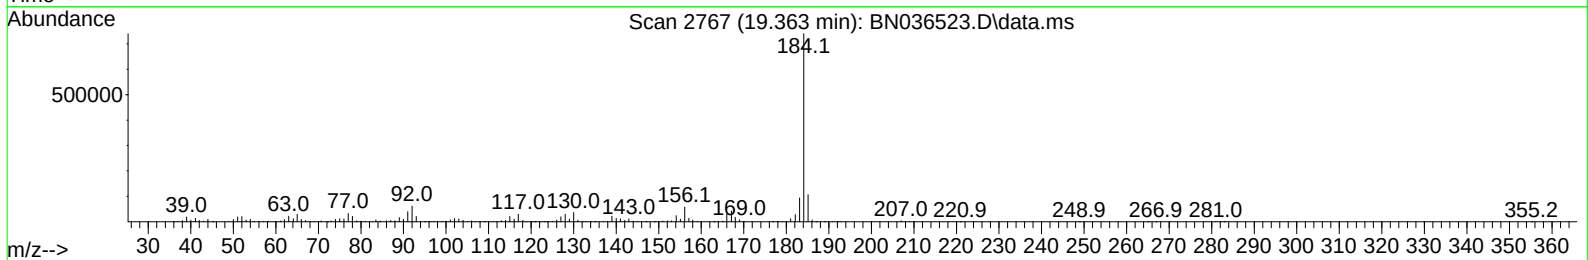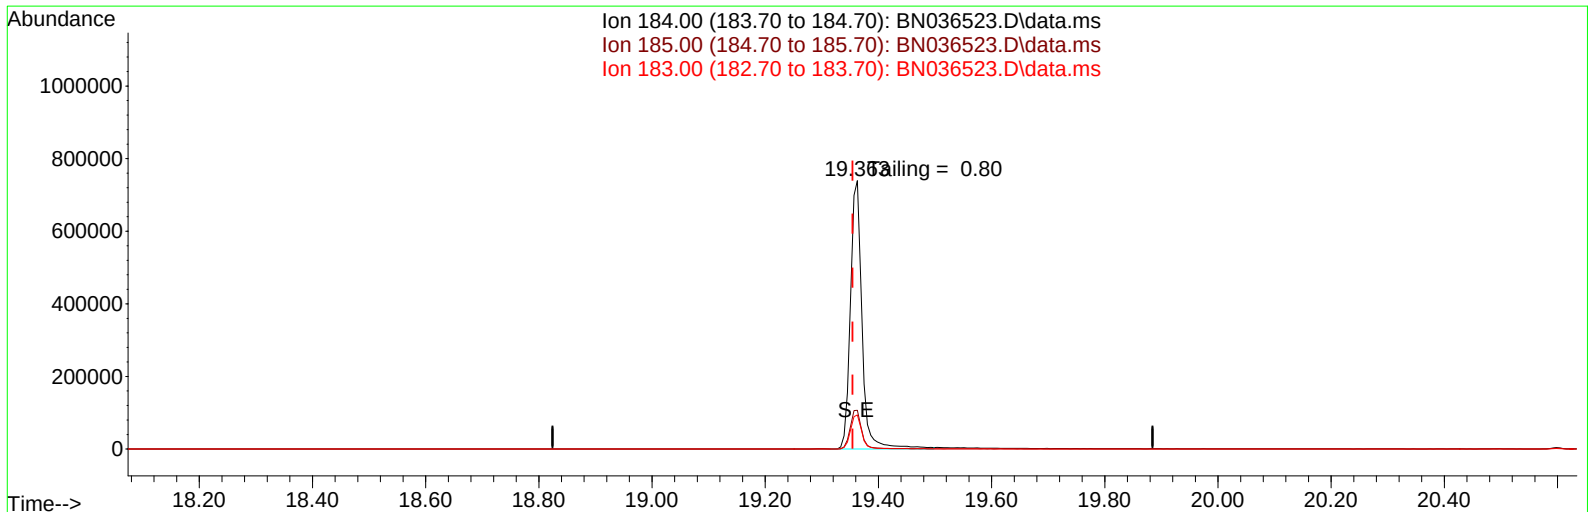

TIC: BN036523.D\data.ms

(77) Benzidine

19.363min (+ 0.009) 0.00 ng

response 1065965

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.43  |
| 183.00 | 13.20  | 12.74  |
| 0.00   | 0.00   | 0.00   |