
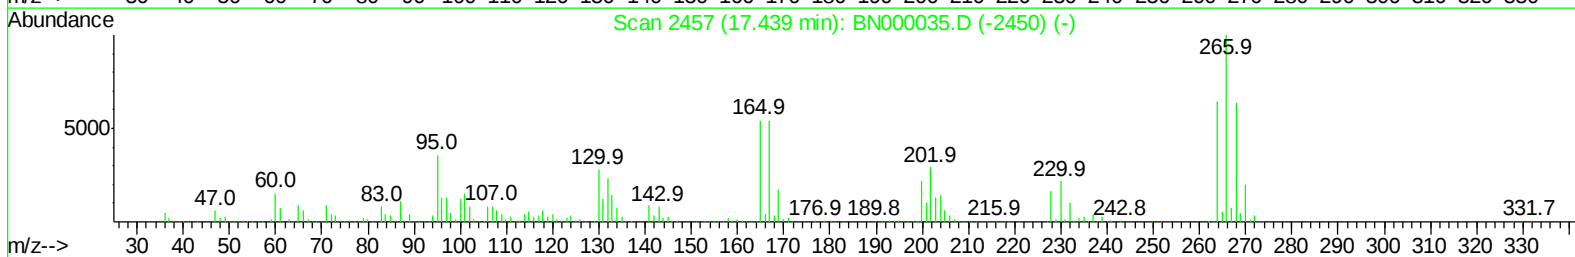
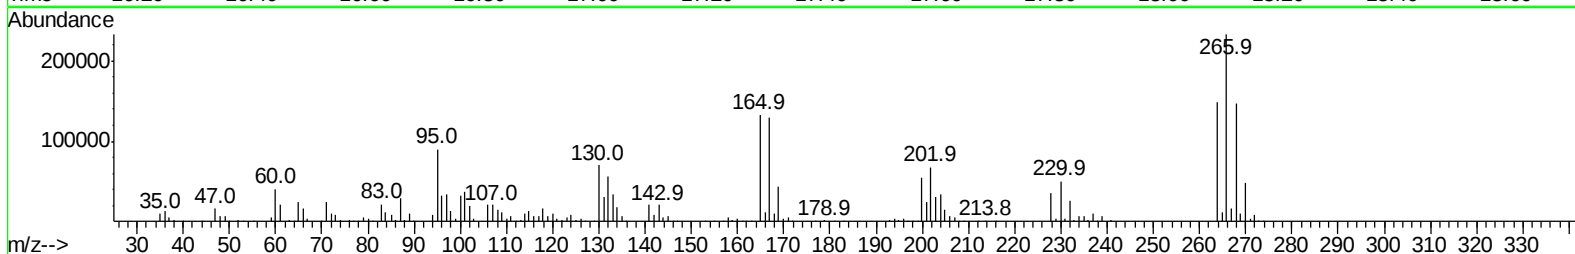


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA N\Data\BN030618\
Data File : BN000254.D
Acq On : 06 Mar 2018 09:05
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 06:04:29 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 07 04:45:19 2018
Response via : Initial Calibration

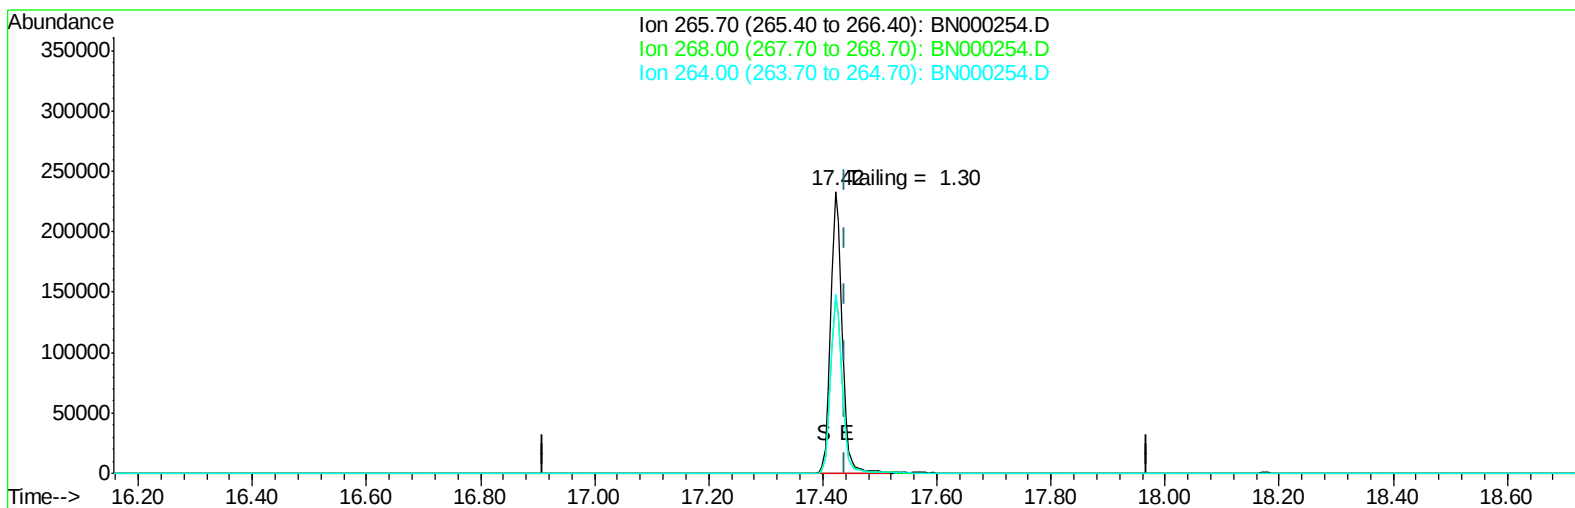

TIC: BN000254.D

(69) Pentachlorophenol (C)




17.422min (-0.017) 16654.28ng

response 324606

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.88
264.00	62.00	63.45
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA N\Data\BN030618\
Data File : BN000254.D
Acq On : 06 Mar 2018 09:05
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 06:04:29 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 07 04:45:19 2018
Response via : Initial Calibration

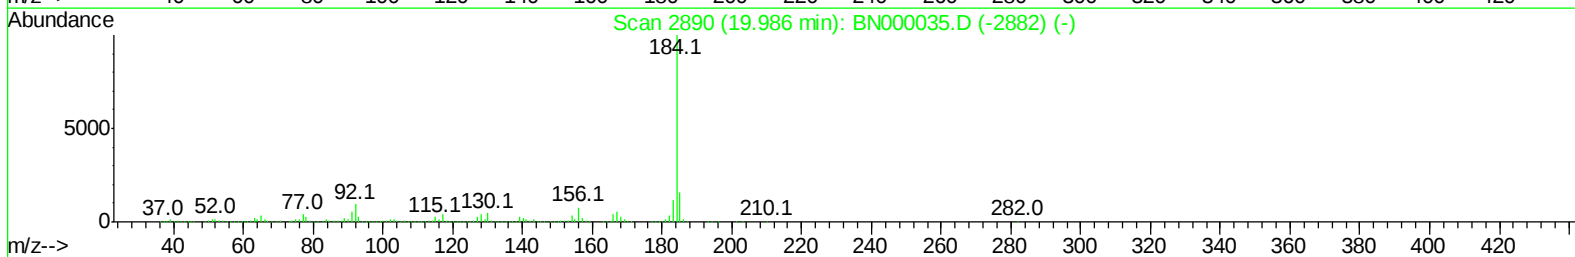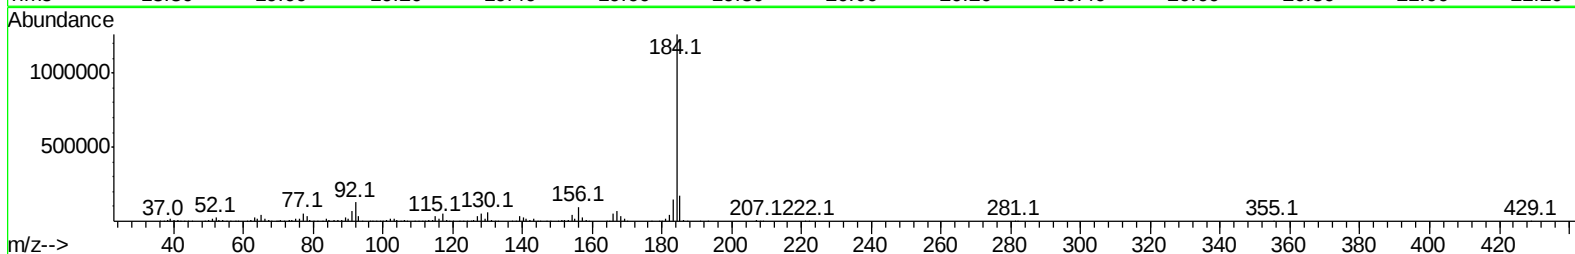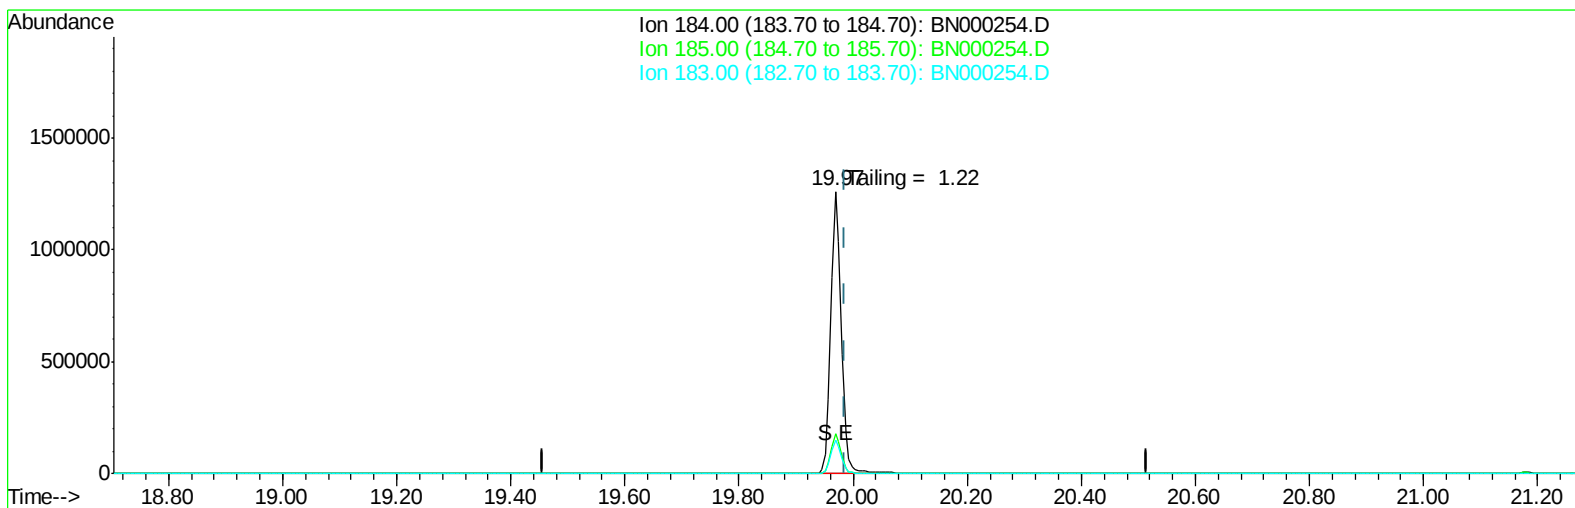

TIC: BN000254.D

(76) Benzidine

19.969min (-0.017) 40919.56ng

response 1596587

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.92
183.00	13.30	11.70
0.00	0.00	0.00