

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA N\DATA\BN030618\
 Data File : BN000257.D
 Acq On : 06 Mar 2018 11:22
 Operator : JU/SJ
 Sample : PB107064BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB107064BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.928	493	500	516	rBV	2945909	4693271	41.61%	7.465%
2	7.575	772	780	793	rBV	3209071	5222566	46.30%	8.307%
3	7.969	839	847	856	rBV	3030204	5083961	45.07%	8.086%
4	8.446	921	928	936	rVB	719105	1213043	10.75%	1.929%
5	8.775	976	984	992	rBV	2190703	3728867	33.06%	5.931%
6	9.628	1120	1129	1137	rBV	1807657	2990702	26.51%	4.757%
7	11.287	1403	1411	1419	rBV	1156206	1933250	17.14%	3.075%
8	13.687	1812	1819	1826	rBV	5420258	8008682	71.00%	12.738%
9	15.057	2046	2052	2062	rVB2	1841685	2740097	24.29%	4.358%
10	16.528	2295	2302	2318	rBV	3578720	4973815	44.10%	7.911%
11	17.780	2508	2515	2525	rBV2	2339347	3408108	30.22%	5.421%
12	20.339	2944	2950	2959	rBV	8816638	11279328	100.00%	17.940%
13	21.892	3208	3214	3221	rBV	2948383	3804974	33.73%	6.052%
14	24.362	3626	3634	3646	rBV2	1862897	3790816	33.61%	6.029%


Sum of corrected areas: 62871480

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA N\DATA\BN030618\
Data File : BN000257.D
Acq On : 06 Mar 2018 11:22
Operator : JU/SJ
Sample : PB107064BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB107064BL

Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

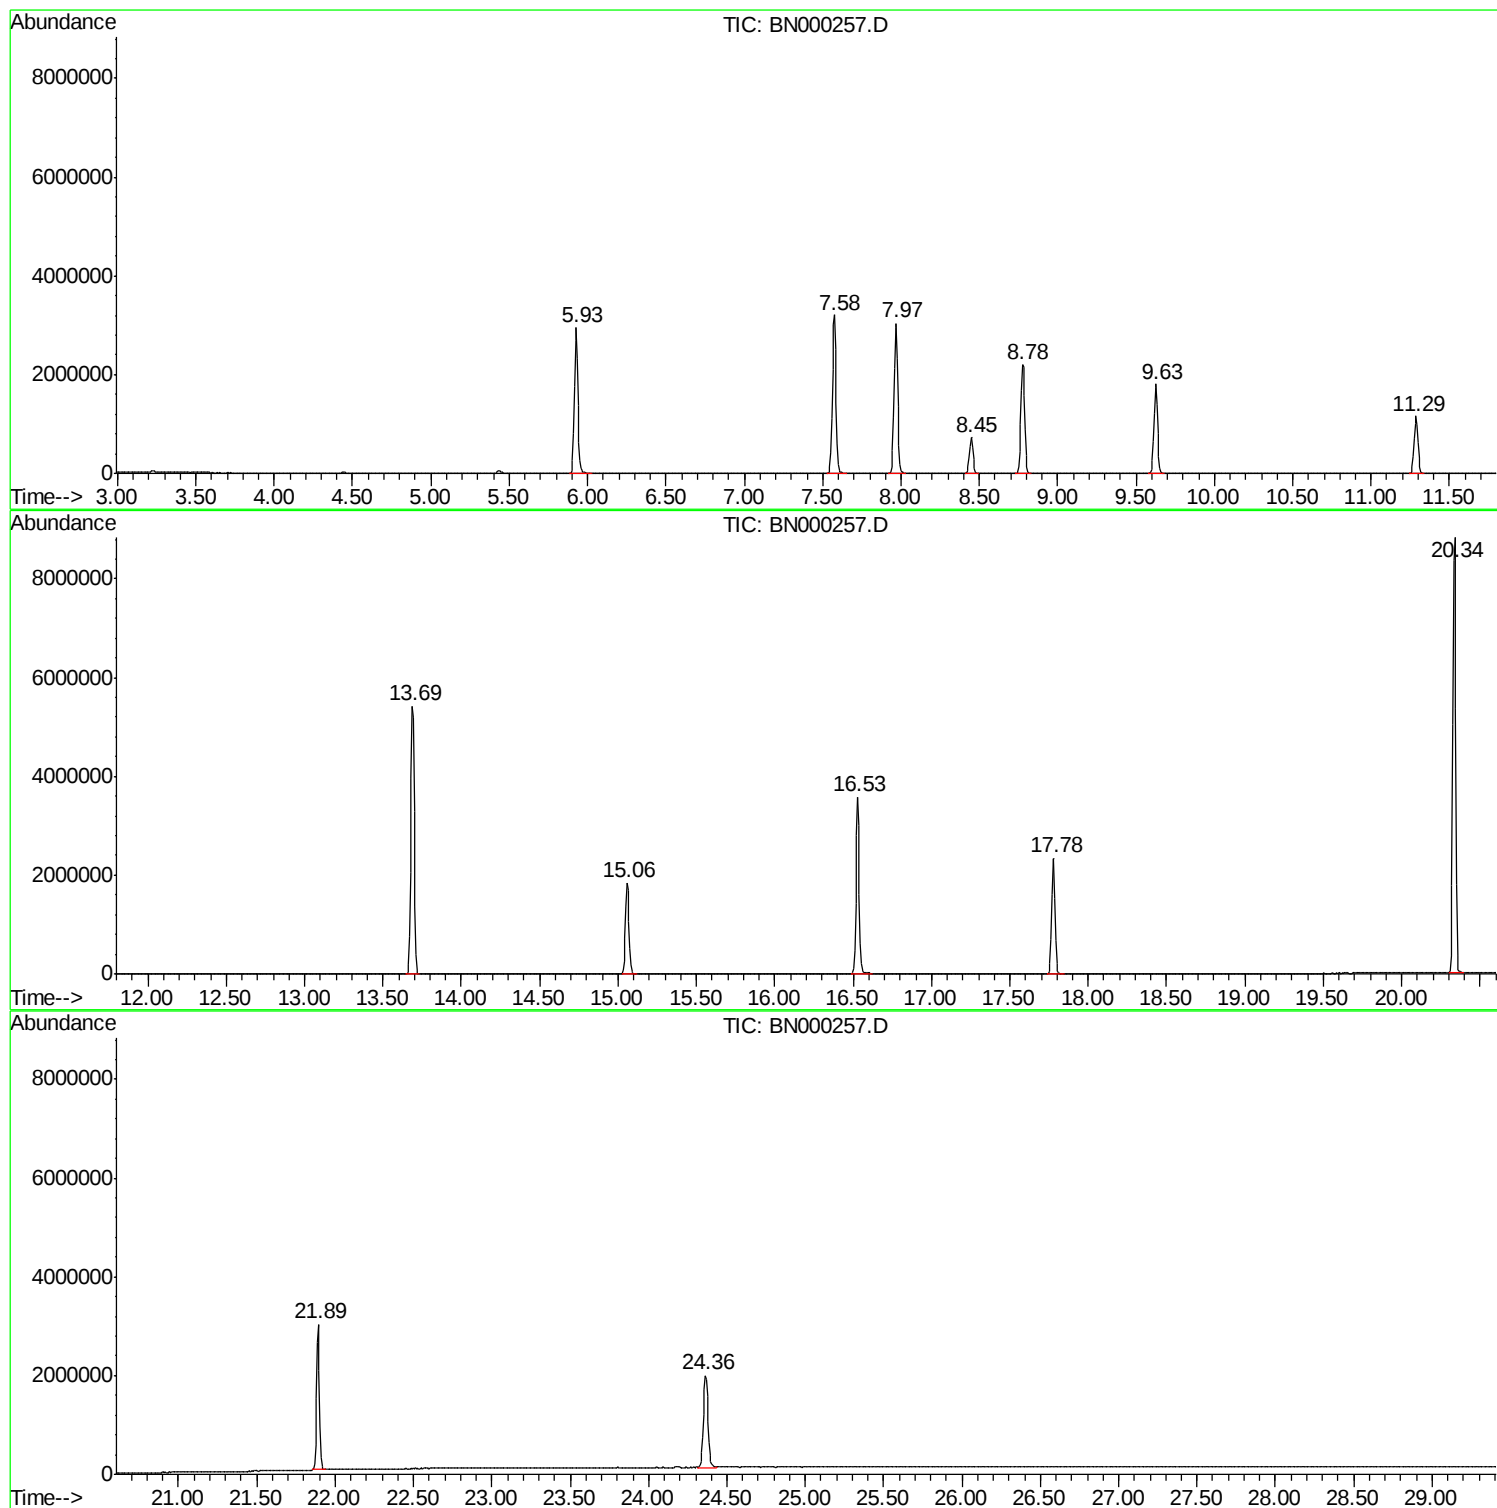

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA N\DATA\BN030618\
Data File : BN000257.D
Acq On : 06 Mar 2018 11:22
Operator : JU/SJ
Sample : PB107064BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB107064BL










Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.97 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.97	83.82 ng	5083960	1,4-Dichlorobenzene-d4	8.45

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	9

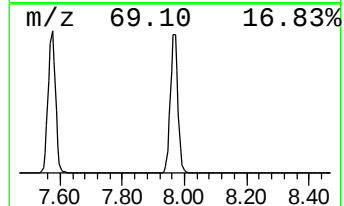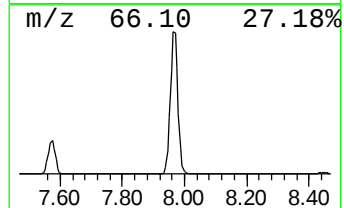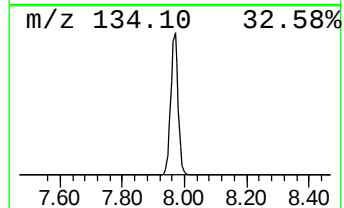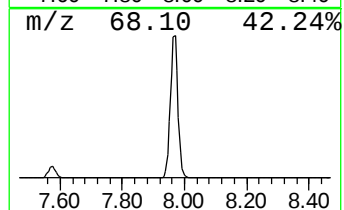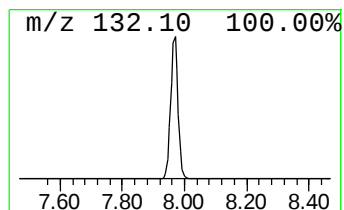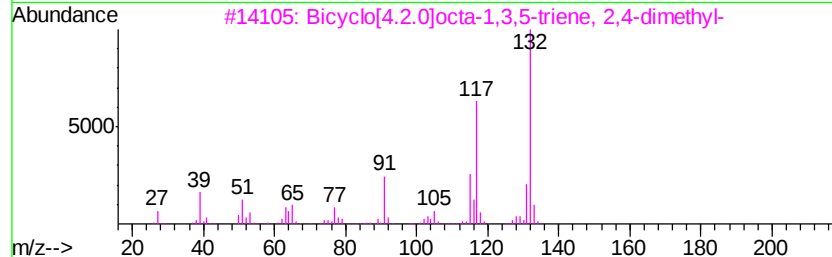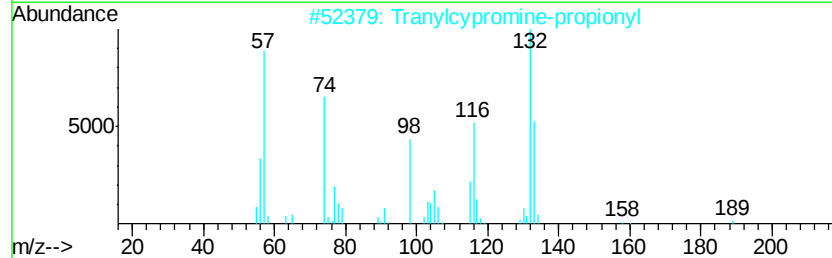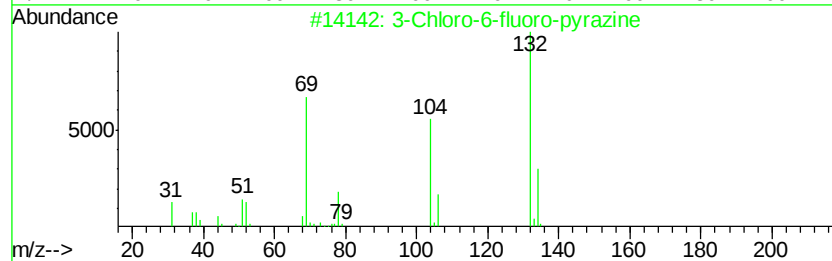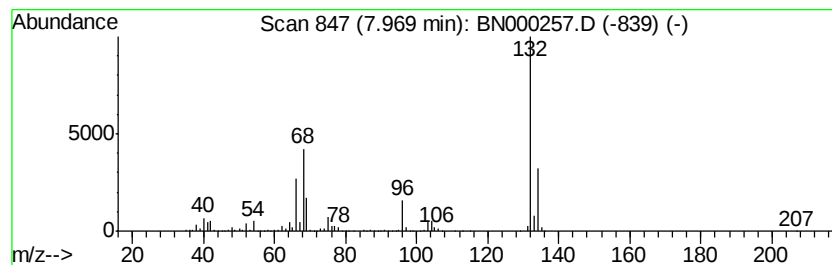

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_N\DATA\BN030618\
Data File : BN000257.D
Acq On : 06 Mar 2018 11:22
Operator : JU/SJ
Sample : PB107064BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB107064BL

Quant Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.97	7.97	83.8	ng	5083960	1	8.45	1213040	20.0