


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA N\Data\BN030618\
 Data File : BN000254.D
 Acq On : 06 Mar 2018 09:05
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 07 04:45:19 2018

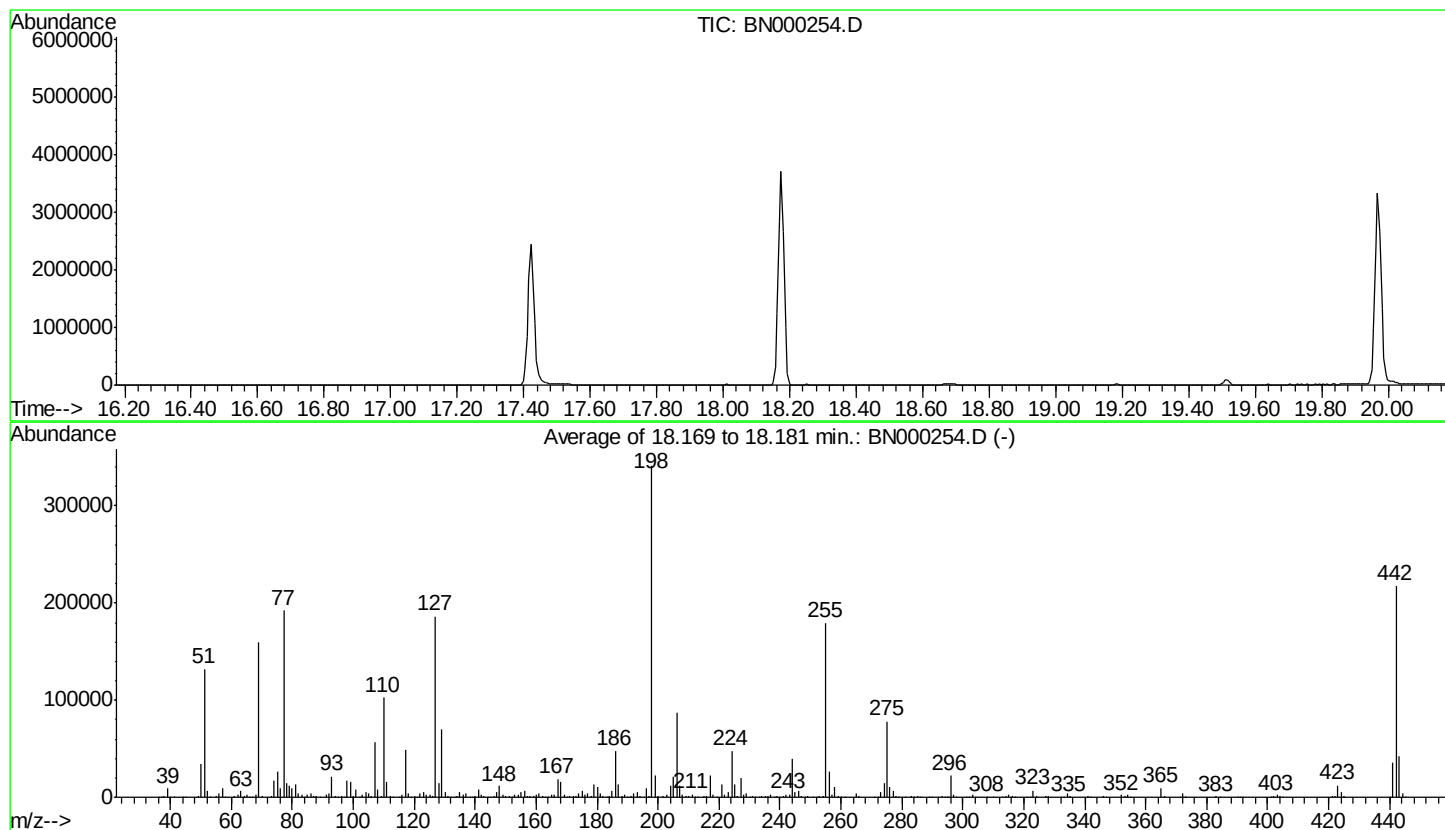

AutoFind: Scans 2581, 2582, 2583; Background Corrected with Scan 2574

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	132032	PASS
68	69	0.00	2	1.9	2953	PASS
69	198	0.00	100	46.7	159509	PASS
70	69	0.00	2	0.5	822	PASS
127	198	10	80	54.5	186304	PASS
197	198	0.00	2	0.4	1387	PASS
198	198	100	100	100.0	341546	PASS
199	198	5	9	6.7	22856	PASS
275	198	10	60	22.9	78178	PASS
365	198	1	100	2.7	9372	PASS
441	443	0.01	100	83.3	35330	PASS
442	198	50	100	63.8	217984	PASS
443	442	15	24	19.4	42389	PASS