
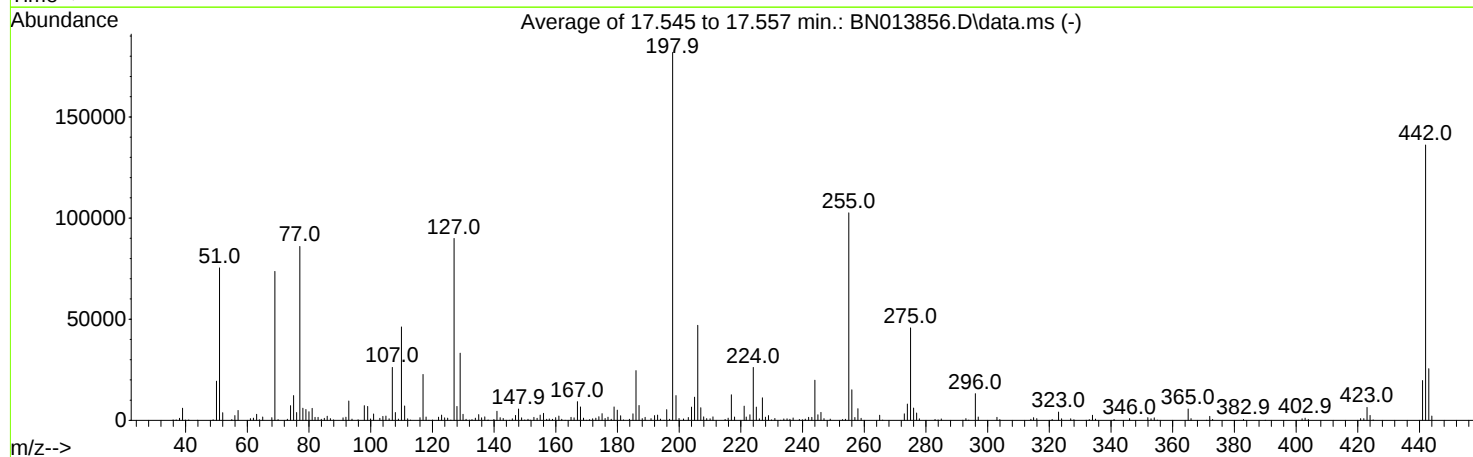


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN030621\  
 Data File : BN013856.D  
 Acq On : 05 Mar 2021 12:11  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN022421.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Mar 05 13:34:35 2021

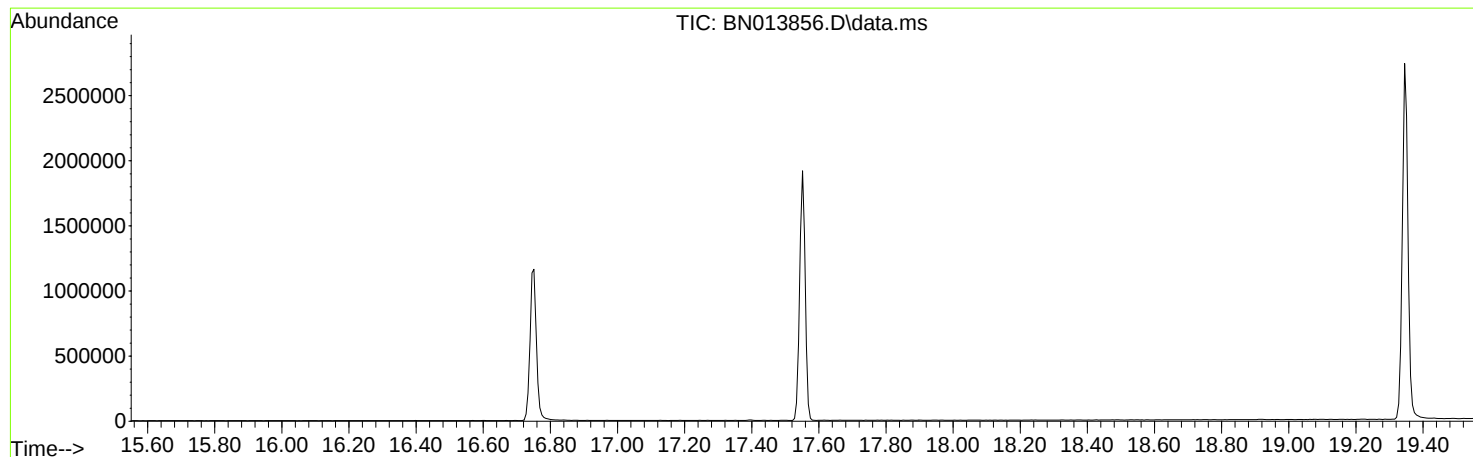

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2452

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 41.5         | 75392      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 1342       | PASS                |
| 69             | 198             | 0.00            | 100             | 40.5         | 73661      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 393        | PASS                |
| 127            | 198             | 10              | 80              | 49.5         | 89928      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.3          | 528        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 181845     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 12301      | PASS                |
| 275            | 198             | 10              | 60              | 25.1         | 45691      | PASS                |
| 365            | 198             | 1               | 100             | 3.1          | 5637       | PASS                |
| 441            | 198             | 0.01            | 100             | 10.8         | 19696      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 136149     | PASS                |
| 443            | 442             | 15              | 24              | 18.7         | 25515      | PASS                |




|                      |                         |                           |
|----------------------|-------------------------|---------------------------|
|                      | <b>DDT Breakdown</b>    |                           |
|                      |                         |                           |
|                      |                         |                           |
| <b>Date</b>          | <b>Instrument Name</b>  | <b>DFTPP Data File</b>    |
| <b>3/6/2021</b>      | <b>BNA_N</b>            | <b><u>BN013856.D</u></b>  |
|                      |                         |                           |
|                      |                         |                           |
| <b>Compound Name</b> | <b>Response</b>         | <b>Retention Time</b>     |
|                      |                         |                           |
| <b>DDT</b>           | <b>633212</b>           | <b>20.586</b>             |
| <b>DDD</b>           | <b>2618</b>             | <b>20.145</b>             |
| <b>DDE</b>           | <b>475</b>              | <b>19.639</b>             |
|                      |                         |                           |
|                      |                         |                           |
| <b>SUM(DDD+DDE)</b>  | <b>SUM(DDT+DDD+DDE)</b> | <b>% Breakdown Of DDT</b> |
|                      |                         |                           |
| <b>3093</b>          | <b>636305</b>           | <b>0.49</b>               |
|                      |                         |                           |

**Instrument :**  
**BNA\_N**  
**ClientSampleId :**  
**DFTPP**

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN030621\  
Data File : BN013856.D  
Acq On : 05 Mar 2021 12:11  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Mar 05 13:12:19 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 05 13:12:06 2021  
Response via : Initial Calibration

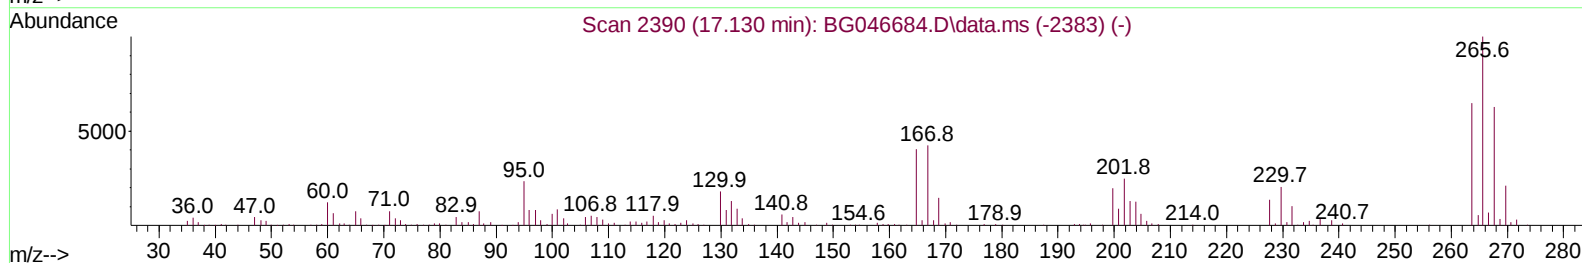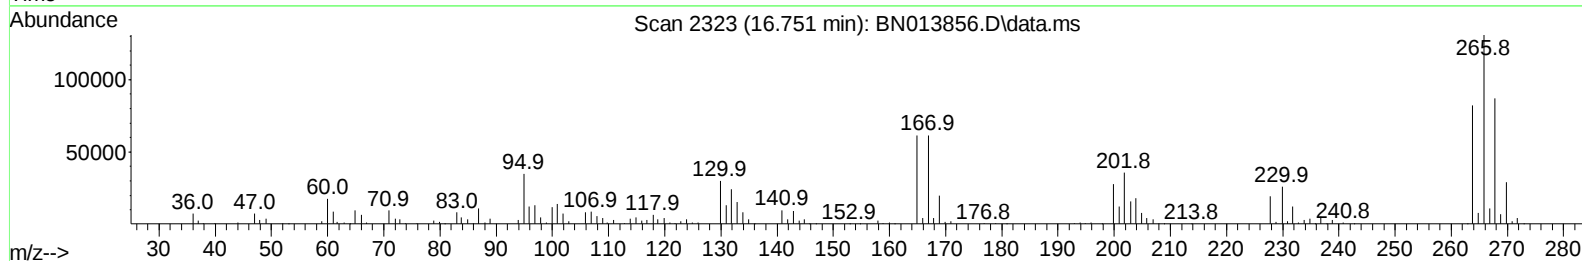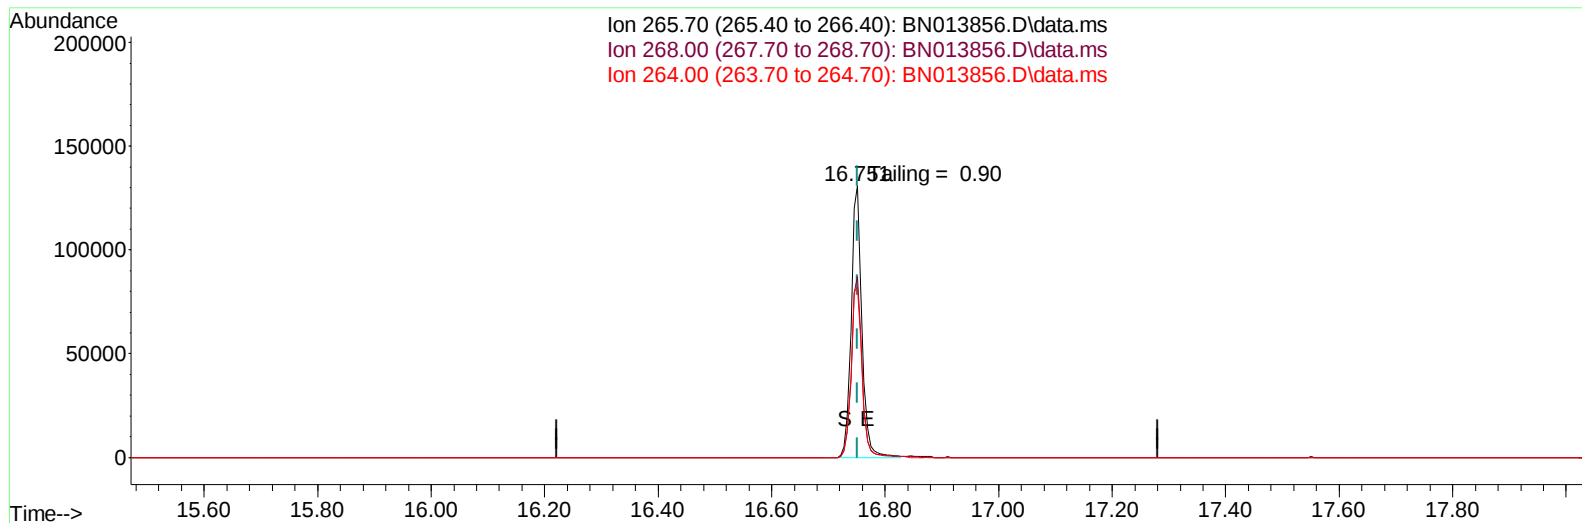

TIC: BN013856.D\data.ms

**(70) Pentachlorophenol (C)**

**16.751min ( 0.000) 18722.30 ng**




**response 173228**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 66.55  |
| 264.00 | 61.60  | 62.74  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN030621\  
Data File : BN013856.D  
Acq On : 05 Mar 2021 12:11  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Mar 05 13:12:19 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 05 13:12:06 2021  
Response via : Initial Calibration

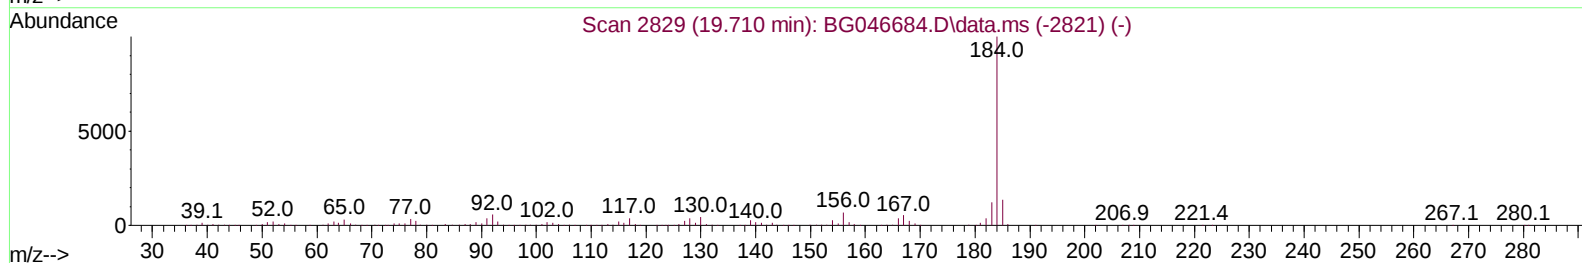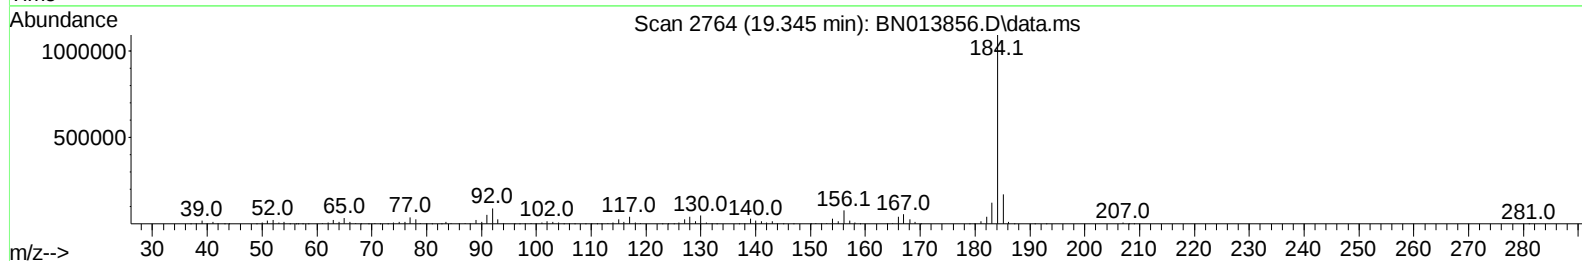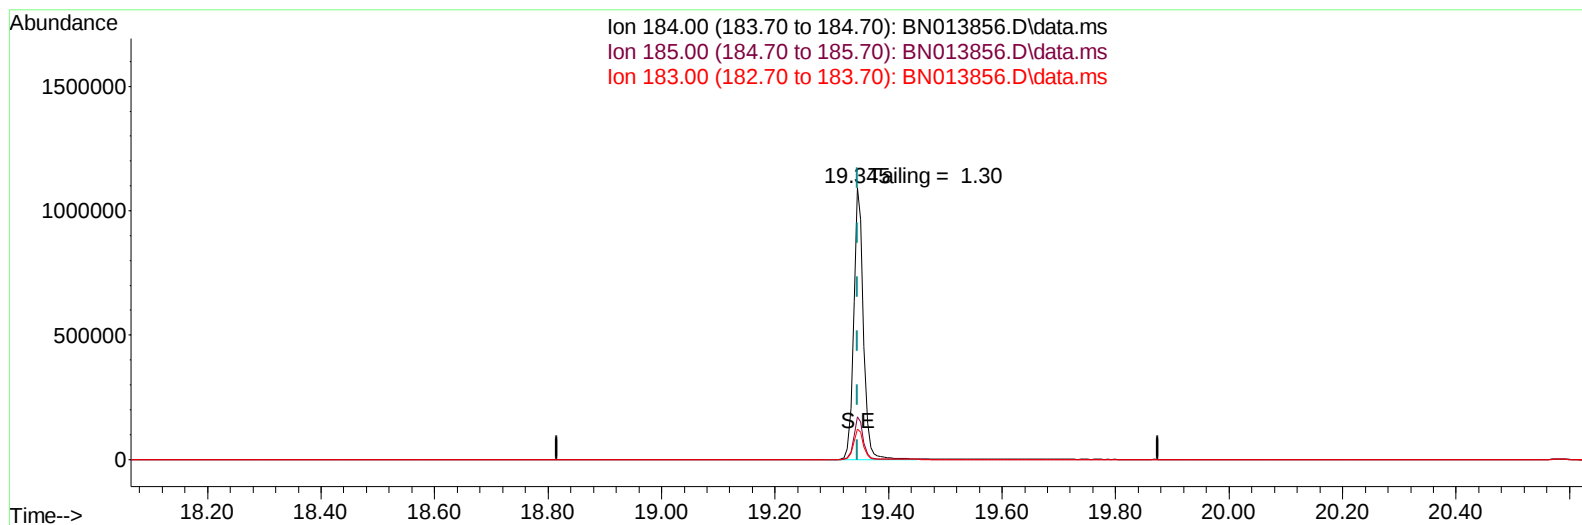

TIC: BN013856.D\data.ms

**(77) Benzidine**

**19.345min ( 0.000) 26890.89 ng**

**response 1292289**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 15.63  |
| 183.00 | 13.20  | 11.27  |
| 0.00   | 0.00   | 0.00   |