
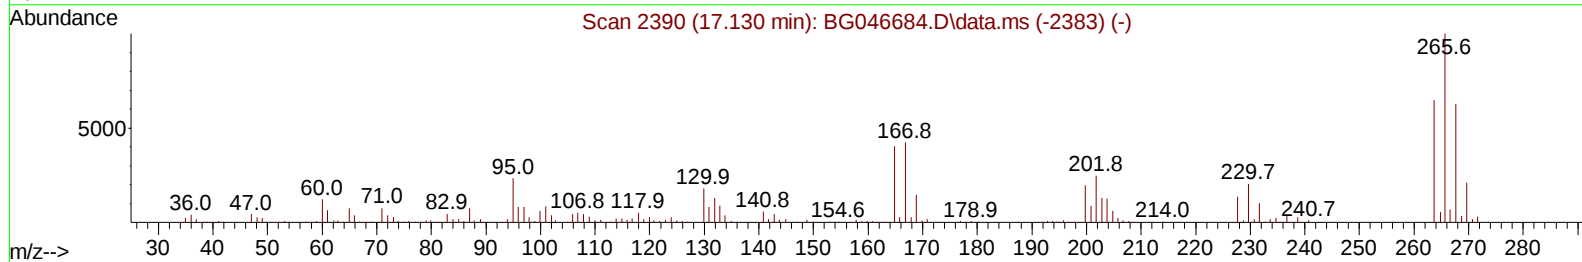
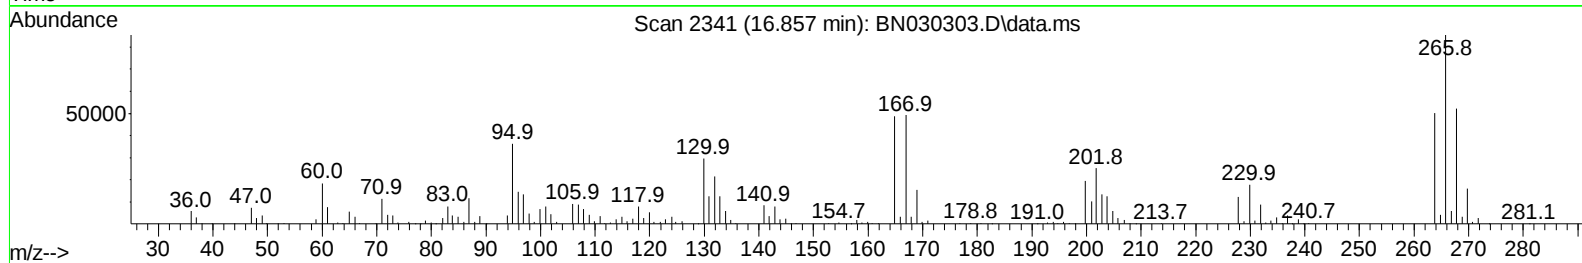


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030624\
Data File : BN030303.D
Acq On : 06 Mar 2024 23:12
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Mar 07 04:37:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 07 04:37:16 2024
Response via : Initial Calibration

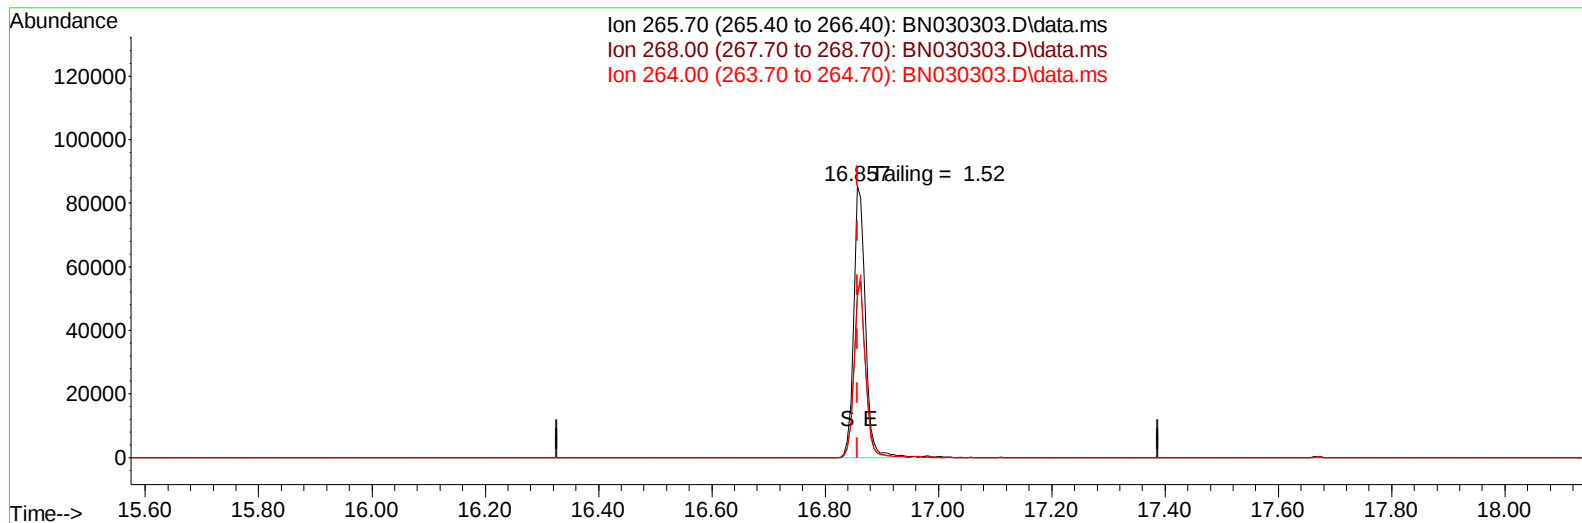




TIC: BN030303.D\data.ms

(70) Pentachlorophenol (C)**16.857min (0.000) 18590.16 ng****response 122986**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.04
264.00	61.60	58.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030624\
Data File : BN030303.D
Acq On : 06 Mar 2024 23:12
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Mar 07 04:37:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 07 04:37:16 2024
Response via : Initial Calibration

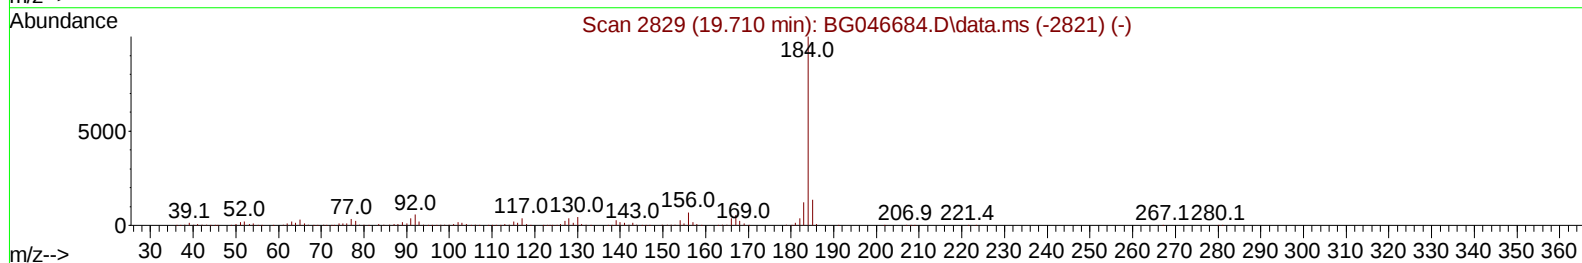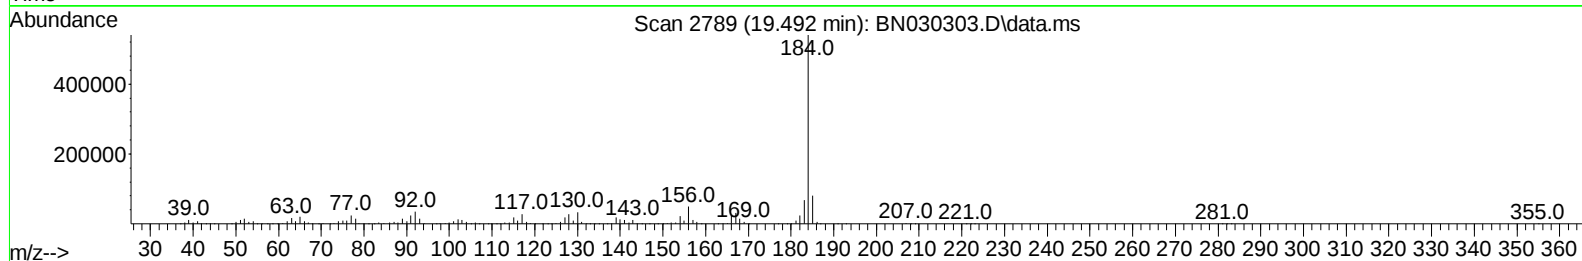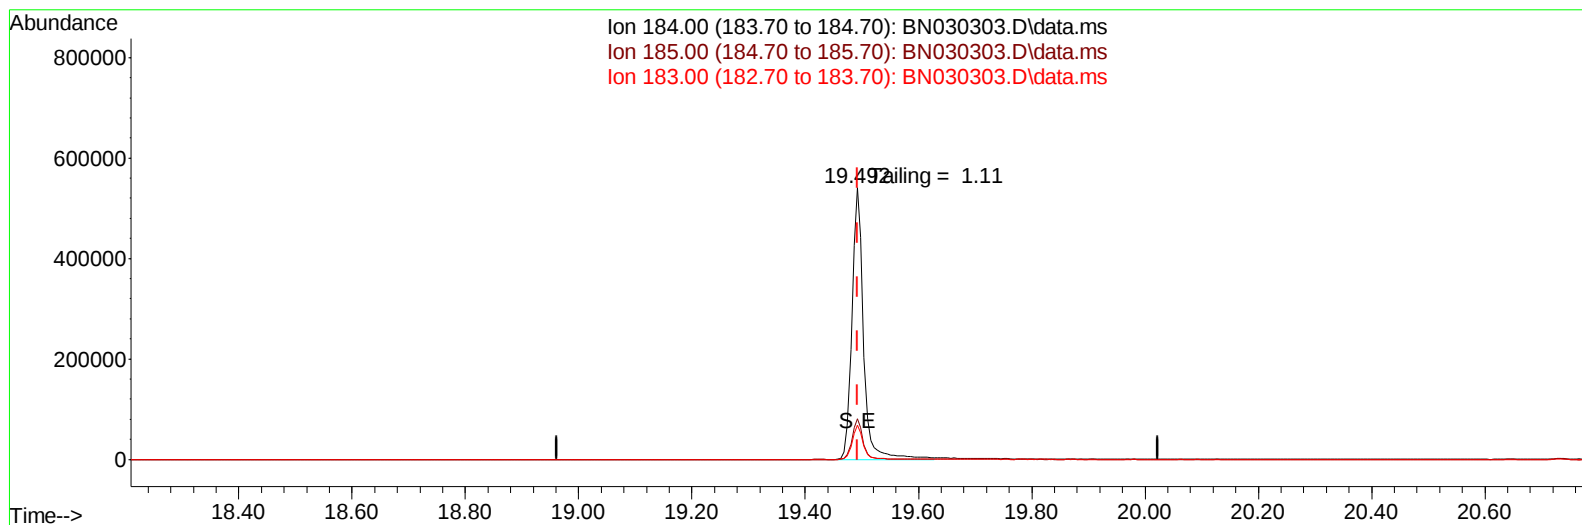

TIC: BN030303.D\data.ms

(77) Benzidine

19.492min (0.000) 0.00 ng

response 776283

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.92
183.00	13.20	12.59
0.00	0.00	0.00