

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030624\
 Data File : BN030316.D
 Acq On : 07 Mar 2024 07:01
 Operator : MA/JU
 Sample : P1590-19
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DUP09-20240222

Quant Time: Mar 07 07:37:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN030524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 05 17:44:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	2060	0.400	ng	0.00
7) Naphthalene-d8	10.605	136	5225	0.400	ng	0.00
13) Acenaphthene-d10	14.458	164	2748	0.400	ng	0.00
19) Phenanthrene-d10	17.218	188	5354	0.400	ng	0.00
29) Chrysene-d12	21.438	240	4312	0.400	ng	0.00
35) Perylene-d12	23.794	264	4855	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.384	112	610	0.113	ng	0.00
5) Phenol-d6	6.981	99	329	0.058	ng	0.00
8) Nitrobenzene-d5	8.982	82	1355	0.284	ng	0.01
11) 2-Methylnaphthalene-d10	12.201	152	2588	0.341	ng	0.00
14) 2,4,6-Tribromophenol	15.965	330	369	0.261	ng	0.00
15) 2-Fluorobiphenyl	13.089	172	3867	0.339	ng	0.00
27) Fluoranthene-d10	19.262	212	5368	0.365	ng	0.00
31) Terphenyl-d14	19.875	244	4395	0.393	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.312	88	3030	1.134	ng	# 94
34) Bis(2-ethylhexyl)phtha...	21.367	149	658	0.055	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030624\
Data File : BN030316.D
Acq On : 07 Mar 2024 07:01
Operator : MA/JU
Sample : P1590-19
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DUP09-20240222


Quant Time: Mar 07 07:37:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN030524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 05 17:44:16 2024
Response via : Initial Calibration

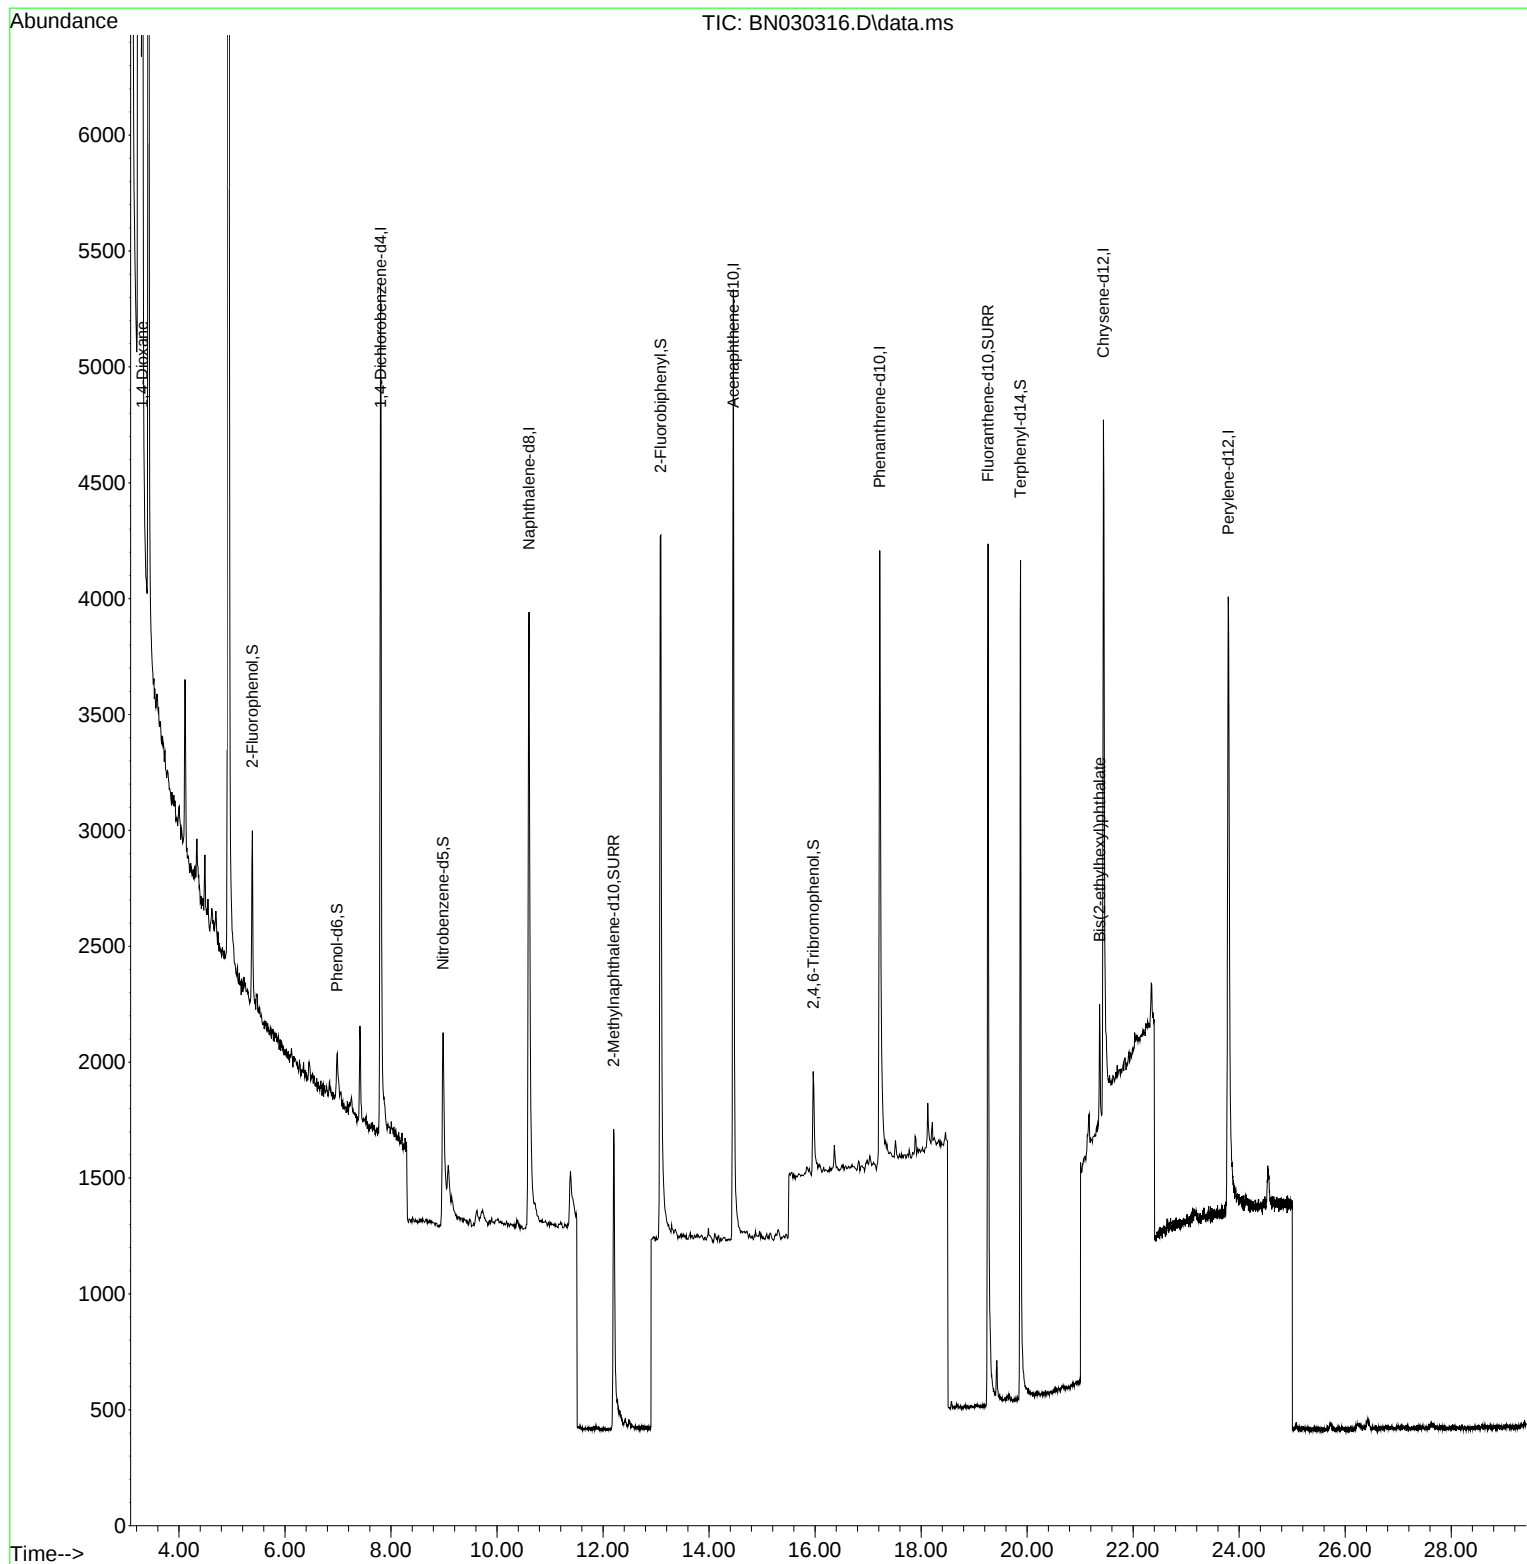






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.804 min Scan# 61
 Delta R.T. -0.007 min
 Lab File: BN030316.D
 Acq: 07 Mar 2024 07:01

Instrument :
 BNA_N
 ClientSampleId :
 DUP09-20240222

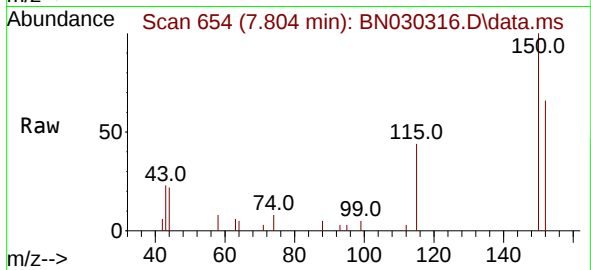

Tgt Ion:152 Resp: 2060




Ion	Ratio	Lower	Upper
152	100		
150	152.6	119.4	179.0
115	66.4	56.9	85.3

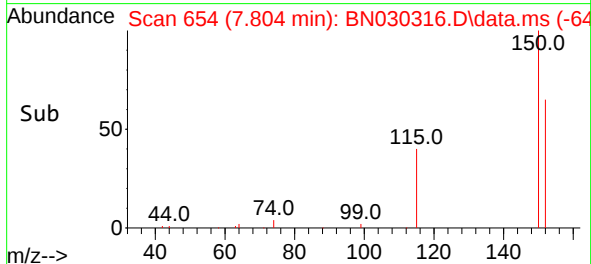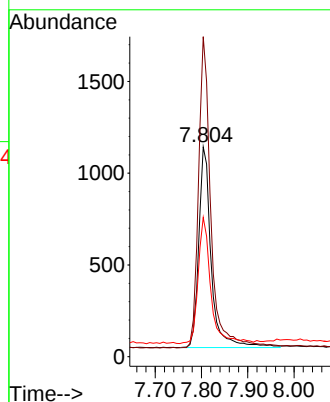


#2
 1,4-Dioxane
 Concen: 1.134 ng
 RT: 3.312 min Scan# 32
 Delta R.T. -0.007 min
 Lab File: BN030316.D
 Acq: 07 Mar 2024 07:01

Tgt Ion: 88 Resp: 3030

Ion	Ratio	Lower	Upper
88	100		
43	38.9	23.8	35.8
58	57.3	46.2	69.4


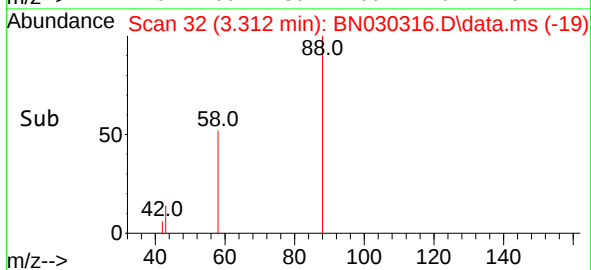
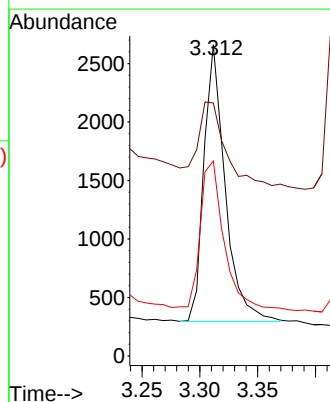
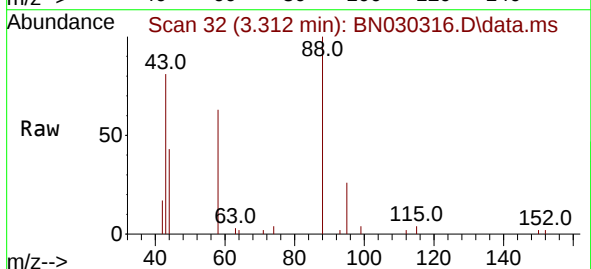




#4
2-Fluorophenol
Concen: 0.113 ng
RT: 5.384 min Scan# 319
Delta R.T. 0.000 min
Lab File: BN030316.D
Acq: 07 Mar 2024 07:01




Instrument :
BNA_N
ClientSampleId :
DUP09-20240222


Tgt Ion:	112	Resp:	610
Ion	Ratio	Lower	Upper
112	100		
64	50.3	41.8	62.8
63	37.9	27.1	40.7

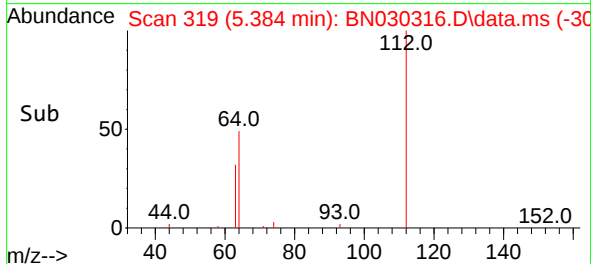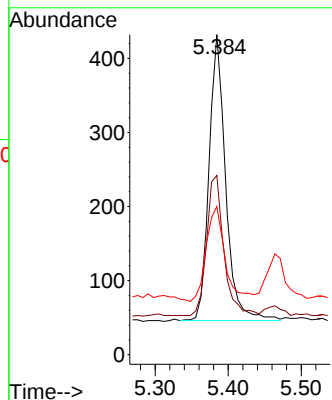

#5
Phenol-d6
Concen: 0.058 ng
RT: 6.981 min Scan# 540
Delta R.T. 0.000 min
Lab File: BN030316.D
Acq: 07 Mar 2024 07:01

Tgt Ion:	99	Resp:	329
Ion	Ratio	Lower	Upper
99	100		
42	20.1	19.0	28.6
71	53.8	36.0	54.0


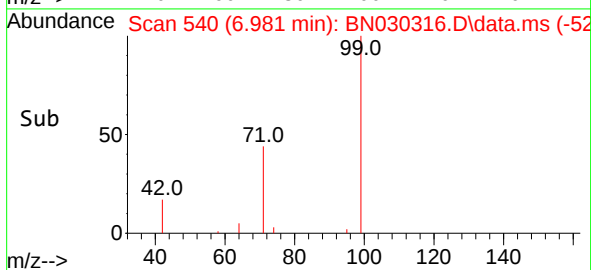
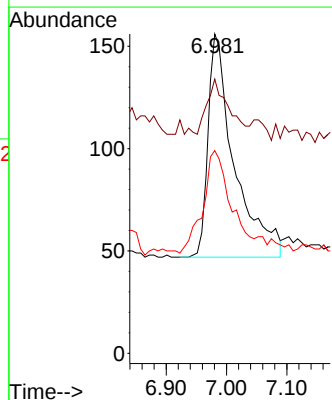
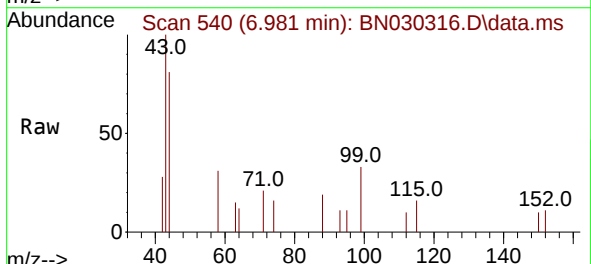




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.605 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN030316.D
Acq: 07 Mar 2024 07:01




Instrument :
BNA_N
ClientSampleId :
DUP09-20240222


Tgt Ion:	136	Resp:	5225
Ion	Ratio	Lower	Upper
136	100		
137	12.6	10.5	15.7
54	7.3	6.4	9.6
68	5.5	5.4	8.2

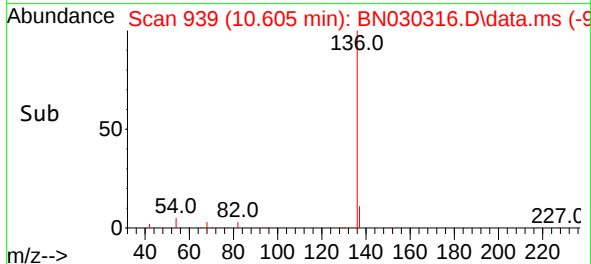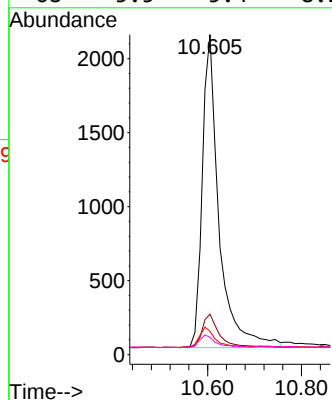

#8
Nitrobenzene-d5
Concen: 0.284 ng
RT: 8.982 min Scan# 787
Delta R.T. 0.011 min
Lab File: BN030316.D
Acq: 07 Mar 2024 07:01

Tgt Ion:	82	Resp:	1355
Ion	Ratio	Lower	Upper
82	100		
128	49.1	32.2	48.2#
54	50.7	47.3	70.9


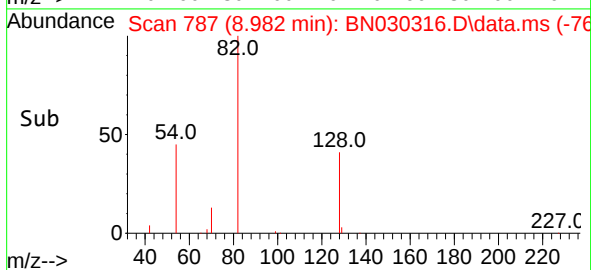
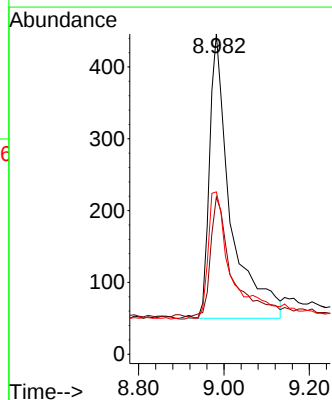
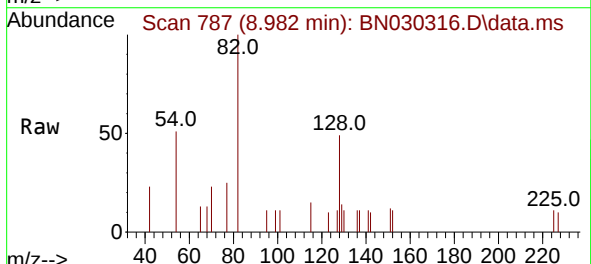




#11
2-Methylnaphthalene-d10
Concen: 0.341 ng
RT: 12.201 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN030316.D
Acq: 07 Mar 2024 07:01




Instrument :
BNA_N
ClientSampleId :
DUP09-20240222


Tgt Ion:152 Resp: 2588
Ion Ratio Lower Upper
152 100
151 20.8 16.7 25.1

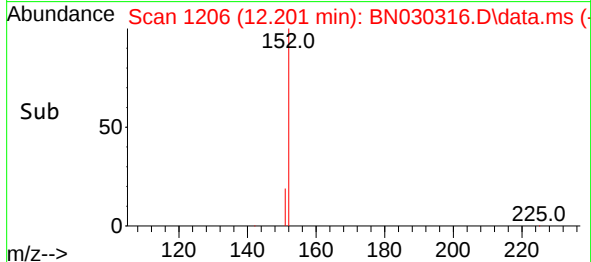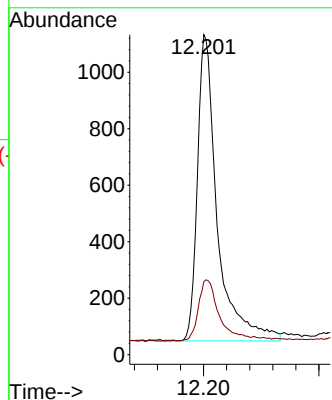

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.458 min Scan# 1538
Delta R.T. 0.000 min
Lab File: BN030316.D
Acq: 07 Mar 2024 07:01

Tgt Ion:164 Resp: 2748
Ion Ratio Lower Upper
164 100
162 105.8 83.4 125.2
160 52.6 41.7 62.5


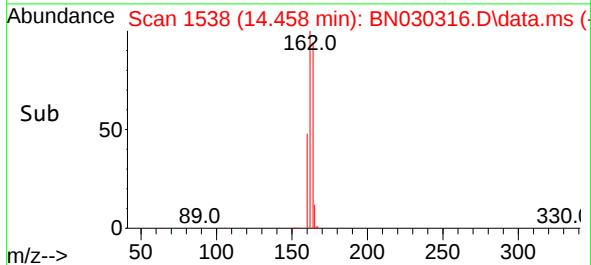
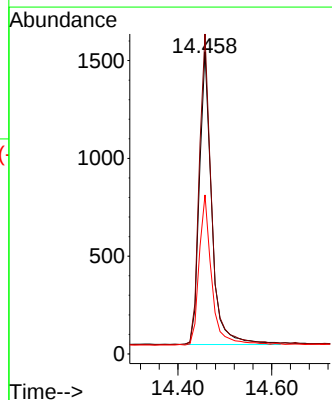
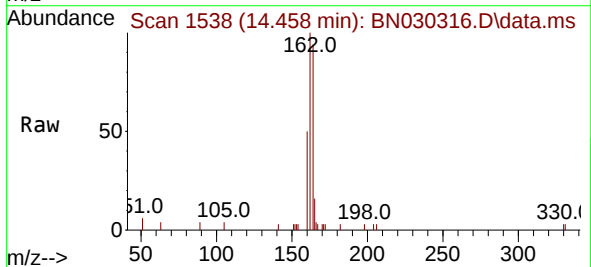




#14
2,4,6-Tribromophenol
Concen: 0.261 ng
RT: 15.965 min Scan# 1673
Delta R.T. 0.000 min
Lab File: BN030316.D
Acq: 07 Mar 2024 07:01




Instrument :
BNA_N
ClientSampleId :
DUP09-20240222


Tgt Ion: 330 Resp: 369
Ion Ratio Lower Upper
330 100
332 94.0 72.6 108.8
141 46.9 41.3 61.9

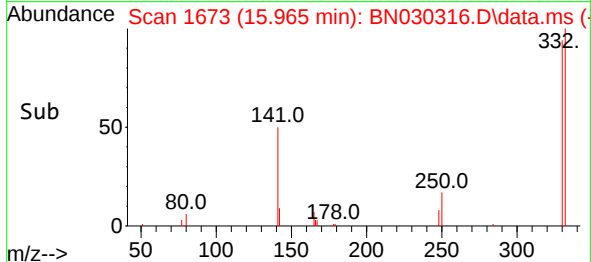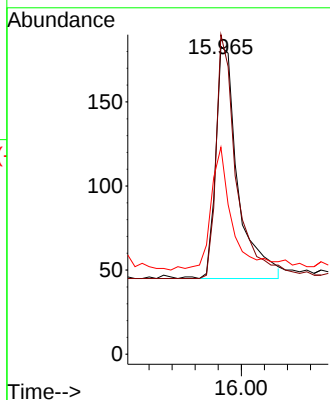

#15
2-Fluorobiphenyl
Concen: 0.339 ng
RT: 13.089 min Scan# 1410
Delta R.T. 0.000 min
Lab File: BN030316.D
Acq: 07 Mar 2024 07:01

Tgt Ion: 172 Resp: 3867
Ion Ratio Lower Upper
172 100
171 35.5 29.0 43.4
170 24.9 20.2 30.2


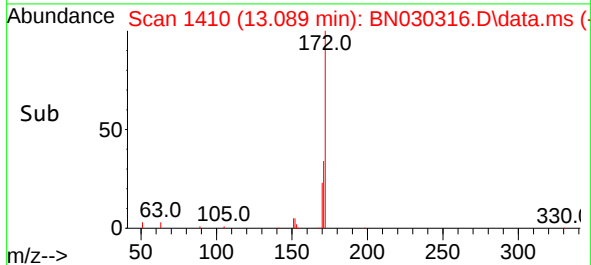
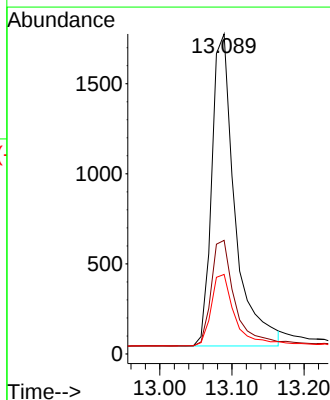
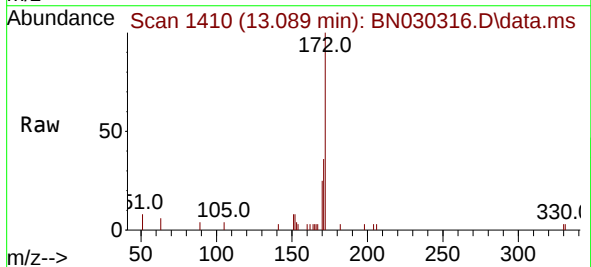




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.218 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN030316.D
Acq: 07 Mar 2024 07:01




Instrument :
BNA_N
ClientSampleId :
DUP09-20240222


Tgt Ion:188 Resp: 5354
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.1 7.8 11.6

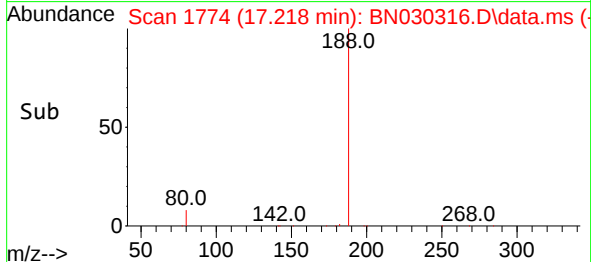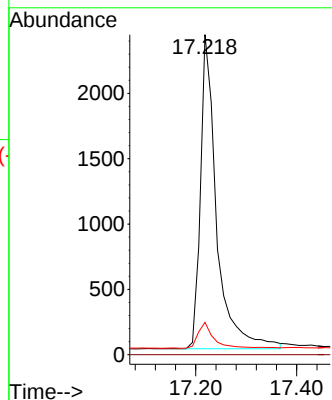

#27
Fluoranthene-d10
Concen: 0.365 ng
RT: 19.262 min Scan# 2040
Delta R.T. 0.000 min
Lab File: BN030316.D
Acq: 07 Mar 2024 07:01

Tgt Ion:212 Resp: 5368
Ion Ratio Lower Upper
212 100
106 10.2 8.2 12.4
104 6.1 4.7 7.1

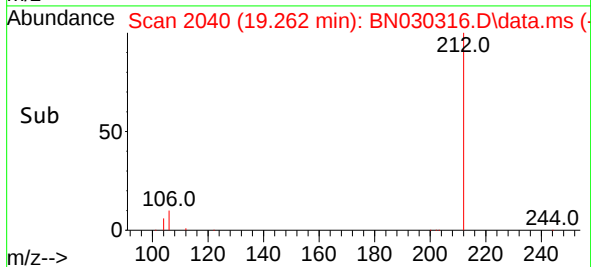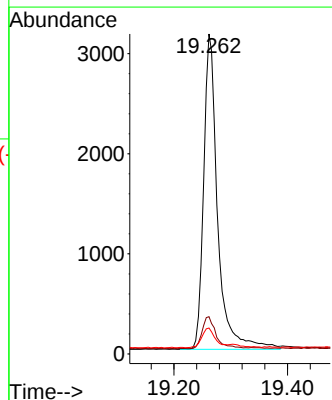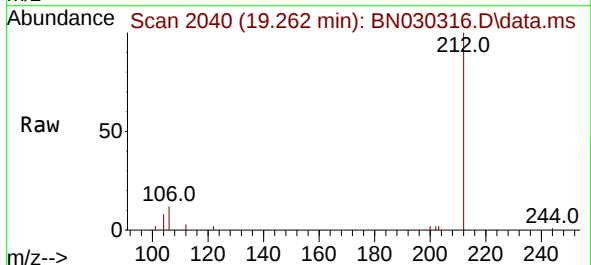



#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.438 min Scan# 2464

Delta R.T. 0.000 min

Lab File: BN030316.D


Acq: 07 Mar 2024 07:01

Instrument :




BNA_N

ClientSampleId :

DUP09-20240222



Tgt Ion:	240	Resp:	4312
Ion Ratio	Lower	Upper	
240	100		
120	15.4	12.2	18.2
236	29.9	25.2	37.8

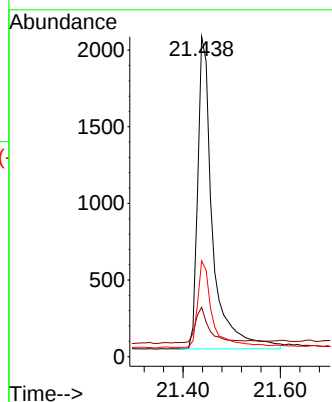

#31

Terphenyl-d14

Concen: 0.393 ng




RT: 19.875 min Scan# 2172


Delta R.T. -0.005 min

Lab File: BN030316.D

Acq: 07 Mar 2024 07:01

Tgt Ion:	244	Resp:	4395
Ion Ratio	Lower	Upper	
244	100		
212	11.2	9.5	14.3
122	13.2	11.8	17.6


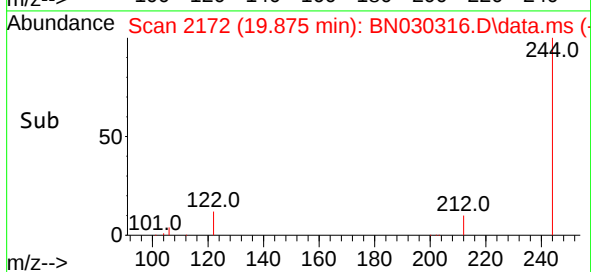

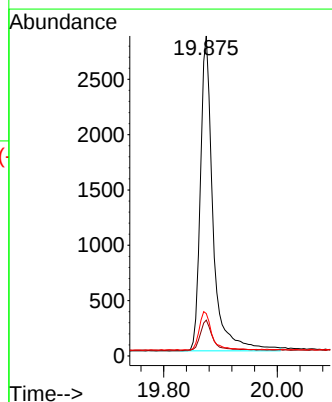


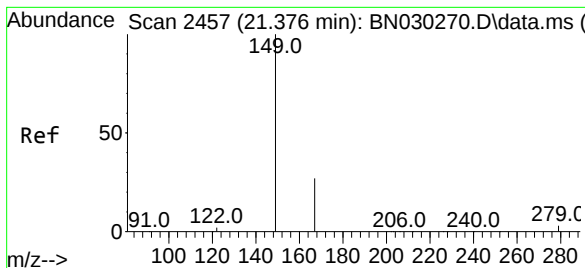

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.055 ng
 RT: 21.367 min Scan# 2456
 Delta R.T. -0.009 min
 Lab File: BN030316.D
 Acq: 07 Mar 2024 07:01

Instrument :
 BNA_N
 ClientSampleId :
 DUP09-20240222

Tgt Ion:149 Resp: 658
 Ion Ratio Lower Upper
 149 100
 167 23.4 20.6 30.8
 279 5.8 4.0 6.0

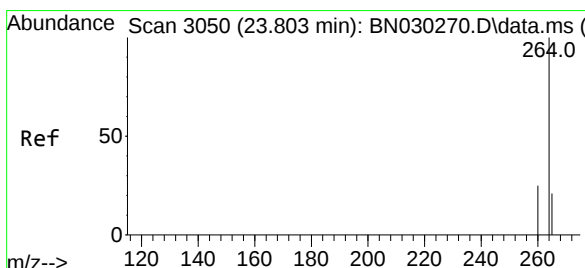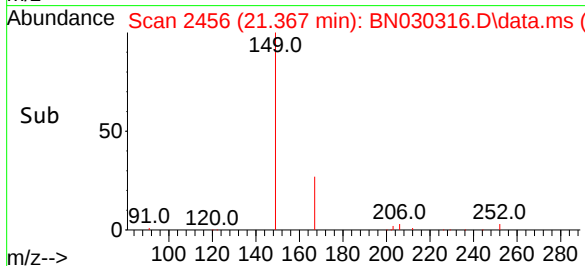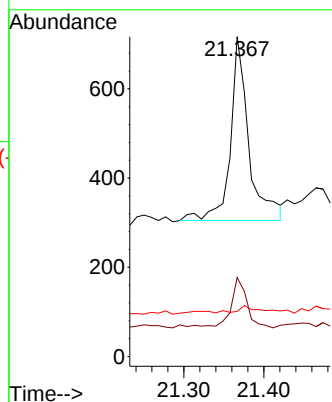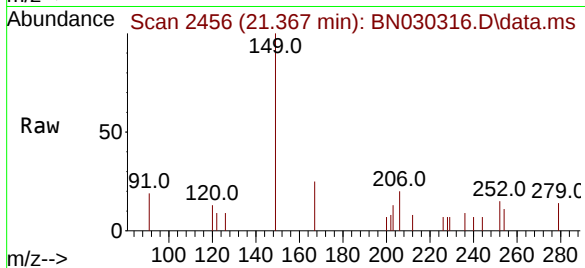

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.794 min Scan# 3047
 Delta R.T. -0.009 min
 Lab File: BN030316.D
 Acq: 07 Mar 2024 07:01

Tgt Ion:264 Resp: 4855
 Ion Ratio Lower Upper
 264 100
 260 27.2 21.7 32.5
 265 56.7 50.8 76.2

