
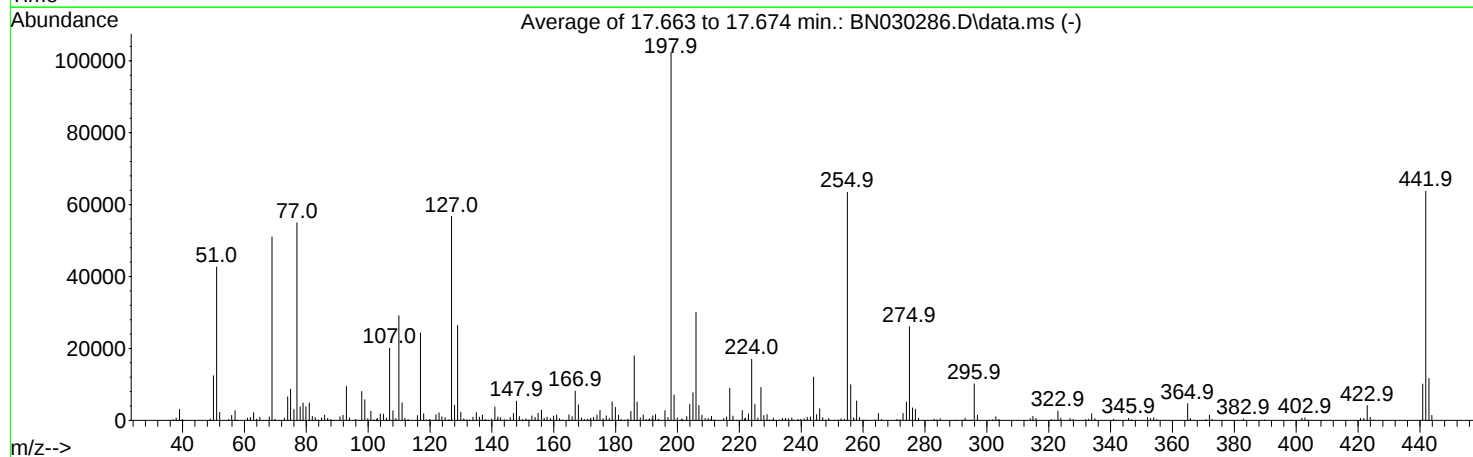


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030624\
Data File : BN030286.D
Acq On : 06 Mar 2024 09:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN030524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 05 17:44:16 2024

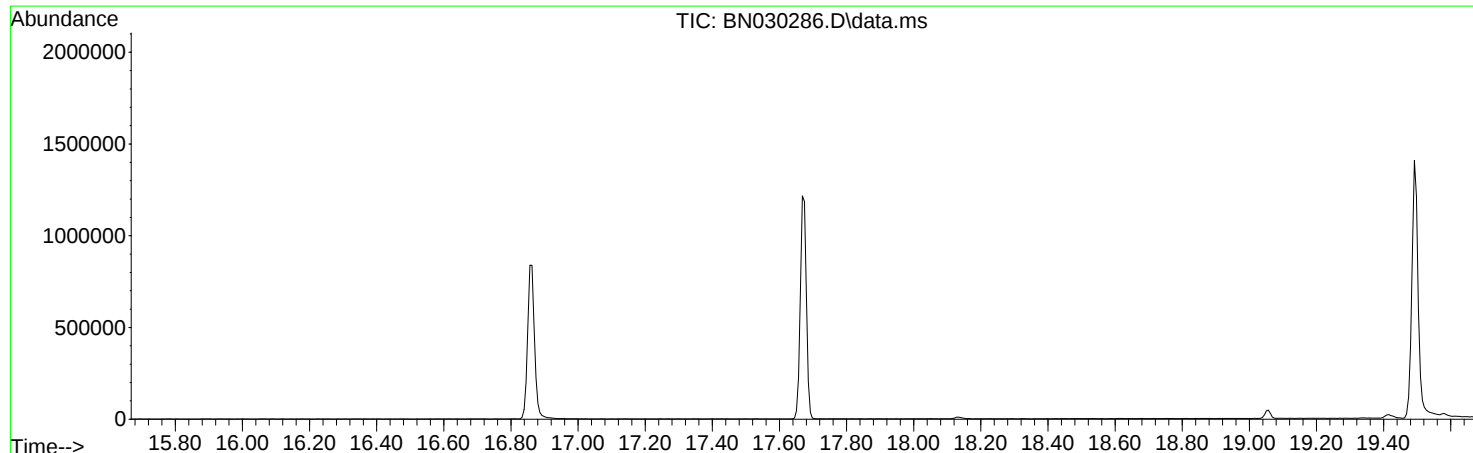




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	42672	PASS
68	69	0.00	2	2.0	996	PASS
69	198	0.00	100	49.8	50981	PASS
70	69	0.00	2	0.4	212	PASS
127	198	10	80	55.4	56725	PASS
197	198	0.00	2	0.8	807	PASS
198	198	100	100	100.0	102301	PASS
199	198	5	9	6.9	7082	PASS
275	198	10	60	25.5	26083	PASS
365	198	1	100	4.5	4633	PASS
441	198	0.01	100	9.9	10122	PASS
442	442	50	100	100.0	63731	PASS
443	442	15	24	18.3	11670	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030624\
Data File : BN030286.D
Acq On : 06 Mar 2024 09:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 07 04:38:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 07 04:37:16 2024
Response via : Initial Calibration

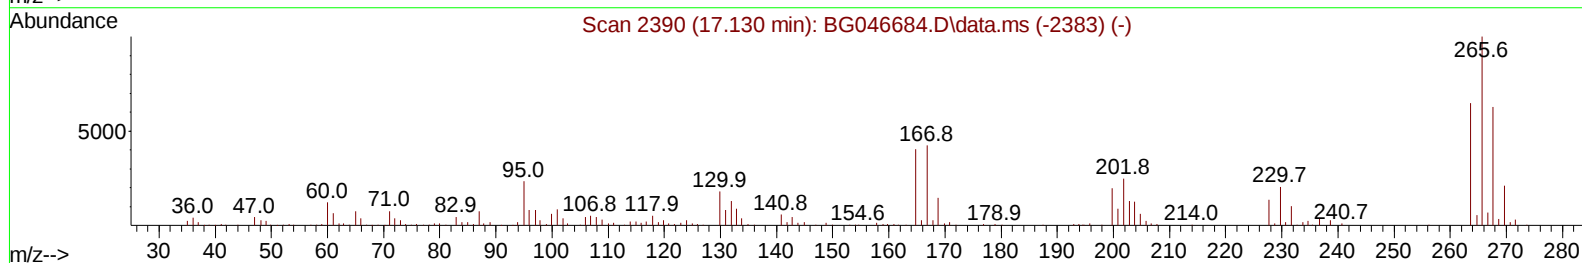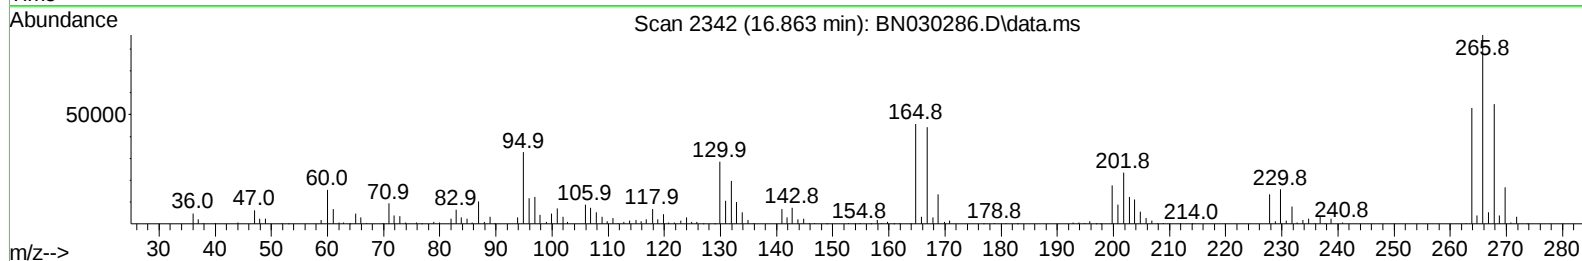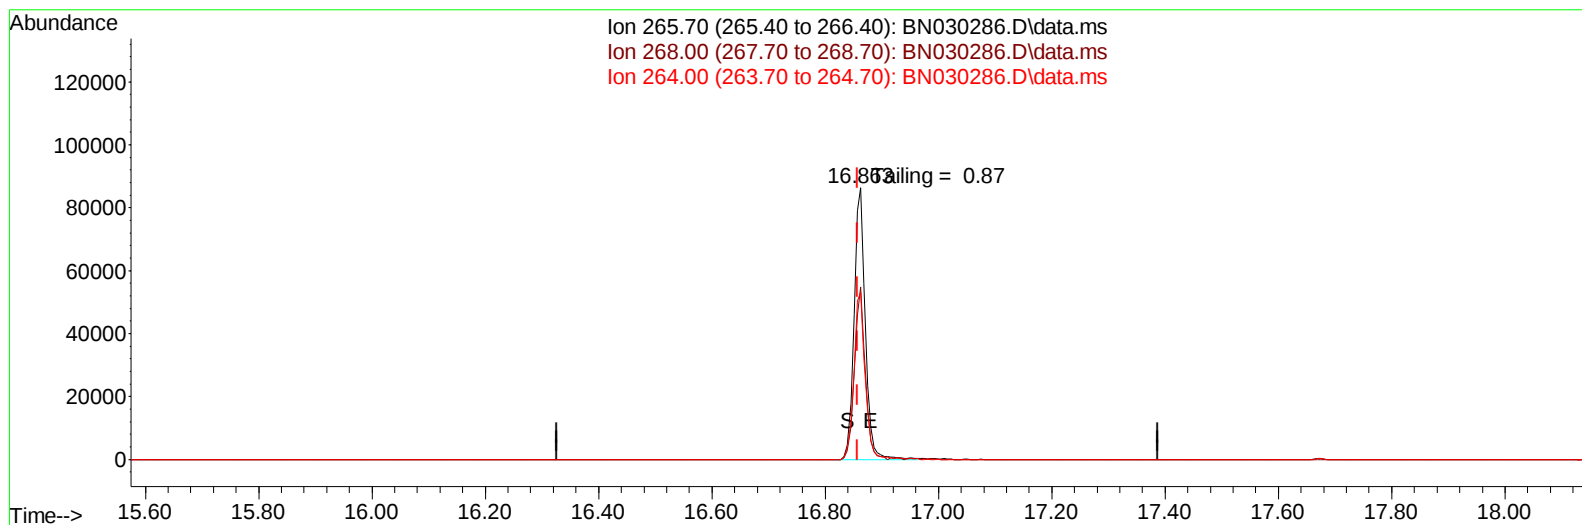

TIC: BN030286.D\data.ms

(70) Pentachlorophenol (C)

16.863min (+ 0.006) 16107.74 ng




response 119457

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.47
264.00	61.60	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030624\
Data File : BN030286.D
Acq On : 06 Mar 2024 09:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 07 04:38:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 07 04:37:16 2024
Response via : Initial Calibration

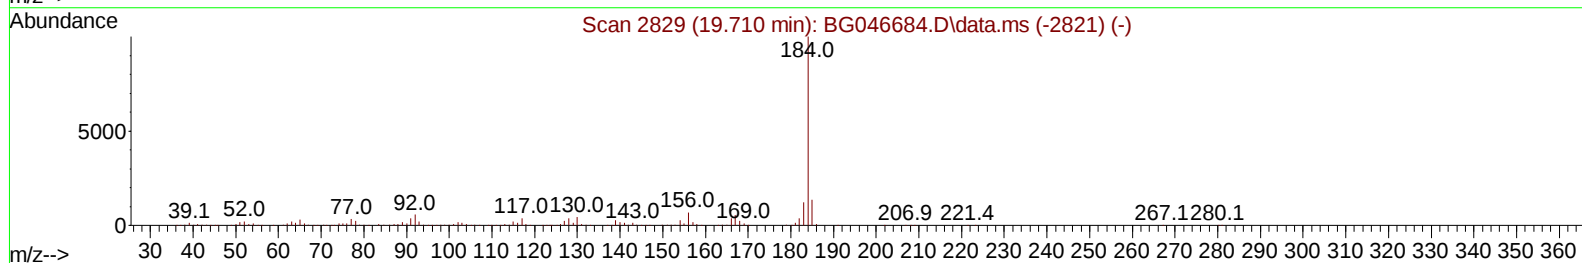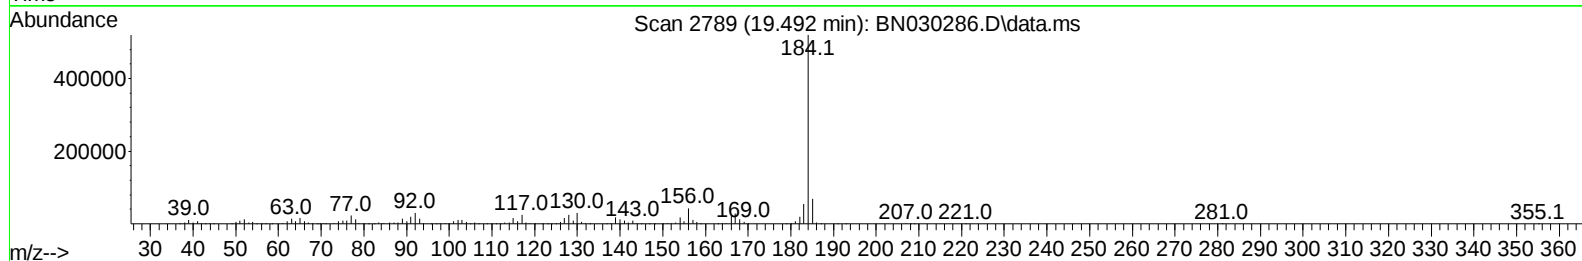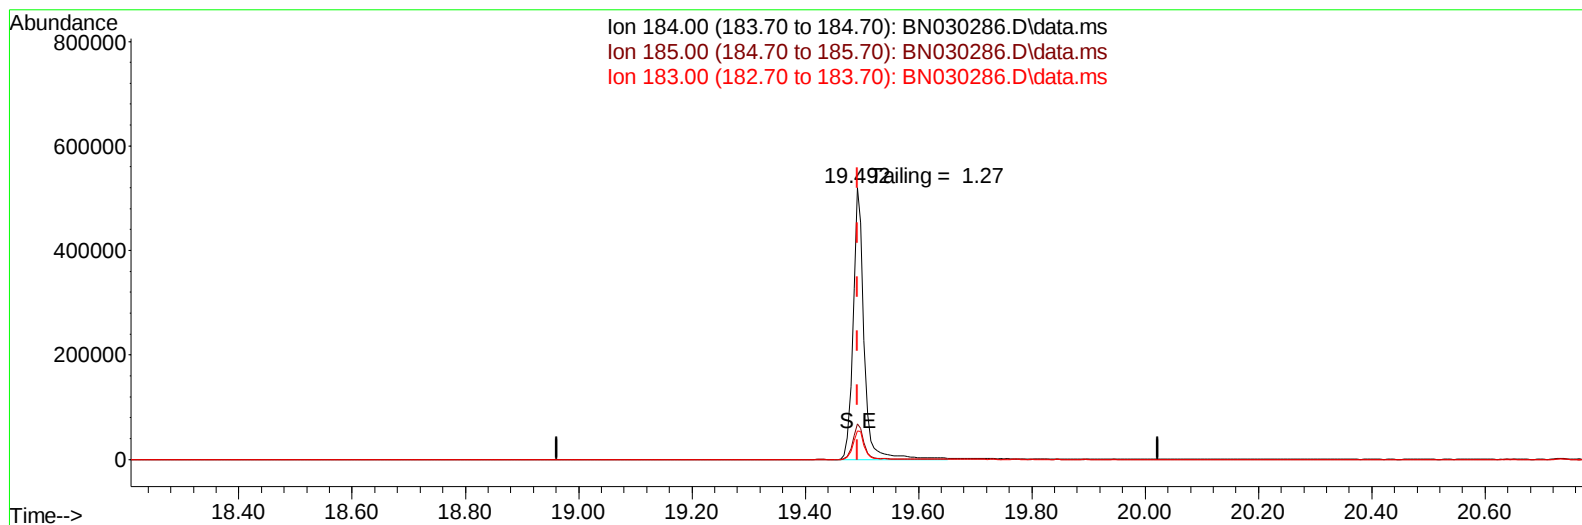

TIC: BN030286.D\data.ms

(77) Benzidine

19.492min (-0.000) 0.00 ng

response 706591

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.15
183.00	13.20	10.50#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/6/2024	BNA_N	<u>BN030286.D</u>
Compound Name	Response	Retention Time
DDT	356405	20.733
DDD	7463	20.292
DDE	415	19.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7878	364283	2.16

Instrument :
BNA_N
ClientSampleId :
DFTPP