
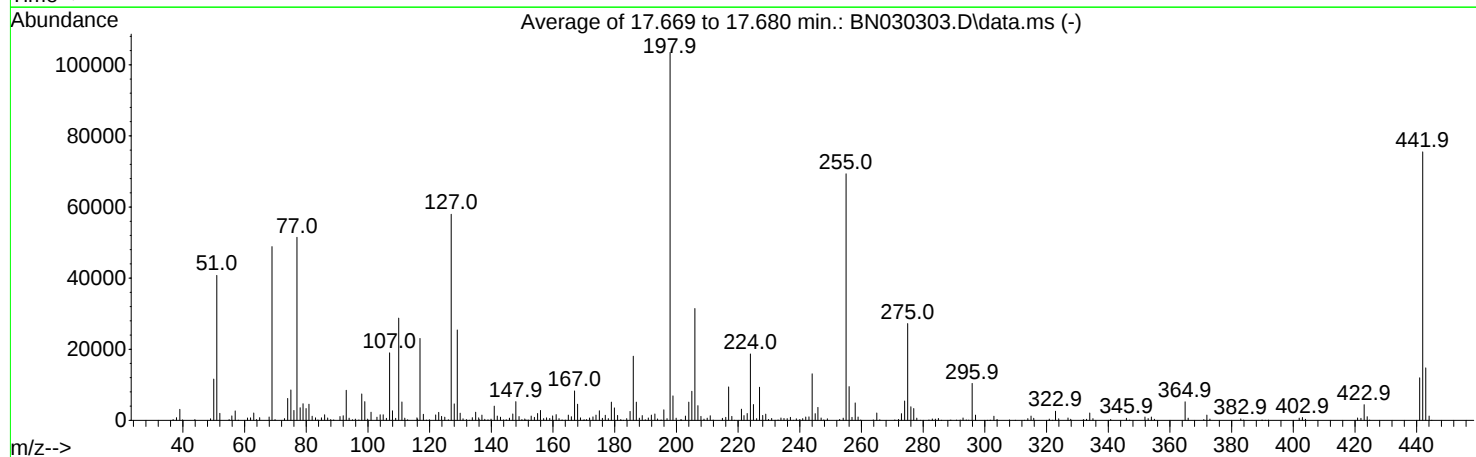


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030624\
Data File : BN030303.D
Acq On : 06 Mar 2024 23:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN030524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 05 17:44:16 2024

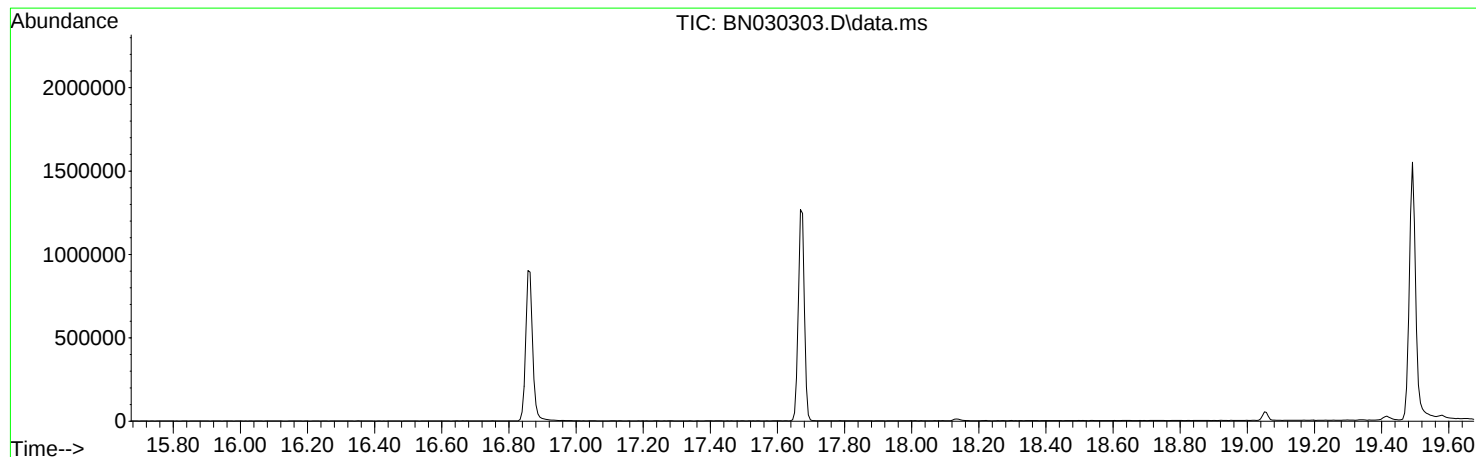




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	40789	PASS
68	69	0.00	2	1.9	927	PASS
69	198	0.00	100	47.2	48856	PASS
70	69	0.00	2	0.5	242	PASS
127	198	10	80	56.0	57952	PASS
197	198	0.00	2	0.5	478	PASS
198	198	100	100	100.0	103453	PASS
199	198	5	9	6.7	6899	PASS
275	198	10	60	26.3	27224	PASS
365	198	1	100	5.1	5229	PASS
441	198	0.01	100	11.6	11984	PASS
442	442	50	100	100.0	75531	PASS
443	442	15	24	19.5	14756	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030624\
Data File : BN030303.D
Acq On : 06 Mar 2024 23:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 07 04:37:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 07 04:37:16 2024
Response via : Initial Calibration

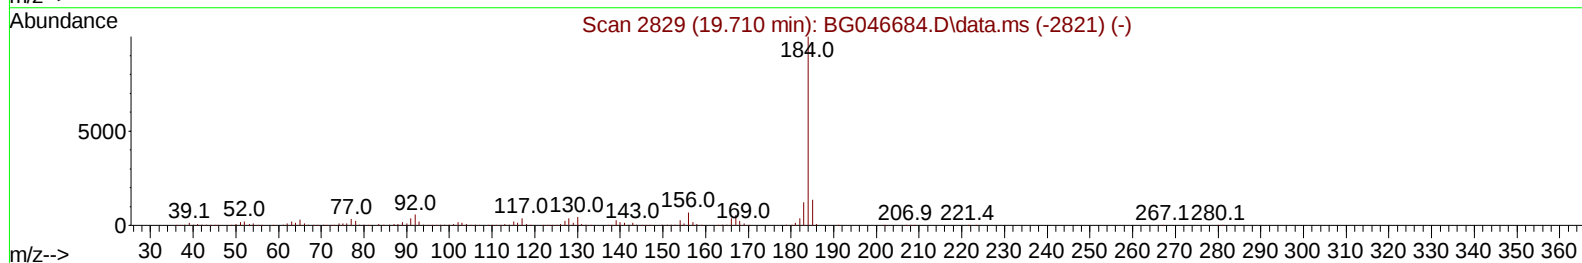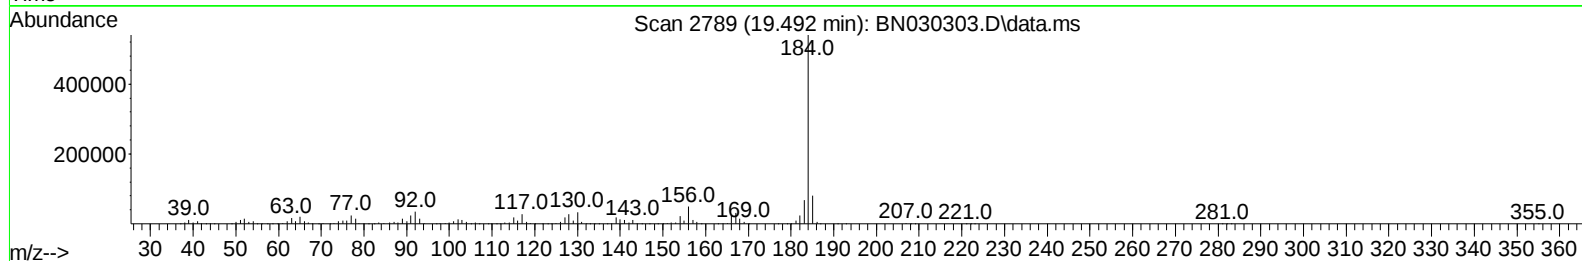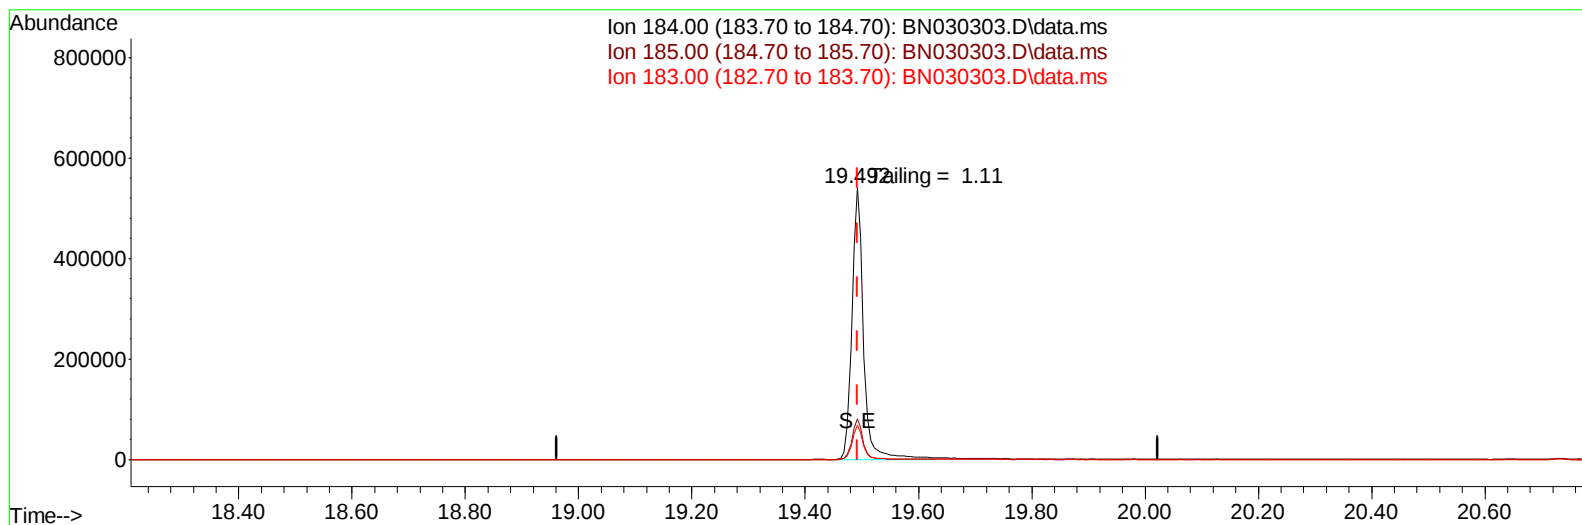

TIC: BN030303.D\data.ms

(77) Benzidine

19.492min (0.000) 0.00 ng

response 776283

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.92
183.00	13.20	12.59
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/6/2024	BNA_N	<u>BN030303.D</u>
Compound Name	Response	Retention Time
DDT	403679	20.733
DDD	9097	20.286
DDE	398	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9495	413174	2.30

Instrument :
BNA_N
ClientSampleId :
DFTPP