
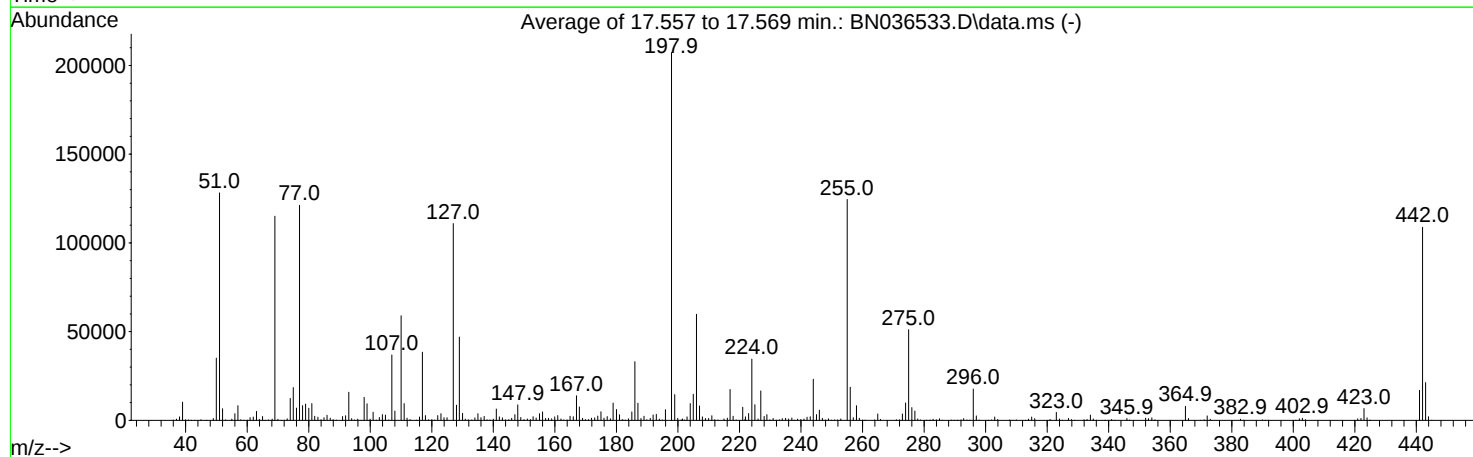


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030625\
Data File : BN036533.D
Acq On : 06 Mar 2025 12:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN021025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 05 16:08:57 2025

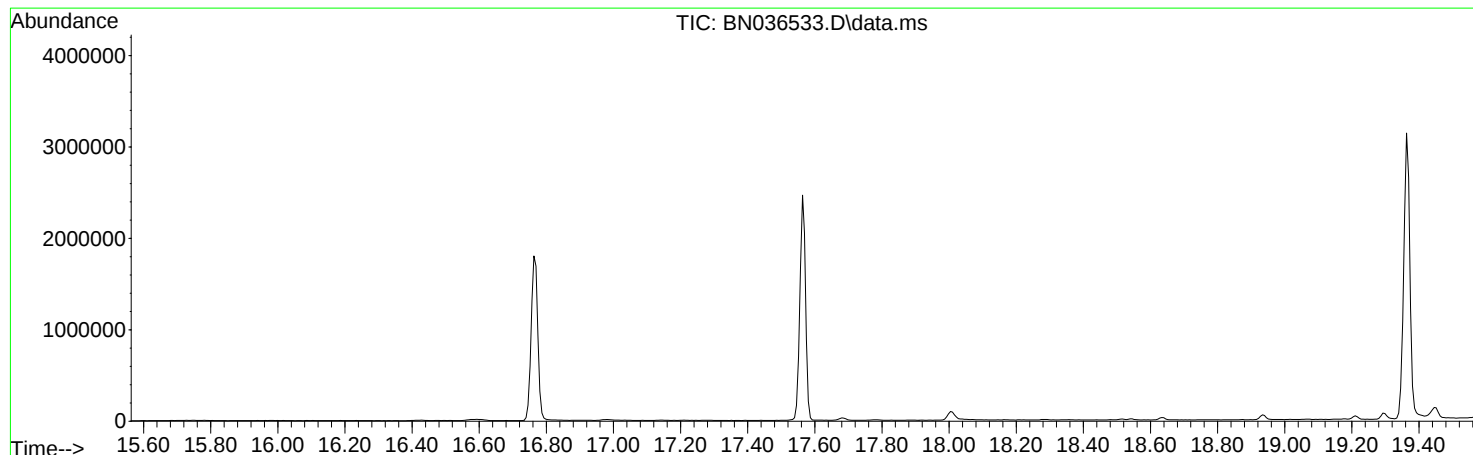

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.8	128173	PASS
68	69	0.00	2	0.6	732	PASS
69	198	0.00	100	55.5	115029	PASS
70	69	0.00	2	0.5	622	PASS
127	198	10	80	53.5	110859	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	207275	PASS
199	198	5	9	7.0	14559	PASS
275	198	10	60	24.7	51104	PASS
365	198	1	100	3.8	7940	PASS
441	198	0.01	100	8.2	16994	PASS
442	442	50	100	100.0	108805	PASS
443	442	15	24	19.5	21267	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/6/2025	BNA_N	<u>BN036533.D</u>
Compound Name	Response	Retention Time
DDT	797297	20.604
DDD	10816	20.216
DDE	504	19.651
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11320	808617	1.40

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030625\
Data File : BN036533.D
Acq On : 06 Mar 2025 12:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 06 17:29:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

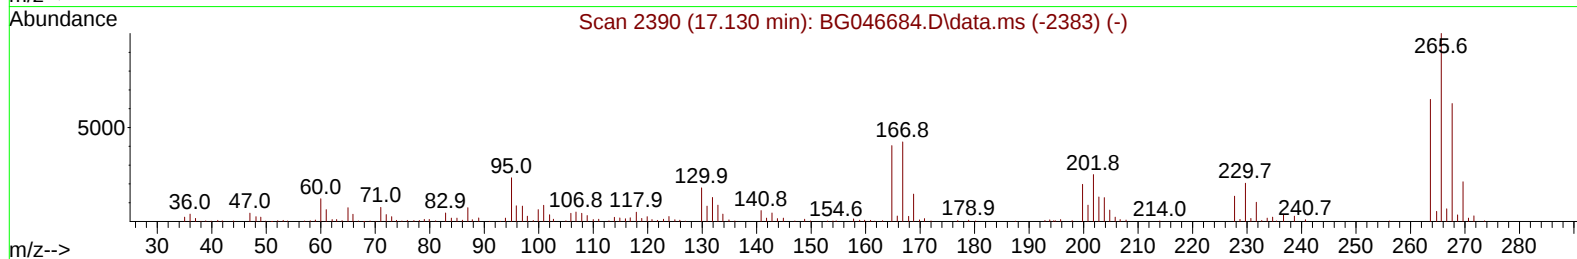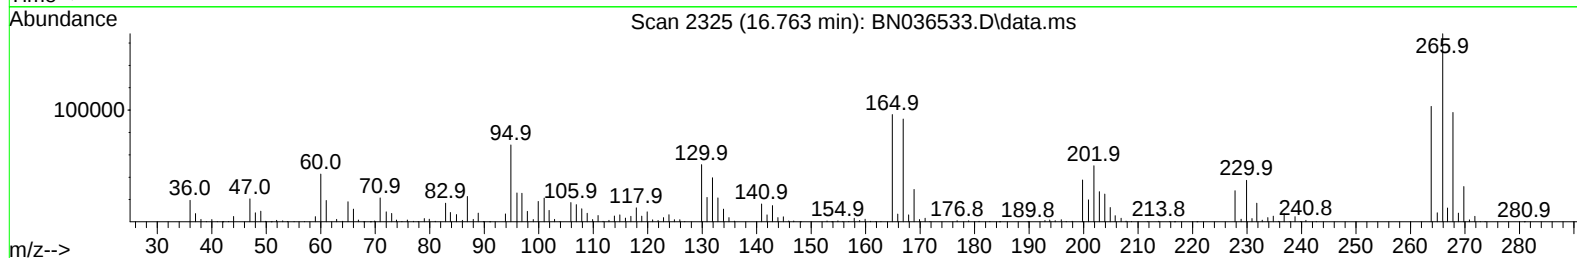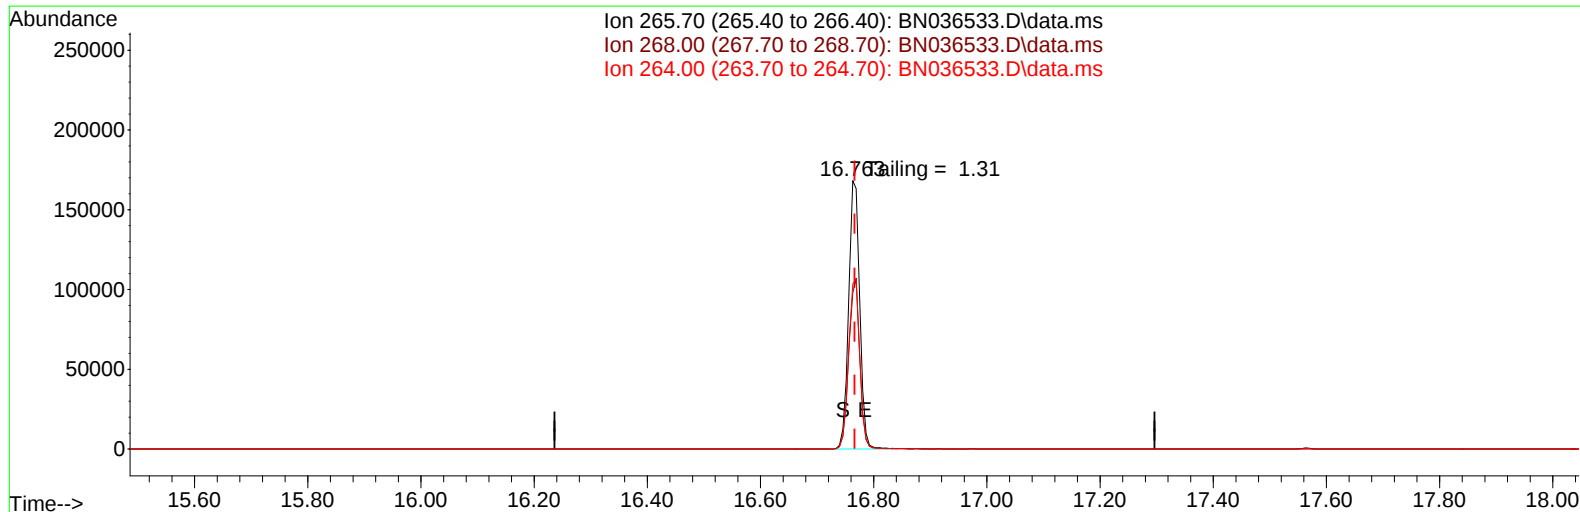

TIC: BN036533.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.003) 20834.00 ng




response 229554

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.20
264.00	61.60	61.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030625\
Data File : BN036533.D
Acq On : 06 Mar 2025 12:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 06 17:29:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

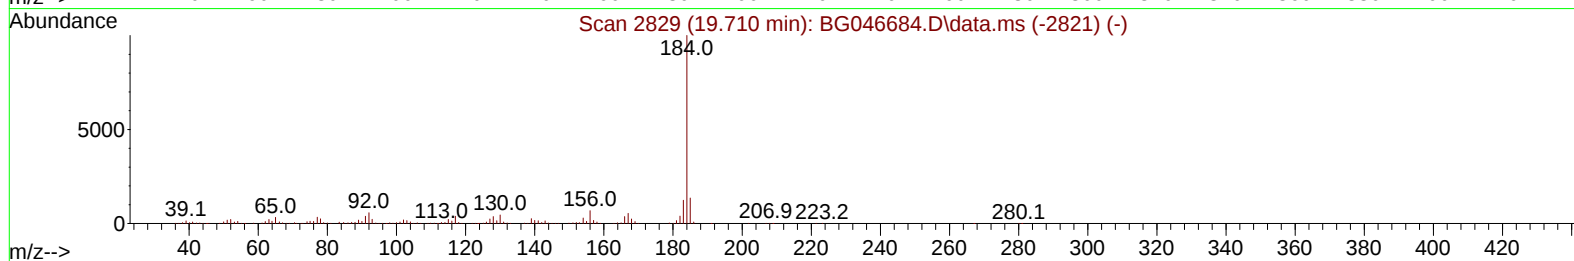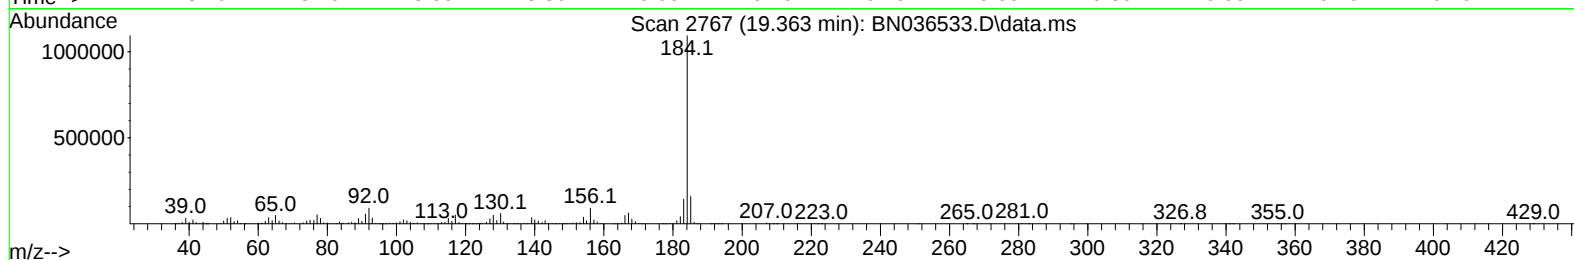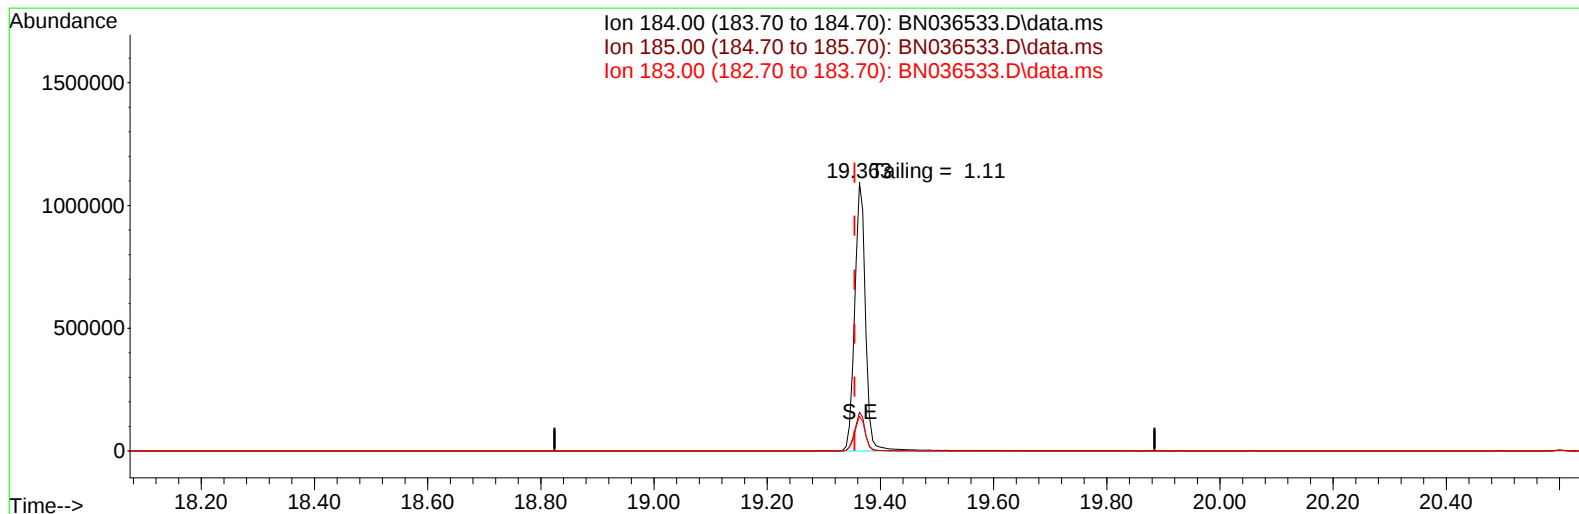

TIC: BN036533.D\data.ms

(77) Benzidine

19.363min (+ 0.009) 0.00 ng

response 1456970

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.50
183.00	13.20	13.03
0.00	0.00	0.00