

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030723\
 Data File : BN024137.D
 Acq On : 07 Mar 2023 09:34
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020259

Quant Time: Mar 08 03:03:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 07 04:27:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.052	152	329327	20.000	ng/u1	0.00
20) Naphthalene-d8	10.881	136	1429968	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.698	164	835910	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	1730698	20.000	ng/u1	0.00
79) Chrysene-d12	21.639	240	1518918	20.000	ng/u1	0.00
88) Perylene-d12	24.151	264	1695639	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	71512	8.471	ng/uL	0.00
4) Pyridine-d5	3.828	84	521309	22.316	ng/u1	0.00
7) Phenol-d5	7.199	99	629185	21.299	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.375	67	423499	22.387	ng/u1	0.00
11) 2-Chlorophenol-d4	7.581	132	493101	21.736	ng/u1	0.00
15) 4-Methylphenol-d8	8.757	113	488911	20.820	ng/u1	0.00
21) Nitrobenzene-d5	9.222	128	204633	22.048	ng/u1	0.00
24) 2-Nitrophenol-d4	9.951	143	224145	22.146	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	469585	21.501	ng/u1	0.00
31) 4-Chloroaniline-d4	11.010	131	683262	20.969	ng/u1	0.00
46) Dimethylphthalate-d6	14.104	166	1344589	20.842	ng/u1	0.00
49) Acenaphthylene-d8	14.392	160	1621951	21.599	ng/u1	0.00
54) 4-Nitrophenol-d4	14.875	143	250519	20.323	ng/u1	0.00
60) Fluorene-d10	15.686	176	1140928	21.043	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	177002	18.983	ng/u1	0.00
73) Anthracene-d10	17.539	188	1727921	21.170	ng/u1	0.00
81) Pyrene-d10	19.833	212	1913352	21.554	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.992	264	1831659	21.730	ng/u1	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.446	88	77756	8.505	ng/uL	93
5) Pyridine	3.852	79	535969	22.164	ng/u1	99
6) Benzaldehyde	7.181	77	379307	26.429	ng/u1	97
8) Phenol	7.228	94	658978	21.519	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.469	93	543787	21.914	ng/u1	98
12) 2-Chlorophenol	7.610	128	506939	21.524	ng/u1	99
13) 2-Methylphenol	8.493	108	491123	21.327	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.587	45	876005	22.251	ng/u1	99
16) Acetophenone	8.881	105	806878	22.133	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.869	70	389706	21.771	ng/u1	98
18) 4-Methylphenol	8.822	108	539735	21.295	ng/u1	100
19) Hexachloroethane	9.151	117	203452	21.997	ng/u1	97
22) Nitrobenzene	9.269	77	565485	22.506	ng/u1	99
23) Isophorone	9.793	82	1163334	21.184	ng/u1	99
25) 2-Nitrophenol	9.981	139	262620	22.588	ng/u1	99
26) 2,4-Dimethylphenol	10.034	107	563033	21.248	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.281	93	724043	21.234	ng/u1	98
29) 2,4-Dichlorophenol	10.516	162	474612	21.531	ng/u1	98
30) Naphthalene	10.928	128	1655159	21.033	ng/u1	99
32) 4-Chloroaniline	11.034	127	691355	21.041	ng/u1	99
33) Hexachlorobutadiene	11.216	225	284679	21.191	ng/u1	92
34) Caprolactam	11.792	113	79831	10.620	ng/u1	96
35) 4-Chloro-3-methylphenol	12.145	107	509172	20.968	ng/u1	98
36) 2-Methylnaphthalene	12.528	142	1098987	21.211	ng/u1	97


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030723\
 Data File : BN024137.D
 Acq On : 07 Mar 2023 09:34
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020259

Quant Time: Mar 08 03:03:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 07 04:27:04 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.751	142	1079945	20.798	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.898	216	525777	20.902	ng/ul	96
40) Hexachlorocyclopentadiene	12.881	237	273811	20.198	ng/ul	99
41) 2,4,6-Trichlorophenol	13.128	196	344251	20.891	ng/ul	98
42) 2,4,5-Trichlorophenol	13.198	196	386980	21.806	ng/ul	93
43) 1,1'-Biphenyl	13.534	154	1421564	21.349	ng/ul	96
44) 2-Chloronaphthalene	13.575	162	1117182	21.534	ng/ul	100
45) 2-Nitroaniline	13.775	65	257862	22.814	ng/ul	97
47) Dimethylphthalate	14.151	163	1359165	20.903	ng/ul	99
48) 2,6-Dinitrotoluene	14.269	165	212690	22.222	ng/ul	95
50) Acenaphthylene	14.416	152	1731558	21.398	ng/ul	99
51) 3-Nitroaniline	14.592	138	243826	20.958	ng/ul	99
52) Acenaphthene	14.757	153	1186492	21.495	ng/ul	97
53) 2,4-Dinitrophenol	14.792	184	112068	16.913	ng/ul	99
55) 4-Nitrophenol	14.886	109	189315	20.160	ng/ul	97
56) Dibenzofuran	15.092	168	1601579	20.653	ng/ul	98
57) 2,4-Dinitrotoluene	15.051	165	334253	22.155	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.310	232	315070	20.653	ng/ul	97
59) Diethylphthalate	15.510	149	1338489	20.651	ng/ul	99
61) Fluorene	15.739	166	1280963	21.085	ng/ul	96
62) 4-Chlorophenyl-phenyle...	15.733	204	600650	20.678	ng/ul	97
63) 4-Nitroaniline	15.757	138	235897	20.968	ng/ul	96
66) 4,6-Dinitro-2-methylph...	15.810	198	182107	19.307	ng/ul	97
67) N-Nitrosodiphenylamine	15.945	169	1099765	21.459	ng/ul	97
68) 4-Bromophenyl-phenylether	16.628	248	346199	20.120	ng/ul	88
69) Hexachlorobenzene	16.745	284	411403	19.654	ng/ul	96
70) Atrazine	16.898	200	354196	20.417	ng/ul	98
71) Pentachlorophenol	17.086	266	264546	20.430	ng/ul	97
72) Phenanthrene	17.486	178	2018672	21.055	ng/ul	97
74) Anthracene	17.580	178	2031130	21.012	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.498	216	543455	21.545	ng/ul	92
76) Pentachlorobenzene	15.010	250	524698	21.348	ng/ul	90
77) Carbazole	17.845	167	1871573	21.619	ng/ul	100
78) Di-n-butylphthalate	18.410	149	2231121	21.652	ng/ul	100
80) Fluoranthene	19.498	202	2278494	22.079	ng/ul	99
82) Pyrene	19.857	202	2372243	21.788	ng/ul	99
83) Butylbenzylphthalate	20.763	149	605556	21.840	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.551	252	636663	21.748	ng/ul	93
85) Benzo(a)anthracene	21.621	228	2265552	21.399	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.545	149	1057189	22.975	ng/ul	99
87) Chrysene	21.680	228	2188482	21.596	ng/ul	98
89) Di-n-octyl phthalate	22.515	149	1754654	19.349	ng/ul	100
90) Benzo(b)fluoranthene	23.386	252	2328884	21.815	ng/ul	95
91) Benzo(k)fluoranthene	23.439	252	2292813	21.715	ng/ul	99
93) Benzo(a)pyrene	24.045	252	2026574	21.436	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.792	276	2400516	20.162	ng/ul	96
95) Dibenzo(a,h)anthracene	26.809	278	2038515	21.027	ng/ul	100
96) Benzo(g,h,i)perylene	27.598	276	1969675	20.051	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed






#2
1,4-Dioxane
Concen: 8.505 ng/uL
RT: 3.446 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Instrument :
BNA_N
ClientSampleId :
SSTD020259







Tgt Ion: 88 Resp: 77756
Ion Ratio Lower Upper
88 100
43 31.0 26.2 39.4
58 73.8 64.9 97.3

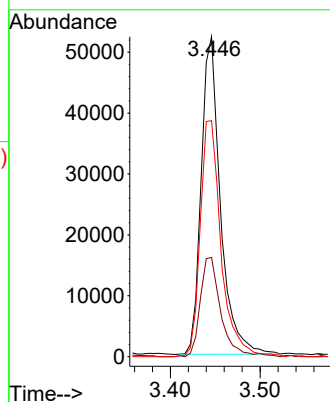

#5
Pyridine
Concen: 22.164 ng/uL
RT: 3.852 min Scan# 130
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion: 79 Resp: 535969
Ion Ratio Lower Upper
79 100
52 82.7 65.1 97.7
51 39.2 31.4 47.0



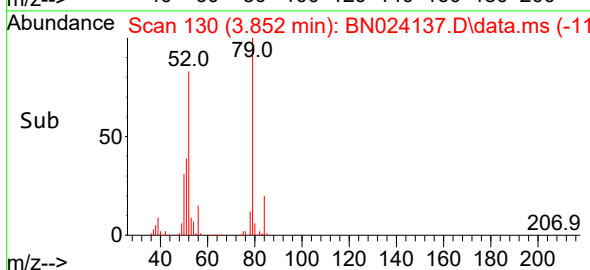





#6
Benzaldehyde
Concen: 26.429 ng/ul
RT: 7.181 min Scan# 697
Delta R.T. -0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion: 77 Resp: 379307
Ion Ratio Lower Upper
77 100
105 95.9 79.2 118.8
106 91.3 75.9 113.9



#8
Phenol
Concen: 21.519 ng/ul
RT: 7.228 min Scan# 704
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion: 94 Resp: 658978
Ion Ratio Lower Upper
94 100
65 28.0 22.9 34.3
66 35.8 29.0 43.6









#10
Bis(2-Chloroethyl)ether
Concen: 21.914 ng/ul
RT: 7.469 min Scan# 746
Delta R.T. -0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion: 93 Resp: 543787
Ion Ratio Lower Upper
93 100
63 80.5 62.6 93.8
95 32.7 25.8 38.6

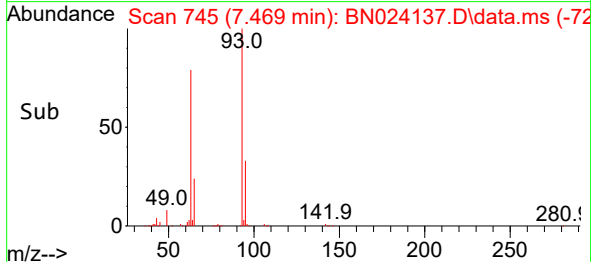

#12
2-Chlorophenol
Concen: 21.524 ng/ul
RT: 7.610 min Scan# 769
Delta R.T. -0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion: 128 Resp: 506939
Ion Ratio Lower Upper
128 100
64 50.1 39.3 58.9
130 31.4 25.1 37.7


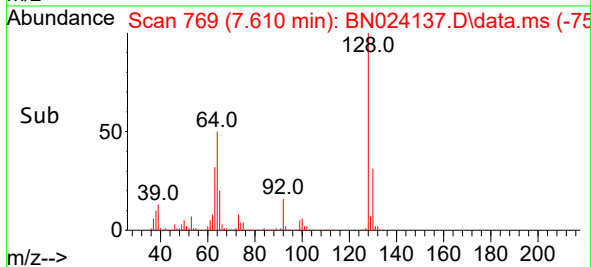

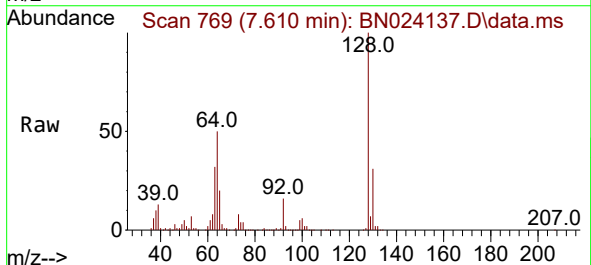




#13
2-Methylphenol
Concen: 21.327 ng/ul
RT: 8.493 min Scan# 919
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:108 Resp: 491123
Ion Ratio Lower Upper
108 100
107 88.7 72.3 108.5

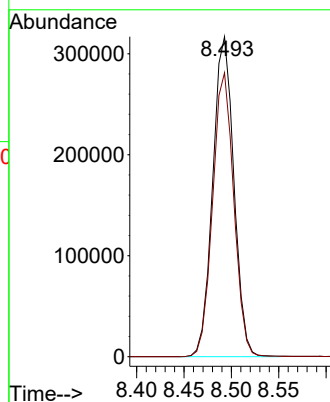

#14
2,2'-oxybis(1-Chloropropane)
Concen: 22.251 ng/ul
RT: 8.587 min Scan# 935
Delta R.T. -0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion: 45 Resp: 876005
Ion Ratio Lower Upper
45 100
77 11.9 9.8 14.6
79 9.0 7.4 11.0









#16
Acetophenone
Concen: 22.133 ng/ul
RT: 8.881 min Scan# 91
Delta R.T. -0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:105 Resp: 806878
Ion Ratio Lower Upper
105 100
77 77.3 61.4 92.0
51 29.7 23.8 35.8

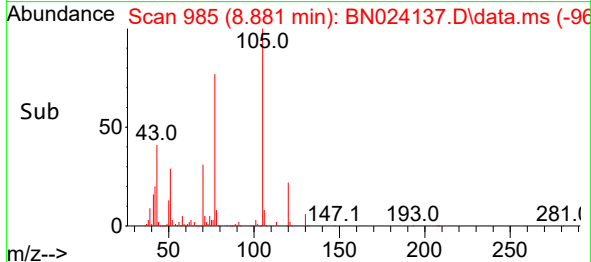

#17
N-Nitroso-di-n-propylamine
Concen: 21.771 ng/ul
RT: 8.869 min Scan# 983
Delta R.T. -0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion: 70 Resp: 389706
Ion Ratio Lower Upper
70 100
42 65.0 50.8 76.2
101 9.0 7.2 10.8
130 18.7 15.8 23.8


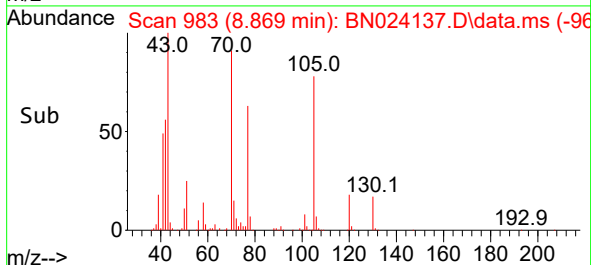
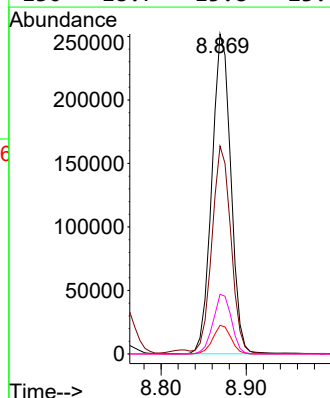
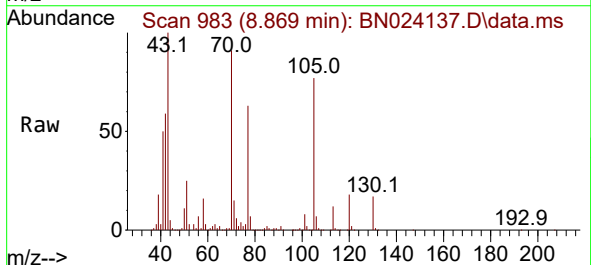




#18
4-Methylphenol
Concen: 21.295 ng/ul
RT: 8.822 min Scan# 91
Delta R.T. -0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:108 Resp: 539735
Ion Ratio Lower Upper
108 100
107 110.2 87.8 131.6



#19
Hexachloroethane
Concen: 21.997 ng/ul
RT: 9.151 min Scan# 1031
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:117 Resp: 203452
Ion Ratio Lower Upper
117 100
201 95.5 73.8 110.6
199 60.5 47.2 70.8









#22
Nitrobenzene
Concen: 22.506 ng/ul
RT: 9.269 min Scan# 110
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion: 77 Resp: 565485
Ion Ratio Lower Upper
77 100
123 43.9 34.8 52.2
65 13.2 11.0 16.4

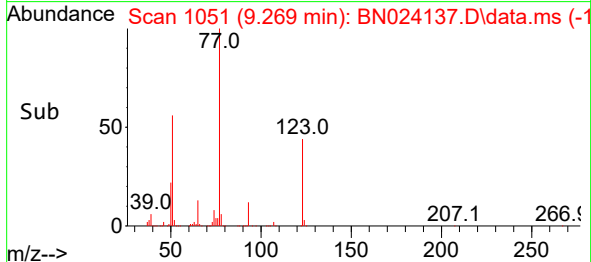

#23
Isophorone
Concen: 21.184 ng/ul
RT: 9.793 min Scan# 1140
Delta R.T. -0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion: 82 Resp: 1163334
Ion Ratio Lower Upper
82 100
95 6.8 5.0 7.6
138 16.9 13.8 20.6


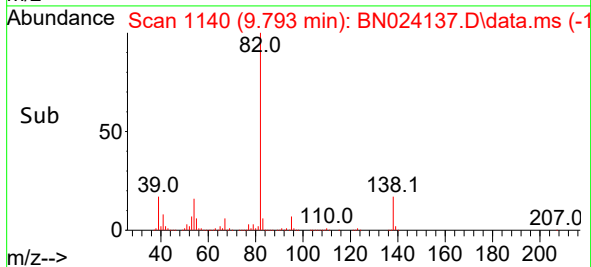

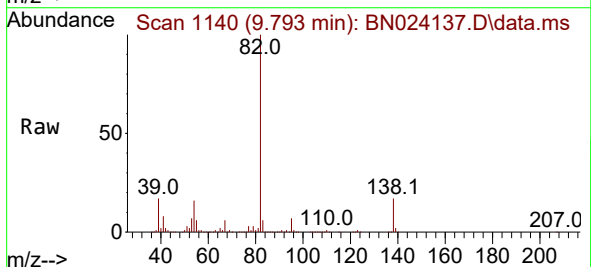




#25
2-Nitrophenol
Concen: 22.588 ng/ul
RT: 9.981 min Scan# 1172
Delta R.T. -0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:139 Resp: 262620
Ion Ratio Lower Upper
139 100
65 54.6 44.5 66.7
109 28.5 23.4 35.2



#26
2,4-Dimethylphenol
Concen: 21.248 ng/ul
RT: 10.034 min Scan# 1181
Delta R.T. -0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:107 Resp: 563033
Ion Ratio Lower Upper
107 100
121 51.8 40.2 60.2
122 91.6 71.8 107.8









#27
 Bis(2-Chloroethoxy)methane
 Concen: 21.234 ng/ul
 RT: 10.281 min Scan# 1223
 Delta R.T. -0.000 min
 Lab File: BN024137.D
 Acq: 07 Mar 2023 09:34

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020259

Tgt Ion: 93 Resp: 724043




Ion	Ratio	Lower	Upper
93	100		
95	32.7	25.4	38.2
123	11.2	8.6	12.8

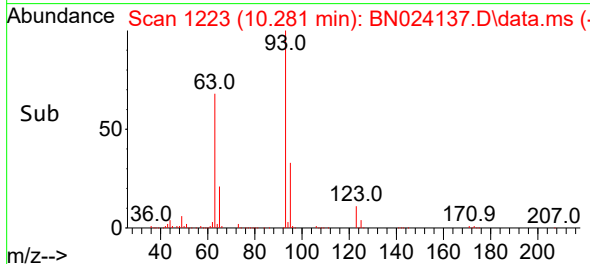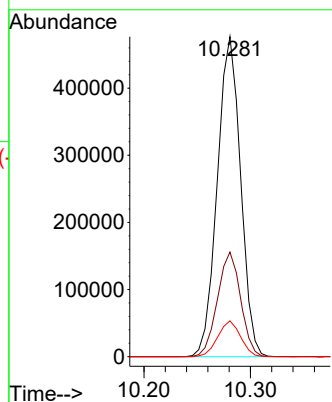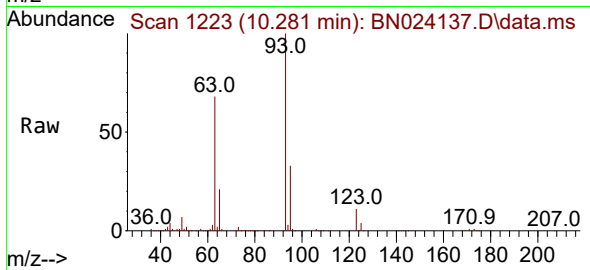


#29
 2,4-Dichlorophenol
 Concen: 21.531 ng/ul
 RT: 10.516 min Scan# 1263
 Delta R.T. -0.000 min
 Lab File: BN024137.D
 Acq: 07 Mar 2023 09:34

Tgt Ion: 162 Resp: 474612

Ion	Ratio	Lower	Upper
162	100		
164	63.6	52.6	78.8
98	37.4	29.8	44.8


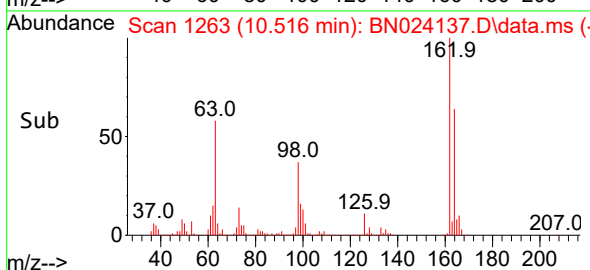




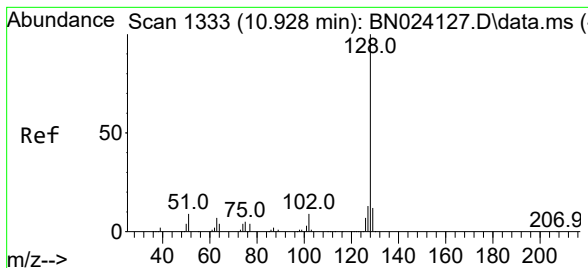

#30
Naphthalene
Concen: 21.033 ng/ul
RT: 10.928 min Scan# 1333
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:128 Resp: 1655159
Ion Ratio Lower Upper
128 100
129 10.8 8.6 12.8
127 13.1 10.1 15.1

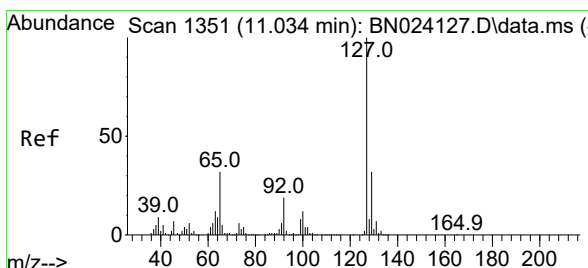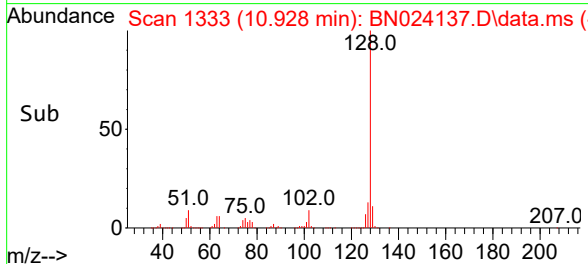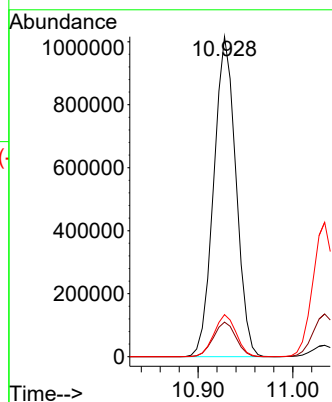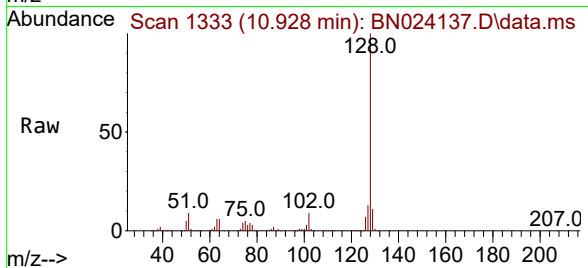

#32
4-Chloroaniline
Concen: 21.041 ng/ul
RT: 11.034 min Scan# 1351
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:127 Resp: 691355
Ion Ratio Lower Upper
127 100
129 31.8 25.1 37.7


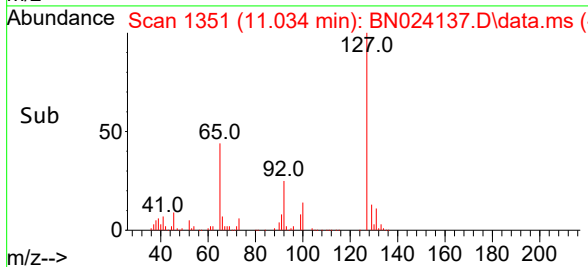
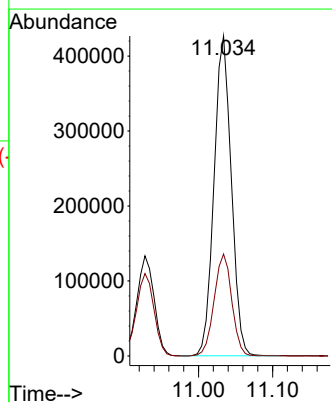
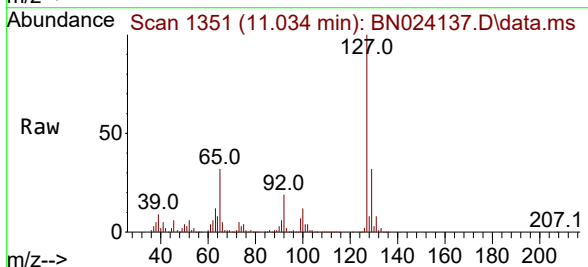




#33
Hexachlorobutadiene
Concen: 21.191 ng/ul
RT: 11.216 min Scan# 1382
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:225 Resp: 284679
Ion Ratio Lower Upper
225 100
223 59.8 53.6 80.4
227 61.1 53.0 79.4



#34
Caprolactam
Concen: 10.620 ng/ul
RT: 11.792 min Scan# 1480
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:113 Resp: 79831
Ion Ratio Lower Upper
113 100
55 196.9 155.4 233.2
56 147.9 111.0 166.6




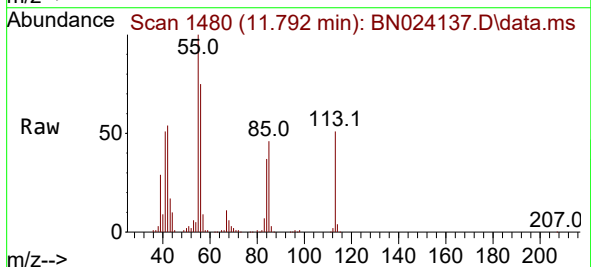




#35
4-Chloro-3-methylphenol
Concen: 20.968 ng/ul
RT: 12.145 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:107 Resp: 509172
Ion Ratio Lower Upper
107 100
144 25.6 21.0 31.4
142 80.3 65.7 98.5

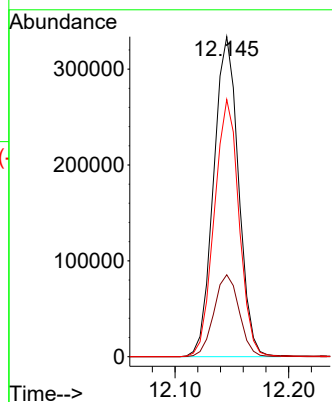

#36
2-Methylnaphthalene
Concen: 21.211 ng/ul
RT: 12.528 min Scan# 1605
Delta R.T. -0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:142 Resp: 1098987
Ion Ratio Lower Upper
142 100
141 88.4 68.2 102.4


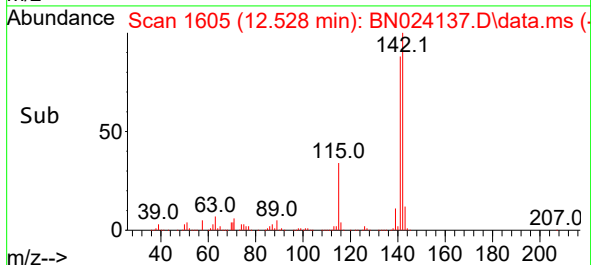

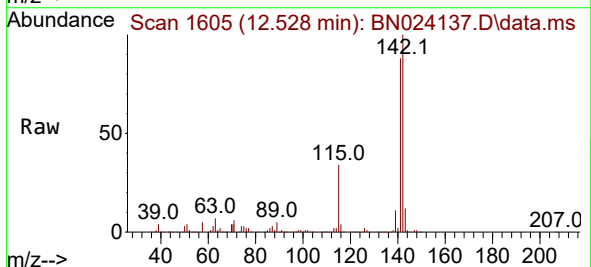




#37
1-Methylnaphthalene
Concen: 20.798 ng/ul
RT: 12.751 min Scan# 1643
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:142 Resp: 1079945
Ion Ratio Lower Upper
142 100
141 94.1 75.5 113.3
116 3.7 3.1 4.7

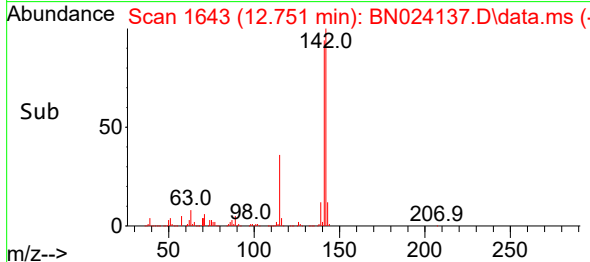

#39
1,2,4,5-Tetrachlorobenzene
Concen: 20.902 ng/ul
RT: 12.898 min Scan# 1668
Delta R.T. 0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:216 Resp: 525777
Ion Ratio Lower Upper
216 100
214 80.5 60.0 90.0
179 21.0 17.0 25.6
108 17.7 14.3 21.5


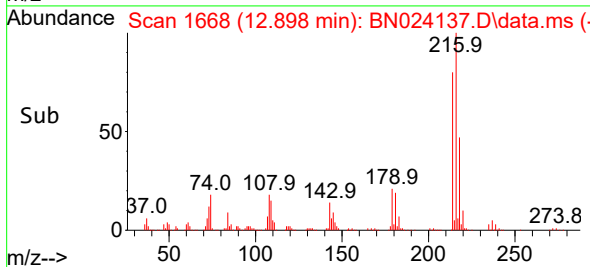

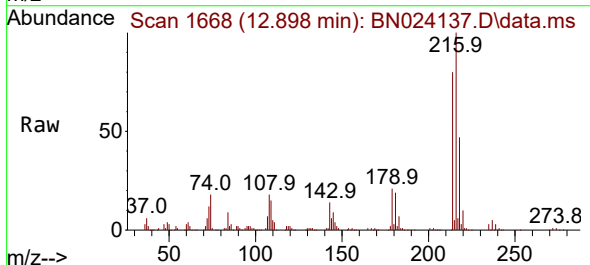




#40
Hexachlorocyclopentadiene
Concen: 20.198 ng/ul
RT: 12.881 min Scan# 1665
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:237 Resp: 273811
Ion Ratio Lower Upper
237 100
235 62.3 50.1 75.1
272 13.5 11.1 16.7

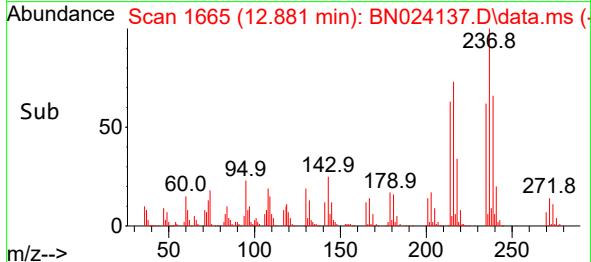

#41
2,4,6-Trichlorophenol
Concen: 20.891 ng/ul
RT: 13.128 min Scan# 1707
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:196 Resp: 344251
Ion Ratio Lower Upper
196 100
198 98.6 80.6 121.0
200 31.5 26.1 39.1


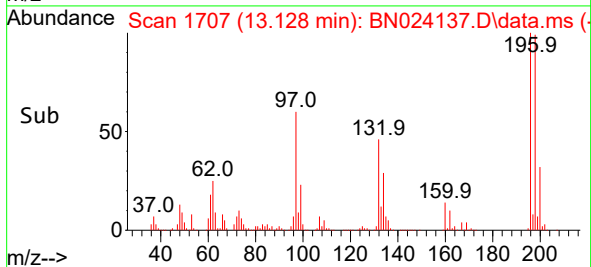

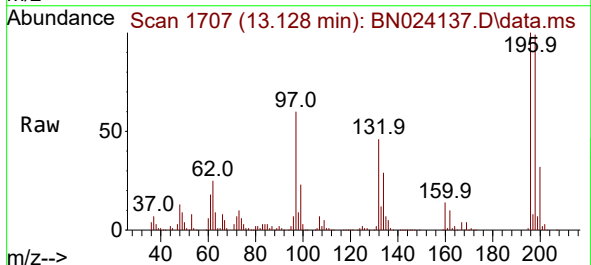




#42
2,4,5-Trichlorophenol
Concen: 21.806 ng/ul
RT: 13.198 min Scan# 1719
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:196 Resp: 386980
Ion Ratio Lower Upper
196 100
198 91.1 79.7 119.5
200 30.6 26.1 39.1

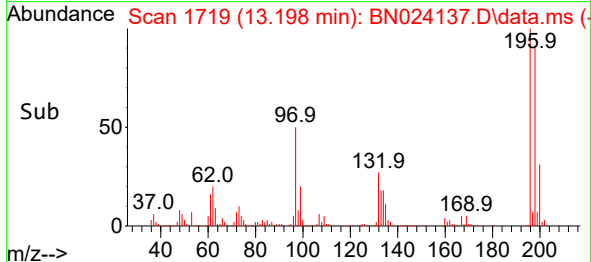

#43
1,1'-Biphenyl
Concen: 21.349 ng/ul
RT: 13.534 min Scan# 1776
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:154 Resp: 1421564
Ion Ratio Lower Upper
154 100
153 41.6 30.8 46.2
76 14.6 11.1 16.7





#44

2-Chloronaphthalene

Concen: 21.534 ng/ul

RT: 13.575 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34

Instrument :

BNA_N

ClientSampleId :

SSTD020259





Tgt Ion:162 Resp: 1117182

Ion Ratio Lower Upper

162 100

164 32.5 25.8 38.6

127 38.8 30.8 46.2

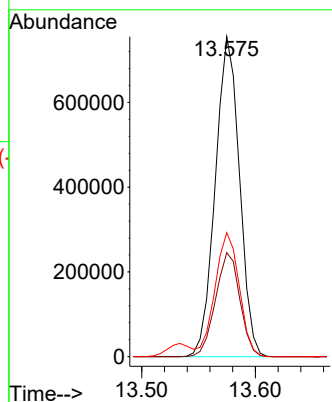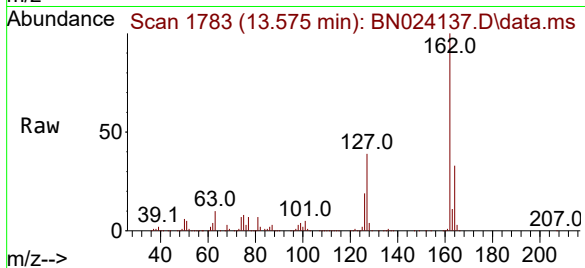

#45

2-Nitroaniline

Concen: 22.814 ng/ul

RT: 13.775 min Scan# 1817

Delta R.T. -0.000 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34




Tgt Ion: 65 Resp: 257862


Ion Ratio Lower Upper

65 100

92 67.1 53.8 80.8

138 100.0 84.1 126.1




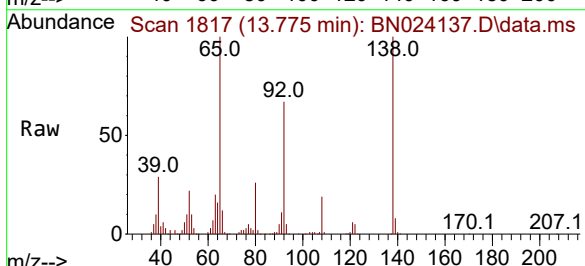




#47
Dimethylphthalate
Concen: 20.903 ng/ul
RT: 14.151 min Scan# 1881
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:163 Resp: 1359165
Ion Ratio Lower Upper
163 100
194 3.7 3.1 4.7
164 9.6 8.1 12.1

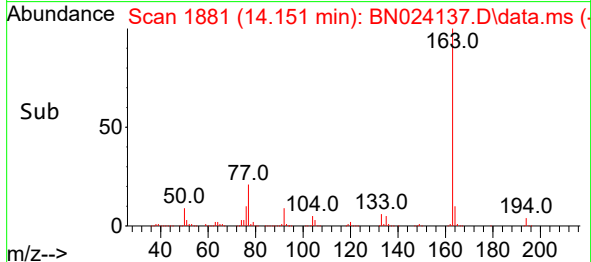

#48
2,6-Dinitrotoluene
Concen: 22.222 ng/ul
RT: 14.269 min Scan# 1901
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:165 Resp: 212690
Ion Ratio Lower Upper
165 100
89 60.9 52.6 78.8
121 23.5 19.4 29.2


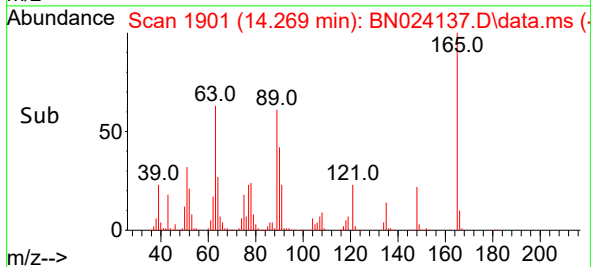

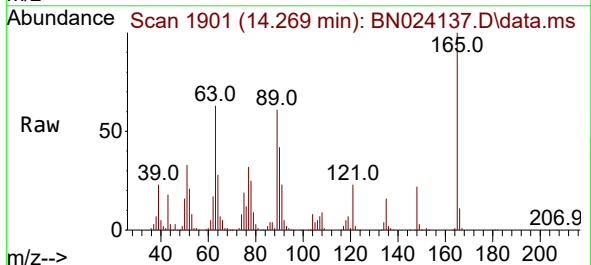




#50
Acenaphthylene
Concen: 21.398 ng/ul
RT: 14.416 min Scan# 1926
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:152 Resp: 1731558
Ion Ratio Lower Upper
152 100
151 19.6 15.6 23.4
153 13.2 10.1 15.1

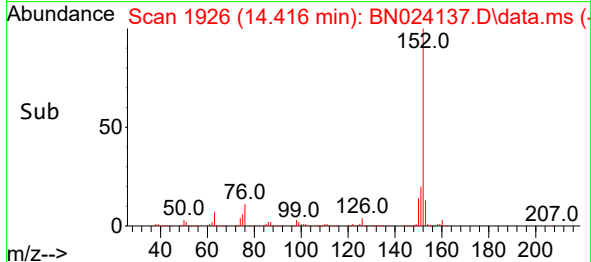

#51
3-Nitroaniline
Concen: 20.958 ng/ul
RT: 14.592 min Scan# 1956
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:138 Resp: 243826
Ion Ratio Lower Upper
138 100
108 11.9 9.6 14.4
92 120.3 95.3 142.9


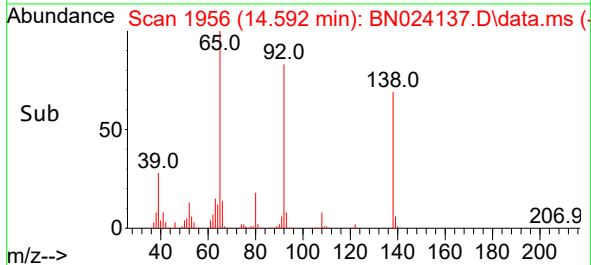

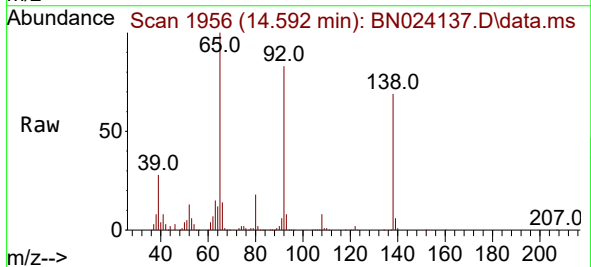




#52
Acenaphthene
Concen: 21.495 ng/ul
RT: 14.757 min Scan# 1984
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:153 Resp: 1186492
Ion Ratio Lower Upper
153 100
152 47.7 39.7 59.5
154 85.6 70.6 106.0

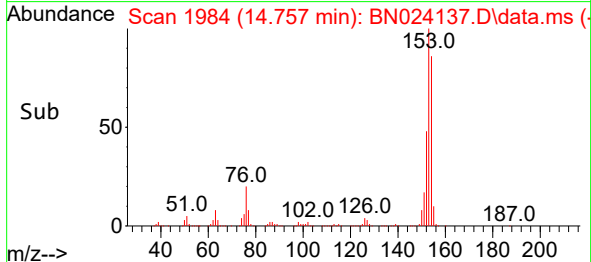

#53
2,4-Dinitrophenol
Concen: 16.913 ng/ul
RT: 14.792 min Scan# 1990
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:184 Resp: 112068
Ion Ratio Lower Upper
184 100
63 75.8 61.6 92.4
154 63.5 50.2 75.4

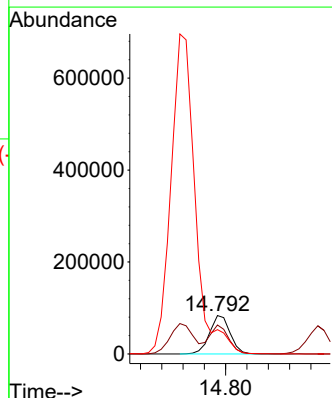



#55

4-Nitrophenol

Concen: 20.160 ng/ul

RT: 14.886 min Scan# 2006

Delta R.T. -0.000 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34

Instrument :

BNA_N

ClientSampleId :

SSTD020259





Tgt Ion:109 Resp: 189315

Ion Ratio Lower Upper

109 100

139 138.6 115.0 172.4

65 141.6 115.7 173.5

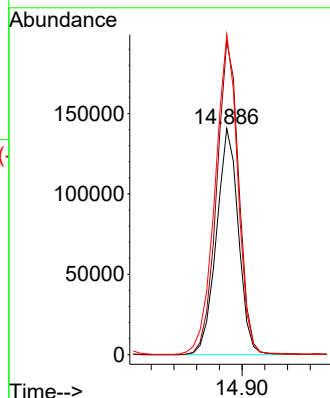

#56

Dibenzofuran

Concen: 20.653 ng/ul

RT: 15.092 min Scan# 2041

Delta R.T. -0.000 min

Lab File: BN024137.D




Acq: 07 Mar 2023 09:34


Tgt Ion:168 Resp: 1601579

Ion Ratio Lower Upper

168 100

139 37.4 30.7 46.1







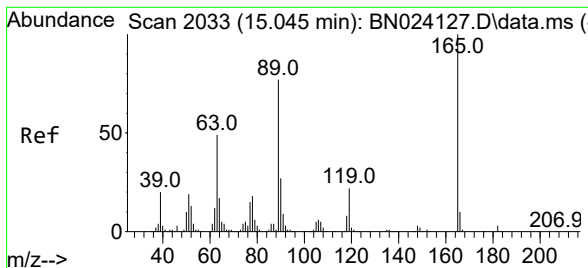

#57
2,4-Dinitrotoluene
Concen: 22.155 ng/ul
RT: 15.051 min Scan# 2033
Delta R.T. 0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:165 Resp: 334253
Ion Ratio Lower Upper
165 100
63 47.1 38.5 57.7
182 2.6 2.2 3.4

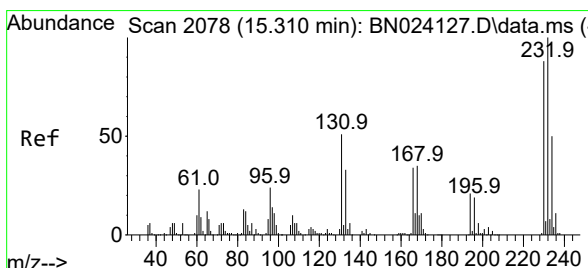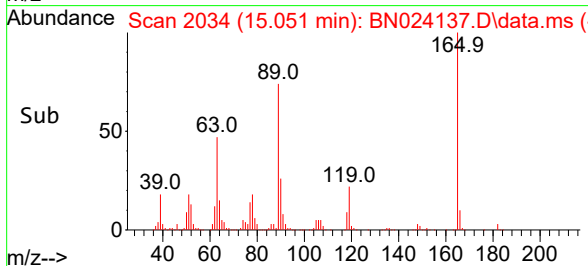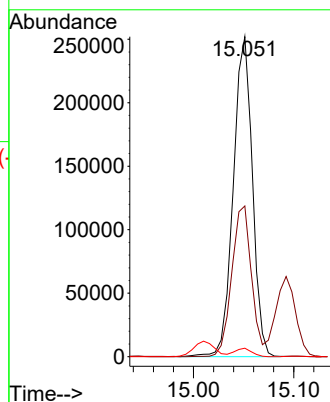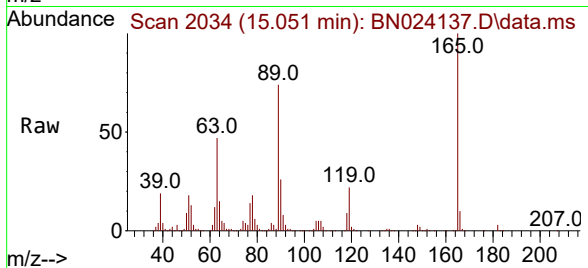

#58
2,3,4,6-Tetrachlorophenol
Concen: 20.653 ng/ul
RT: 15.310 min Scan# 2078
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:232 Resp: 315070
Ion Ratio Lower Upper
232 100
131 49.3 38.5 57.7
130 2.7 2.0 3.0
166 34.6 26.0 39.0


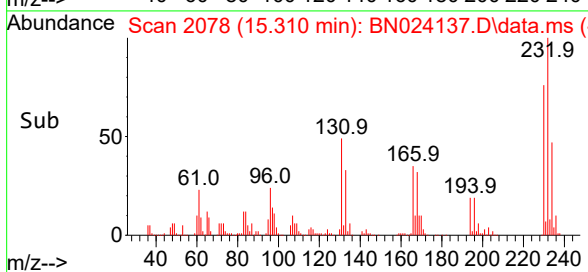

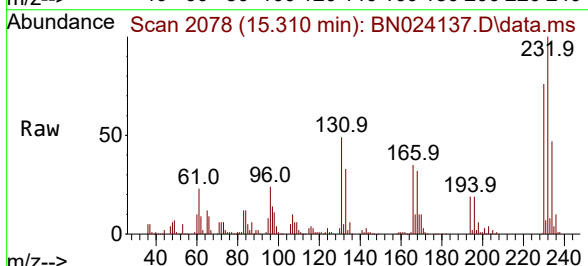




#59
Diethylphthalate
Concen: 20.651 ng/ul
RT: 15.510 min Scan# 2112
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:149 Resp: 1338489
Ion Ratio Lower Upper
149 100
177 21.6 16.9 25.3
150 12.2 9.7 14.5

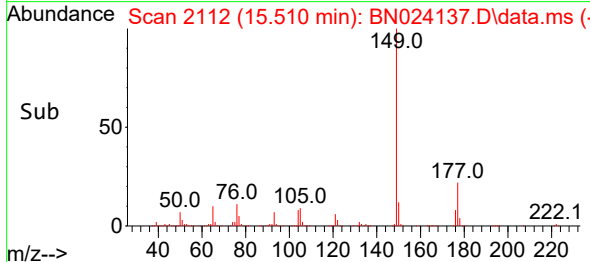

#61
Fluorene
Concen: 21.085 ng/ul
RT: 15.739 min Scan# 2151
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:166 Resp: 1280963
Ion Ratio Lower Upper
166 100
165 98.9 75.6 113.4
167 13.7 11.2 16.8


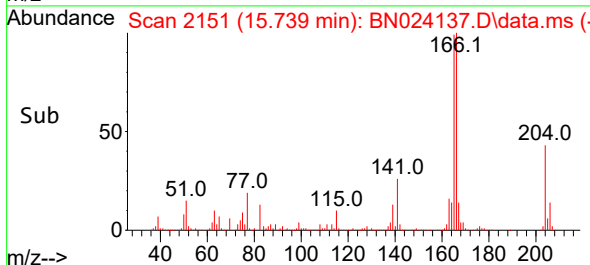
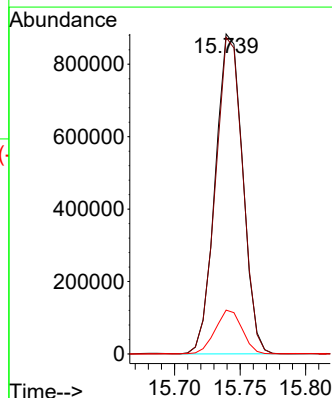
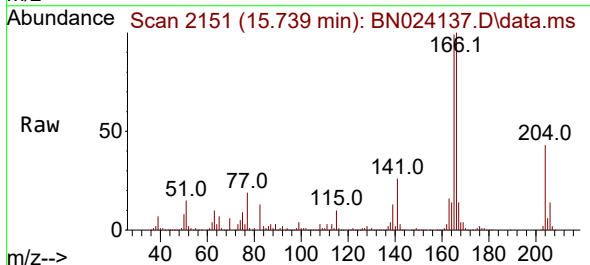




#62
4-Chlorophenyl-phenylether
Concen: 20.678 ng/ul
RT: 15.733 min Scan# 2150
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:204 Resp: 600650
Ion Ratio Lower Upper
204 100
206 32.4 27.1 40.7
141 61.1 47.4 71.0

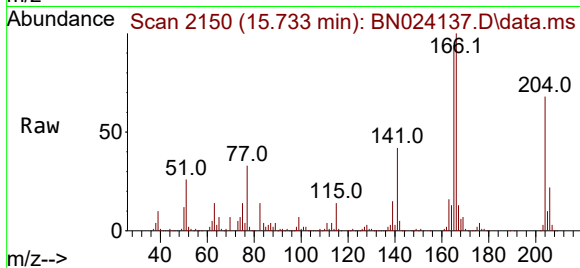

#63
4-Nitroaniline
Concen: 20.968 ng/ul
RT: 15.757 min Scan# 2154
Delta R.T. 0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:138 Resp: 235897
Ion Ratio Lower Upper
138 100
92 52.9 40.0 60.0
108 79.2 60.4 90.6


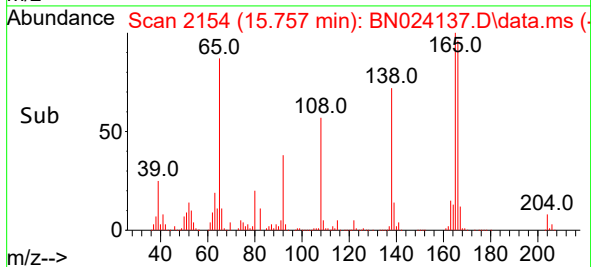

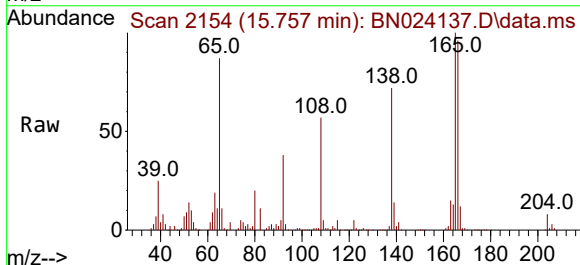




#66
 4,6-Dinitro-2-methylphenol
 Concen: 19.307 ng/ul
 RT: 15.810 min Scan# 2163
 Delta R.T. -0.000 min
 Lab File: BN024137.D
 Acq: 07 Mar 2023 09:34




Instrument :
 BNA_N
 ClientSampleId :
 SSTD020259


Tgt Ion:198 Resp: 182107
 Ion Ratio Lower Upper
 198 100
 182 4.4 3.4 5.0
 77 27.1 20.4 30.6

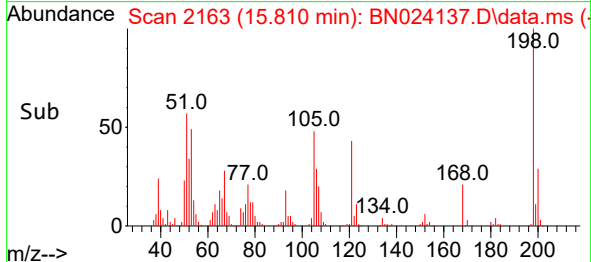

#67
 N-Nitrosodiphenylamine
 Concen: 21.459 ng/ul
 RT: 15.945 min Scan# 2186
 Delta R.T. -0.000 min
 Lab File: BN024137.D
 Acq: 07 Mar 2023 09:34

Tgt Ion:169 Resp: 1099765
 Ion Ratio Lower Upper
 169 100
 168 65.6 54.5 81.7
 167 37.1 28.3 42.5


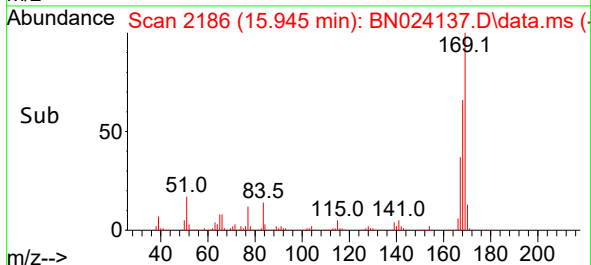
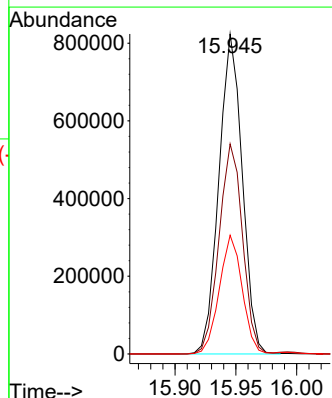
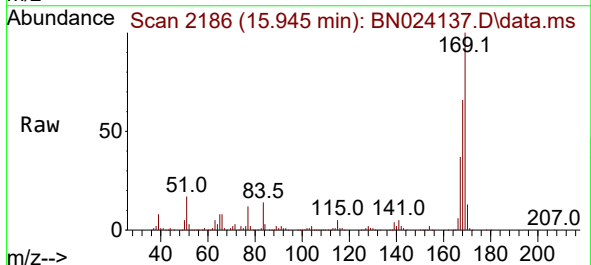




#68
4-Bromophenyl-phenylether
Concen: 20.120 ng/ul
RT: 16.628 min Scan# 2111
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:248 Resp: 346199
Ion Ratio Lower Upper
248 100
250 107.5 76.6 115.0
141 87.5 61.4 92.0

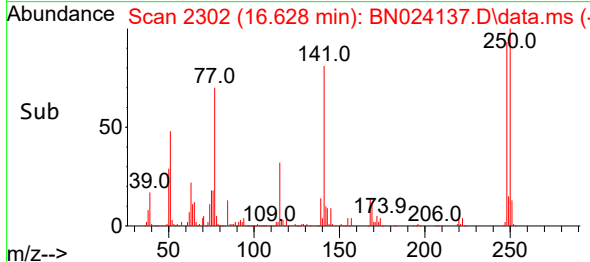

#69
Hexachlorobenzene
Concen: 19.654 ng/ul
RT: 16.745 min Scan# 2322
Delta R.T. 0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:284 Resp: 411403
Ion Ratio Lower Upper
284 100
142 39.6 29.0 43.6
249 30.3 25.0 37.6

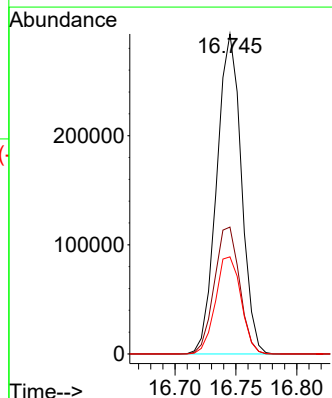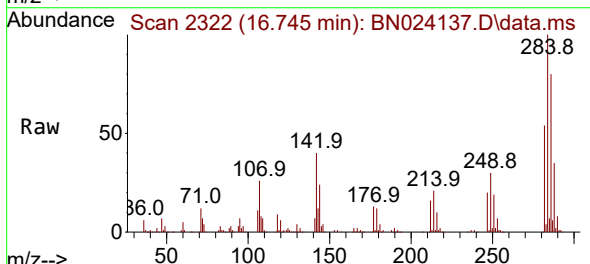



#70

Atrazine

Concen: 20.417 ng/ul

RT: 16.898 min Scan# 21

Delta R.T. 0.006 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34

Instrument :

BNA_N

ClientSampleId :

SSTD020259





Tgt Ion:200 Resp: 354196

Ion Ratio Lower Upper

200 100

173 27.4 20.7 31.1

215 49.5 38.8 58.2

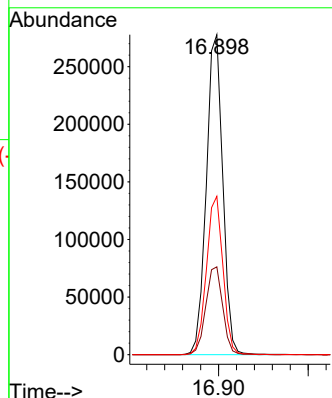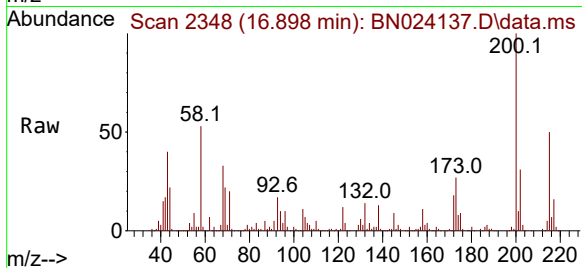

#71

Pentachlorophenol

Concen: 20.430 ng/ul

RT: 17.086 min Scan# 2380

Delta R.T. 0.006 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34




Tgt Ion:266 Resp: 264546


Ion Ratio Lower Upper

266 100

264 59.4 49.5 74.3

268 61.8 51.3 76.9




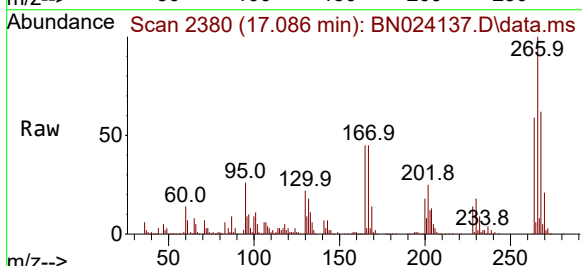




#72
Phenanthrene
Concen: 21.055 ng/ul
RT: 17.486 min Scan# 2448
Delta R.T. 0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:178 Resp: 2018672
Ion Ratio Lower Upper
178 100
179 15.9 11.6 17.4
176 19.5 14.9 22.3

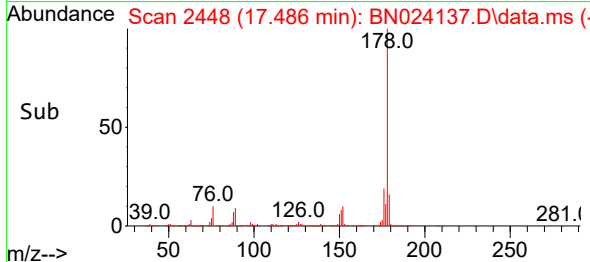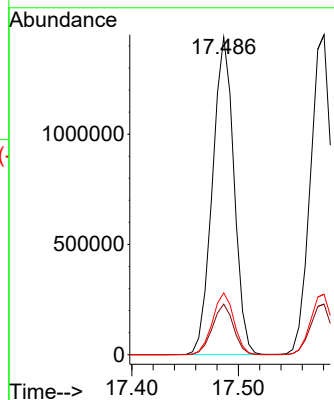

#74
Anthracene
Concen: 21.012 ng/ul
RT: 17.580 min Scan# 2464
Delta R.T. 0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:178 Resp: 2031130
Ion Ratio Lower Upper
178 100
179 15.8 11.9 17.9
176 18.9 14.6 21.8


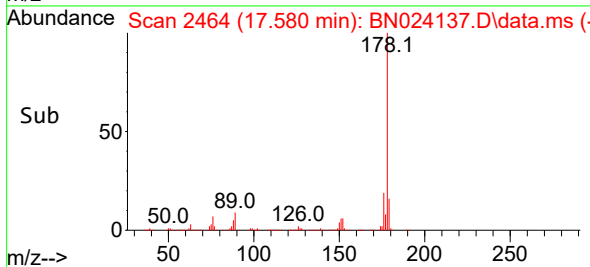
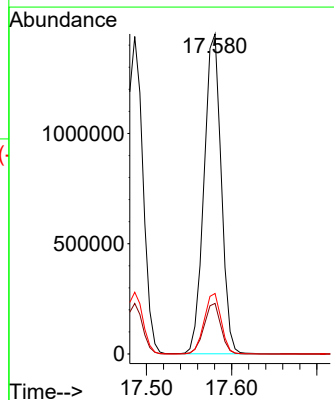
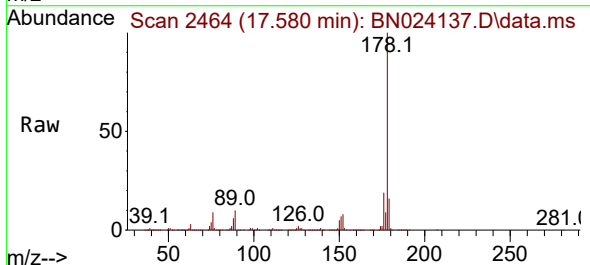




#75
1,2,3,4-Tetrachlorobenzene
Concen: 21.545 ng/uL
RT: 13.498 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:216 Resp: 543455
Ion Ratio Lower Upper
216 100
214 84.8 59.6 89.4
218 47.1 37.0 55.4



#76
Pentachlorobenzene
Concen: 21.348 ng/uL
RT: 15.010 min Scan# 2027
Delta R.T. -0.000 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:250 Resp: 524698
Ion Ratio Lower Upper
250 100
248 59.5 53.0 79.4
252 58.7 54.6 81.8









#77
 Carbazole
 Concen: 21.619 ng/ul
 RT: 17.845 min Scan# 2509
 Delta R.T. 0.006 min
 Lab File: BN024137.D
 Acq: 07 Mar 2023 09:34




Instrument :
 BNA_N
 ClientSampleId :
 SSTD020259


Tgt Ion:167 Resp: 1871573
 Ion Ratio Lower Upper
 167 100
 166 21.8 17.3 25.9
 139 13.0 10.5 15.7

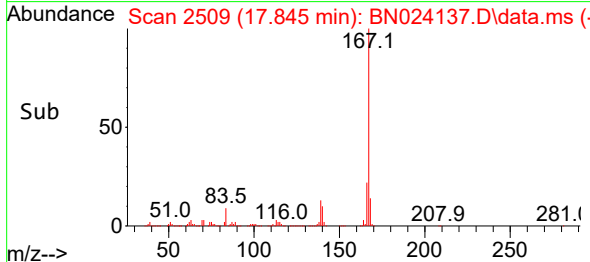

#78
 Di-n-butylphthalate
 Concen: 21.652 ng/ul
 RT: 18.410 min Scan# 2605
 Delta R.T. -0.000 min
 Lab File: BN024137.D
 Acq: 07 Mar 2023 09:34

Tgt Ion:149 Resp: 2231121
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.4 11.0
 104 5.1 4.0 6.0

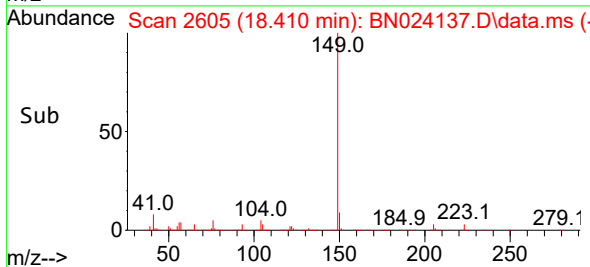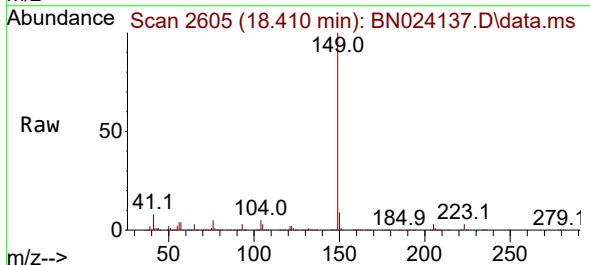



#80

Fluoranthene

Concen: 22.079 ng/ul

RT: 19.498 min Scan# 21

Delta R.T. 0.006 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34

Instrument :

BNA_N

ClientSampleId :

SSTD020259





Tgt Ion:202 Resp: 2278494

Ion Ratio Lower Upper

202 100

101 13.2 10.0 15.0

100 9.7 7.6 11.4



#82

Pyrene

Concen: 21.788 ng/ul

RT: 19.857 min Scan# 2851

Delta R.T. -0.000 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34




Tgt Ion:202 Resp: 2372243


Ion Ratio Lower Upper

202 100

101 14.7 11.9 17.9

100 12.2 9.9 14.9





#83

Butylbenzylphthalate

Concen: 21.840 ng/ul

RT: 20.763 min Scan# 3005

Delta R.T. 0.012 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34

Instrument :

BNA_N

ClientSampleId :

SSTD020259





Tgt Ion:149 Resp: 605556

Ion Ratio Lower Upper

149 100

91 77.0 62.2 93.2

206 21.0 16.4 24.6



#84

3,3'-Dichlorobenzidine

Concen: 21.748 ng/ul

RT: 21.551 min Scan# 3139

Delta R.T. 0.012 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34




Tgt Ion:252 Resp: 636663


Ion Ratio Lower Upper

252 100

254 62.6 54.6 81.8

126 11.9 11.0 16.6





#85

Benzo(a)anthracene

Concen: 21.399 ng/ul

RT: 21.621 min Scan# 3151

Delta R.T. 0.012 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34

Instrument :

BNA_N

ClientSampleId :

SSTD020259





Tgt Ion:228 Resp: 2265552

Ion Ratio Lower Upper

228 100

229 20.5 16.3 24.5

226 27.1 22.6 34.0

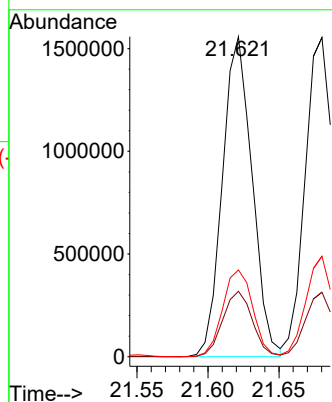

#86

Bis(2-ethylhexyl)phthalate

Concen: 22.975 ng/ul

RT: 21.545 min Scan# 3138

Delta R.T. 0.012 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34




Tgt Ion:149 Resp: 1057189


Ion Ratio Lower Upper

149 100

167 27.2 21.6 32.4

279 3.6 3.4 5.2





#87

Chrysene

Concen: 21.596 ng/ul

RT: 21.680 min Scan# 31

Delta R.T. 0.012 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34

Instrument :

BNA_N

ClientSampleId :

SSTD020259





Tgt Ion:228 Resp: 2188482

Ion Ratio Lower Upper

228 100

226 31.5 25.8 38.6

229 20.2 17.5 26.3



#89

Di-n-octyl phthalate

Concen: 19.349 ng/ul




RT: 22.515 min Scan# 3303


Delta R.T. 0.012 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34

Tgt Ion:149 Resp: 1754654









#90
Benzo(b)fluoranthene
Concen: 21.815 ng/ul
RT: 23.386 min Scan# 3450
Delta R.T. 0.006 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34




Instrument :
BNA_N
ClientSampleId :
SSTD020259


Tgt Ion:252 Resp: 2328884
Ion Ratio Lower Upper
252 100
253 20.7 18.3 27.5
125 9.9 9.5 14.3

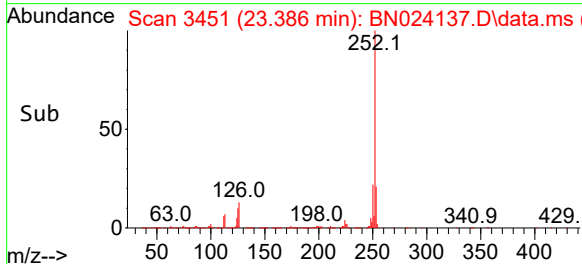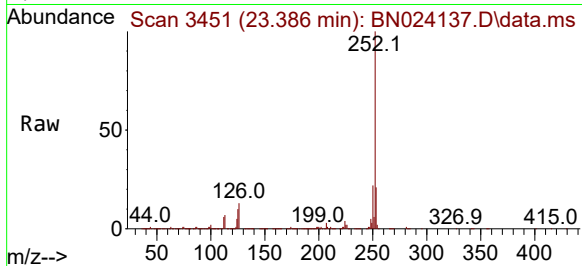

#91
Benzo(k)fluoranthene
Concen: 21.715 ng/ul
RT: 23.439 min Scan# 3460
Delta R.T. 0.012 min
Lab File: BN024137.D
Acq: 07 Mar 2023 09:34

Tgt Ion:252 Resp: 2292813
Ion Ratio Lower Upper
252 100
253 21.5 17.4 26.0
125 10.9 9.0 13.6

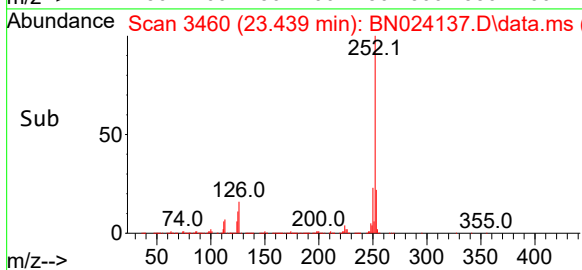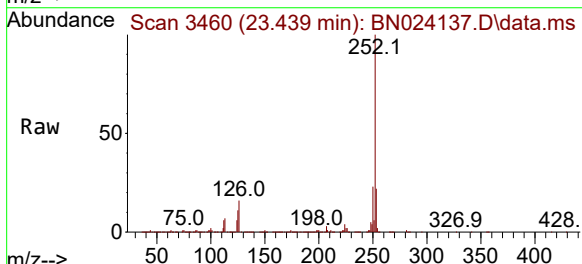



#93

Benzo(a)pyrene

Concen: 21.436 ng/ul

RT: 24.045 min Scan# 3563

Delta R.T. -0.000 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34

Instrument :

BNA_N

ClientSampleId :

SSTD020259





Tgt Ion:252 Resp: 2026574

Ion Ratio Lower Upper

252 100

253 21.4 17.0 25.4

125 12.8 9.5 14.3

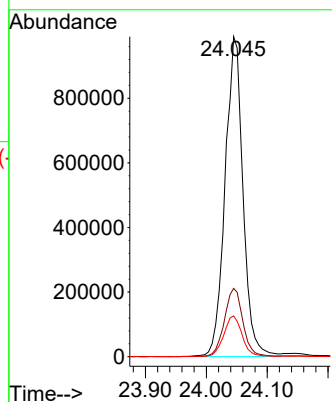

#94

Indeno(1,2,3-cd)pyrene

Concen: 20.162 ng/ul

RT: 26.792 min Scan# 4030

Delta R.T. -0.018 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34




Tgt Ion:276 Resp: 2400516


Ion Ratio Lower Upper

276 100

138 27.9 19.6 29.4

277 23.9 19.7 29.5





#95

Dibenzo(a,h)anthracene

Concen: 21.027 ng/ul

RT: 26.809 min Scan# 4036

Delta R.T. -0.018 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34

Instrument :

BNA_N

ClientSampleId :

SSTD020259





Tgt Ion:278 Resp: 2038515

Ion Ratio Lower Upper

278 100

139 18.3 14.4 21.6

279 22.7 18.2 27.2

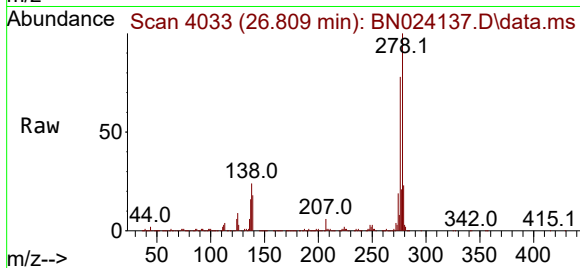

#96

Benzo(g,h,i)perylene

Concen: 20.051 ng/ul

RT: 27.598 min Scan# 4167

Delta R.T. -0.024 min

Lab File: BN024137.D

Acq: 07 Mar 2023 09:34

Tgt Ion:276 Resp: 1969675

Ion Ratio Lower Upper

276 100

138 23.4 18.8 28.2

277 23.0 18.6 27.8

