
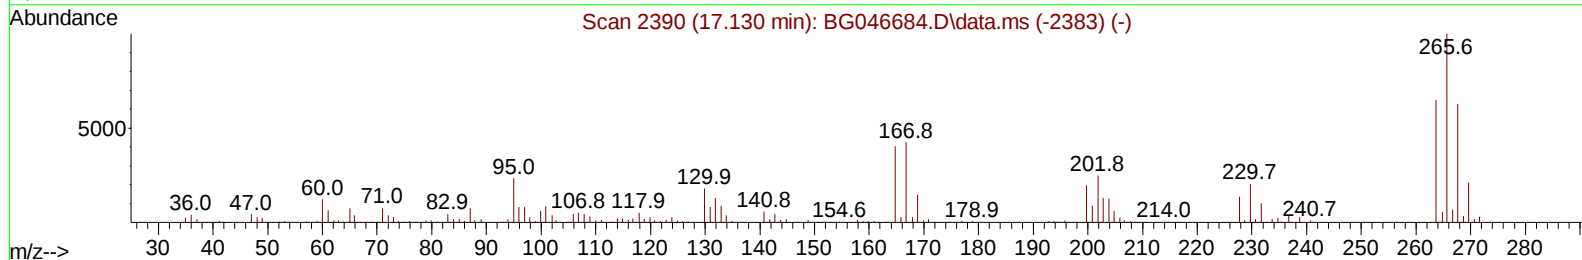
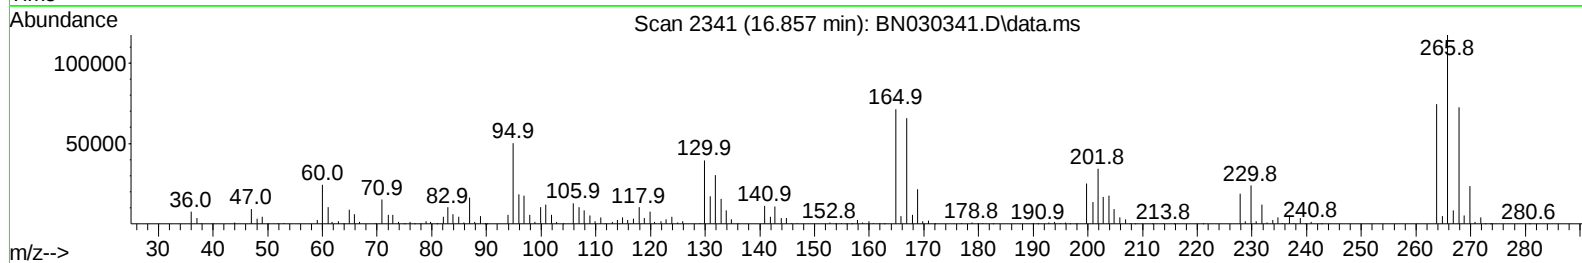


Quant Time: Mar 08 04:34:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 08 04:34:38 2024
Response via : Initial Calibration

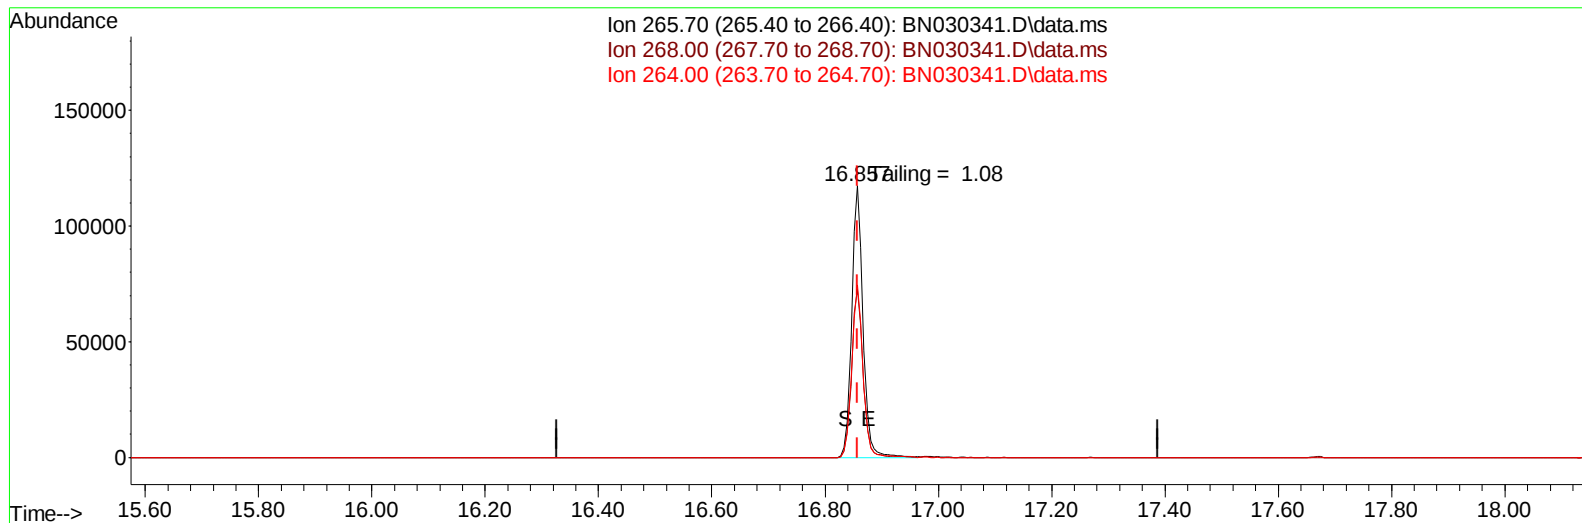

TIC: BN030341.D\data.ms

(70) Pentachlorophenol (C)




16.857min (0.000) 21020.12 ng

response **163311**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.84
264.00	61.60	63.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030724\
Data File : BN030341.D
Acq On : 08 Mar 2024 01:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 60 Sample Multiplier: 1

Quant Time: Mar 08 04:34:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 08 04:34:38 2024
Response via : Initial Calibration

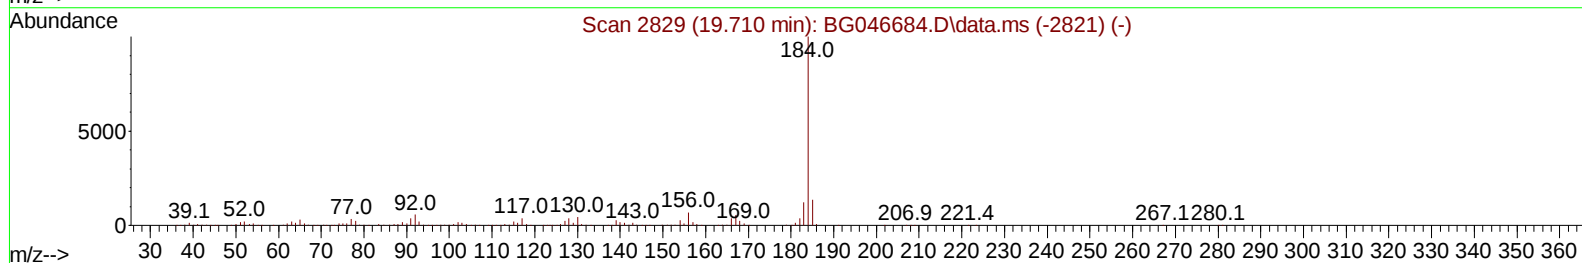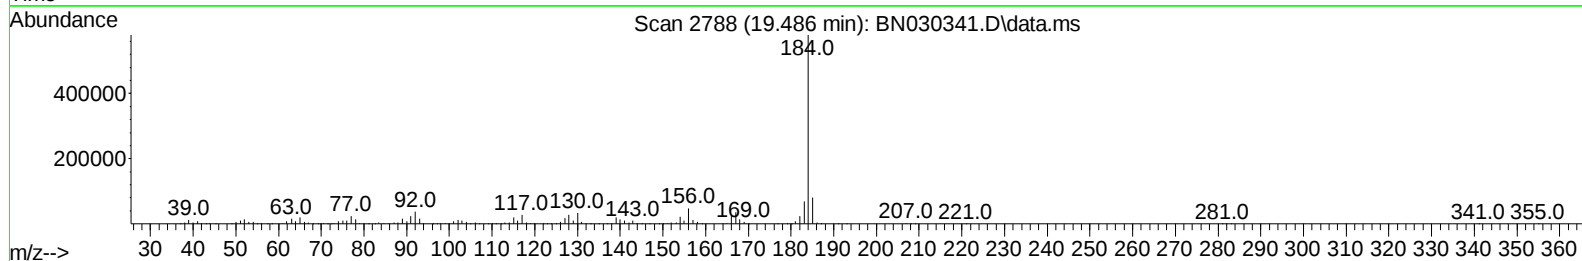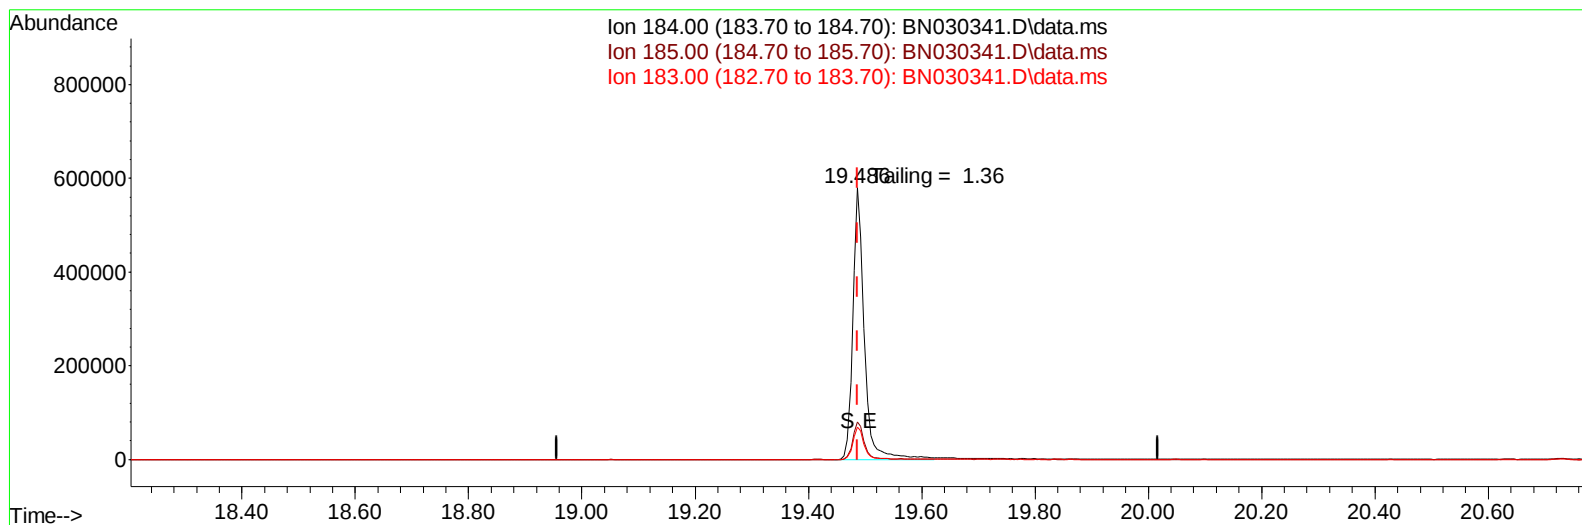

TIC: BN030341.D\data.ms

(77) Benzidine

19.486min (0.000) 0.00 ng

response 830486

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.84
183.00	13.20	11.86
0.00	0.00	0.00