


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030724\
Data File : BN030322.D
Acq On : 07 Mar 2024 12:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN030524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 05 17:44:16 2024

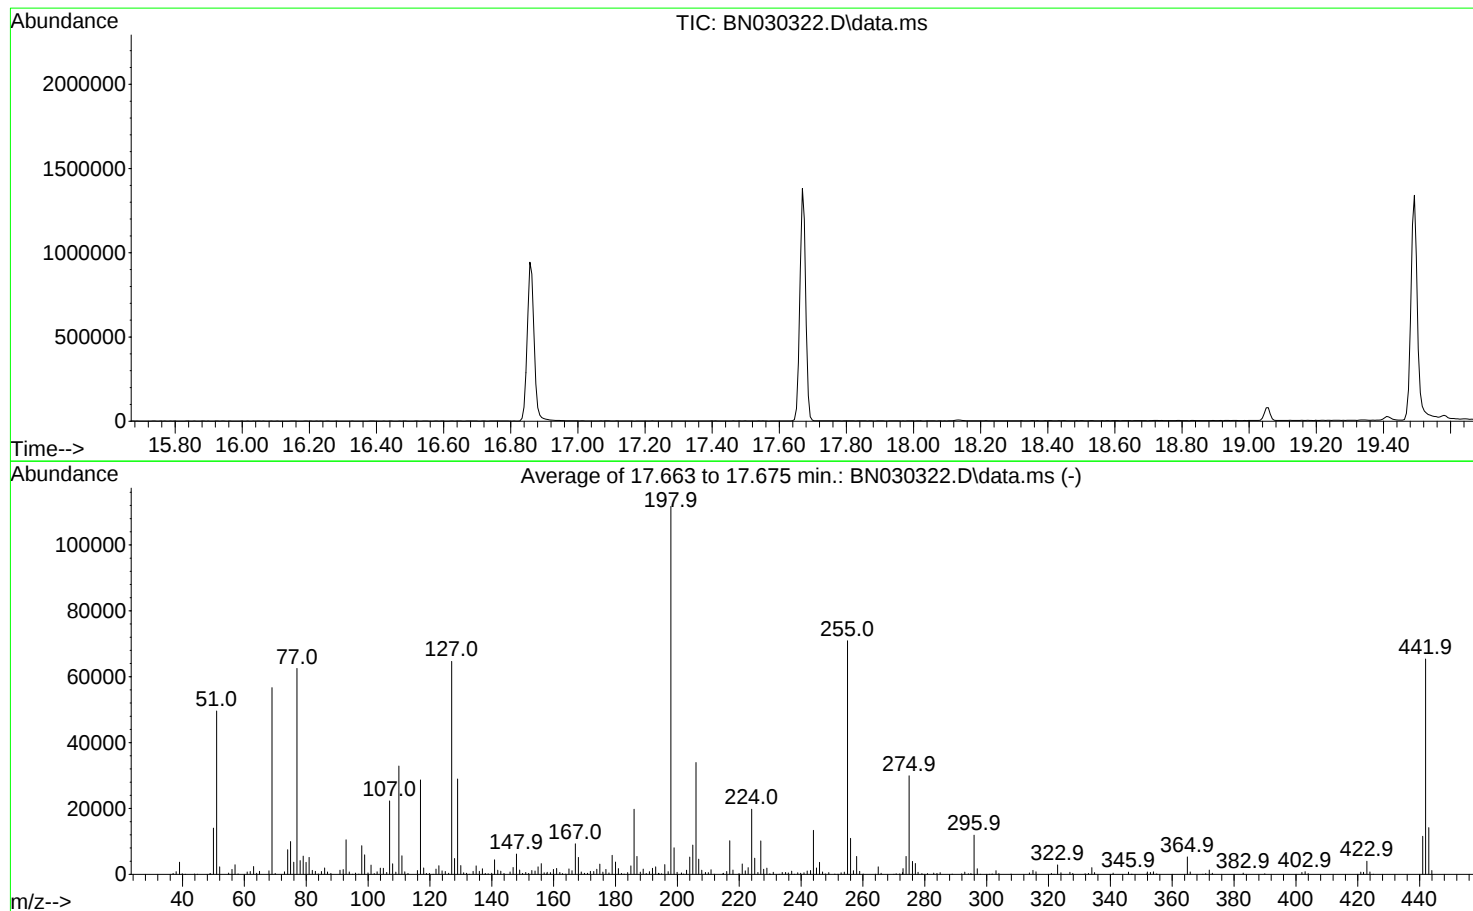




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	49605	PASS
68	69	0.00	2	1.9	1058	PASS
69	198	0.00	100	50.8	56680	PASS
70	69	0.00	2	0.5	292	PASS
127	198	10	80	57.9	64661	PASS
197	198	0.00	2	0.8	844	PASS
198	198	100	100	100.0	111675	PASS
199	198	5	9	7.2	8089	PASS
275	198	10	60	26.8	29917	PASS
365	198	1	100	4.7	5279	PASS
441	198	0.01	100	10.4	11566	PASS
442	442	50	100	100.0	65400	PASS
443	442	15	24	21.7	14172	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030724\
Data File : BN030322.D
Acq On : 07 Mar 2024 12:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 08 00:05:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 08 00:05:51 2024
Response via : Initial Calibration

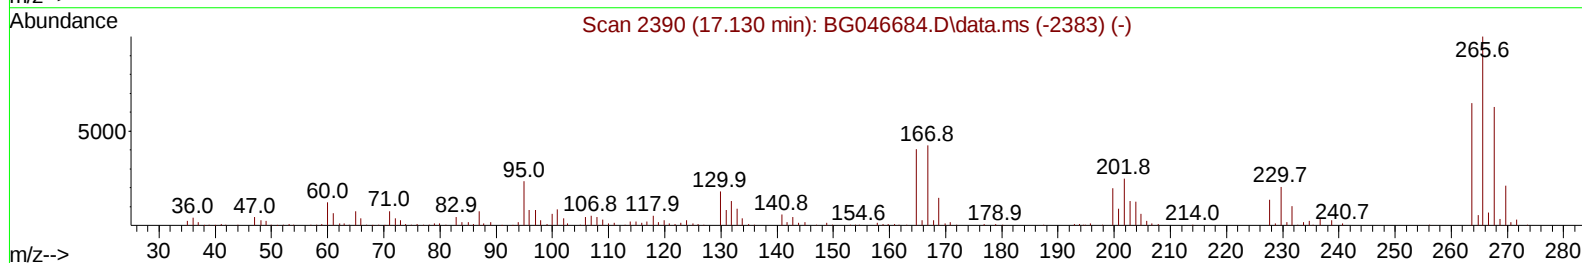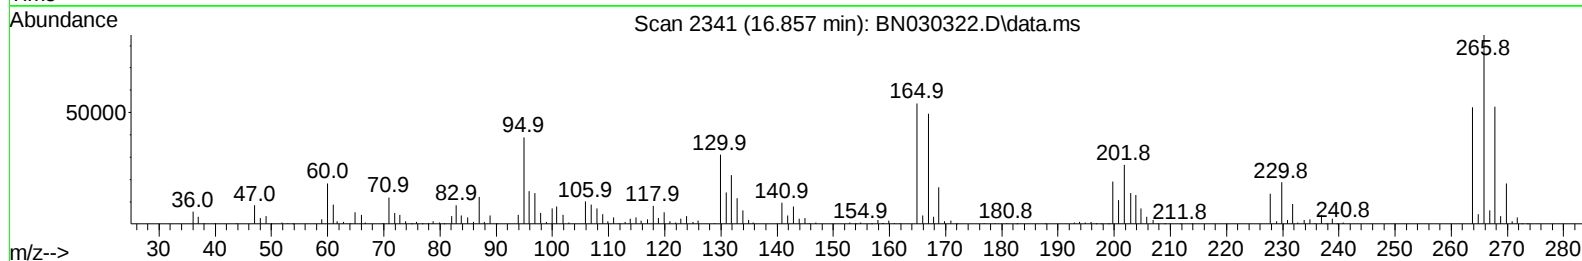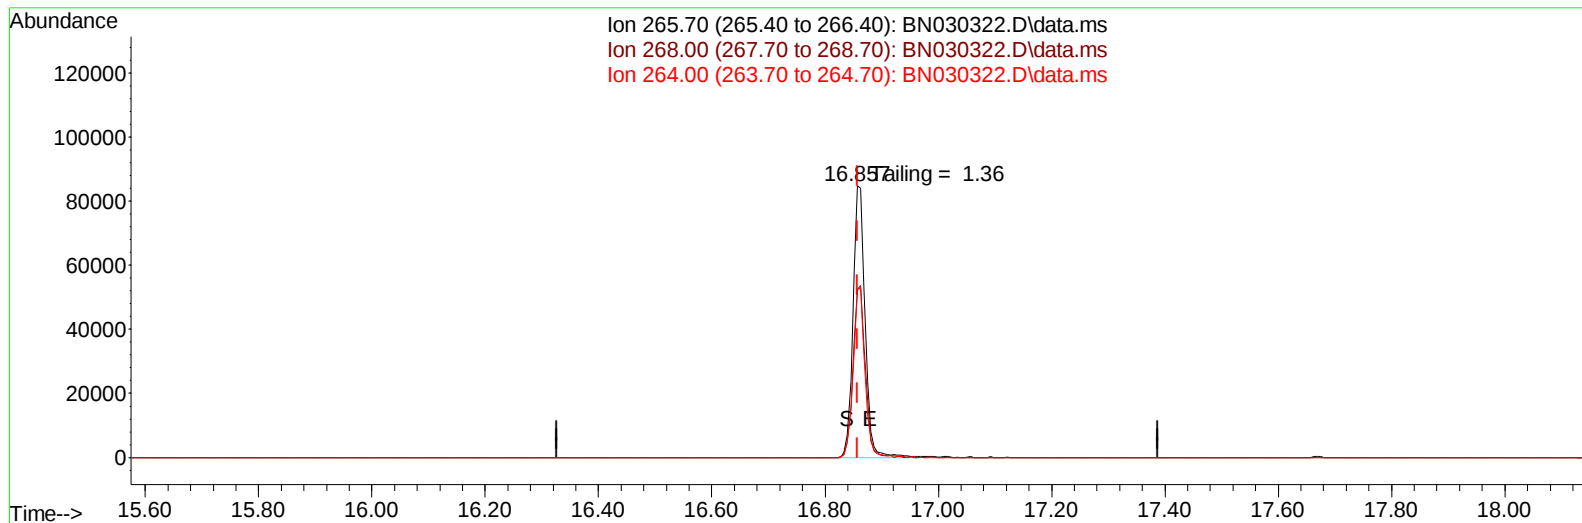

TIC: BN030322.D\data.ms

(70) Pentachlorophenol (C)

16.857min (0.000) 17740.98 ng




response 127114

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.95
264.00	61.60	61.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030724\
Data File : BN030322.D
Acq On : 07 Mar 2024 12:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 08 00:05:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 08 00:05:51 2024
Response via : Initial Calibration

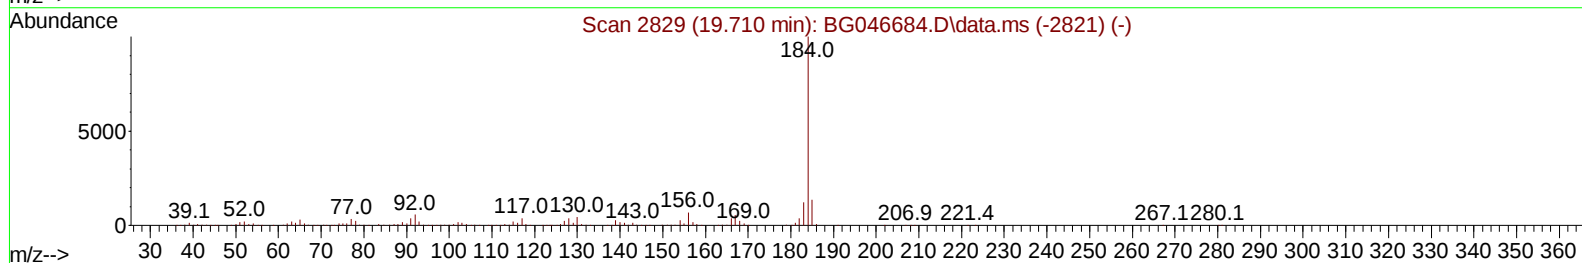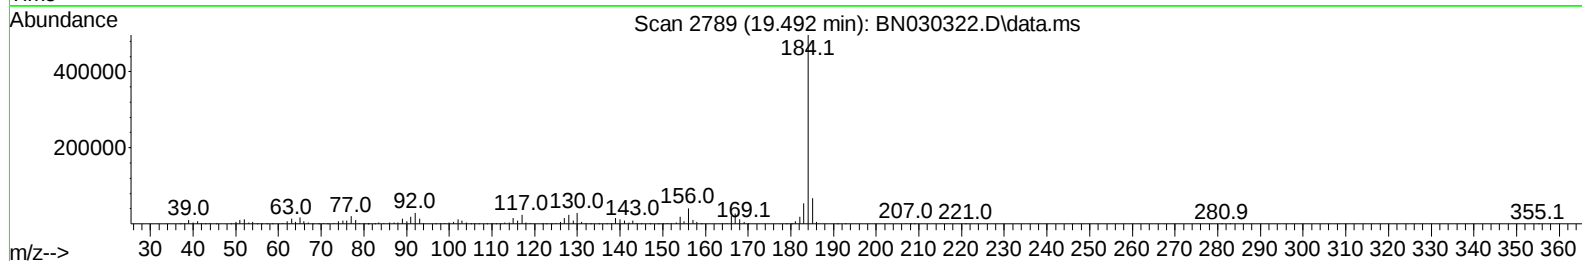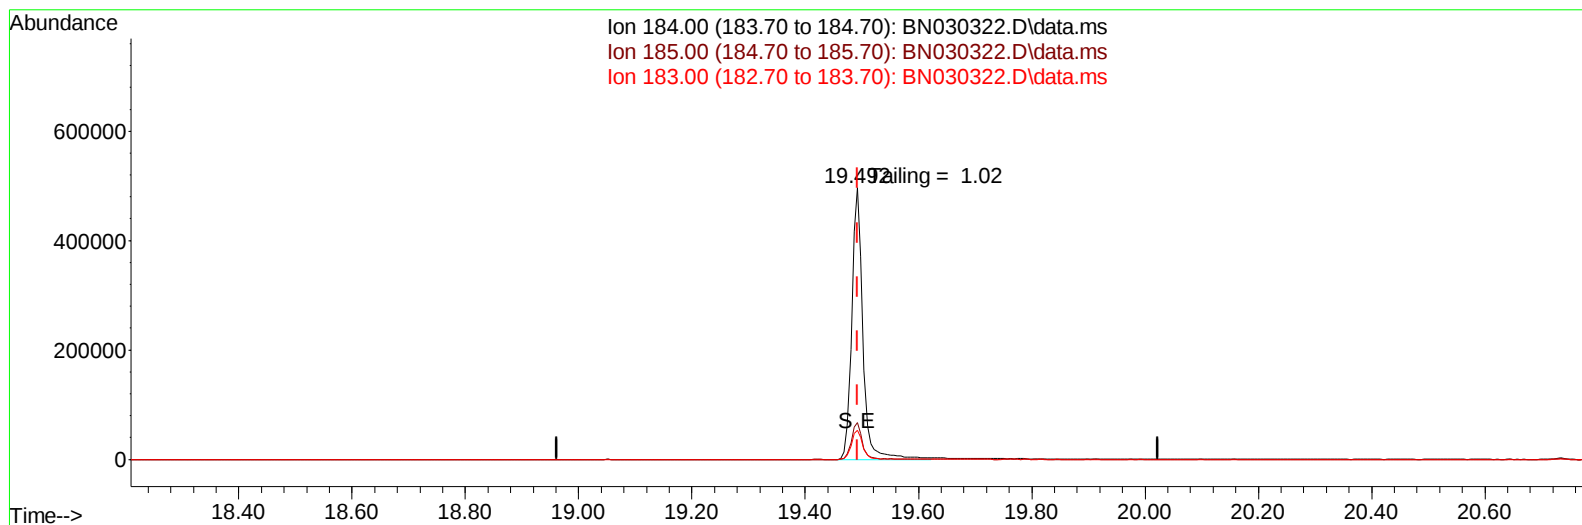

TIC: BN030322.D\data.ms

(77) Benzidine

19.492min (0.000) 0.00 ng

response 685078

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.58
183.00	13.20	10.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/7/2024	BNA_N	<u>BN030322.D</u>
Compound Name	Response	Retention Time
DDT	379758	20.733
DDD	8531	20.292
DDE	294	19.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8825	388583	2.27

Instrument :
BNA_N
ClientSampleId :
DFTPP