

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA N\DATA\BN030918\
 Data File : BN000291.D
 Acq On : 09 Mar 2018 20:36
 Operator : JU/SJ
 Sample : J1844-10MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAM79MS

Manual Integrations
 APPROVED

Sohil
 3/12/2018 3:52:52 PM

Quant Time: Mar 12 01:05:33 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN030918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 09 23:47:40 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.45	152	235674	20.00	ng/ul	0.00
2) Naphthalene-d8	11.29	136	1190667	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.06	164	685416	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.78	188	1463487	20.00	ng/ul	0.00
17) Chrysene-d12	21.89	240	1527577	20.00	ng/ul	0.00
22) Perylene-d12	24.37	264	1636308	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	14.76	160	1574942	23.15	ng/ul	0.00
10) Fluorene-d10	16.03	176	1065603	23.13	ng/ul	0.00
14) Anthracene-d10	17.87	188	1577620	23.07	ng/ul	0.00
18) Pyrene-d10	20.13	212	1759768	23.55	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.21	264	1790442	23.96	ng/ul	0.00
Target Compounds						
9) Acenaphthene	15.12	153	1021921	21.478	ng/ul	95
13) Phenanthrene	17.82	178	542562	6.464	ng/ul	99
15) Anthracene	17.91	178	108589	1.275	ng/ul	98
16) Fluoranthene	19.80	202	1125887	12.416	ng/ul#	94
19) Pyrene	20.16	202	2989593m	30.998	ng/ul	
20) Benzo(a)anthracene	21.87	228	454652m	4.788	ng/ul	
21) Chrysene	21.93	228	450497	4.999	ng/ul	97
23) Benzo(b)fluoranthene	23.62	252	546540m	5.601	ng/ul	
24) Benzo(k)fluoranthene	23.66	252	185542m	2.031	ng/ul	
26) Benzo(a)pyrene	24.26	252	341527	3.678	ng/ul#	94
27) Indeno(1,2,3-cd)pyrene	26.92	276	214046	2.138	ng/ul#	83
29) Benzo(g,h,i)perylene	27.70	276	207502	2.482	ng/ul#	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA N\DATA\BN030918\
Data File : BN000291.D
Acq On : 09 Mar 2018 20:36
Operator : JU/SJ
Sample : J1844-10MS
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DAM79MS

Manual Integrations
APPROVED

Sohil
3/12/2018 3:52:52 PM

Quant Time: Mar 12 01:05:33 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN030918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 09 23:47:40 2018
Response via : Initial Calibration

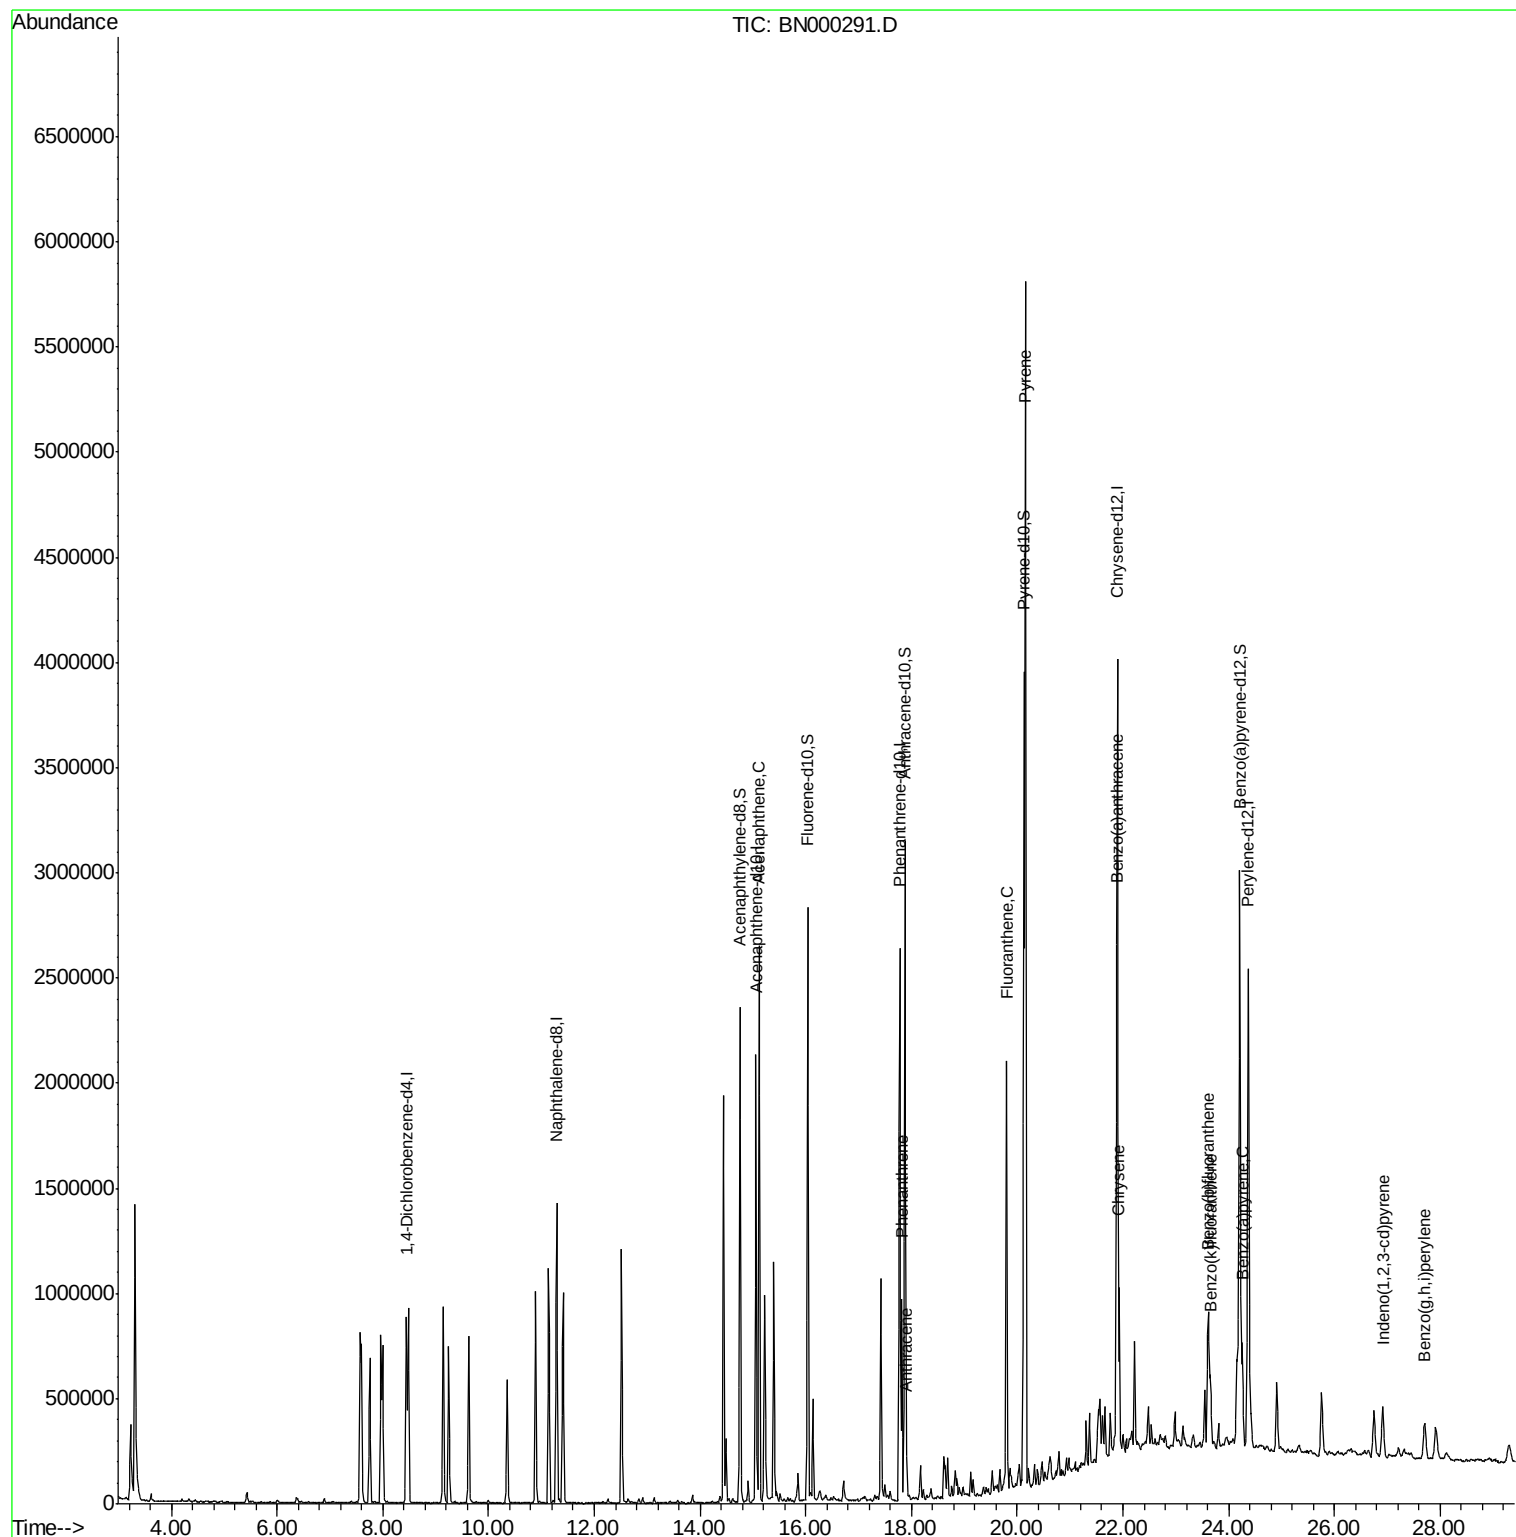

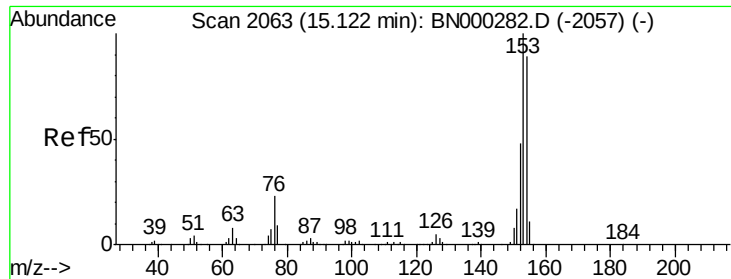

#9

Acenaphthene

Concen: 21.478 ng/ul

RT: 15.12 min Scan# 2063

Delta R.T. -0.00 min

Lab File: BN000291.D

Acq: 09 Mar 2018 20:36

Instrument :

BNA_N

ClientSampleId :

DAM79MS

Tot Ion:153 Resp: 1021921

Ion Ratio Lower Upper

153 100


152 47.1 39.0 58.6

154 88.7 66.8 100.2

Manual Integrations
APPROVED

Sohil




3/12/2018 3:52:52 PM

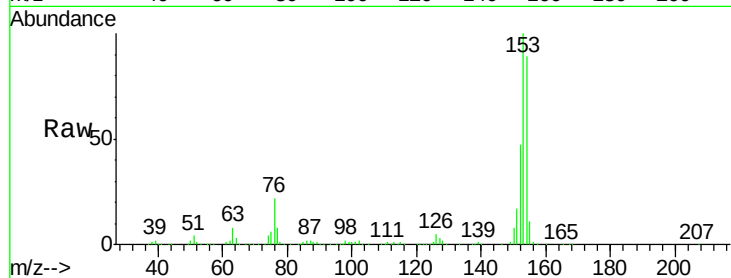

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

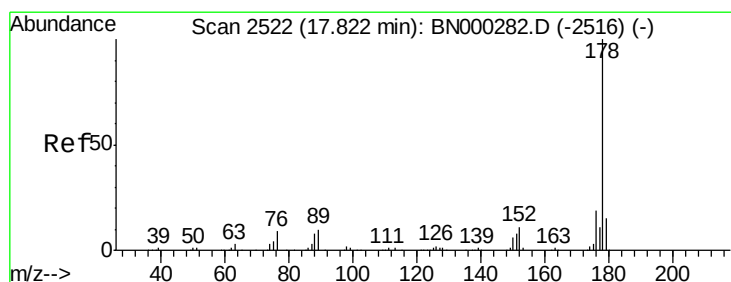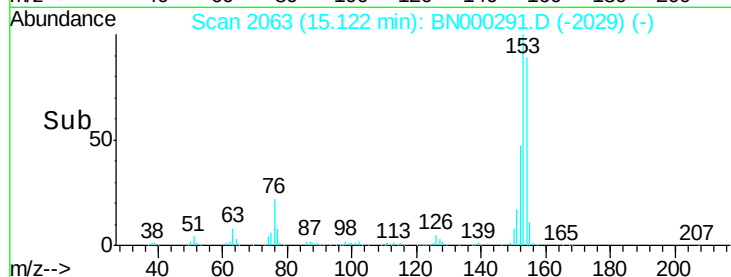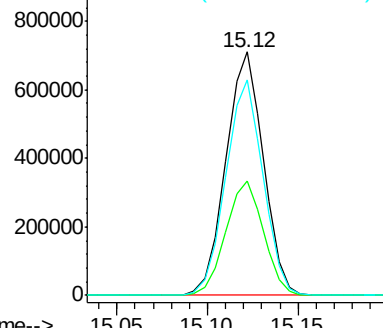

#13

Phenanthrene

Concen: 6.464 ng/ul

RT: 17.82 min Scan# 2522

Delta R.T. -0.00 min

Lab File: BN000291.D

Acq: 09 Mar 2018 20:36


Tgt Ion:178 Resp: 542562

Ion Ratio Lower Upper

178 100

179 15.3 12.3 18.5



176 19.3 15.1 22.7

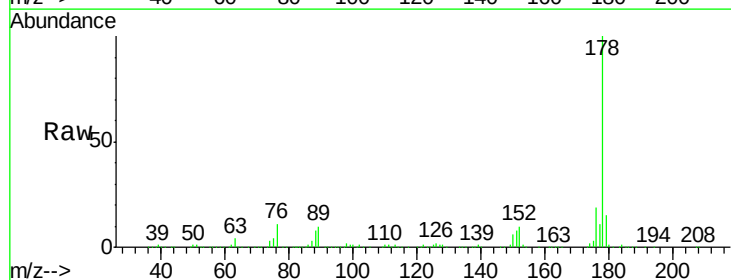


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

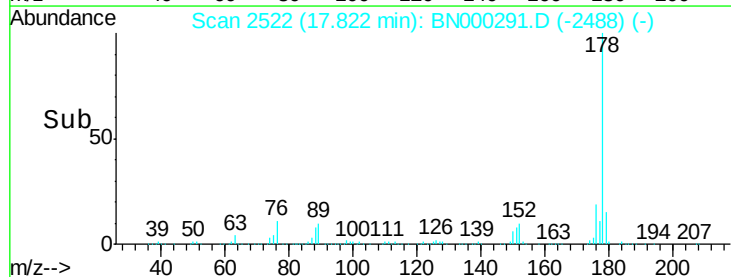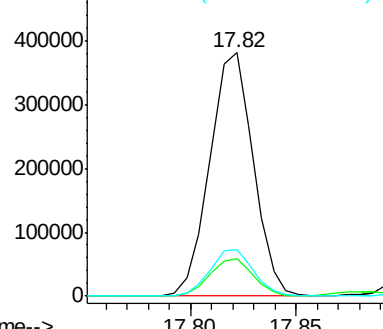

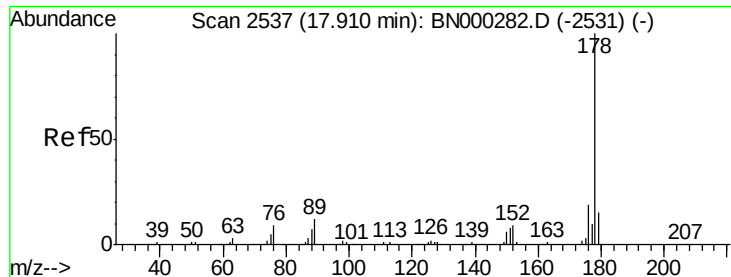





#15
 Anthracene
 Concen: 1.275 ng/ul
 RT: 17.91 min Scan# 2537
 Delta R.T. -0.00 min
 Lab File: BN000291.D
 Acq: 09 Mar 2018 20:36

Instrument :
 BNA_N
 ClientSampleId :
 DAM79MS

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.4	11.8	17.8
176	17.8	15.2	22.8




Manual Integrations
 APPROVED


Sohil
 3/12/2018 3:52:52 PM

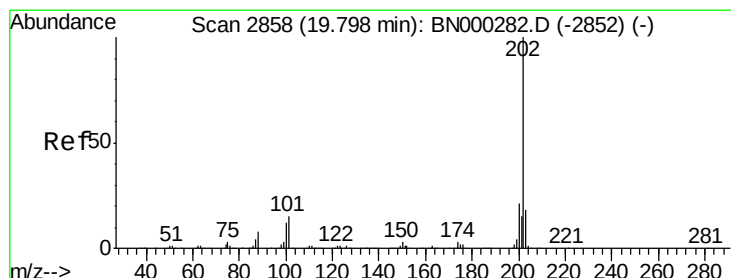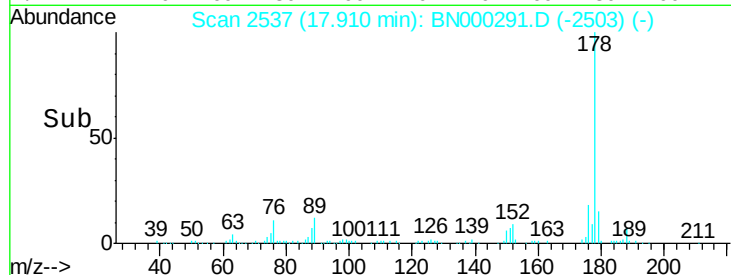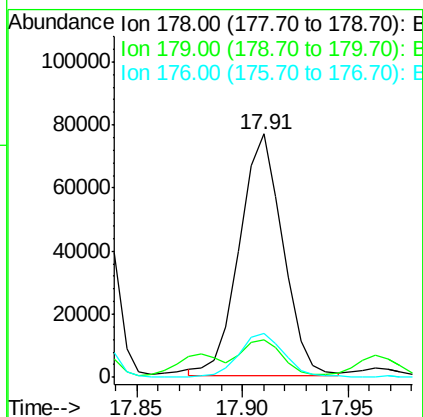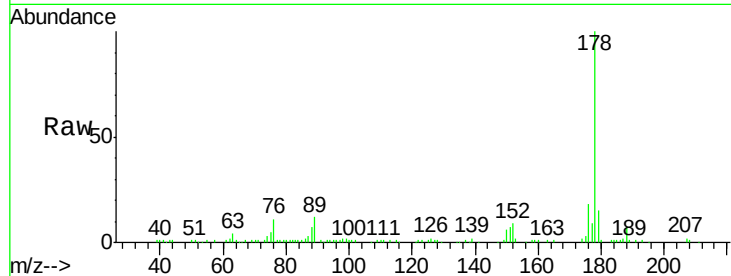

#16
 Fluoranthene
 Concen: 12.416 ng/ul
 RT: 19.80 min Scan# 2858
 Delta R.T. -0.00 min
 Lab File: BN000291.D
 Acq: 09 Mar 2018 20:36

Tgt Ion	Ratio	Lower	Upper
202	100		
101	14.7	9.9	14.9
100	11.1	7.4	11.0#

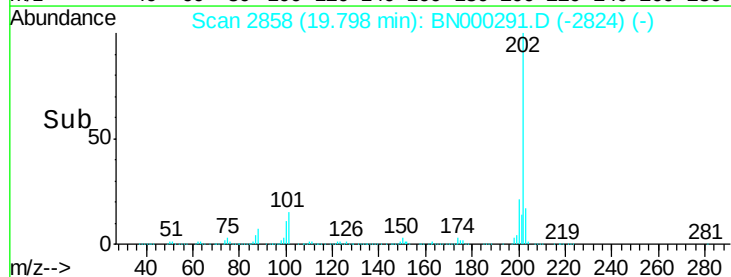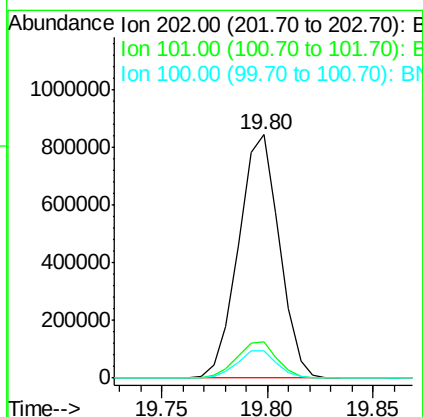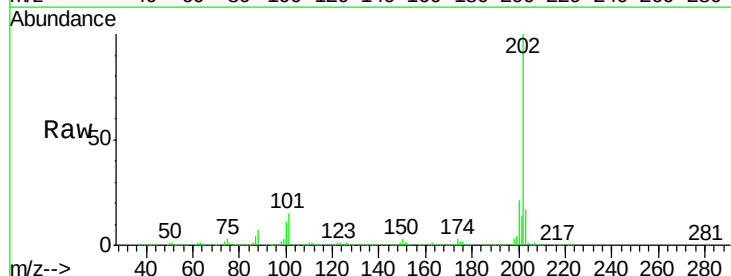

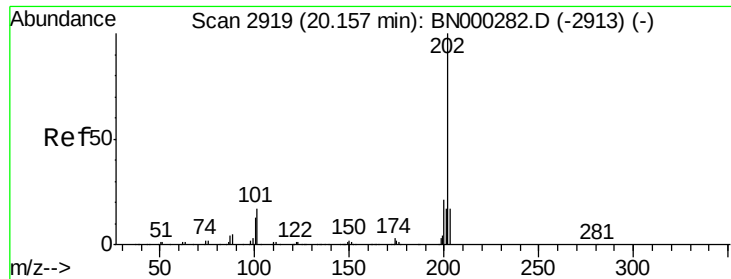


#19
Pvrene
Concen: 30.998 ng/ul m
RT: 20.16 min Scan# 2919
Delta R.T. -0.00 min
Lab File: BN000291.D
Acq: 09 Mar 2018 20:36

Instrument :
BNA_N
ClientSampleId :
DAM79MS

Tot Ion	Ratio	Lower	Upper
202	100		
101	17.8	11.0	16.4#
100	14.8	8.1	12.1#

Manual Integrations
APPROVED

Sohil
3/12/2018 3:52:52 PM



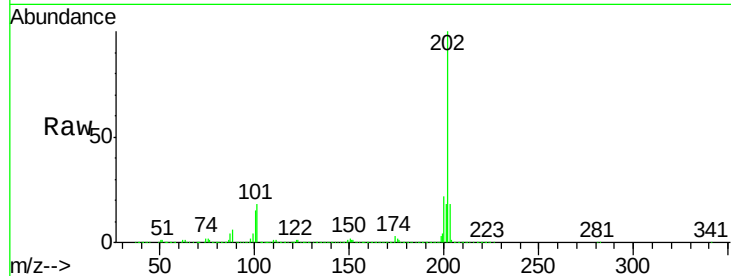


Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

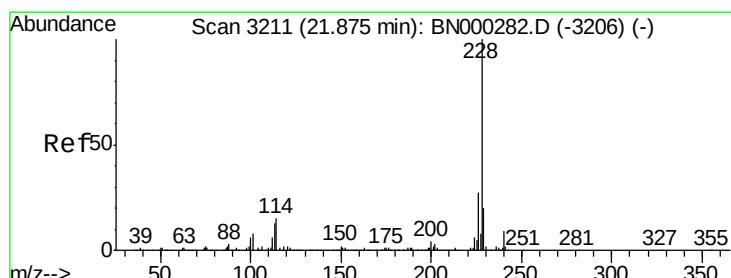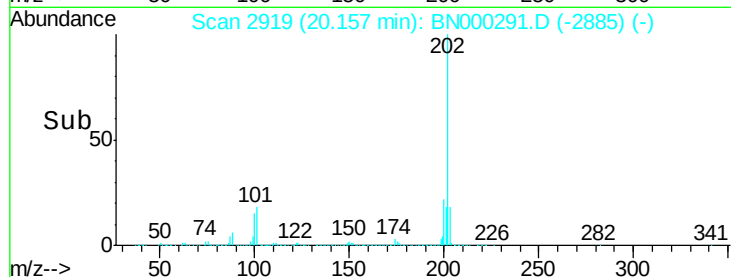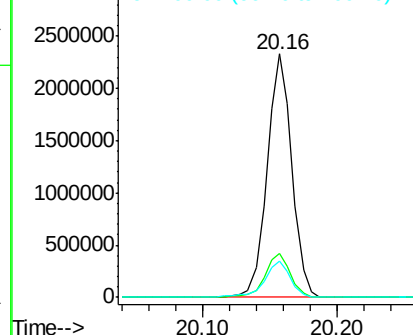

#20
Benzo(a)anthracene
Concen: 4.788 ng/ul m
RT: 21.87 min Scan# 3211
Delta R.T. -0.00 min
Lab File: BN000291.D
Acq: 09 Mar 2018 20:36




Tgt Ion	Ratio	Lower	Upper
228	100		
229	20.4	15.7	23.5
226	26.9	21.1	31.7


Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

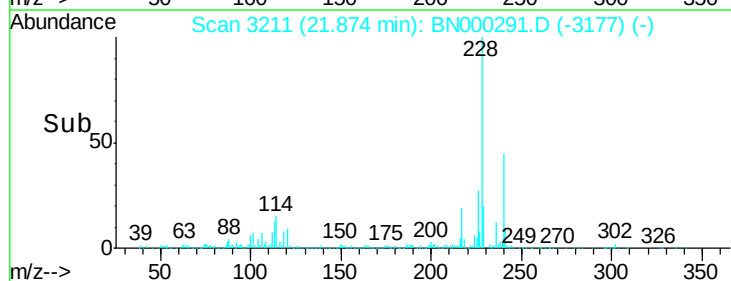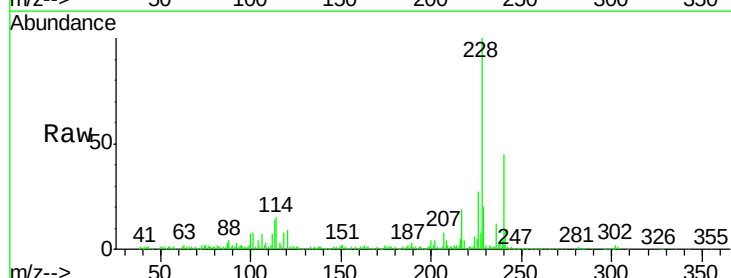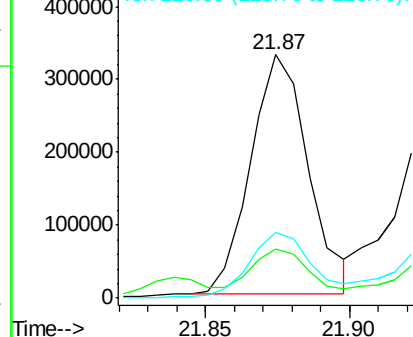

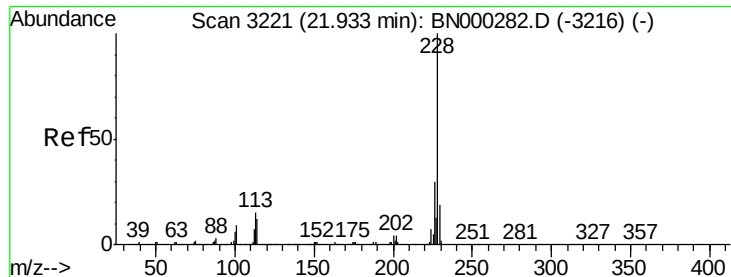





#21
Chrysene
Concen: 4.999 ng/ul
RT: 21.93 min Scan# 3220
Delta R.T. -0.01 min
Lab File: BN000291.D
Acq: 09 Mar 2018 20:36

Instrument :
BNA_N
ClientSampled :
DAM79MS

Tot Ion	Ratio	Lower	Upper
228	100		
226	29.7	24.5	36.7
229	22.2	15.8	23.8




Manual Integrations
APPROVED


Sohil
3/12/2018 3:52:52 PM

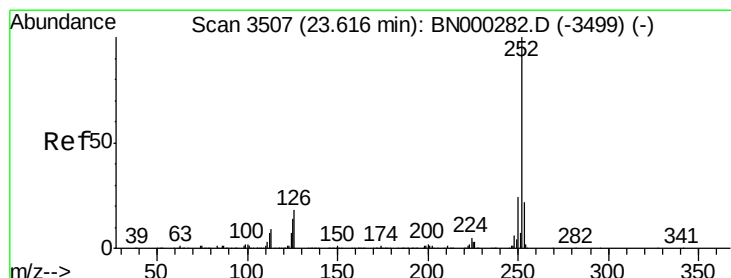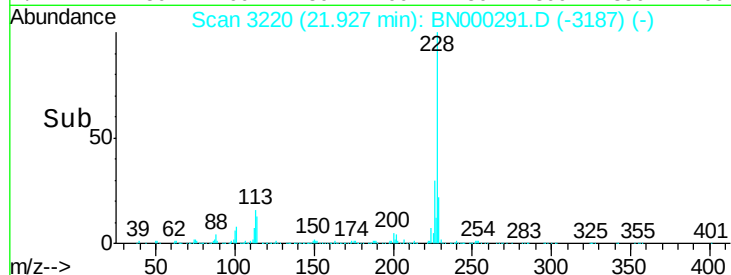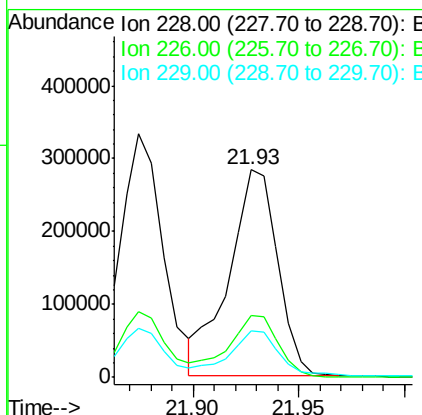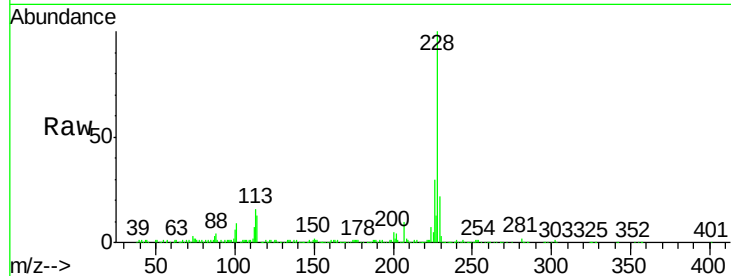

#23
Benzo(b)fluoranthene
Concen: 5.601 ng/ul m
RT: 23.62 min Scan# 3507
Delta R.T. -0.00 min
Lab File: BN000291.D
Acq: 09 Mar 2018 20:36

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.2	18.0	27.0
125	15.1	8.0	12.0

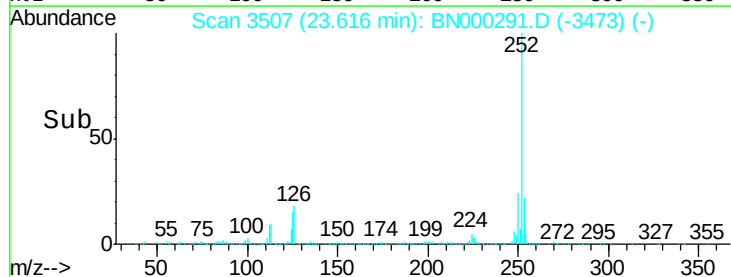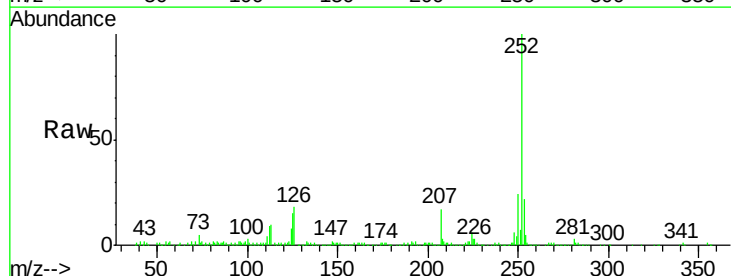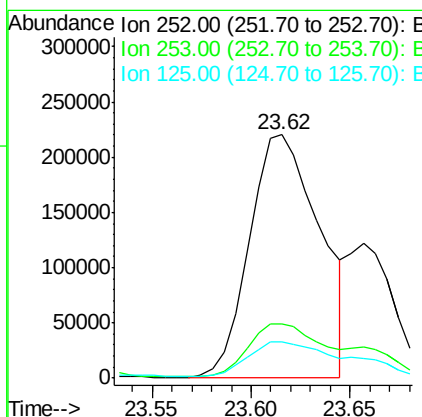

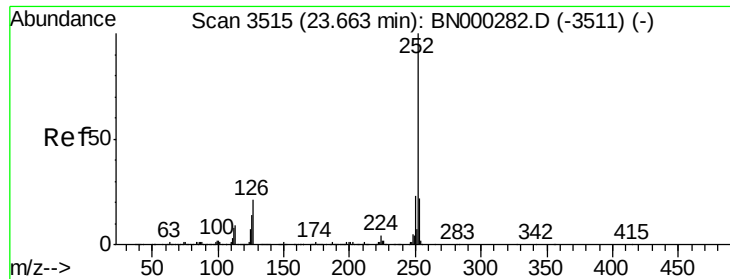





#24
Benzo(k)fluoranthene
Concen: 2.031 ng/ul m
RT: 23.66 min Scan# 3514
Delta R.T. -0.01 min
Lab File: BN000291.D
Acq: 09 Mar 2018 20:36

Instrument :
BNA_N
ClientSampled :
DAM79MS

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.2	18.0	27.0
125	14.8	8.1	12.1




Manual Integrations
APPROVED


Sohil
3/12/2018 3:52:52 PM

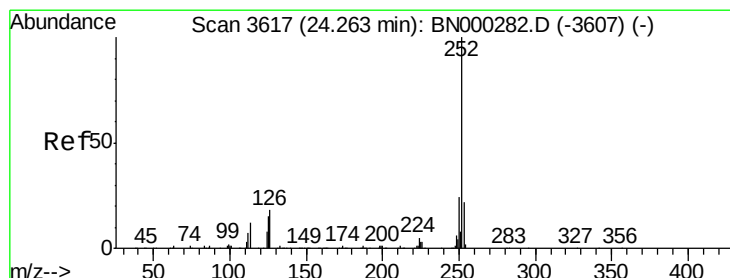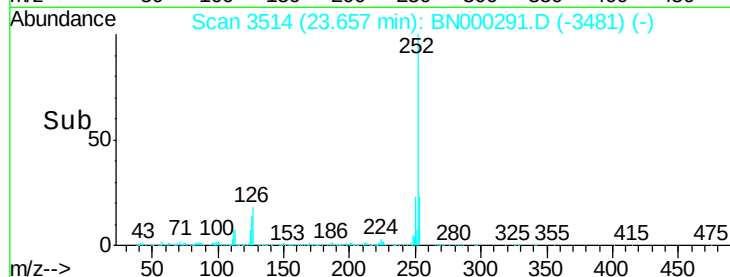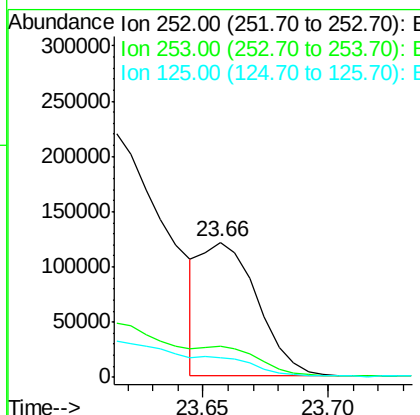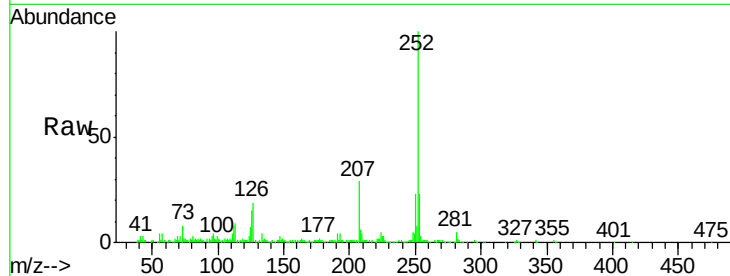

#26
Benzo(a)pyrene
Concen: 3.678 ng/ul
RT: 24.26 min Scan# 3617
Delta R.T. -0.00 min
Lab File: BN000291.D
Acq: 09 Mar 2018 20:36

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.9	17.2	25.8
125	15.0	8.2	12.4

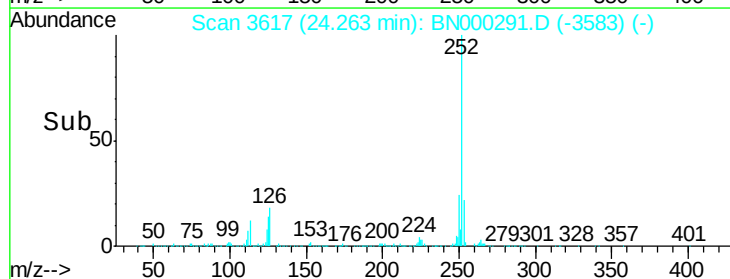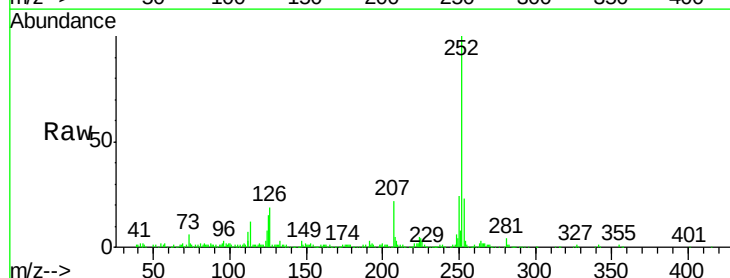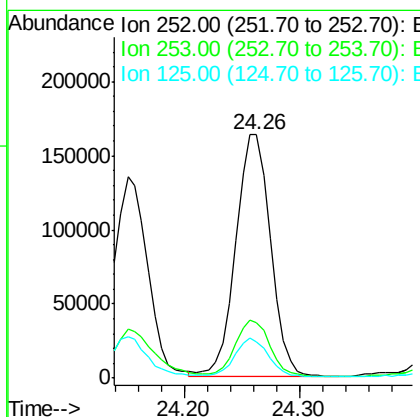

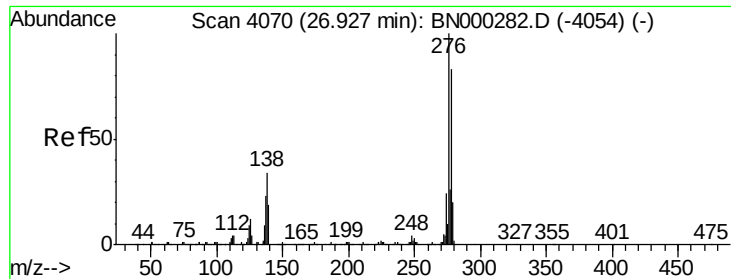





#27
 Indeno(1,2,3-cd)pyrene
 Concen: 2.138 ng/ul
 RT: 26.92 min Scan# 4068
 Delta R.T. -0.01 min
 Lab File: BN000291.D
 Acq: 09 Mar 2018 20:36

Instrument :
 BNA_N
 ClientSampleId :
 DAM79MS

Tot Ion	Ratio	Lower	Upper
276	100		
138	32.1	14.4	21.6#
277	24.6	18.0	27.0

Manual Integrations
 APPROVED

Sohil
 3/12/2018 3:52:52 PM

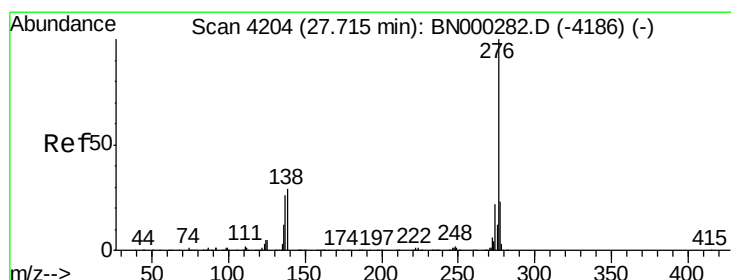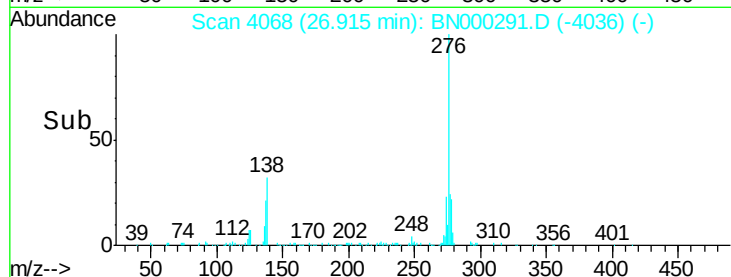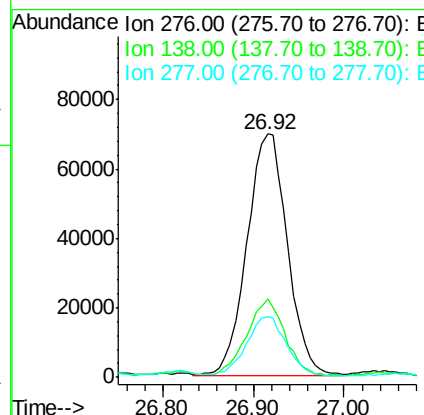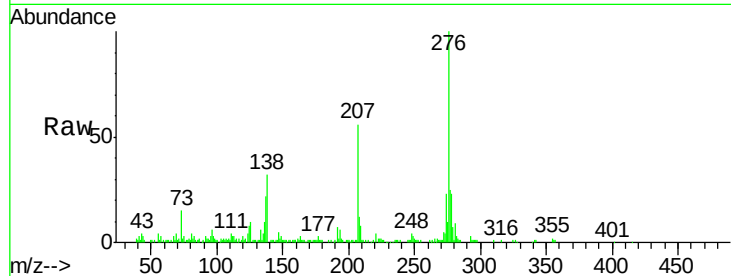

#29
 Benzo(g,h,i)perylene
 Concen: 2.482 ng/ul
 RT: 27.70 min Scan# 4202
 Delta R.T. -0.01 min
 Lab File: BN000291.D
 Acq: 09 Mar 2018 20:36

Tgt Ion	Ratio	Lower	Upper
276	100		
138	29.0	15.3	22.9#
277	24.2	19.0	28.4

