

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA N\DATA\BN030918\
 Data File : BN000293.D
 Acq On : 09 Mar 2018 21:45
 Operator : JU/SJ
 Sample : J1844-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAMA1

Manual Integrations
 APPROVED

Sohil
 3/12/2018 3:52:58 PM

Quant Time: Mar 12 01:17:15 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN030918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 09 23:47:40 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.45	152	289482	20.00	ng/ul	0.00
2) Naphthalene-d8	11.29	136	1400001	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.06	164	797704	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.78	188	1674712	20.00	ng/ul	0.00
17) Chrysene-d12	21.89	240	1680457	20.00	ng/ul	0.00
22) Perylene-d12	24.37	264	1690462	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	14.76	160	1472922	18.60	ng/ul	0.00
10) Fluorene-d10	16.03	176	1003766	18.72	ng/ul	0.00
14) Anthracene-d10	17.87	188	1482262	18.94	ng/ul	0.00
18) Pyrene-d10	20.13	212	1612124	19.61	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.21	264	1507718	19.53	ng/ul	0.00
Target Compounds				Ovalue		
13) Phenanthrene	17.82	178	118452	1.233	ng/ul	99
16) Fluoranthene	19.80	202	306910	2.958	ng/ul	95
19) Pyrene	20.16	202	261014m	2.460	ng/ul	
20) Benzo(a)anthracene	21.87	228	148619m	1.423	ng/ul	
21) Chrysene	21.93	228	159076	1.605	ng/ul	97
23) Benzo(b)fluoranthene	23.62	252	238958	2.371	ng/ul#	95
26) Benzo(a)pyrene	24.26	252	140184	1.461	ng/ul#	93
29) Benzo(g,h,i)perylene	27.71	276	92122	1.067	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA N\DATA\BN030918\
Data File : BN000293.D
Acq On : 09 Mar 2018 21:45
Operator : JU/SJ
Sample : J1844-13
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DAMA1

Manual Integrations
APPROVED

Sohil
3/12/2018 3:52:58 PM

Quant Time: Mar 12 01:17:15 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN030918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 09 23:47:40 2018
Response via : Initial Calibration

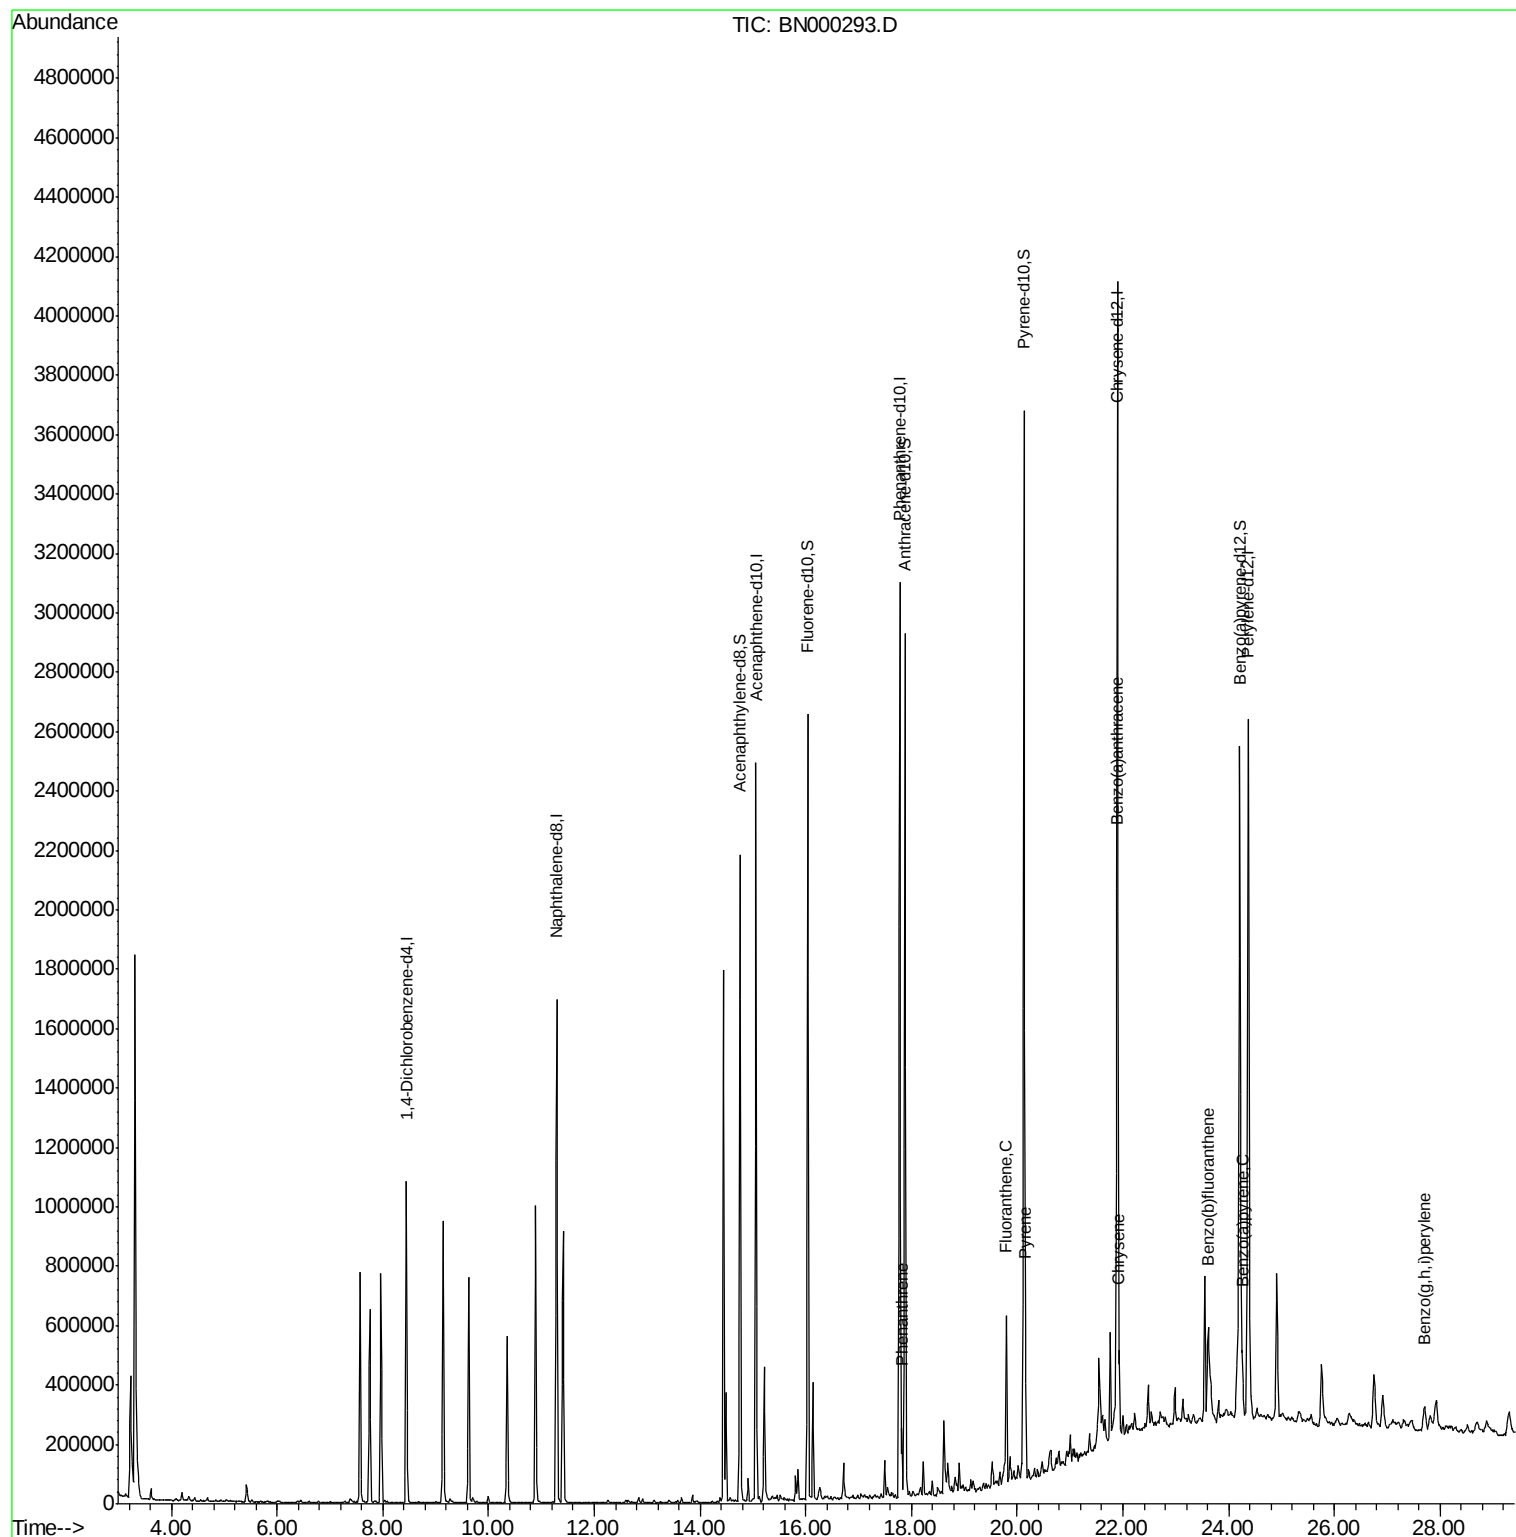

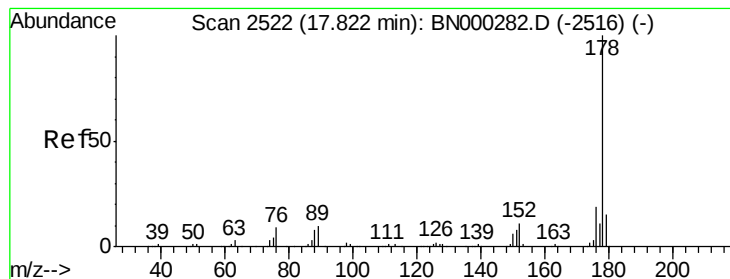

#13

Phenanthrene

Concen: 1.233 ng/ul

RT: 17.82 min Scan# 2522

Delta R.T. -0.00 min

Lab File: BN000293.D

Acq: 09 Mar 2018 21:45

Instrument :

BNA_N


ClientSampled :

DAMA1




Tot Ion:	178	Resp:	118452
Ion Ratio	Lower	Upper	
178	100		
179	16.3	12.3	18.5
176	18.9	15.1	22.7

Manual Integrations
APPROVED

Sohil
3/12/2018 3:52:58 PM

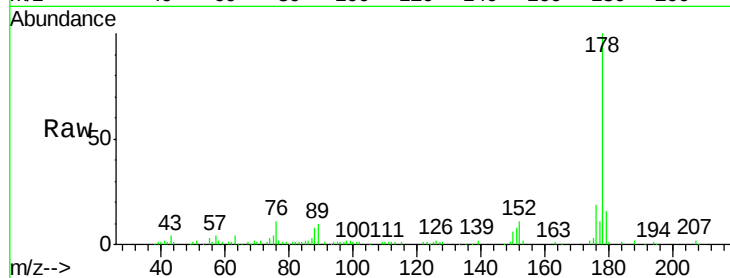

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

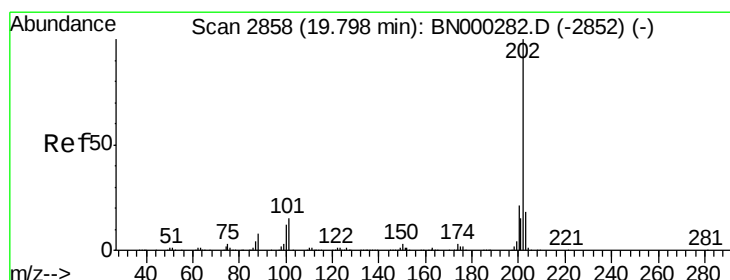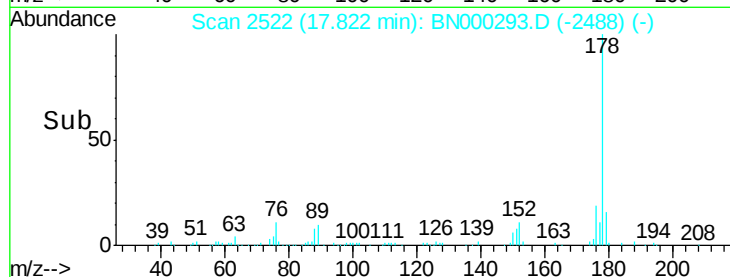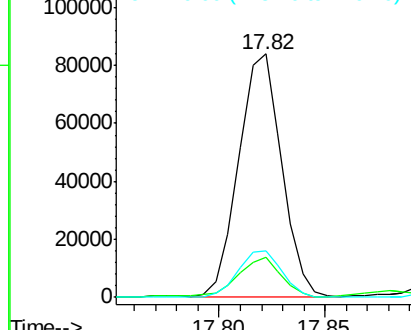

#16

Fluoranthene

Concen: 2.958 ng/ul


RT: 19.80 min Scan# 2858

Delta R.T. 0.00 min



Lab File: BN000293.D


Acq: 09 Mar 2018 21:45

Tgt Ion:	202	Resp:	306910
Ion Ratio	Lower	Upper	
202	100		
101	14.8	9.9	14.9
100	10.5	7.4	11.0

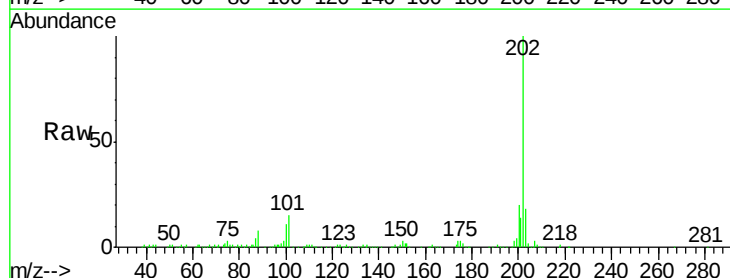

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

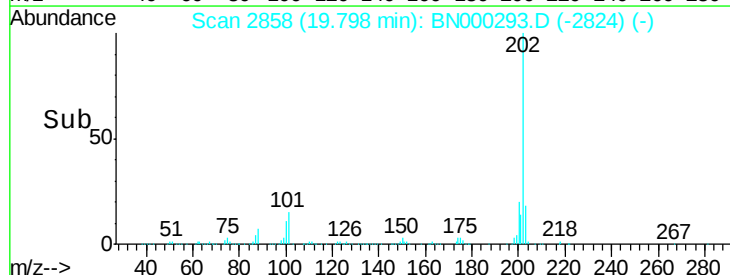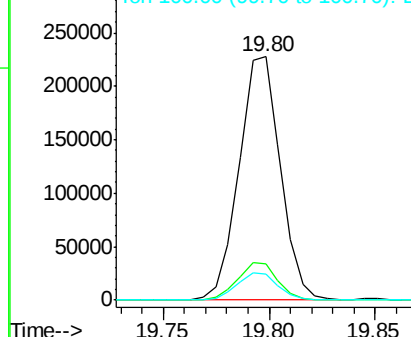

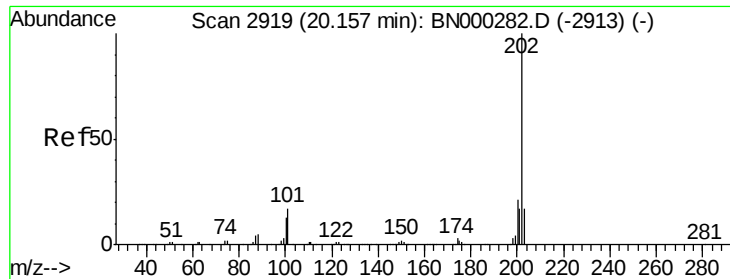





#19
Pvrene
Concen: 2.460 ng/ul m
RT: 20.16 min Scan# 2919
Delta R.T. -0.00 min
Lab File: BN000293.D
Acq: 09 Mar 2018 21:45

Instrument :
BNA_N
ClientSampled :
DAMA1

Tot Ion	Ratio	Lower	Upper
202	100		
101	17.0	11.0	16.4#
100	13.5	8.1	12.1#




Manual Integrations
APPROVED


Sohil
3/12/2018 3:52:58 PM

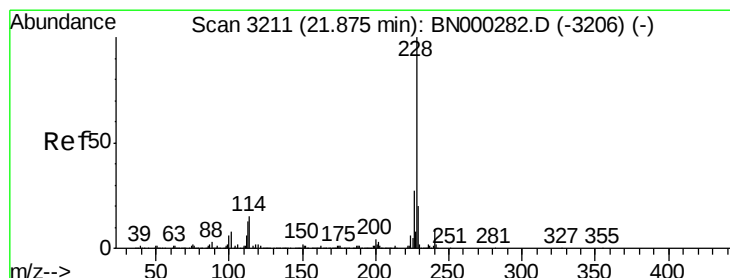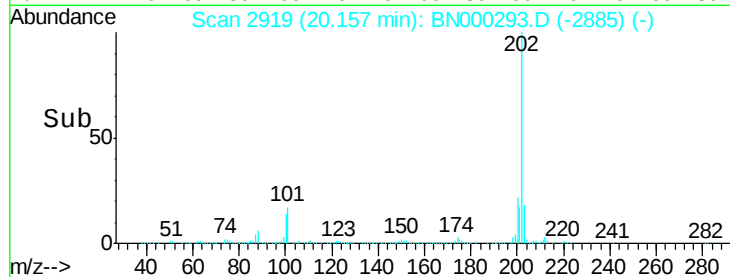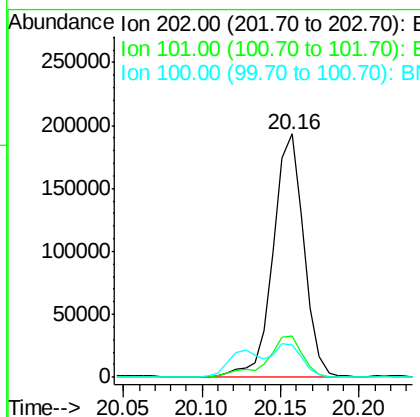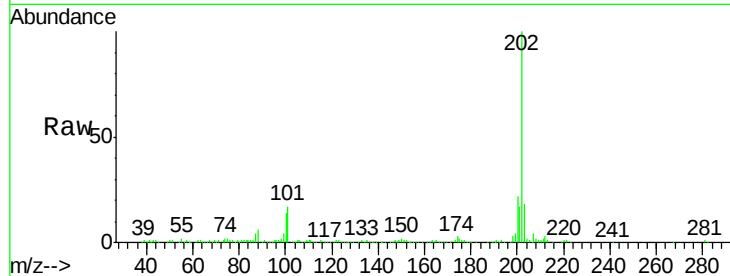

#20
Benzo(a)anthracene
Concen: 1.423 ng/ul m
RT: 21.87 min Scan# 3211
Delta R.T. 0.00 min
Lab File: BN000293.D
Acq: 09 Mar 2018 21:45

Tgt Ion	Ratio	Lower	Upper
228	100		
229	21.8	15.7	23.5
226	27.9	21.1	31.7

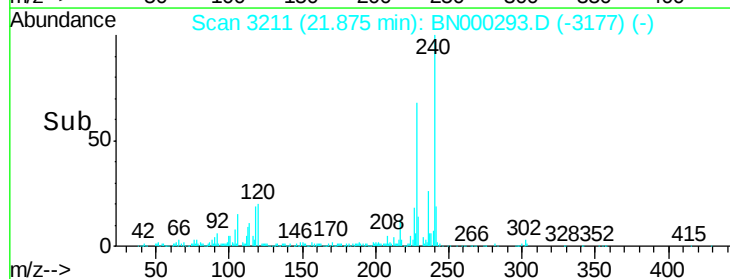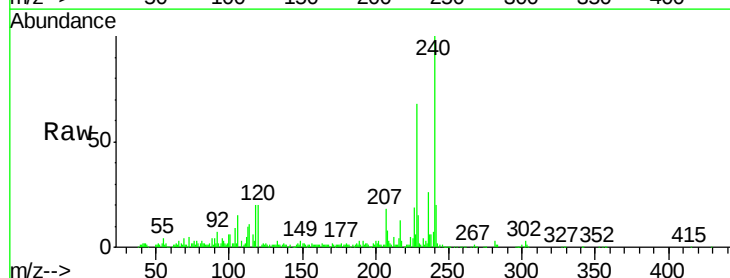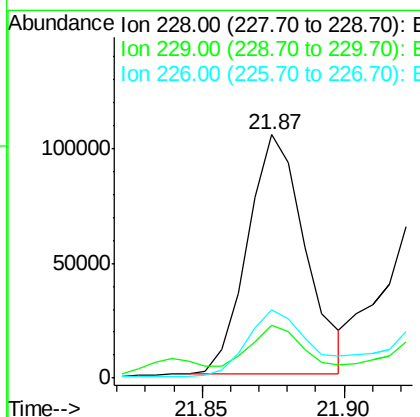

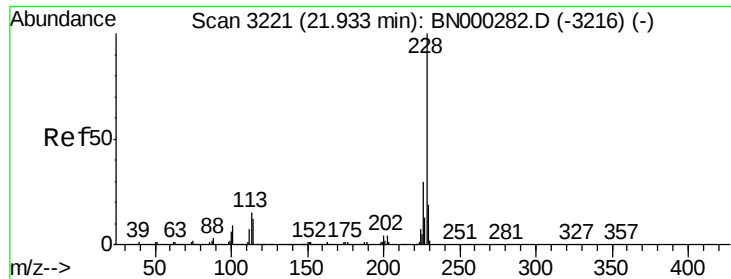





#21
Chrysene
Concen: 1.605 ng/ul
RT: 21.93 min Scan# 3221
Delta R.T. 0.00 min
Lab File: BN000293.D
Acq: 09 Mar 2018 21:45

Instrument :
BNA_N
ClientSampleId :
DAMA1

Tot Ion	Ratio	Lower	Upper
228	100		
226	31.7	24.5	36.7
229	22.1	15.8	23.8




Manual Integrations
APPROVED


Sohil
3/12/2018 3:52:58 PM

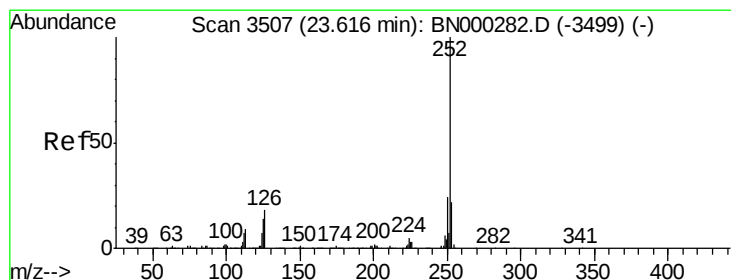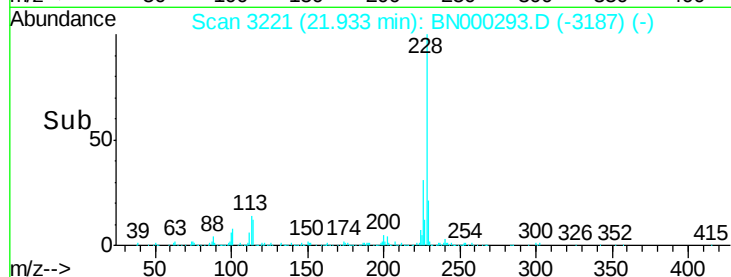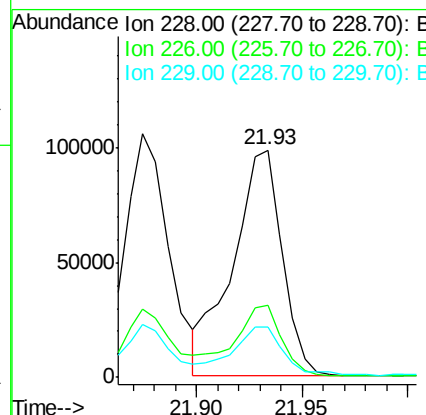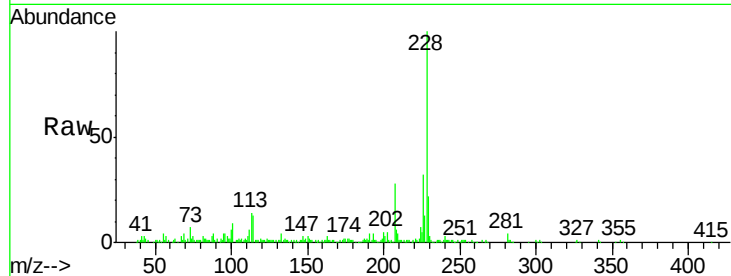

#23
Benzo(b)fluoranthene
Concen: 2.371 ng/ul
RT: 23.62 min Scan# 3507
Delta R.T. 0.00 min
Lab File: BN000293.D
Acq: 09 Mar 2018 21:45

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.3	18.0	27.0
125	15.3	8.0	12.0

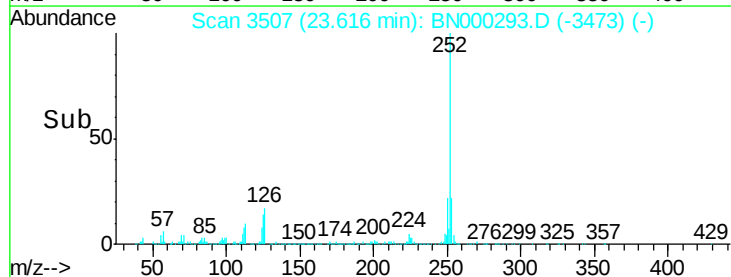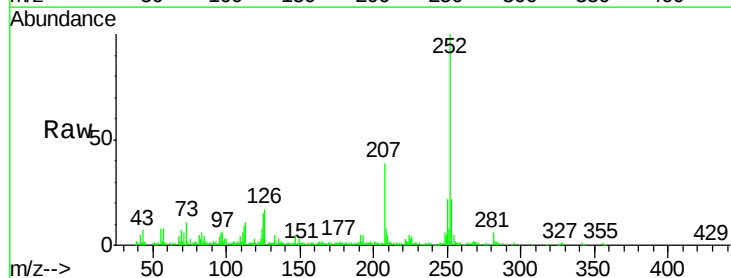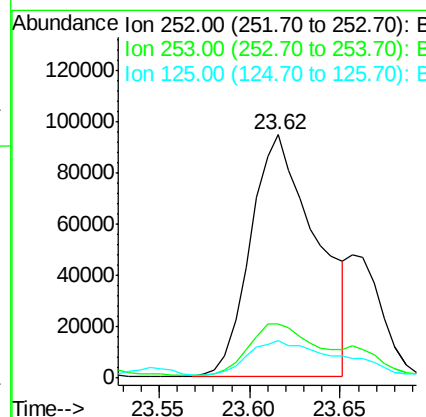

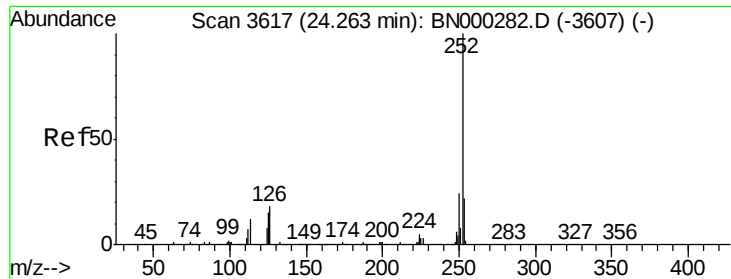

#26

Benzo(a)pyrene

Concen: 1.461 ng/ul

RT: 24.26 min Scan# 3616

Delta R.T. -0.01 min

Lab File: BN000293.D

Acq: 09 Mar 2018 21:45

Instrument :

BNA_N


ClientSampleId :

DAMA1




Tot Ion:	252	Resp:	140184
Ion Ratio		Lower	Upper
252	100		
253	22.7	17.2	25.8
125	16.4	8.2	12.4#

Manual Integrations
APPROVED

Sohil
3/12/2018 3:52:58 PM

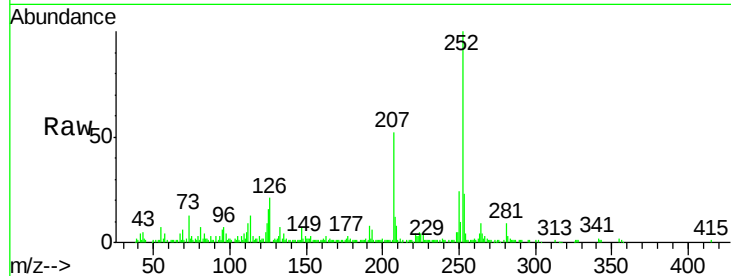

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

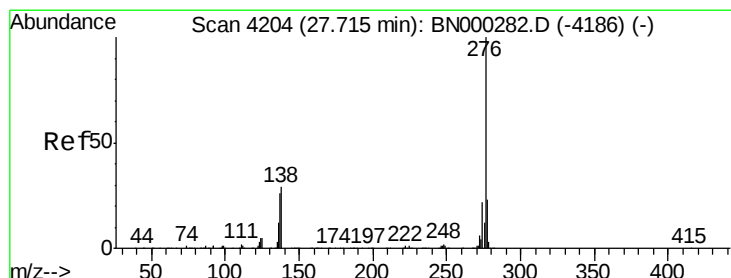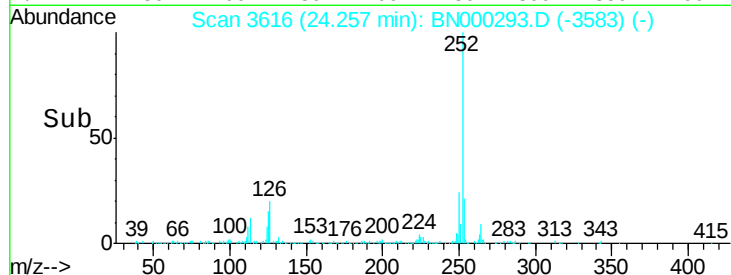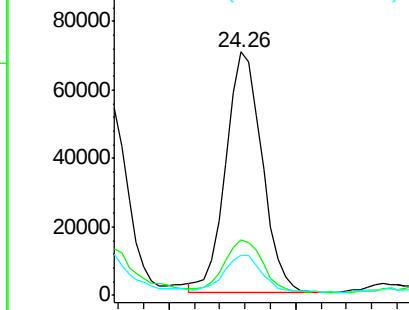

#29

Benzo(g,h,i)perylene

Concen: 1.067 ng/ul


RT: 27.71 min Scan# 4203

Delta R.T. -0.01 min

Lab File: BN000293.D

Acq: 09 Mar 2018 21:45

Tgt Ion:	276	Resp:	92122
Ion Ratio		Lower	Upper
276	100		
138	32.2	15.3	22.9#
277	23.5	19.0	28.4

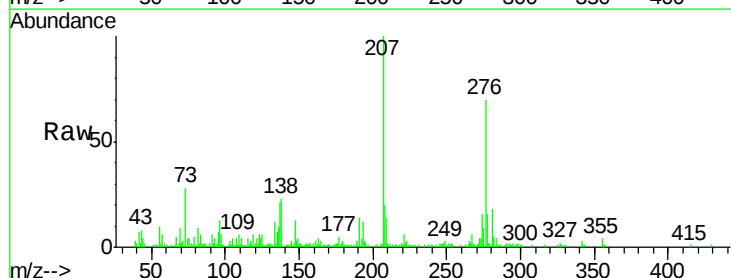

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

