


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030920\
 Data File : BN010142.D
 Acq On : 09 Mar 2020 10:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN021920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 19 15:57:43 2020

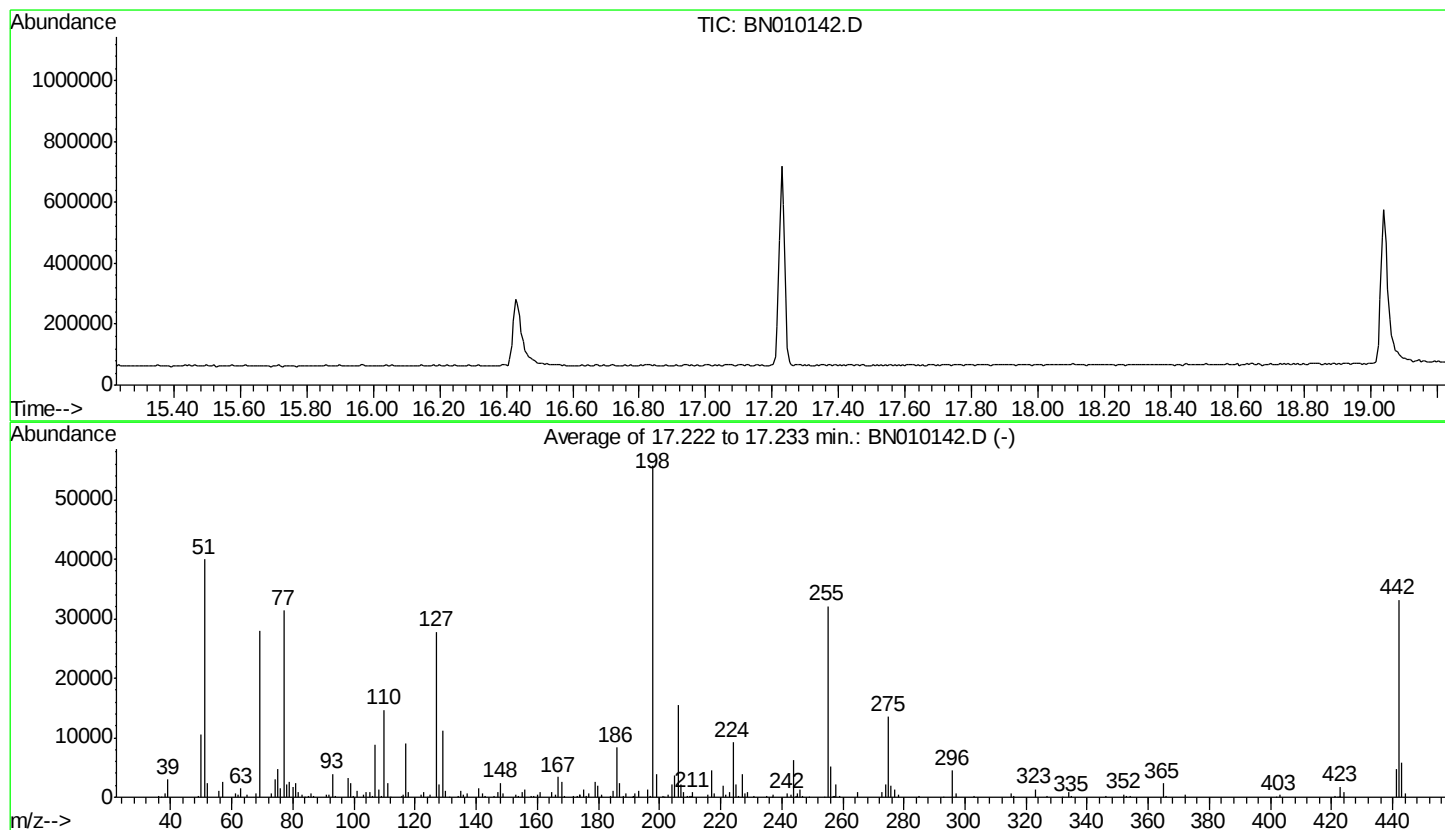

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	71.7	39928	PASS
68	69	0.00	2	2.0	568	PASS
69	198	0.00	100	50.3	27997	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.8	27752	PASS
197	198	0.00	2	0.2	138	PASS
198	198	100	100	100.0	55704	PASS
199	198	5	9	7.0	3922	PASS
275	198	10	60	24.1	13452	PASS
365	198	1	100	4.1	2281	PASS
441	198	0.01	100	8.5	4733	PASS
442	198	50	100	59.5	33160	PASS
443	442	15	24	17.5	5792	PASS