




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030922\
 Data File : BN018890.D
 Acq On : 09 Mar 2022 18:33
 Operator : CG/JU
 Sample : PB143185TB 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLEB185

Manual IntegrationsAPPROVED

Quant Time: Mar 10 01:37:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 08 14:15:20 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/10/2022
 Supervised By :Yogesh Patel 03/11/2022

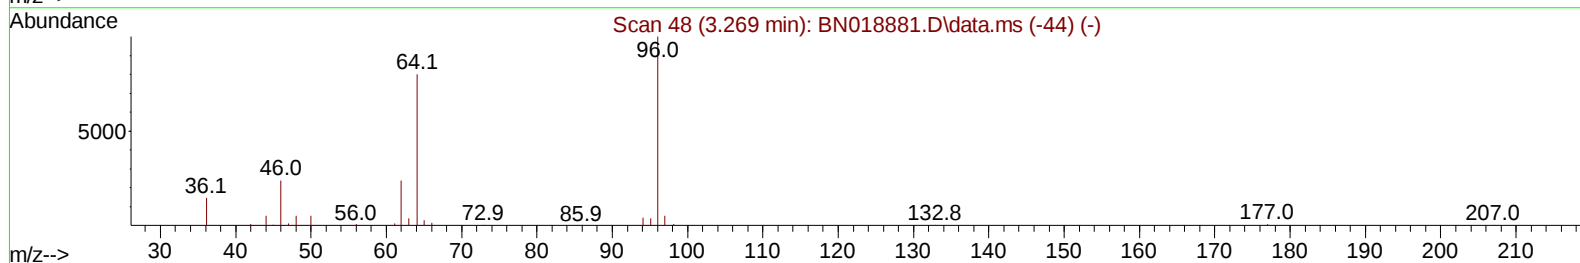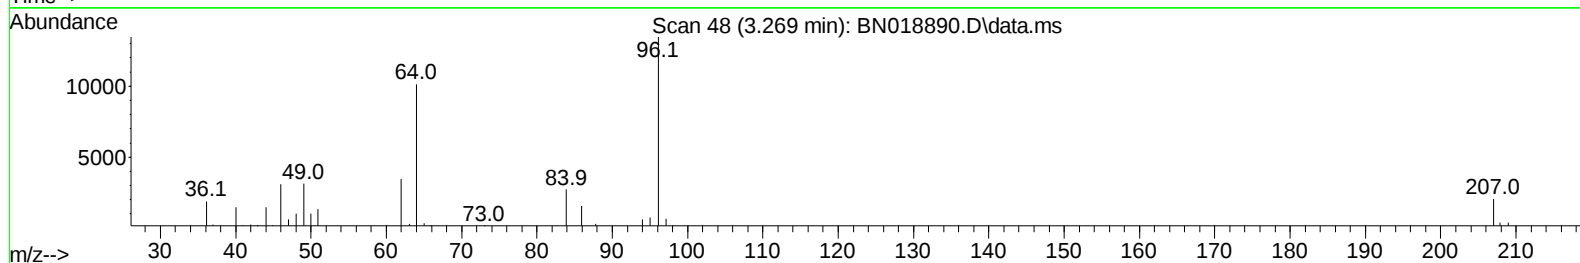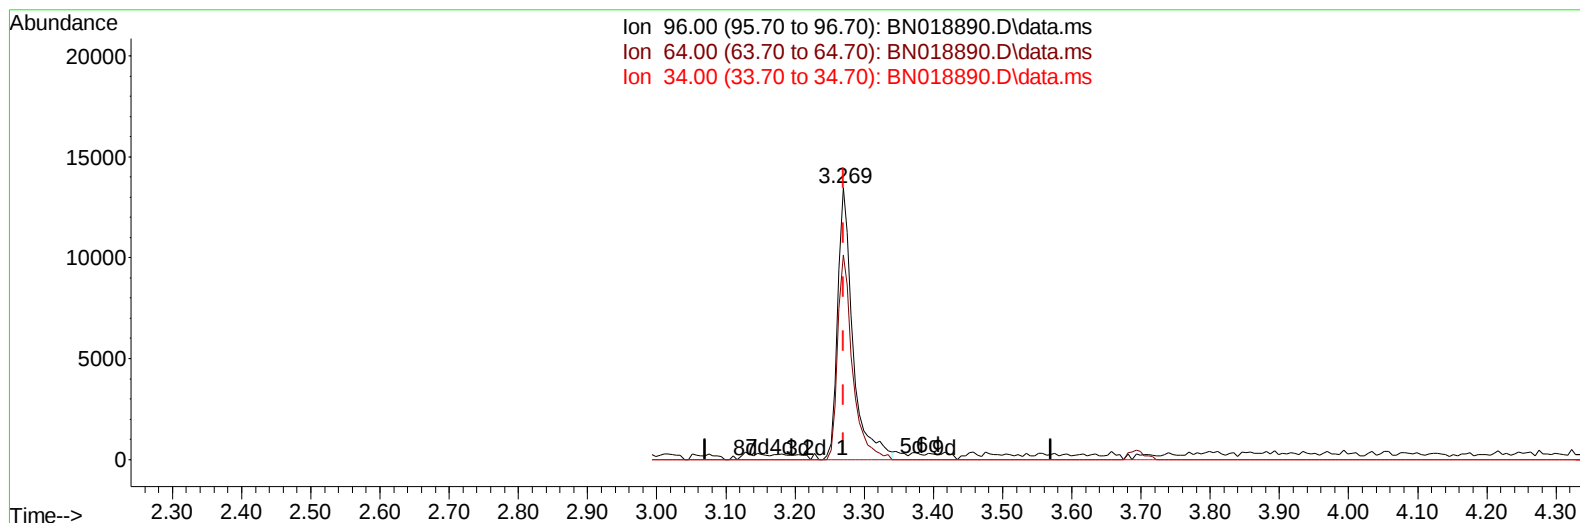

TIC: BN018890.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.269min (-0.001) 5.96 ng/uL

response 20638

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	80.20	75.23
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030922\
 Data File : BN018890.D
 Acq On : 09 Mar 2022 18:33
 Operator : CG/JU
 Sample : PB143185TB 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLEB185

Manual IntegrationsAPPROVED

Quant Time: Mar 10 01:37:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 08 14:15:20 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/10/2022
 Supervised By :Yogesh Patel 03/11/2022

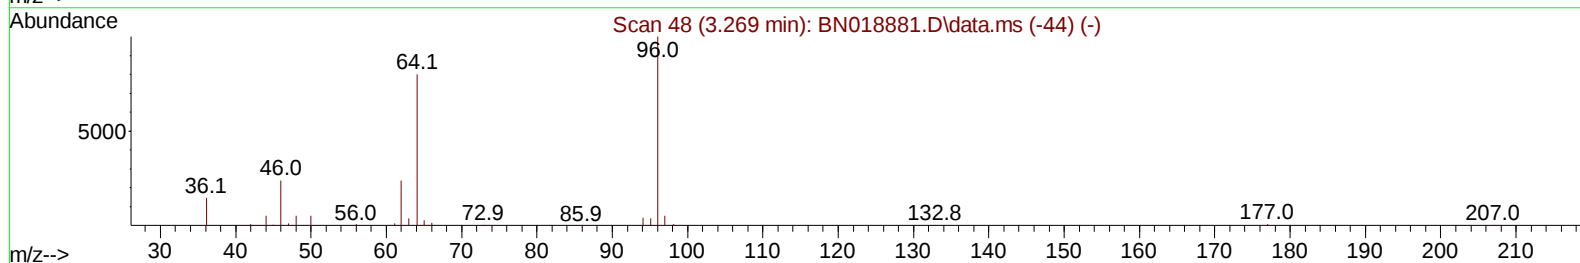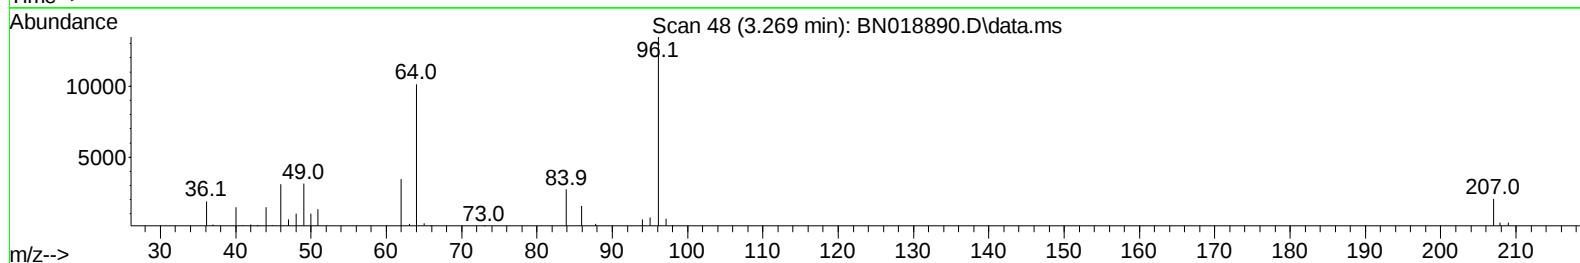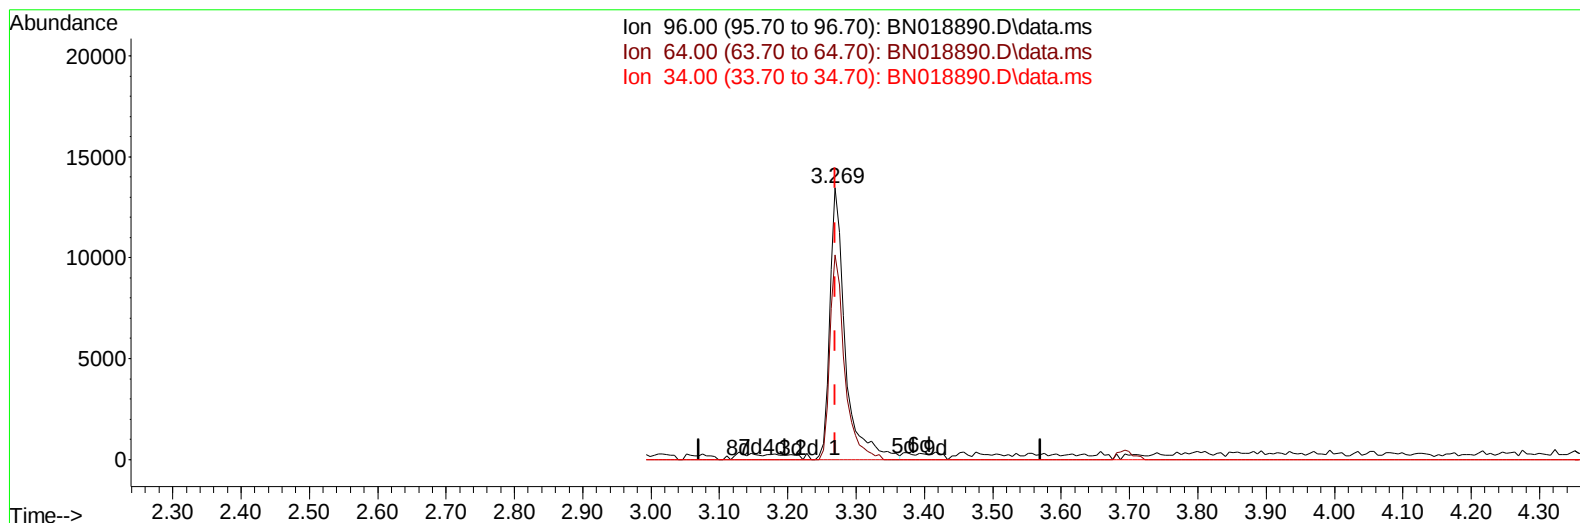

TIC: BN018890.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.269min (-0.001) 6.08 ng/uL m

response 21053

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	80.20	75.23
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030922\
 Data File : BN018890.D
 Acq On : 09 Mar 2022 18:33
 Operator : CG/JU
 Sample : PB143185TB 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLEB185

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/10/2022
 Supervised By :Yogesh Patel 03/11/2022

Quant Time: Mar 10 01:37:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 08 14:15:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	138522	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	651672	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.539	164	458402	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.275	188	1014075	20.000	ng/ul	0.00
79) Chrysene-d12	21.451	240	1117850	20.000	ng/ul	0.00
88) Perylene-d12	23.845	264	1210072	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	21053m	6.079	ng/uL	0.00
4) Pyridine-d5	3.687	84	285109	26.903	ng/ul	0.00
7) Phenol-d5	7.058	99	360215	26.636	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	236706	29.059	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	277208	28.602	ng/ul	0.00
15) 4-Methylphenol-d8	8.604	113	292681	26.615	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	138157	27.600	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	155111	28.203	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	283584	26.957	ng/ul	0.00
31) 4-Chloroaniline-d4	10.840	131	439500	27.744	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	1047846	30.191	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	1261943	29.211	ng/ul	0.00
54) 4-Nitrophenol-d4	14.716	143	166326	23.664	ng/ul	0.00
60) Fluorene-d10	15.528	176	904086	29.968	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.639	200	146208	23.265	ng/ul	0.00
73) Anthracene-d10	17.375	188	1493572	30.793	ng/ul	0.00
81) Pyrene-d10	19.663	212	1819515	30.078	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	1993912	31.616	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030922\
Data File : BN018890.D
Acq On : 09 Mar 2022 18:33
Operator : CG/JU
Sample : PB143185TB 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB185

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/10/2022
Supervised By :Yogesh Patel 03/11/2022

Quant Time: Mar 10 01:37:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 08 14:15:20 2022
Response via : Initial Calibration

