

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030922\
 Data File : BN018886.D
 Acq On : 09 Mar 2022 16:05
 Operator : CG/JU
 Sample : PB142786BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK786

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018886.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	44	48	55	rBV	33207	48475	0.99%	0.106%
2	3.687	116	119	148	rBV	446242	780389	15.88%	1.713%
3	4.046	176	180	186	rVB	7900	11413	0.23%	0.025%
4	7.052	685	691	704	rVB	588350	957061	19.47%	2.101%
5	7.222	714	720	732	rVB	490837	781111	15.89%	1.715%
6	7.428	748	755	764	rBV	589592	935317	19.03%	2.053%
7	7.905	829	836	845	rVB	465399	732714	14.91%	1.609%
8	8.605	946	955	966	rBV	765134	1203243	24.48%	2.642%
9	9.058	1025	1032	1041	rBV	583433	943736	19.20%	2.072%
10	9.787	1149	1156	1169	rBV	476583	772743	15.72%	1.697%
11	10.328	1240	1248	1259	rBV	732352	1205195	24.52%	2.646%
12	10.710	1304	1313	1321	rBV	721723	1186825	24.15%	2.606%
13	10.840	1325	1335	1348	rBV	780793	1324184	26.94%	2.907%
14	12.299	1578	1583	1590	rBV2	11245	20170	0.41%	0.044%
15	13.940	1856	1862	1869	rBV	1477872	1974130	40.17%	4.334%
16	14.234	1905	1912	1923	rBV	1578282	2340423	47.62%	5.138%
17	14.540	1956	1964	1972	rBV	1165153	1736664	35.33%	3.813%
18	14.716	1987	1994	2004	rBV	640293	918703	18.69%	2.017%
19	15.528	2125	2132	2142	rBV	2124258	2993693	60.91%	6.573%
20	15.634	2144	2150	2163	rBV	631388	849312	17.28%	1.865%
21	15.769	2169	2173	2179	rVB5	10211	14588	0.30%	0.032%
22	17.057	2391	2392	2396	rVB3	5217	5827	0.12%	0.013%
23	17.275	2423	2429	2439	rBV	1561075	2158889	43.93%	4.740%
24	17.375	2439	2446	2460	rVV	2410286	3337162	67.90%	7.327%
25	19.233	2757	2762	2767	rVB2	26612	38078	0.77%	0.084%
26	19.298	2769	2773	2780	rVV	29236	39445	0.80%	0.087%
27	19.598	2820	2824	2827	rBV5	5206	6259	0.13%	0.014%
28	19.663	2829	2835	2848	rVV	3066541	4138465	84.20%	9.086%
29	20.663	3002	3005	3010	rVB3	13925	16830	0.34%	0.037%
30	21.451	3134	3139	3149	rBV	2338745	2717288	55.29%	5.966%
31	22.069	3241	3244	3248	rVB	45093	52406	1.07%	0.115%
32	22.569	3325	3329	3334	rVB	116717	154732	3.15%	0.340%
33	23.116	3417	3422	3429	rBV	198743	326547	6.64%	0.717%
34	23.692	3512	3520	3526	rBV2	2478250	4914937	100.00%	10.791%
35	23.745	3526	3529	3536	rVB	292566	461977	9.40%	1.014%
36	23.845	3538	3546	3556	rVV	1471672	3002465	61.09%	6.592%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030922\
Data File : BN018886.D
Acq On : 09 Mar 2022 16:05
Operator : CG/JU
Sample : PB142786BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK786

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Title : SVOA CALIBRATION

37	24.463	3644	3651	3661	rBV	293052	602679	12.26%	1.323%
38	25.304	3786	3794	3807	rVB	280120	704122	14.33%	1.546%
39	26.286	3953	3961	3973	rVB2	205304	604598	12.30%	1.327%
40	27.451	4152	4159	4175	rVB2	163248	535777	10.90%	1.176%




Sum of corrected areas: 45548572

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030922\
Data File : BN018886.D
Acq On : 09 Mar 2022 16:05
Operator : CG/JU
Sample : PB142786BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK786

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

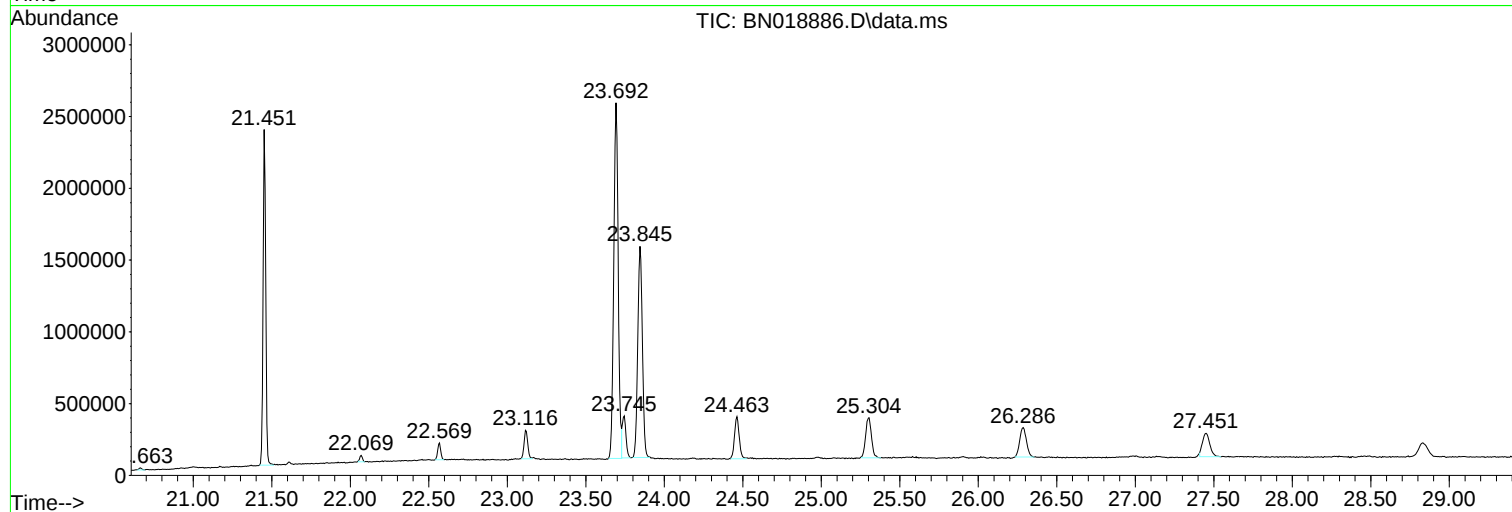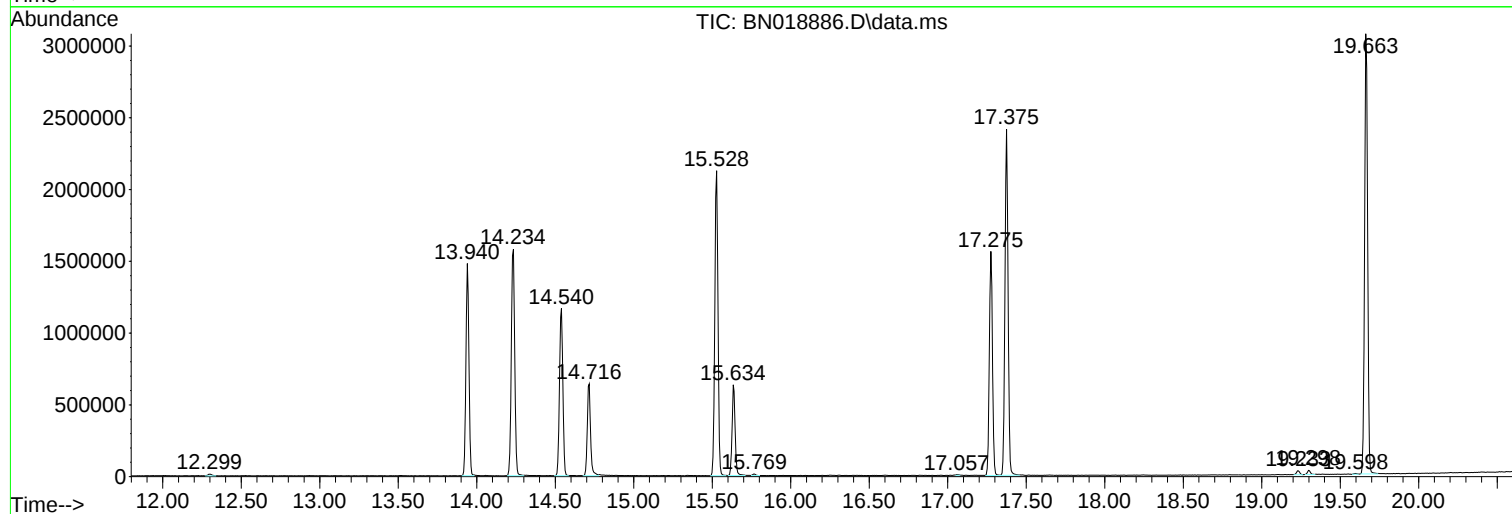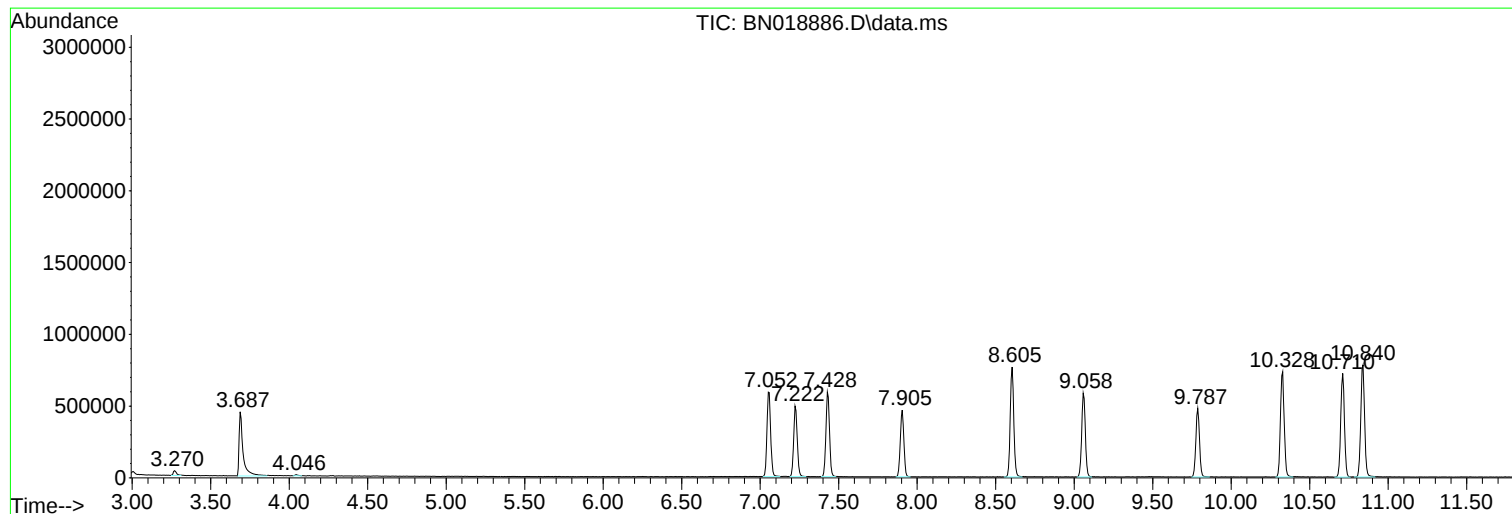

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030922\
Data File : BN018886.D
Acq On : 09 Mar 2022 16:05
Operator : CG/JU
Sample : PB142786BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK786

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030922\
Data File : BN018886.D
Acq On : 09 Mar 2022 16:05
Operator : CG/JU
Sample : PB142786BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK786

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc