

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030922\
 Data File : BN018889.D
 Acq On : 09 Mar 2022 17:57
 Operator : CG/JU
 Sample : PB143227BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK227

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018889.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	44	48	53	rBV	34163	45297	0.84%	0.101%
2	3.687	115	119	141	rBV	446804	769822	14.33%	1.717%
3	4.046	176	180	189	rVB	9405	16460	0.31%	0.037%
4	7.057	685	692	706	rBV	611543	974837	18.14%	2.175%
5	7.222	713	720	730	rBV	485617	785726	14.62%	1.753%
6	7.428	748	755	767	rBV	587401	957080	17.81%	2.135%
7	7.904	829	836	846	rVB	473742	750613	13.97%	1.675%
8	8.604	948	955	967	rBV	798497	1237708	23.04%	2.761%
9	9.057	1025	1032	1041	rBV	600529	976443	18.17%	2.178%
10	9.787	1149	1156	1165	rBV	504221	814433	15.16%	1.817%
11	10.328	1241	1248	1262	rBV	768265	1262878	23.50%	2.817%
12	10.710	1305	1313	1321	rBV	741925	1215971	22.63%	2.713%
13	10.840	1327	1335	1345	rBV	830544	1416527	26.36%	3.160%
14	12.298	1578	1583	1590	rVB2	13618	21916	0.41%	0.049%
15	13.939	1856	1862	1869	rBV	1586292	2129376	39.63%	4.750%
16	14.234	1904	1912	1933	rBV	1726849	2544122	47.35%	5.676%
17	14.539	1957	1964	1973	rBV	1224279	1801825	33.54%	4.020%
18	14.716	1987	1994	2009	rBV	751363	1046972	19.49%	2.336%
19	15.528	2125	2132	2144	rBV	2322798	3219258	59.92%	7.182%
20	15.639	2144	2151	2165	rVV	691737	968003	18.02%	2.160%
21	15.769	2169	2173	2177	rVB2	9238	13117	0.24%	0.029%
22	16.257	2251	2256	2259	rBV6	2682	5413	0.10%	0.012%
23	17.063	2391	2393	2397	rVB3	5911	7071	0.13%	0.016%
24	17.275	2423	2429	2437	rBV	1590781	2256422	42.00%	5.034%
25	17.375	2439	2446	2464	rVB	2584791	3616086	67.30%	8.067%
26	19.233	2757	2762	2767	rBV3	31063	45698	0.85%	0.102%
27	19.304	2769	2774	2780	rVV	31635	44745	0.83%	0.100%
28	19.669	2829	2836	2853	rVV	3287892	4507324	83.89%	10.056%
29	20.663	3001	3005	3010	rBV3	19048	26721	0.50%	0.060%
30	20.998	3059	3062	3069	rVB2	36278	60674	1.13%	0.135%
31	21.451	3134	3139	3145	rBV2	2229265	2827700	52.63%	6.308%
32	23.692	3512	3520	3535	rBV2	2696048	5372827	100.00%	11.986%
33	23.845	3538	3546	3558	rVB2	1532139	3085215	57.42%	6.883%




Sum of corrected areas: 44824280

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030922\
Data File : BN018889.D
Acq On : 09 Mar 2022 17:57
Operator : CG/JU
Sample : PB143227BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK227

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

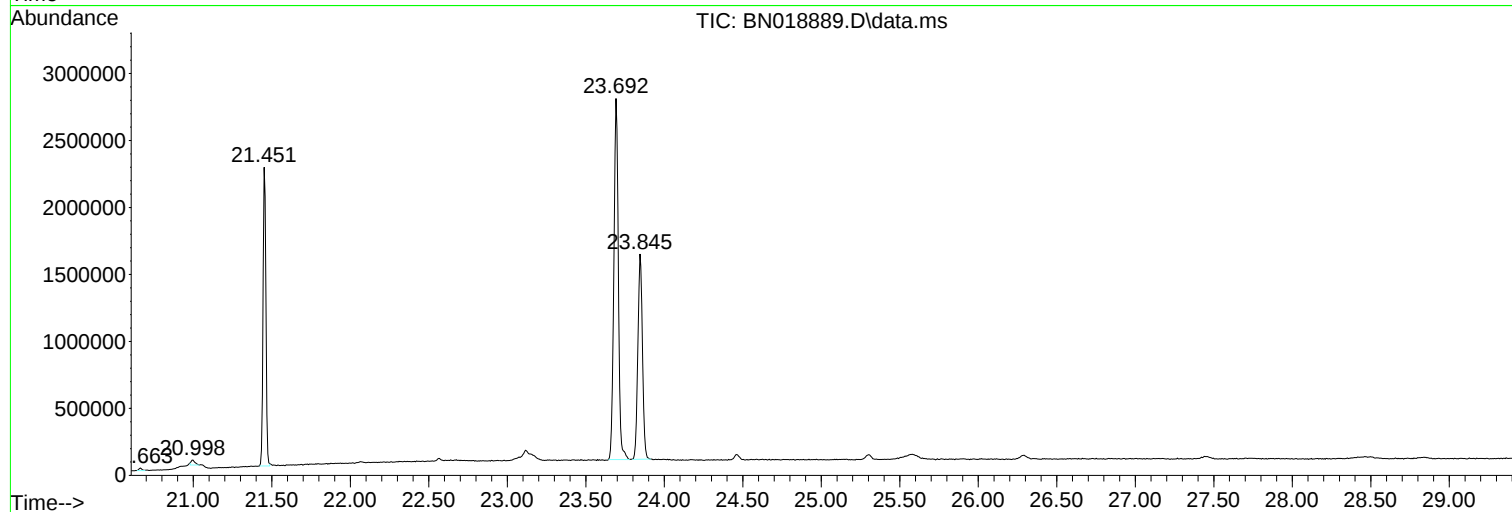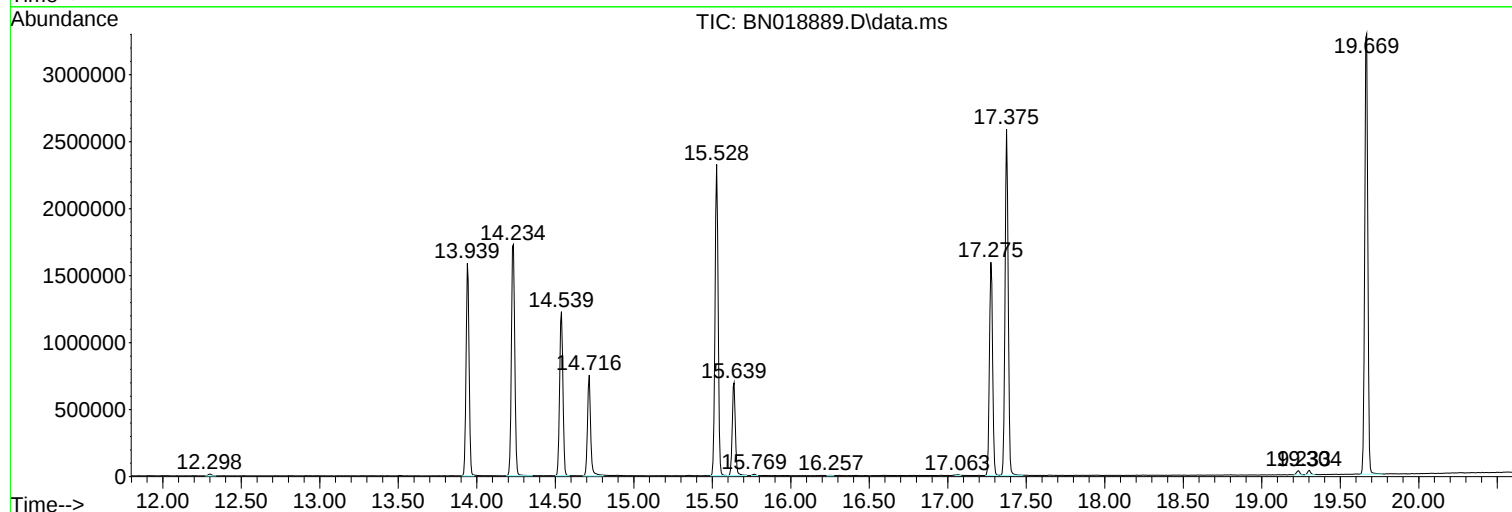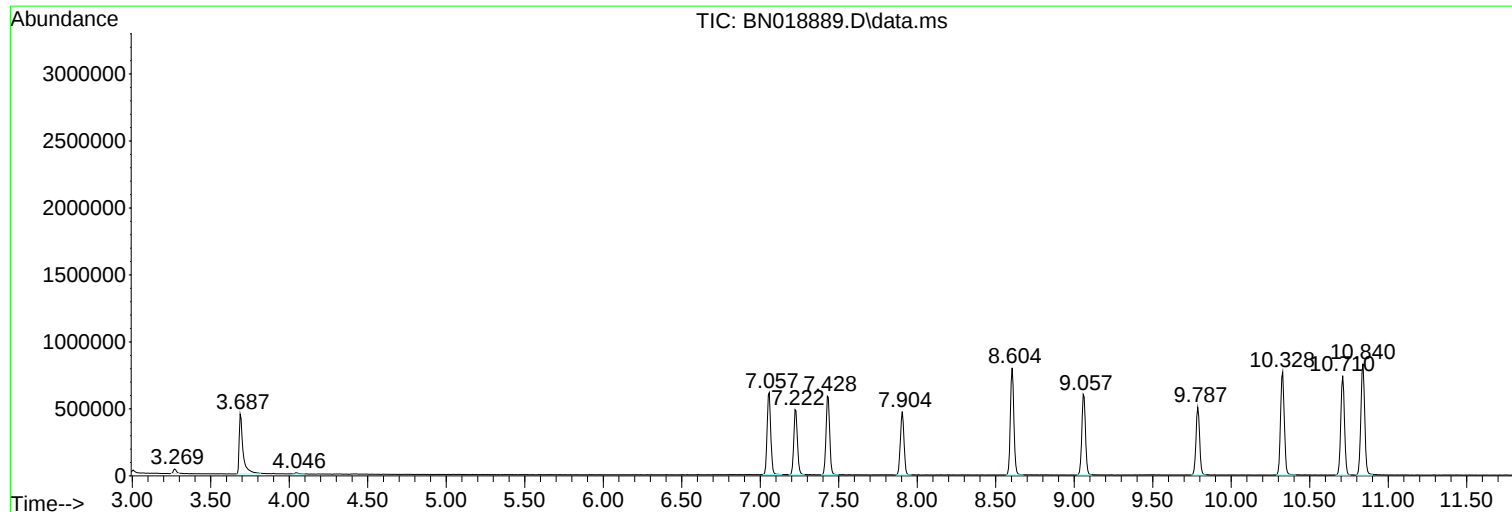

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030922\
Data File : BN018889.D
Acq On : 09 Mar 2022 17:57
Operator : CG/JU
Sample : PB143227BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK227

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030922\
Data File : BN018889.D
Acq On : 09 Mar 2022 17:57
Operator : CG/JU
Sample : PB143227BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK227

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------