

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031021\
 Data File : BN013897.D
 Acq On : 10 Mar 2021 09:07
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Mar 10 09:53:08 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 08 10:32:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.716	152	6085	0.40	ng	0.00
7) Naphthalene-d8	10.492	136	22415	0.40	ng	-0.01
13) Acenaphthene-d10	14.346	164	11953	0.40	ng	0.00
19) Phenanthrene-d10	17.092	188	25445	0.40	ng	# 0.00
29) Chrysene-d12	21.261	240	24779	0.40	ng	0.00
36) Perylene-d12	23.486	264	22130	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.308	112	5824	0.36	ng	0.00
5) Phenol-d6	6.879	99	7578	0.35	ng	0.00
8) Nitrobenzene-d5	8.857	82	5954	0.41	ng	0.00
11) 2-Methylnaphthalene-d10	12.089	152	14262	0.39	ng	0.00
14) 2,4,6-Tribromophenol	15.831	330	1450	0.30	ng	-0.01
15) 2-Fluorobiphenyl	12.963	172	18801	0.44	ng	-0.01
27) Fluoranthene-d10	19.119	212	28453	0.38	ng	0.00
31) Terphenyl-d14	19.719	244	22151	0.40	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.255	88	2956	0.40	ng	97
3) n-Nitrosodimethylamine	3.585	42	1899	0.33	ng	# 95
6) bis(2-Chloroethyl)ether	7.145	93	6682	0.43	ng	96
9) Naphthalene	10.543	128	23107	0.42	ng	100
10) Hexachlorobutadiene	10.834	225	4339	0.41	ng	# 99
12) 2-Methylnaphthalene	12.160	142	15258	0.39	ng	98
16) Acenaphthylene	14.067	152	18587	0.35	ng	99
17) Acenaphthene	14.410	154	13839	0.42	ng	99
18) Fluorene	15.399	166	17033	0.40	ng	99
20) 4,6-Dinitro-2-methylph...	15.475	198	1009	0.57	ng	# 80
21) 4-Bromophenyl-phenylether	16.289	248	5478	0.40	ng	# 86
22) Hexachlorobenzene	16.398	284	6543	0.45	ng	99
23) Atrazine	16.556	200	3256	0.25	ng	99
24) Pentachlorophenol	16.739	266	1264	0.27	ng	96
25) Phenanthrene	17.128	178	28725	0.43	ng	100
26) Anthracene	17.214	178	22917	0.35	ng	100
28) Fluoranthene	19.149	202	31222	0.39	ng	99
30) Pyrene	19.511	202	31335	0.41	ng	100
32) Benzo(a)anthracene	21.250	228	26794	0.35	ng	99
33) Chrysene	21.303	228	32595	0.44	ng	97
34) Bis(2-ethylhexyl)phtha...	21.186	149	7495	0.21	ng	98
35) Indeno(1,2,3-cd)pyrene	25.717	276	36015	0.40	ng	98
37) Benzo(b)fluoranthene	22.818	252	31242	0.44	ng	96
38) Benzo(k)fluoranthene	22.863	252	31225	0.46	ng	# 94
39) Benzo(a)pyrene	23.390	252	27174	0.43	ng	95
40) Dibenzo(a,h)anthracene	25.728	278	29912	0.44	ng	98
41) Benzo(g,h,i)perylene	26.395	276	31291	0.46	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031021\
Data File : BN013897.D
Acq On : 10 Mar 2021 09:07
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Quant Time: Mar 10 09:53:08 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 08 10:32:09 2021
Response via : Initial Calibration

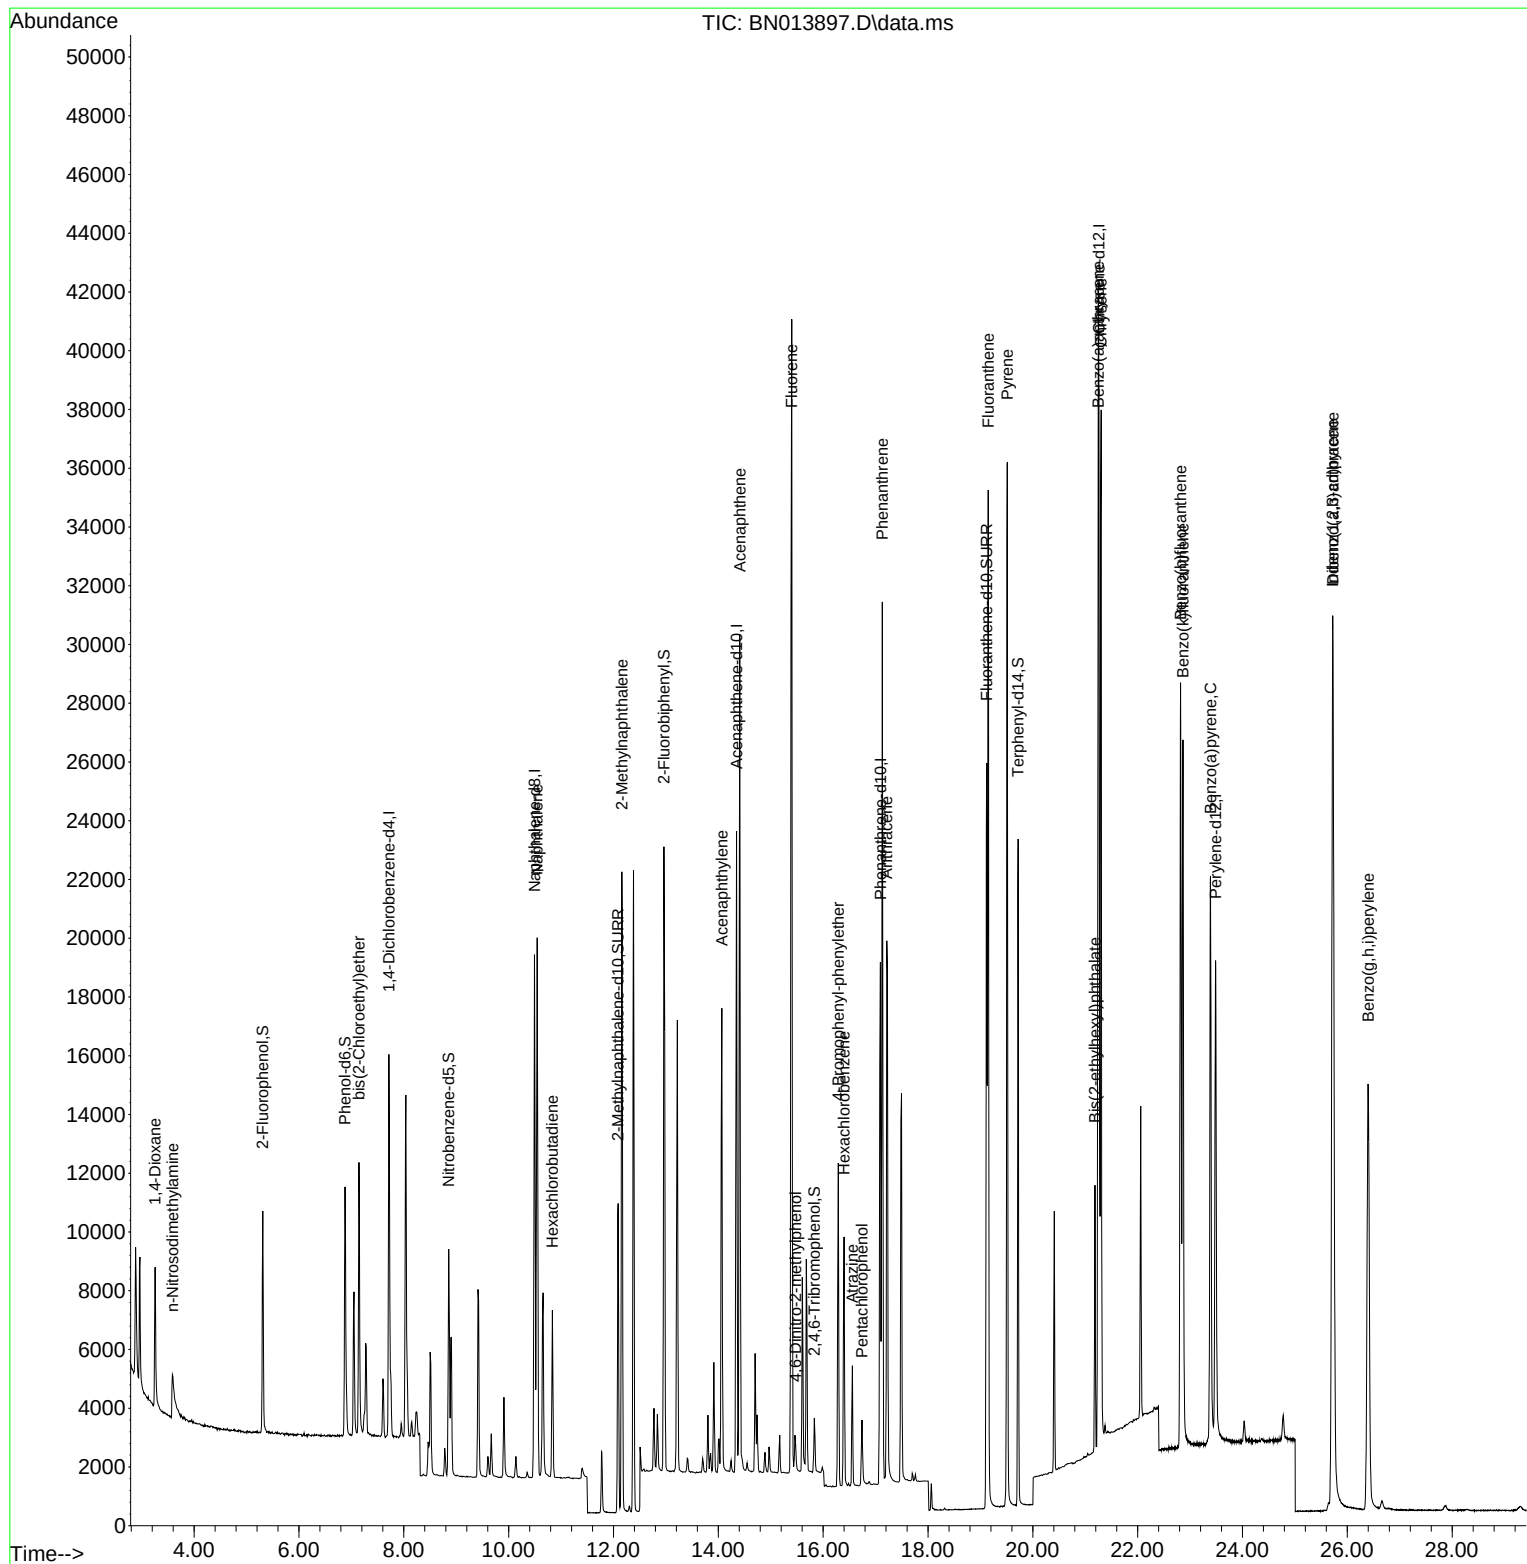






#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.716 min Scan# 613
Delta R.T. -0.008 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

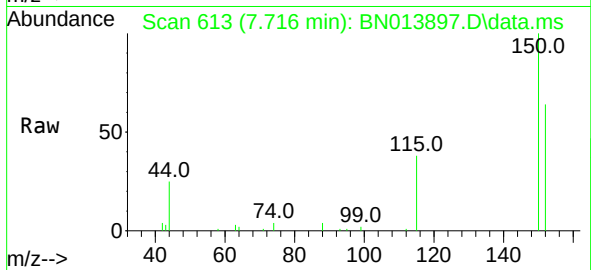


Tgt Ion: 152 Resp: 6085

Ion	Ratio	Lower	Upper
152	100		
150	155.8	121.8	182.8
115	59.2	46.6	69.8

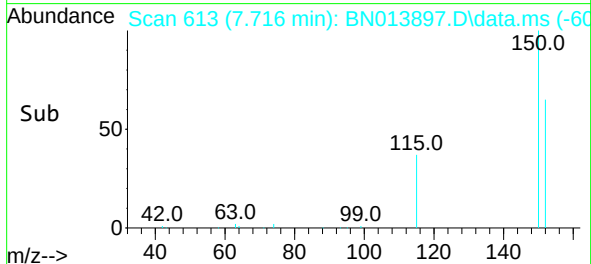




#2
1,4-Dioxane
Concen: 0.40 ng
RT: 3.255 min Scan# 59
Delta R.T. 0.000 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

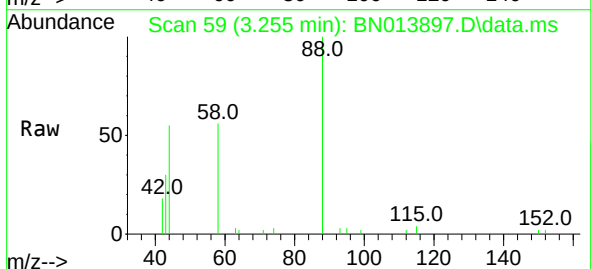

Tgt Ion: 88 Resp: 2956

Ion	Ratio	Lower	Upper
88	100		
58	82.8	64.6	96.8
43	35.7	26.6	40.0



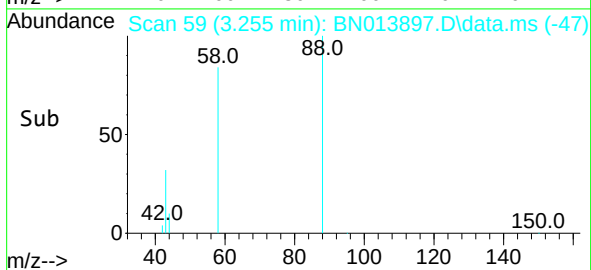





#3
n-Nitrosodimethylamine
Concen: 0.33 ng
RT: 3.585 min Scan# 100
Delta R.T. 0.008 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 42 Resp: 1899
Ion Ratio Lower Upper
42 100
74 113.5 95.0 142.6
44 9.0 5.8 8.8#

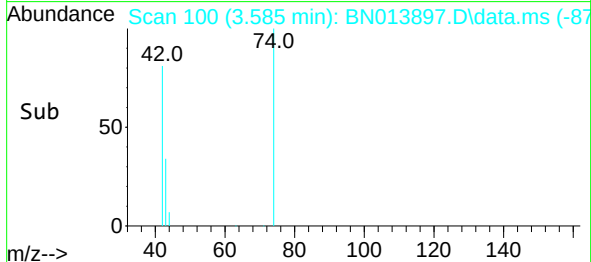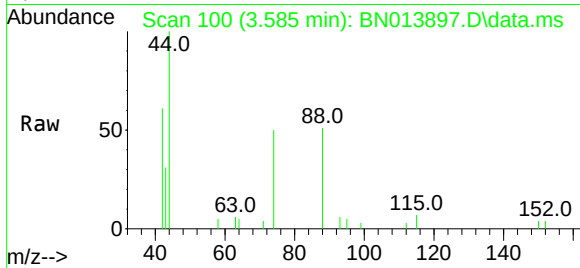

#4
2-Fluorophenol
Concen: 0.36 ng
RT: 5.308 min Scan# 314
Delta R.T. 0.000 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Tgt Ion: 112 Resp: 5824
Ion Ratio Lower Upper
112 100
64 60.2 44.3 66.5
63 31.8 23.0 34.6


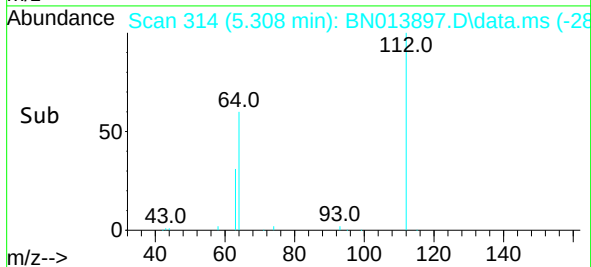

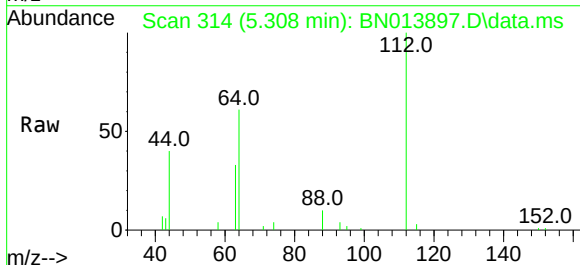




#5
Phenol-d6
Concen: 0.35 ng
RT: 6.879 min Scan# 509
Delta R.T. 0.000 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	99	Resp:	7578
Ion	Ratio	Lower	Upper
99	100		
42	22.4	15.2	22.8
71	33.1	26.1	39.1

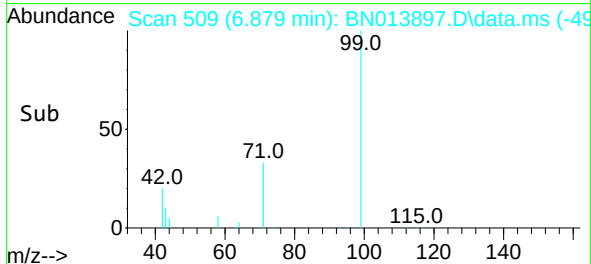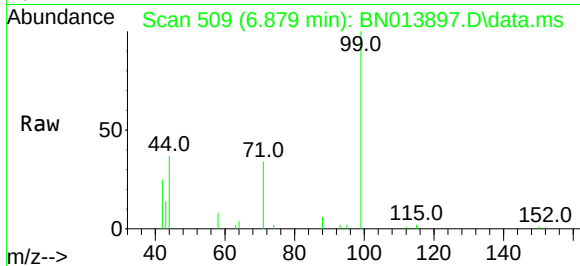

#6
bis(2-Chloroethyl)ether
Concen: 0.43 ng
RT: 7.145 min Scan# 542
Delta R.T. 0.000 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Tgt Ion:	93	Resp:	6682
Ion	Ratio	Lower	Upper
93	100		
63	80.3	60.8	91.2
95	33.2	26.0	39.0




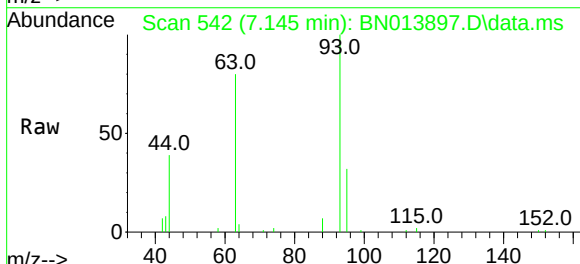




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.492 min Scan# 859
Delta R.T. -0.013 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	22415
Ion Ratio	Lower	Upper	
136	100		
137	11.5	9.0	13.6
54	8.8	6.4	9.6
68	6.5	4.5	6.7

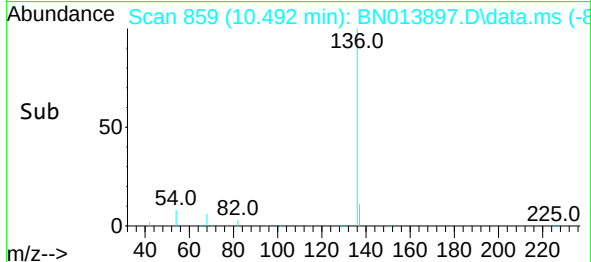

#8
Nitrobenzene-d5
Concen: 0.41 ng
RT: 8.857 min Scan# 730
Delta R.T. 0.000 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Tgt Ion:	82	Resp:	5954
Ion Ratio	Lower	Upper	
82	100		
128	35.1	39.2	58.8#
54	56.7	40.1	60.1


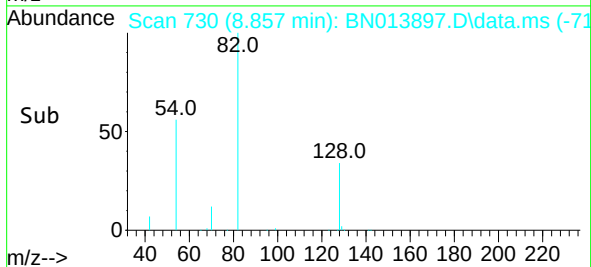

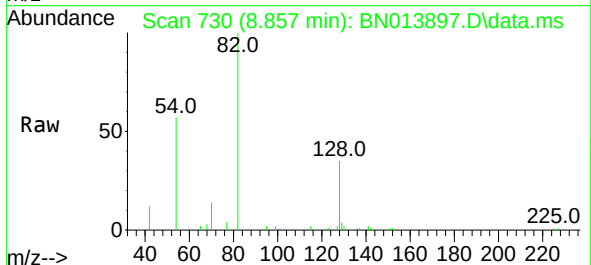




#9
Naphthalene
Concen: 0.42 ng
RT: 10.543 min Scan# 863
Delta R.T. 0.000 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:128	Resp:	23107
Ion Ratio	Lower	Upper
128	100	
129	11.2	9.0 13.4
127	13.3	10.4 15.6

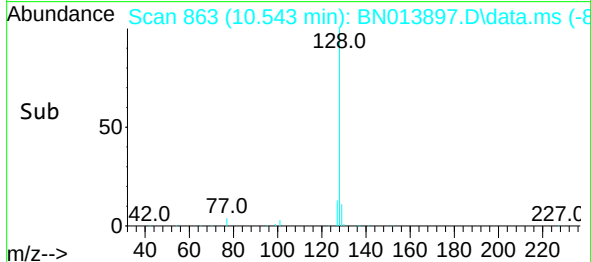

#10
Hexachlorobutadiene
Concen: 0.41 ng
RT: 10.834 min Scan# 886
Delta R.T. 0.000 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Tgt Ion:225	Resp:	4339
Ion Ratio	Lower	Upper
225	100	
223	0.0	0.0 0.0
227	64.4	51.2 76.8


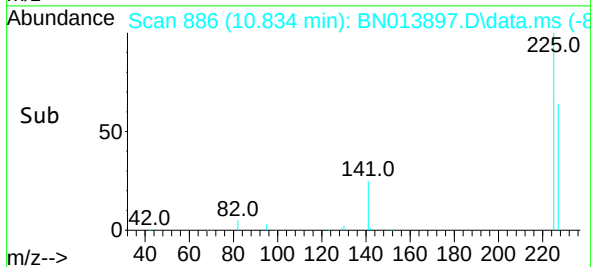

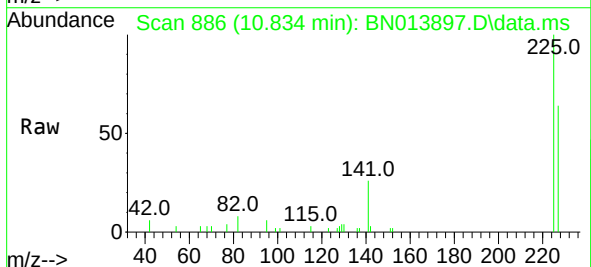




#11
2-Methylnaphthalene-d10
Concen: 0.39 ng
RT: 12.089 min Scan# 1070
Delta R.T. -0.004 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 14262
Ion Ratio Lower Upper
152 100
151 20.0 16.2 24.2

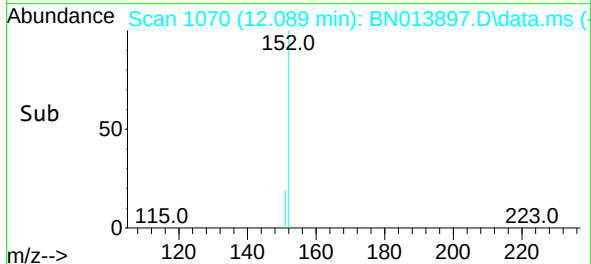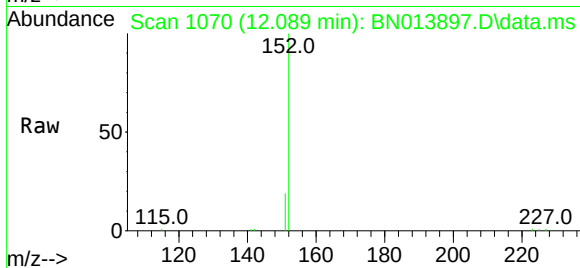

#12
2-Methylnaphthalene
Concen: 0.39 ng
RT: 12.160 min Scan# 1086
Delta R.T. -0.004 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Tgt Ion:142 Resp: 15258
Ion Ratio Lower Upper
142 100
141 89.5 70.5 105.7
115 36.1 27.4 41.0


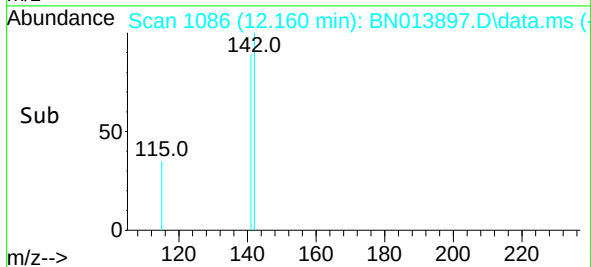

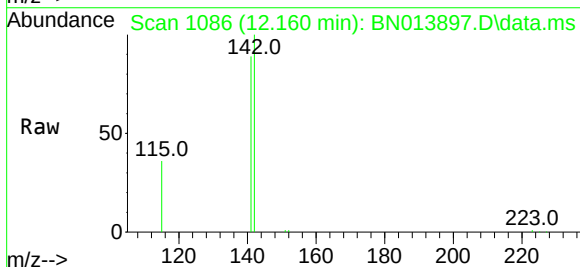




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.346 min Scan# 1309
Delta R.T. 0.000 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164 Resp: 11953
Ion Ratio Lower Upper
164 100
162 101.0 79.6 119.4
160 46.3 36.0 54.0

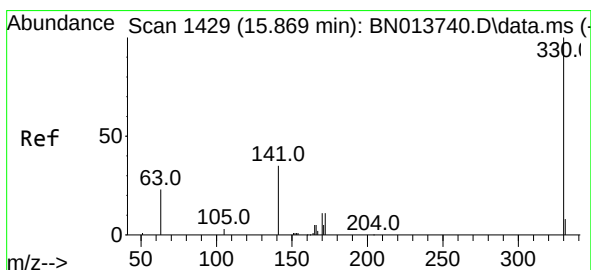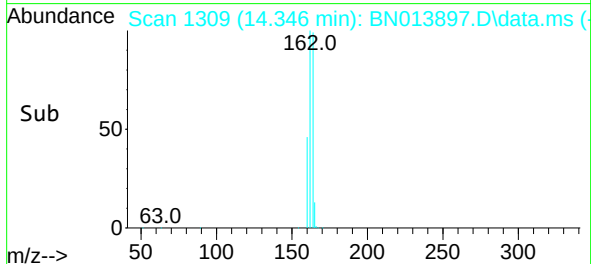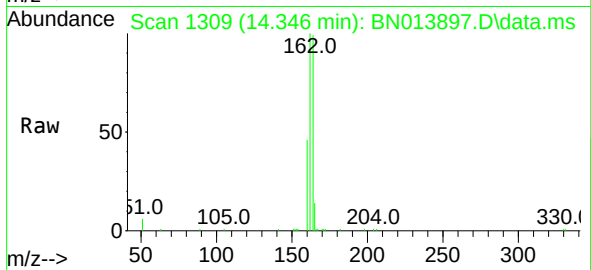

#14
2,4,6-Tribromophenol
Concen: 0.30 ng
RT: 15.831 min Scan# 1426
Delta R.T. -0.013 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Tgt Ion:330 Resp: 1450
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 35.7 26.8 40.2


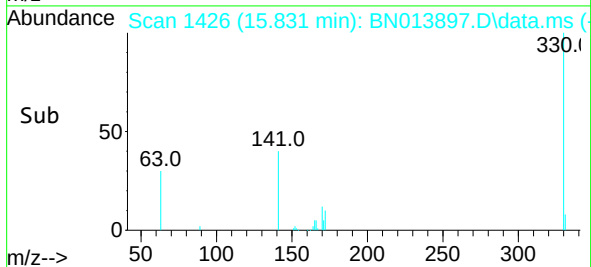

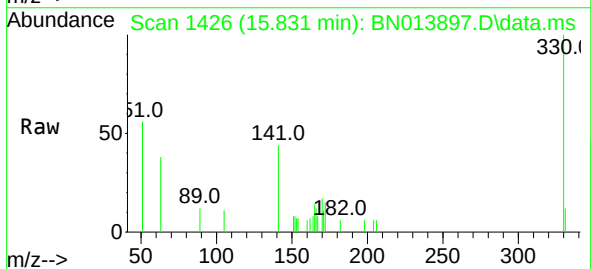


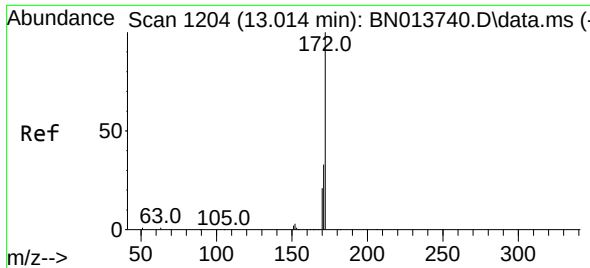

#15
2-Fluorobiphenyl
Concen: 0.44 ng
RT: 12.963 min Scan# 1200
Delta R.T. -0.013 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:172	Resp:	18801
Ion Ratio	Lower	Upper
172	100	
171	35.4	28.6 42.8
170	24.9	18.9 28.3

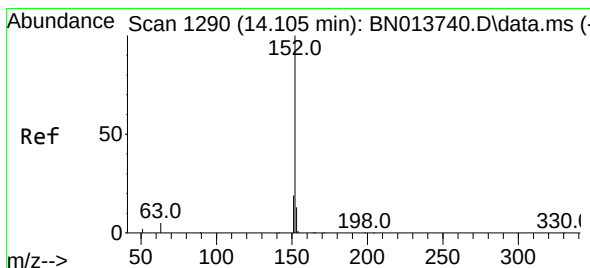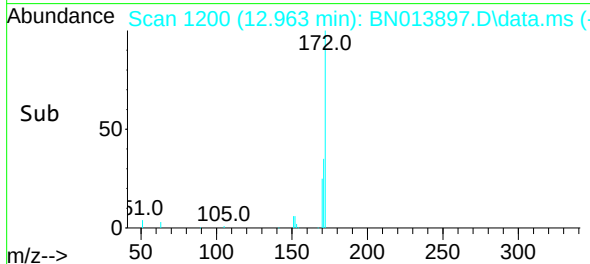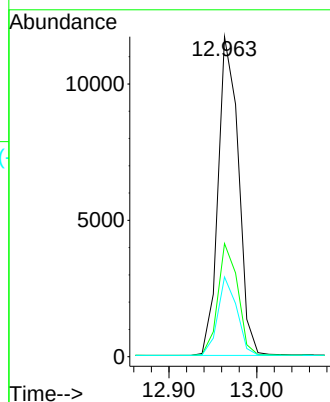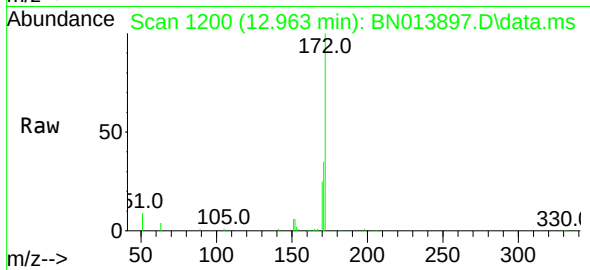

#16
Acenaphthylene
Concen: 0.35 ng
RT: 14.067 min Scan# 1287
Delta R.T. 0.000 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Tgt Ion:152	Resp:	18587
Ion Ratio	Lower	Upper
152	100	
151	19.3	15.7 23.5
153	12.9	10.5 15.7


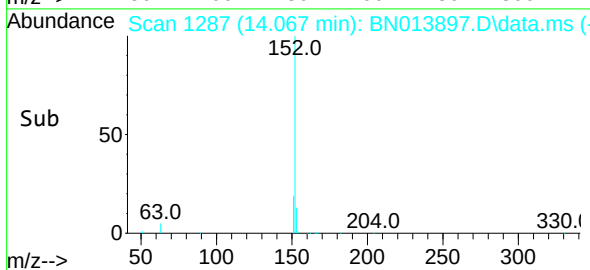
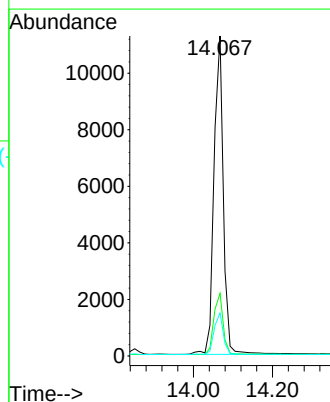
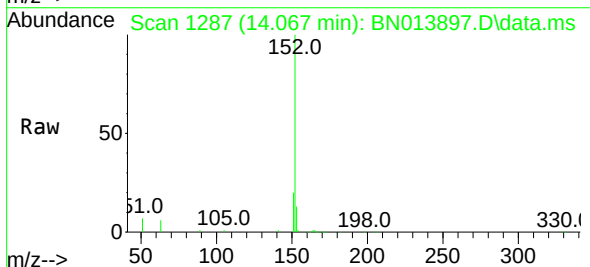


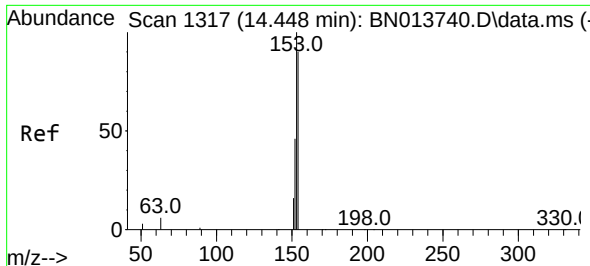

#17
Acenaphthene
Concen: 0.42 ng
RT: 14.410 min Scan# 1314
Delta R.T. 0.000 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 13839
Ion Ratio Lower Upper
154 100
153 111.1 88.4 132.6
152 54.9 43.0 64.4

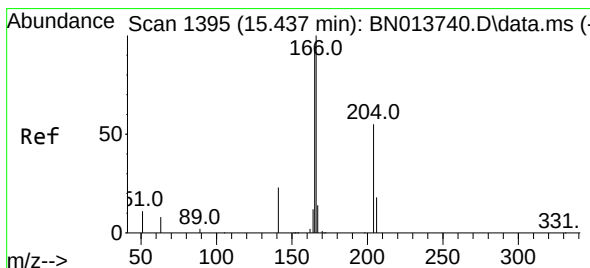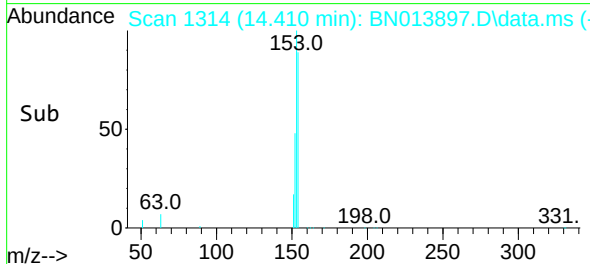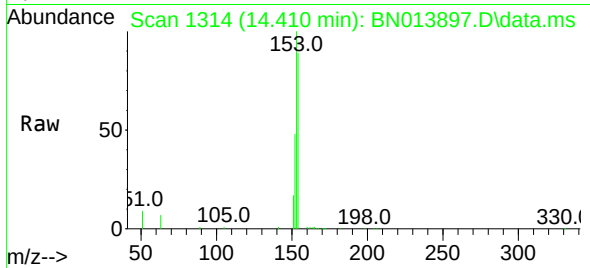

#18
Fluorene
Concen: 0.40 ng
RT: 15.399 min Scan# 1392
Delta R.T. 0.000 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Tgt Ion:166 Resp: 17033
Ion Ratio Lower Upper
166 100
165 97.9 77.8 116.8
167 13.5 10.6 16.0


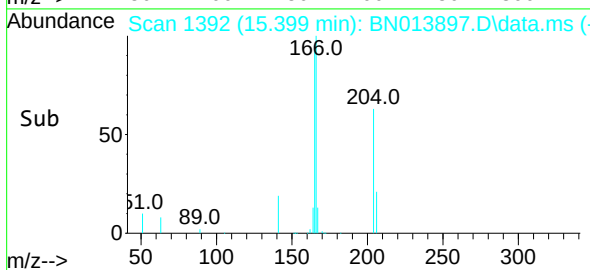

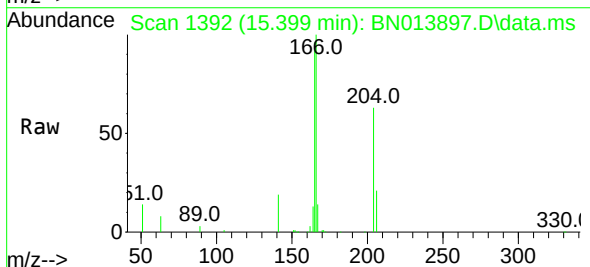


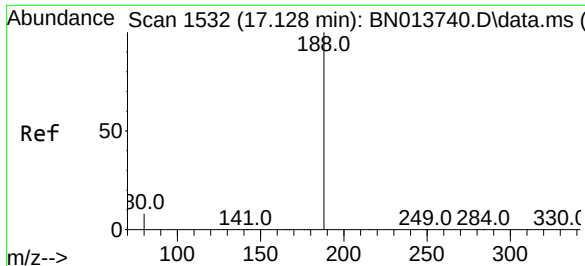

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.092 min Scan# 1529
Delta R.T. 0.001 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 25445
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.0 9.0 13.6#

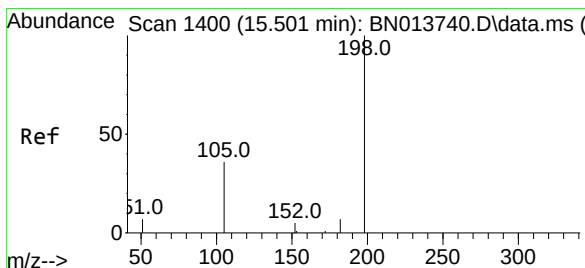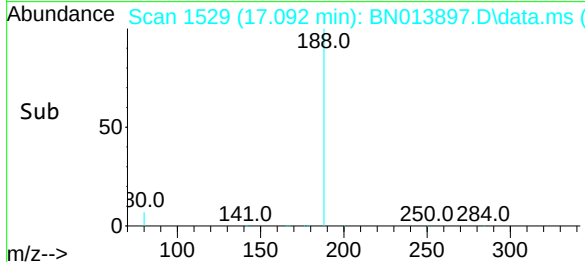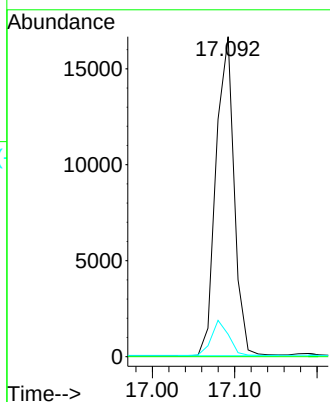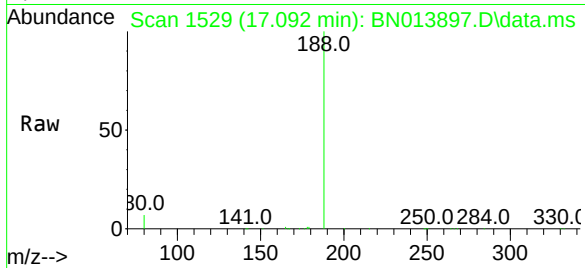

#20
4,6-Dinitro-2-methylphenol
Concen: 0.57 ng
RT: 15.475 min Scan# 1398
Delta R.T. 0.000 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Tgt Ion:198 Resp: 1009
Ion Ratio Lower Upper
198 100
51 98.5 61.7 92.5#
105 34.8 33.0 49.6


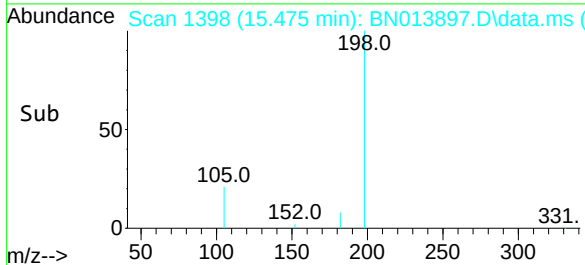
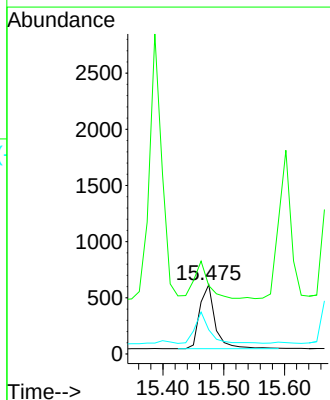
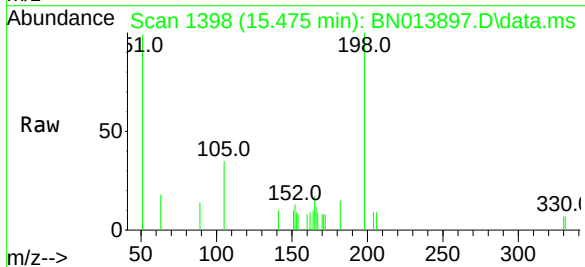


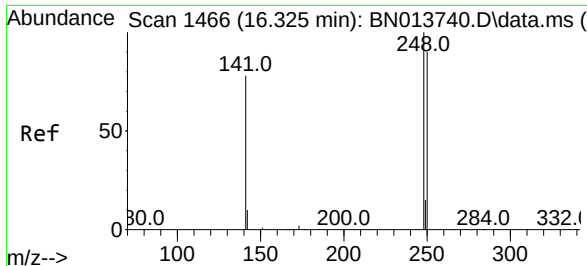

#21
4-Bromophenyl-phenylether
Concen: 0.40 ng
RT: 16.289 min Scan# 1463
Delta R.T. 0.001 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 5478
Ion Ratio Lower Upper
248 100
250 100.5 75.5 113.3
141 47.4 53.8 80.8#

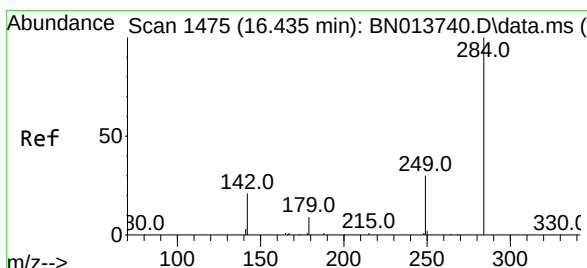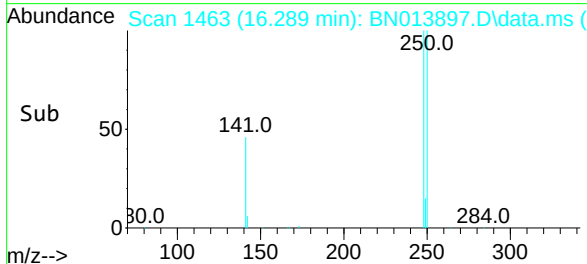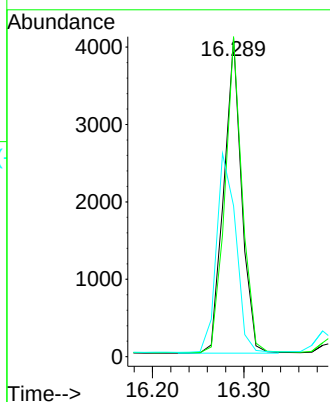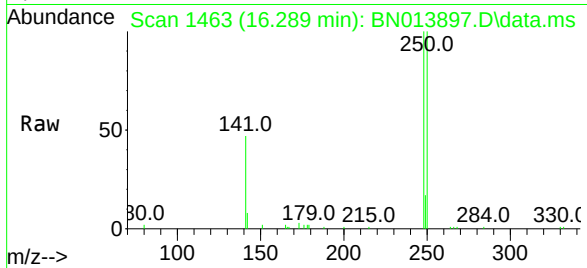

#22
Hexachlorobenzene
Concen: 0.45 ng
RT: 16.398 min Scan# 1472
Delta R.T. 0.001 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Tgt Ion:284 Resp: 6543
Ion Ratio Lower Upper
284 100
142 34.7 27.9 41.9
249 30.6 24.2 36.2

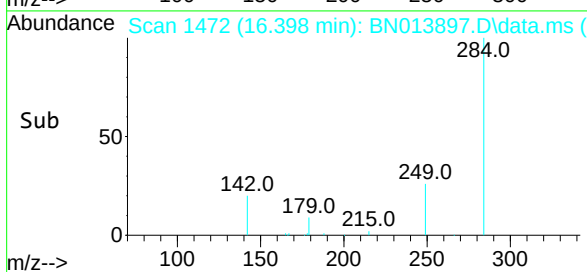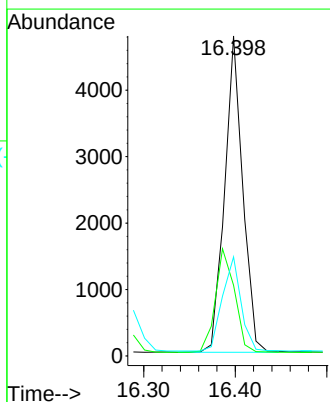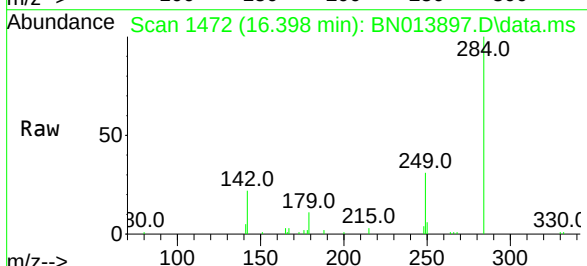

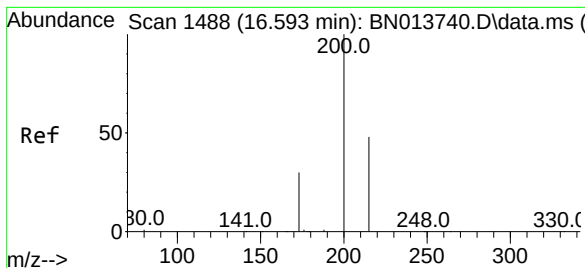

#23

Atrazine

Concen: 0.25 ng

RT: 16.556 min Scan# 1485

Delta R.T. 0.001 min

Lab File: BN013897.D

Acq: 10 Mar 2021 09:07





Tgt Ion:	200	Resp:	3256
Ion Ratio	Lower	Upper	
200	100		
173	24.0	18.6	28.0
215	51.7	41.0	61.6

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4

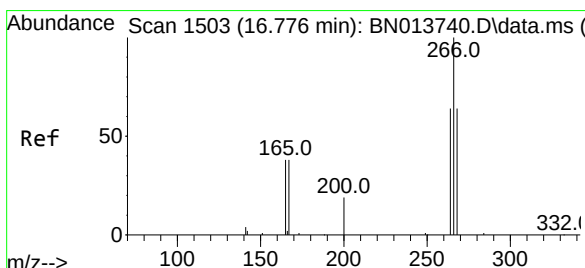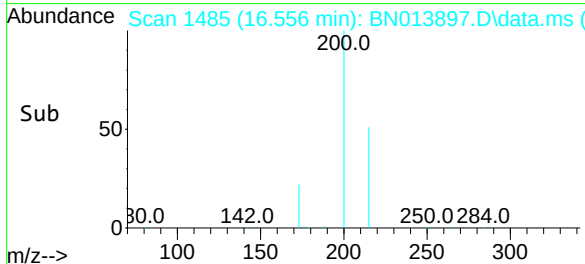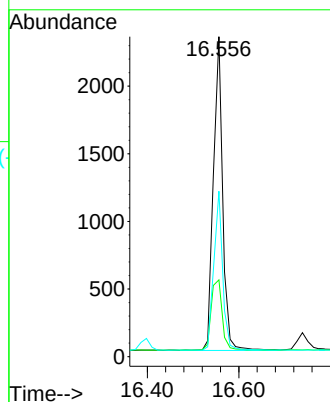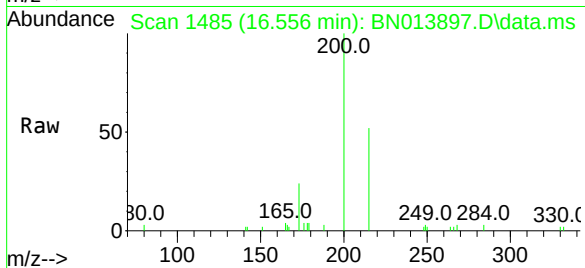

#24

Pentachlorophenol

Concen: 0.27 ng




RT: 16.739 min Scan# 1500


Delta R.T. 0.001 min

Lab File: BN013897.D

Acq: 10 Mar 2021 09:07

Tgt Ion:	266	Resp:	1264
Ion Ratio	Lower	Upper	
266	100		
264	62.0	51.6	77.4
268	65.2	54.6	82.0


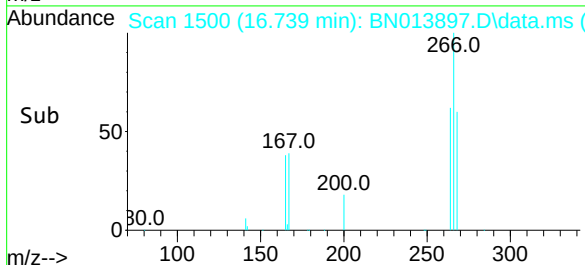
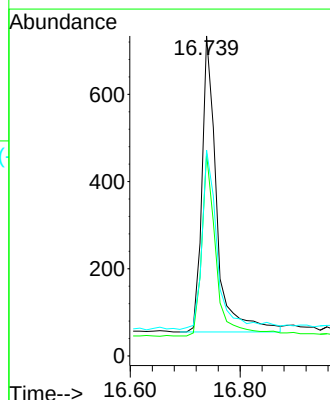
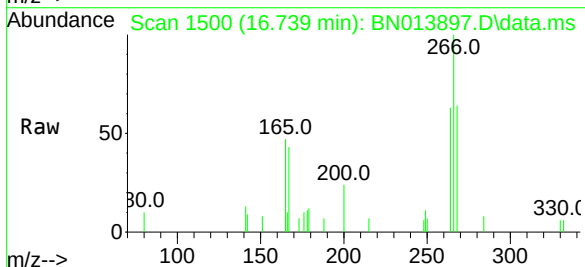


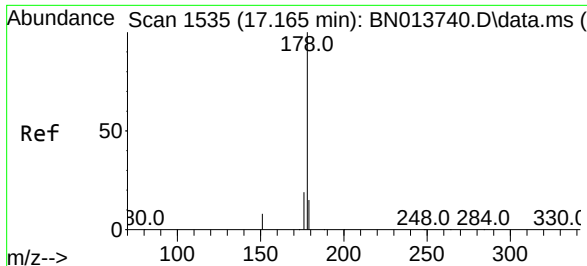

#25
Phenanthrene
Concen: 0.43 ng
RT: 17.128 min Scan# 1532
Delta R.T. 0.001 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:178 Resp: 28725
Ion Ratio Lower Upper
178 100
176 18.9 15.0 22.4
179 15.4 12.3 18.5

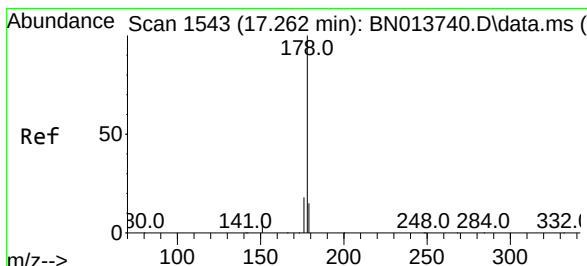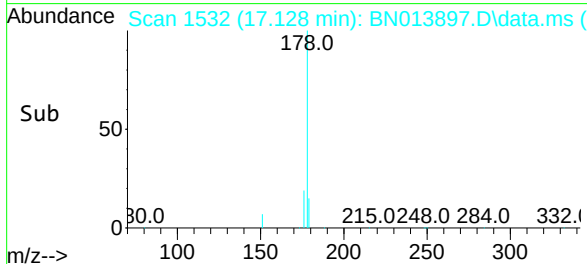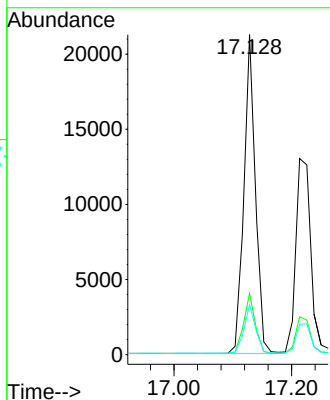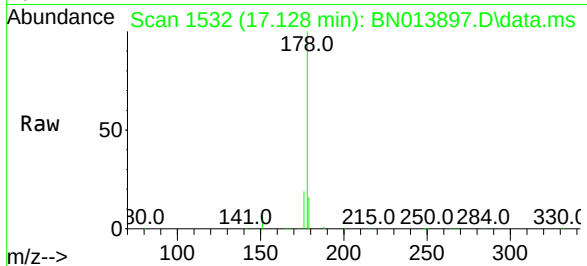

#26
Anthracene
Concen: 0.35 ng
RT: 17.214 min Scan# 1539
Delta R.T. -0.012 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Tgt Ion:178 Resp: 22917
Ion Ratio Lower Upper
178 100
176 18.5 14.6 21.8
179 15.3 12.2 18.2


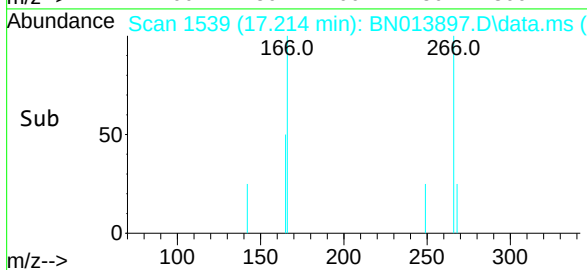
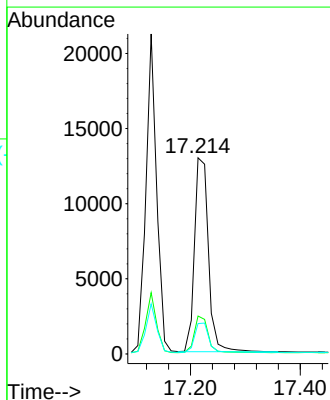
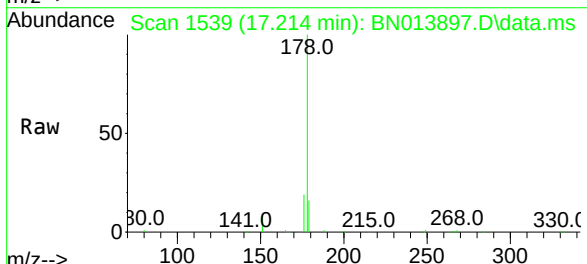


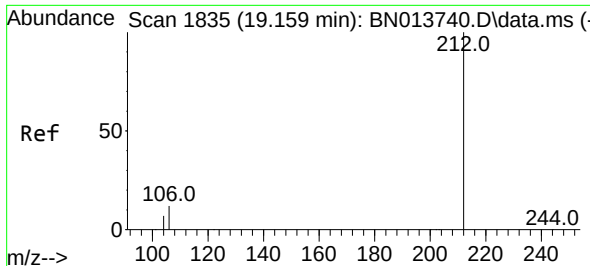

#27
Fluoranthene-d10
Concen: 0.38 ng
RT: 19.119 min Scan# 1827
Delta R.T. -0.002 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 28453
Ion Ratio Lower Upper
212 100
106 12.5 9.7 14.5
104 7.1 5.5 8.3

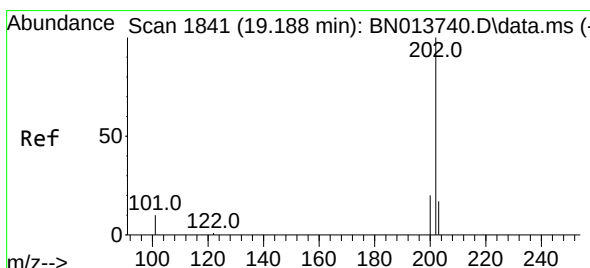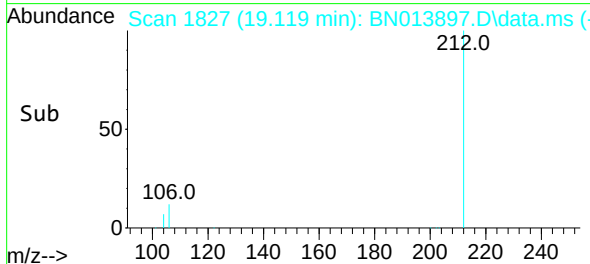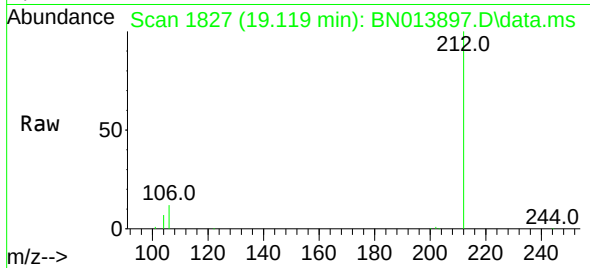

#28
Fluoranthene
Concen: 0.39 ng
RT: 19.149 min Scan# 1833
Delta R.T. -0.002 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Tgt Ion:202 Resp: 31222
Ion Ratio Lower Upper
202 100
101 10.9 8.1 12.1
203 17.3 13.9 20.9


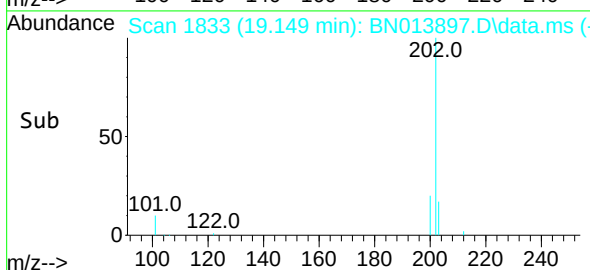

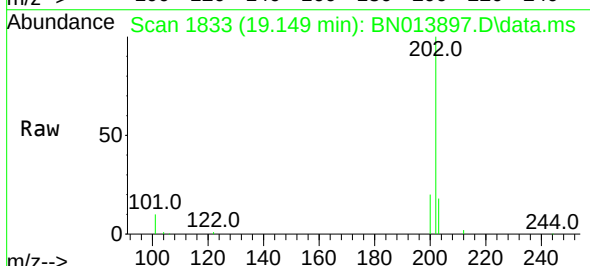


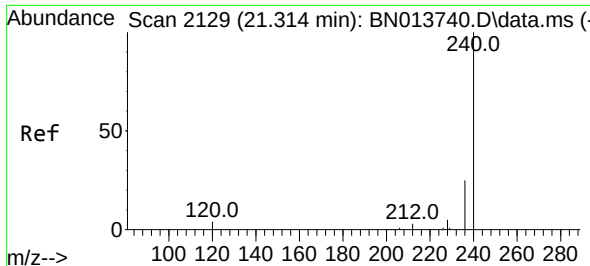

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.261 min Scan# 2124
Delta R.T. -0.008 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:240 Resp: 24779
Ion Ratio Lower Upper
240 100
120 11.8 10.2 15.4
236 26.9 21.3 31.9

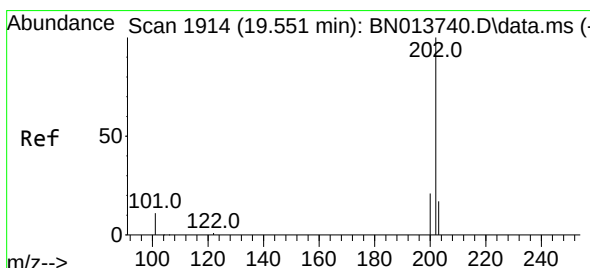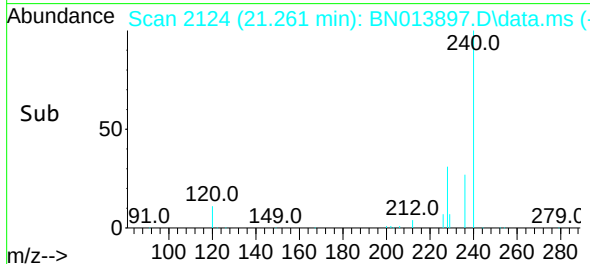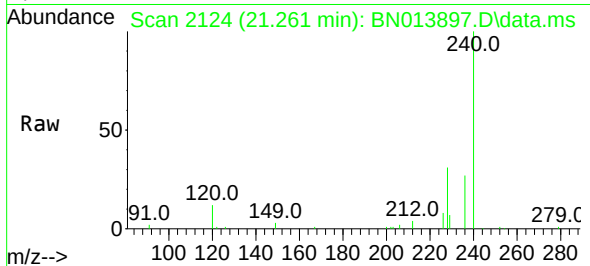

#30
Pyrene
Concen: 0.41 ng
RT: 19.511 min Scan# 1906
Delta R.T. -0.002 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Tgt Ion:202 Resp: 31335
Ion Ratio Lower Upper
202 100
200 20.4 16.3 24.5
203 17.4 14.0 21.0


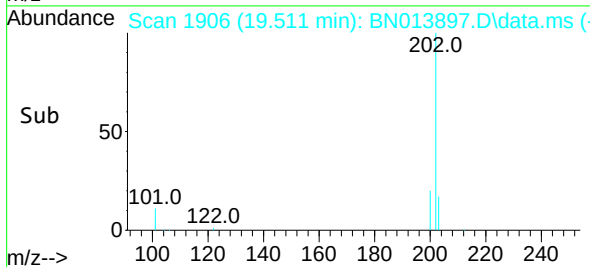

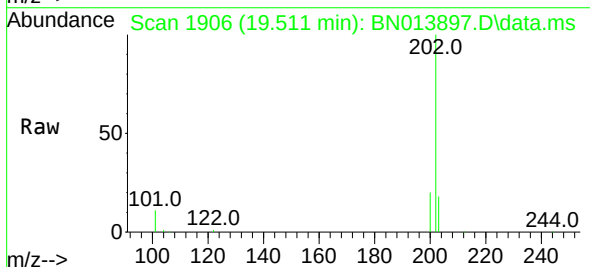




#31
 Terphenyl-d14
 Concen: 0.40 ng
 RT: 19.719 min Scan# 1948
 Delta R.T. -0.002 min
 Lab File: BN013897.D
 Acq: 10 Mar 2021 09:07




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:244 Resp: 22151
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.1 9.1
 122 10.7 9.8 14.8

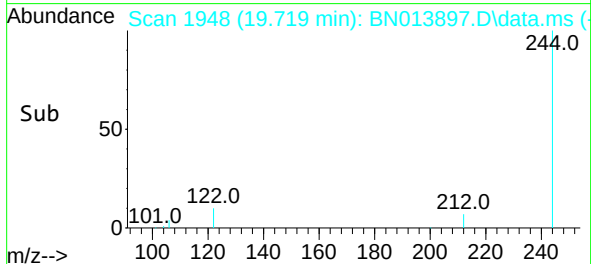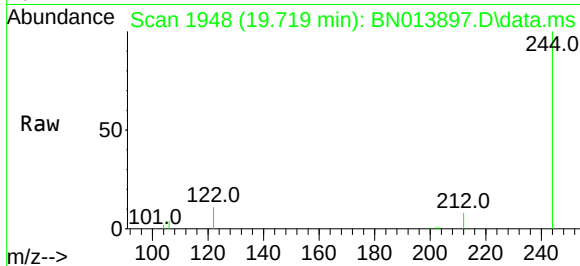

#32
 Benzo(a)anthracene
 Concen: 0.35 ng
 RT: 21.250 min Scan# 2123
 Delta R.T. 0.003 min
 Lab File: BN013897.D
 Acq: 10 Mar 2021 09:07

Tgt Ion:228 Resp: 26794
 Ion Ratio Lower Upper
 228 100
 226 26.1 20.5 30.7
 229 19.9 16.2 24.4

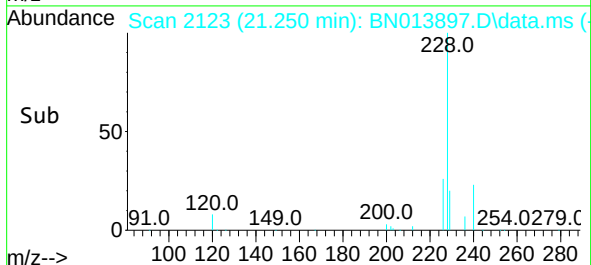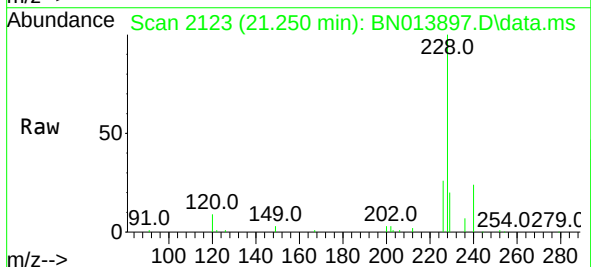

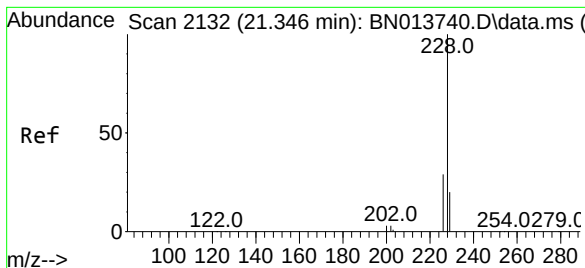

#33

Chrysene

Concen: 0.44 ng

RT: 21.303 min Scan# 2128

Delta R.T. 0.003 min

Lab File: BN013897.D

Acq: 10 Mar 2021 09:07





Tgt Ion:228 Resp: 32595

Ion Ratio Lower Upper

228 100

226 28.5 24.3 36.5

229 20.4 15.1 22.7

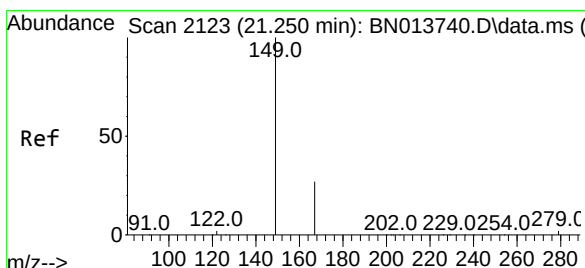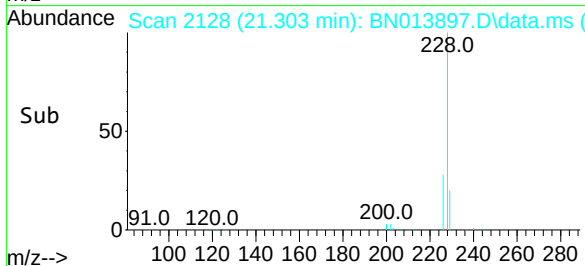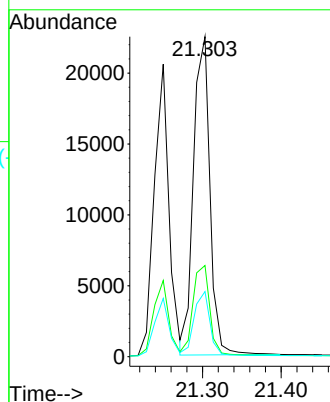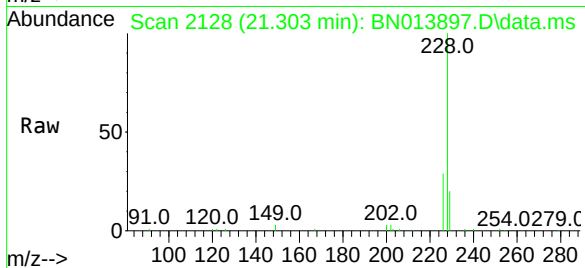

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.21 ng

RT: 21.186 min Scan# 2117

Delta R.T. -0.008 min

Lab File: BN013897.D

Acq: 10 Mar 2021 09:07




Tgt Ion:149 Resp: 7495


Ion Ratio Lower Upper

149 100

167 26.2 22.1 33.1


279 3.9 3.5 5.3

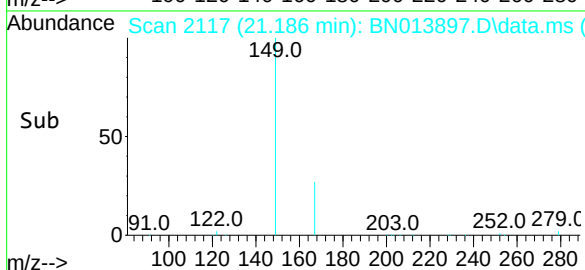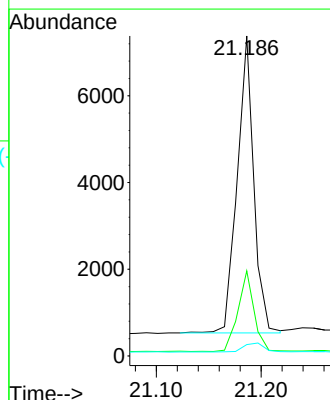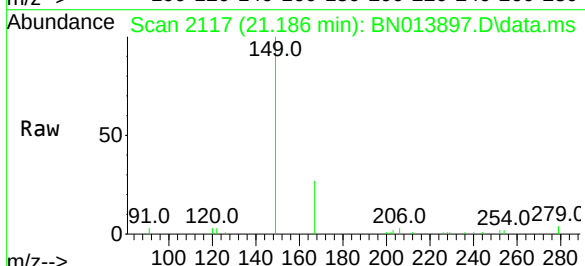






#35
Indeno(1,2,3-cd)pyrene
Concen: 0.40 ng
RT: 25.717 min Scan# 3199
Delta R.T. -0.011 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:276 Resp: 36015
Ion Ratio Lower Upper
276 100
138 22.7 19.8 29.6
277 24.8 19.9 29.9

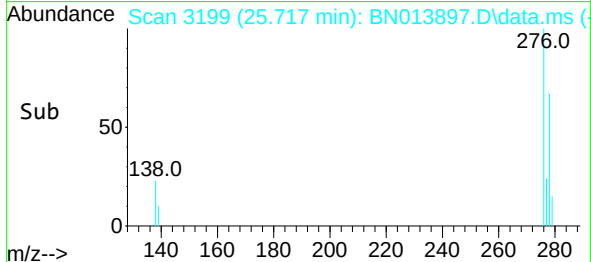

#36
Perylene-d12
Concen: 0.40 ng
RT: 23.486 min Scan# 2547
Delta R.T. -0.007 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Tgt Ion:264 Resp: 22130
Ion Ratio Lower Upper
264 100
260 24.6 19.3 28.9
265 35.2 66.2 99.4#


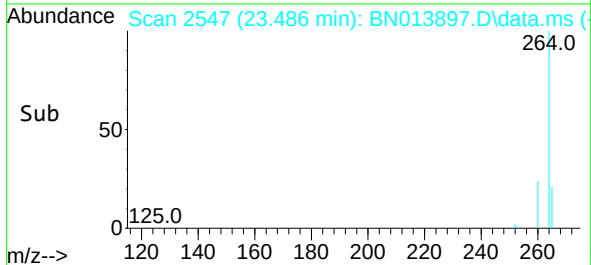

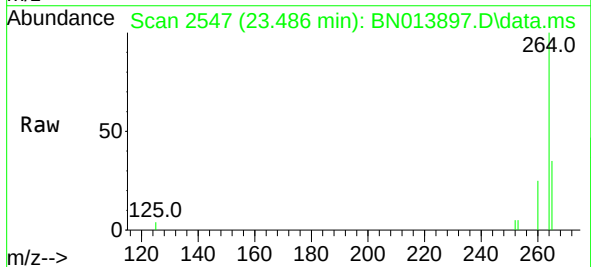




#37
Benzo(b)fluoranthene
Concen: 0.44 ng
RT: 22.818 min Scan# 2352
Delta R.T. -0.007 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252 Resp: 31242
Ion Ratio Lower Upper
252 100
253 23.7 20.4 30.6
125 12.0 11.6 17.4

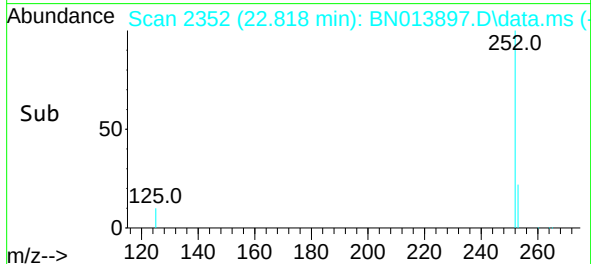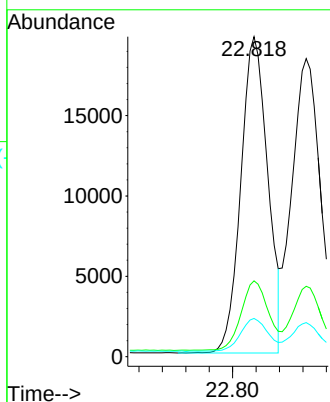

#38
Benzo(k)fluoranthene
Concen: 0.46 ng
RT: 22.863 min Scan# 2365
Delta R.T. -0.004 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Tgt Ion:252 Resp: 31225
Ion Ratio Lower Upper
252 100
253 23.6 20.5 30.7
125 11.4 12.3 18.5#

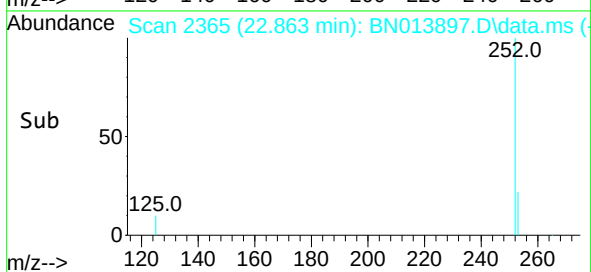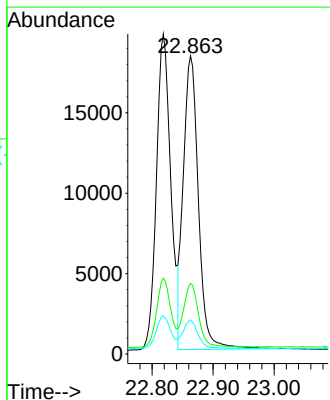



#39

Benzo(a)pyrene

Concen: 0.43 ng

RT: 23.390 min Scan# 2519





Delta R.T. -0.007 min

Lab File: BN013897.D

Acq: 10 Mar 2021 09:07

Tgt Ion:	252	Resp:	27174
Ion Ratio	Lower	Upper	
252	100		
253	24.9	21.8	32.6
125	15.1	14.6	21.8

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

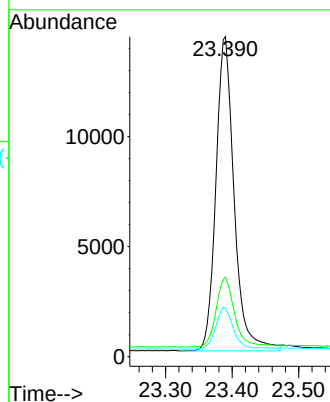

#40

Dibenzo(a,h)anthracene

Concen: 0.44 ng




RT: 25.728 min Scan# 3202


Delta R.T. -0.014 min

Lab File: BN013897.D

Acq: 10 Mar 2021 09:07

Tgt Ion:	278	Resp:	29912
Ion Ratio	Lower	Upper	
278	100		
139	16.4	13.1	19.7
279	24.9	21.4	32.0

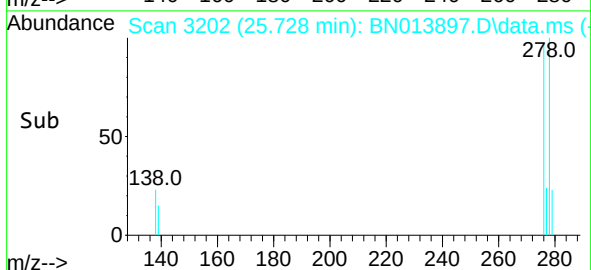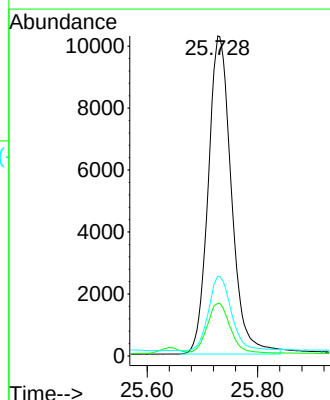

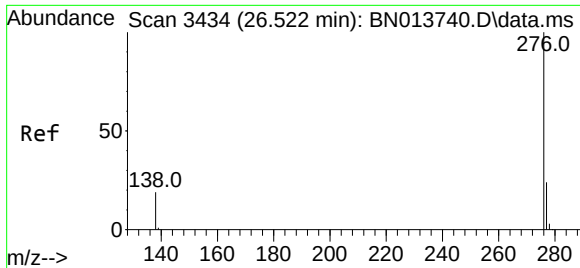

#41
Benzo(g,h,i)perylene
Concen: 0.46 ng
RT: 26.395 min Scan# 3397
Delta R.T. -0.014 min
Lab File: BN013897.D
Acq: 10 Mar 2021 09:07

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	276	Resp:	31291
Ion	Ratio	Lower	Upper
276	100		
277	24.1	20.0	30.0
138	20.8	17.8	26.8

