
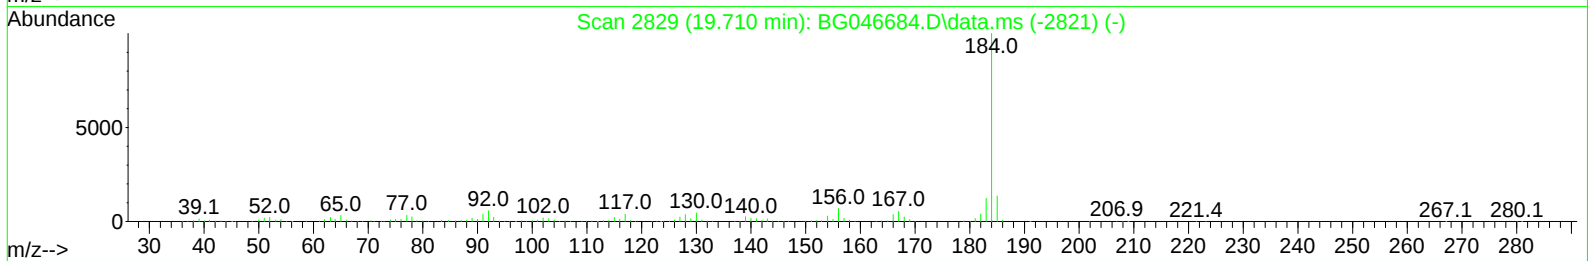
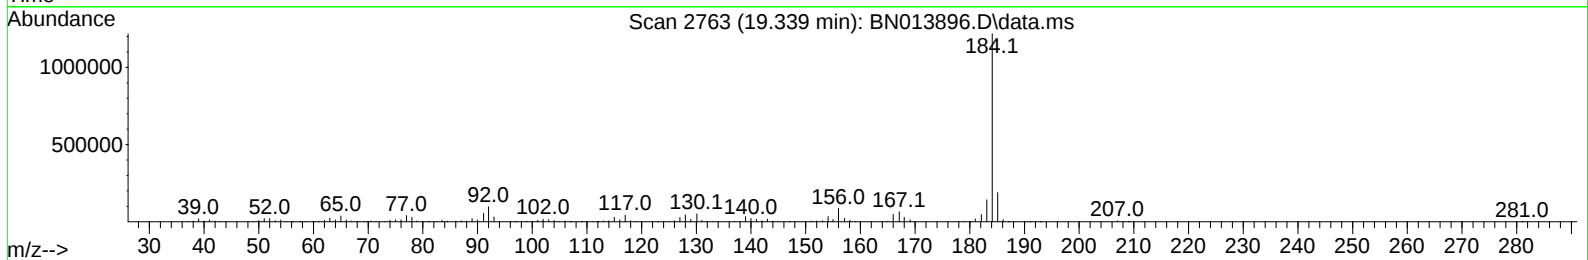


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031021\
Data File : BN013896.D
Acq On : 10 Mar 2021 08:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 09:50:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

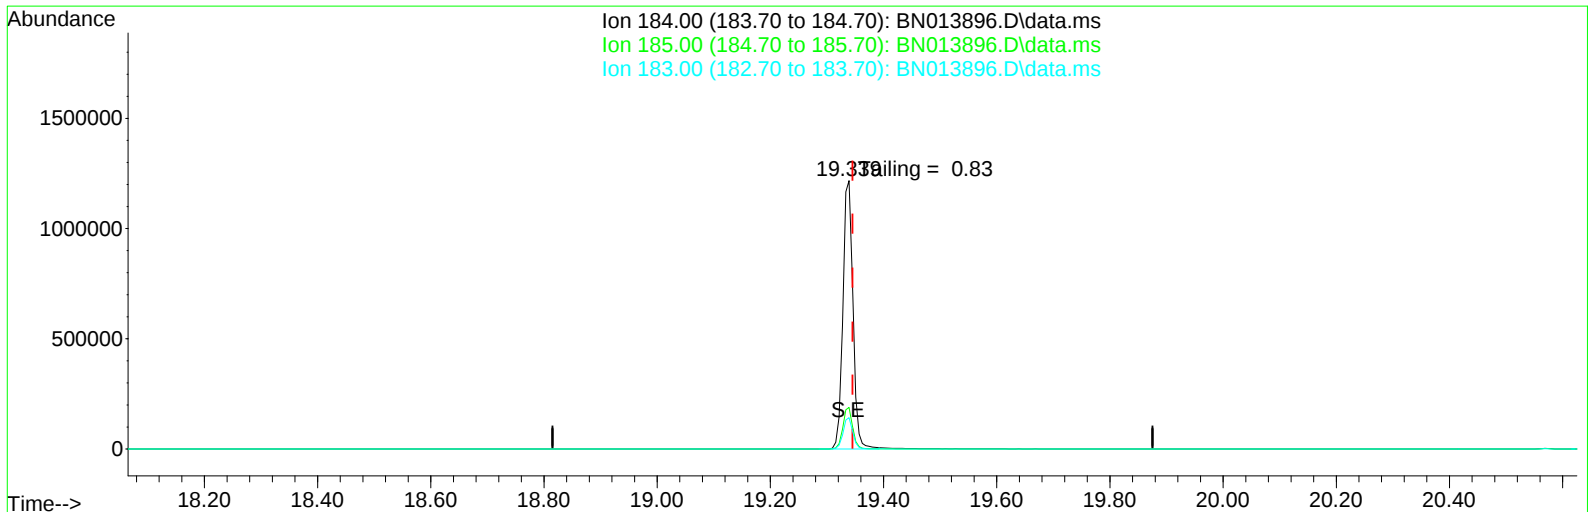




TIC: BN013896.D\data.ms

(77) Benzidine**19.339min (-0.006) 2171.13 ng****response 1508374**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.52
183.00	13.20	11.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031021\
Data File : BN013896.D
Acq On : 10 Mar 2021 08:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 09:50:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

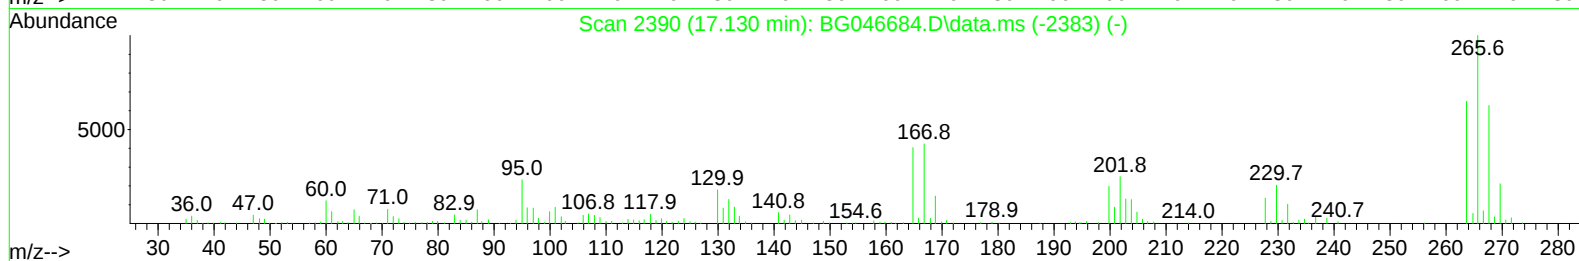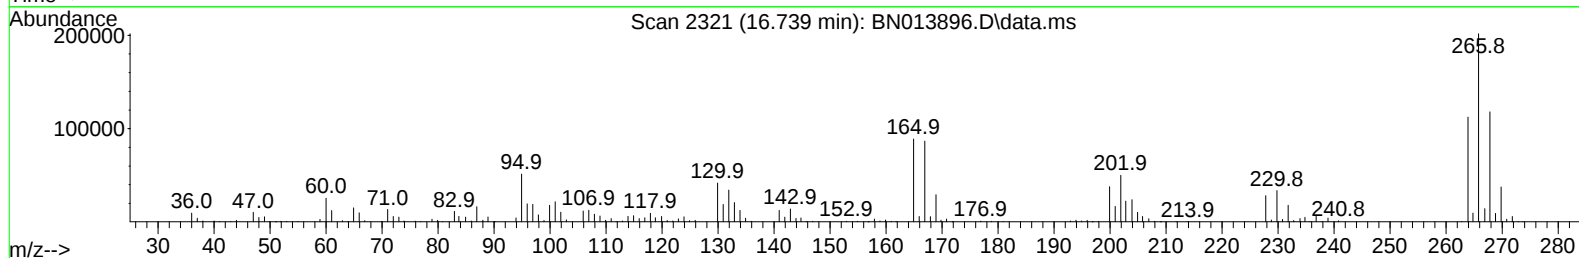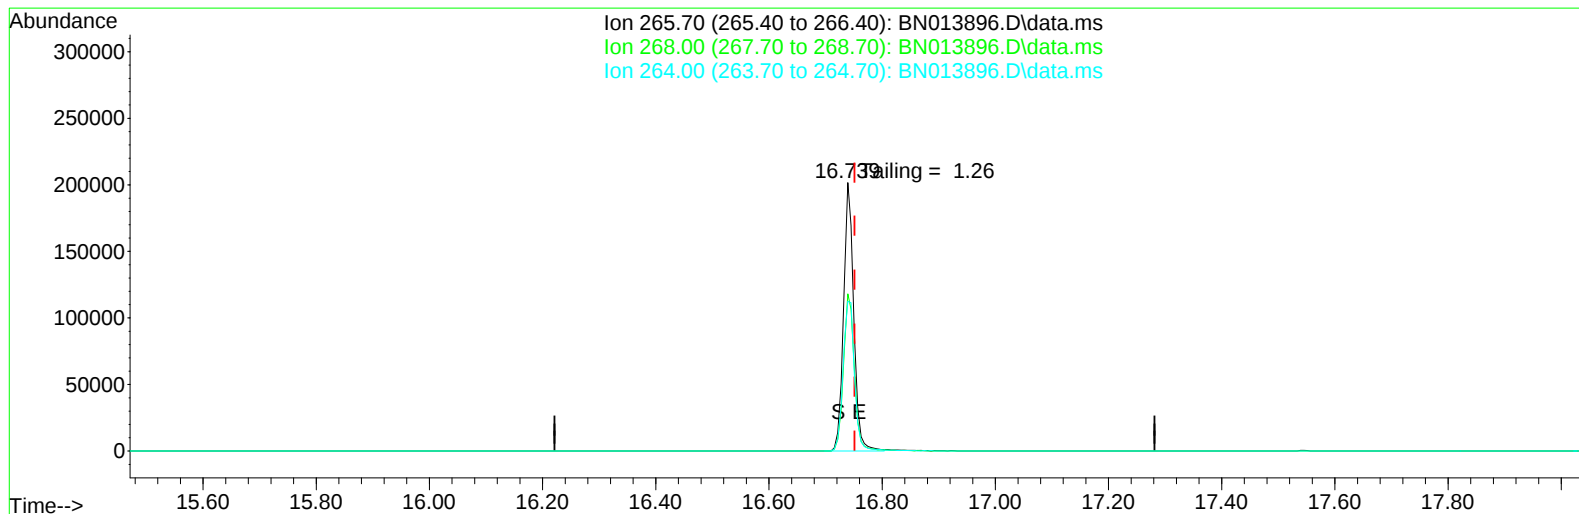

TIC: BN013896.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.012) 22662.12 ng

response 255032

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------

268.00	62.20	58.54
--------	-------	-------

264.00	61.60	55.75
--------	-------	-------

0.00 0.00 0.00