
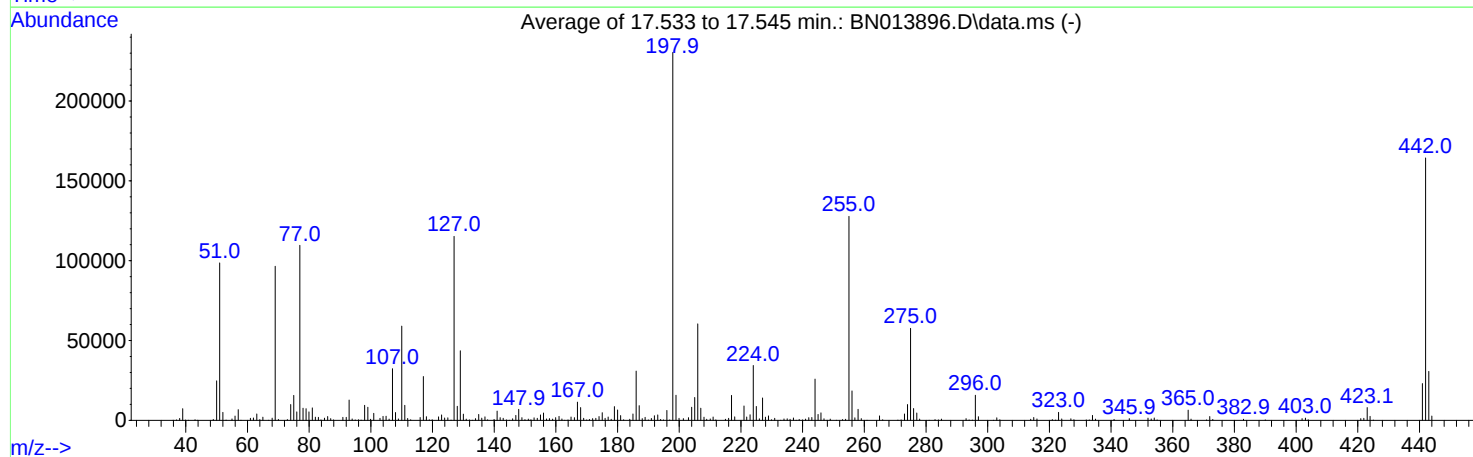


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031021\
 Data File : BN013896.D
 Acq On : 10 Mar 2021 08:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 08 10:32:09 2021

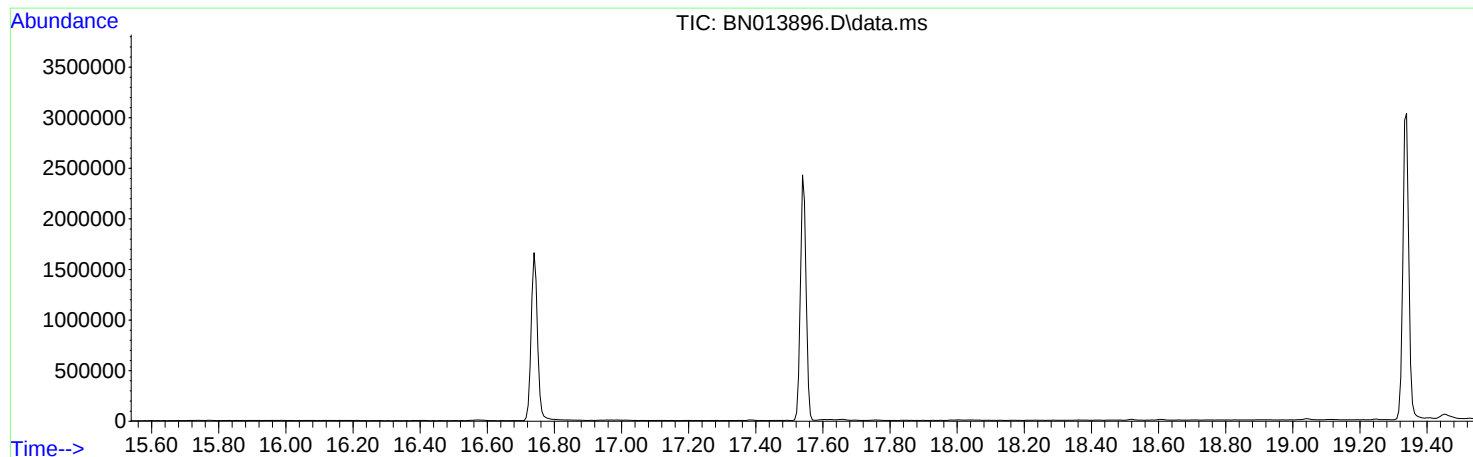




AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	98571	PASS
68	69	0.00	2	1.5	1433	PASS
69	198	0.00	100	41.9	96560	PASS
70	69	0.00	2	0.6	574	PASS
127	198	10	80	50.0	115256	PASS
197	198	0.00	2	0.1	325	PASS
198	198	100	100	100.0	230400	PASS
199	198	5	9	6.8	15701	PASS
275	198	10	60	25.0	57635	PASS
365	198	1	100	2.8	6457	PASS
441	198	0.01	100	10.0	23074	PASS
442	442	50	100	100.0	164405	PASS
443	442	15	24	18.7	30711	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031021\
 Data File : BN013896.D
 Acq On : 10 Mar 2021 08:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 10 09:50:30 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 05 13:12:06 2021
 Response via : Initial Calibration

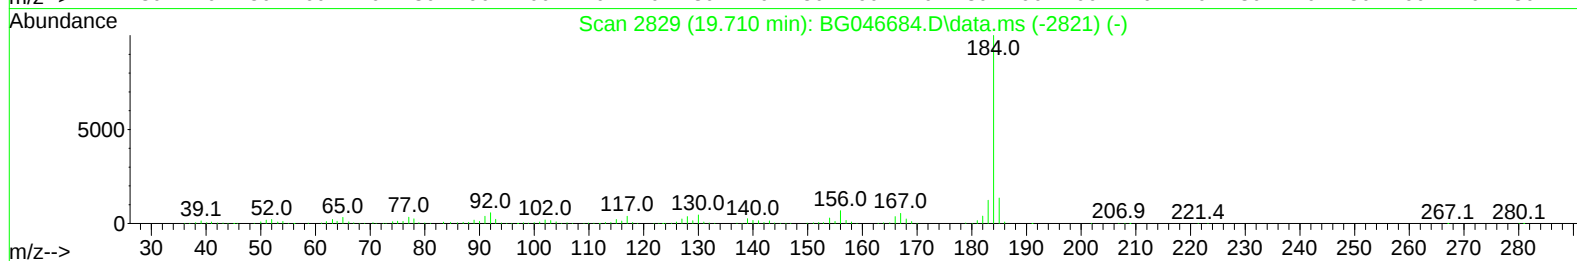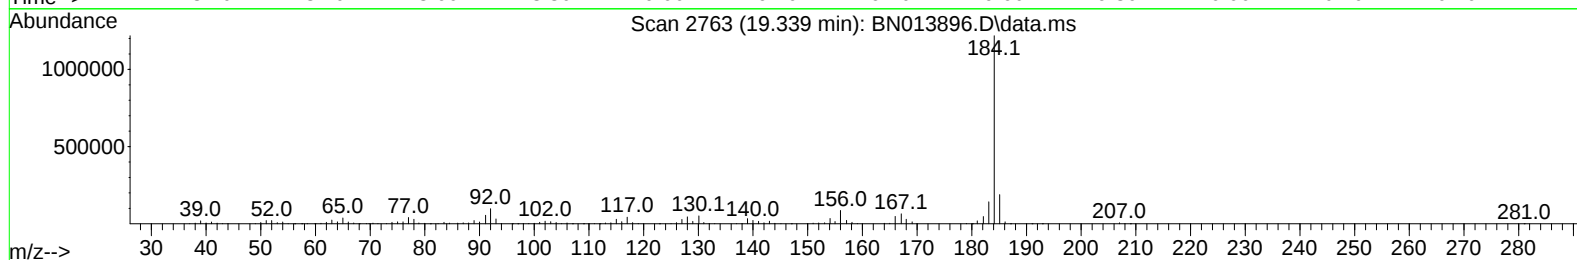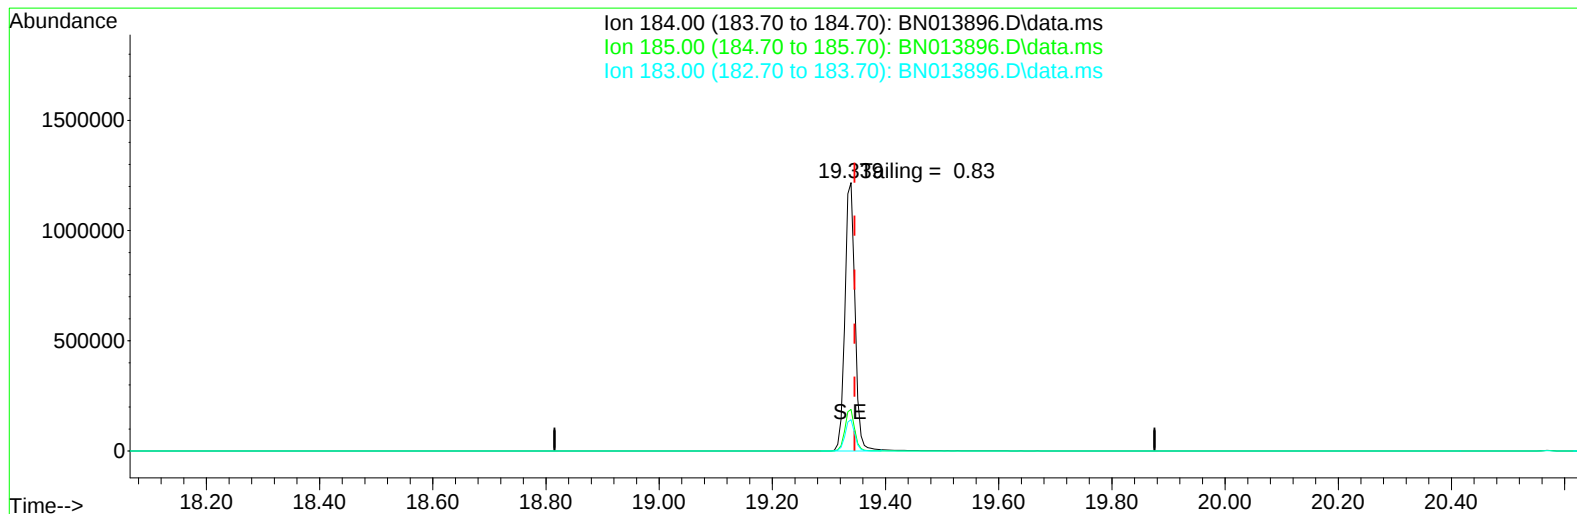

TIC: BN013896.D\data.ms

(77) Benzidine

19.339min (-0.006) 2171.13 ng




response 1508374

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.52
183.00	13.20	11.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031021\
Data File : BN013896.D
Acq On : 10 Mar 2021 08:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 10 09:50:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

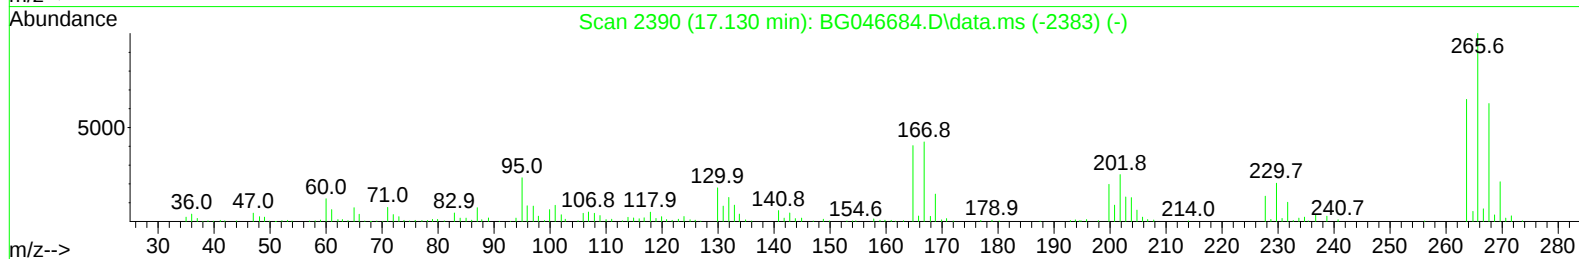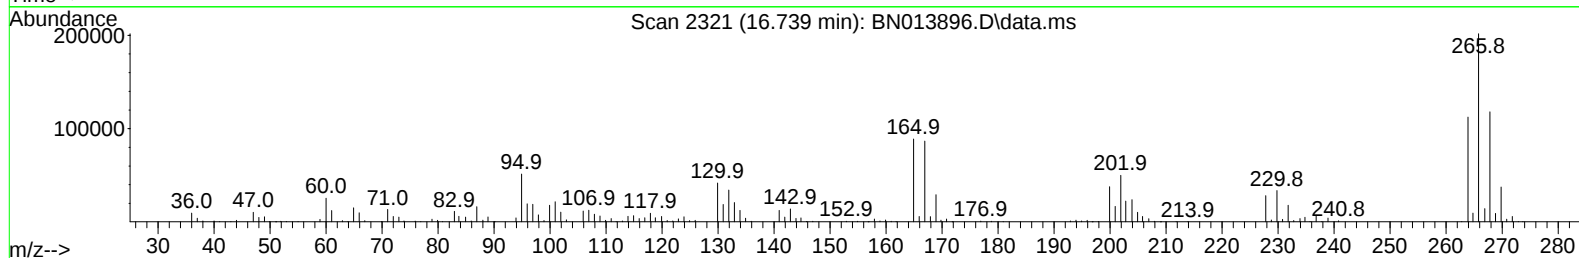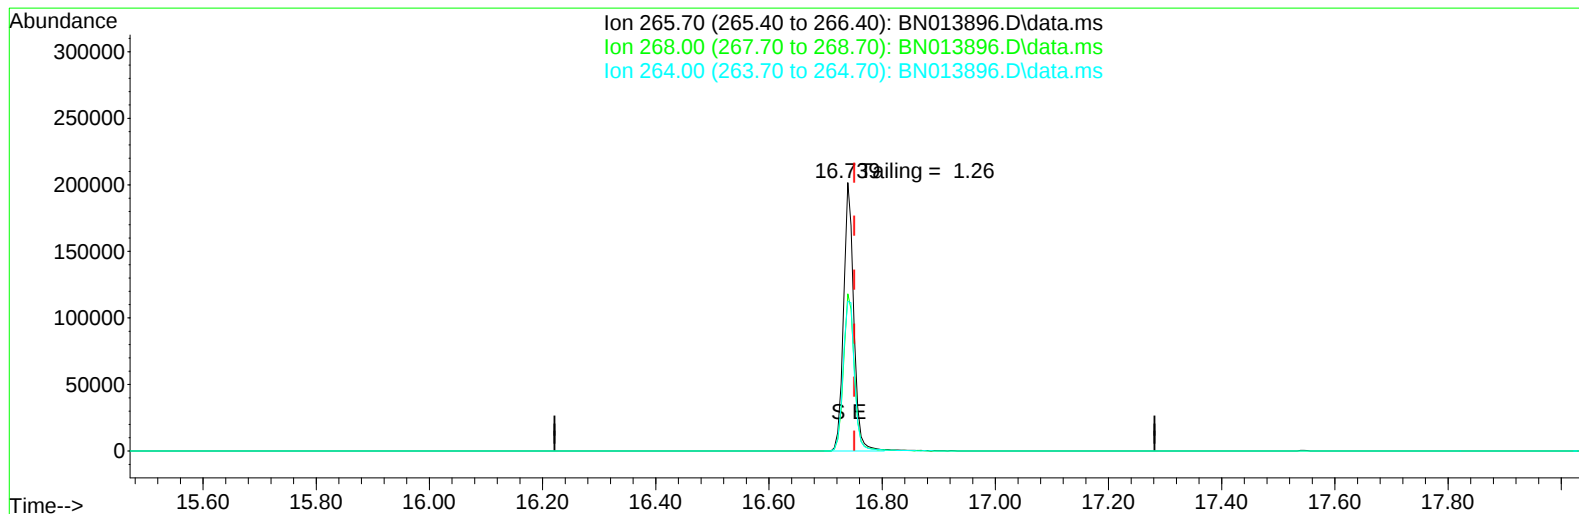

TIC: BN013896.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.012) 22662.12 ng

response 255032

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.54
264.00	61.60	55.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/10/2021	BNA_N	<u>BN013896.D</u>
Compound Name	Response	Retention Time
DDT	810144	20.57
DDD	4316	20.13
DDE	1360	19.62
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5676	815820	0.70