

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031022\
 Data File : BN018897.D
 Acq On : 10 Mar 2022 10:41
 Operator : CG/JU
 Sample : PB142853BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK853

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018897.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	44	48	56	rBV	37161	56820	0.90%	0.102%
2	3.687	115	119	147	rBV	529872	1017238	16.10%	1.828%
3	4.040	175	179	185	rVB2	10722	17086	0.27%	0.031%
4	7.052	684	691	703	rVB	779573	1246656	19.73%	2.241%
5	7.222	714	720	730	rVB	629236	996561	15.77%	1.791%
6	7.428	748	755	767	rBV	769757	1223097	19.36%	2.198%
7	7.899	828	835	844	rBV	620856	998078	15.80%	1.794%
8	8.604	948	955	965	rBV	962325	1567789	24.81%	2.818%
9	9.057	1024	1032	1040	rBV	771817	1237906	19.59%	2.225%
10	9.781	1149	1155	1164	rBV	618961	1018341	16.12%	1.830%
11	10.322	1240	1247	1257	rBV	979983	1596491	25.27%	2.869%
12	10.704	1304	1312	1322	rBV	962359	1617746	25.60%	2.907%
13	10.834	1327	1334	1351	rBV	1026609	1726576	27.33%	3.103%
14	12.298	1577	1583	1589	rBV	17631	29125	0.46%	0.052%
15	13.940	1855	1862	1868	rBV	1958095	2592185	41.02%	4.659%
16	14.228	1904	1911	1925	rBV	2135611	3080984	48.76%	5.537%
17	14.534	1957	1963	1974	rBV	1599652	2327504	36.84%	4.183%
18	14.710	1986	1993	2012	rBV	931803	1295522	20.50%	2.328%
19	15.528	2124	2132	2143	rBV	2628008	3880619	61.42%	6.974%
20	15.634	2144	2150	2162	rVV	886149	1177967	18.64%	2.117%
21	15.763	2166	2172	2177	rVB3	13110	18897	0.30%	0.034%
22	17.057	2385	2392	2399	rBV3	8461	19198	0.30%	0.035%
23	17.275	2422	2429	2437	rBV	2020585	2872527	45.46%	5.163%
24	17.375	2439	2446	2456	rBV	2908238	4373924	69.22%	7.861%
25	18.798	2681	2688	2692	rBV6	4113	7484	0.12%	0.013%
26	19.227	2757	2761	2766	rBV2	39883	53818	0.85%	0.097%
27	19.298	2768	2773	2779	rVV	38123	52776	0.84%	0.095%
28	19.592	2819	2823	2828	rBV4	7839	11348	0.18%	0.020%
29	19.663	2829	2835	2849	rVV	3982430	5456904	86.36%	9.807%
30	20.280	2938	2940	2945	rVB4	8629	9789	0.15%	0.018%
31	20.657	2998	3004	3011	rBV3	23305	36584	0.58%	0.066%
32	20.910	3045	3047	3051	rVB3	17636	19446	0.31%	0.035%
33	21.445	3133	3138	3150	rBV	2740431	3533383	55.92%	6.350%
34	23.110	3417	3421	3426	rVB2	47905	70847	1.12%	0.127%
35	23.686	3510	3519	3535	rBV2	3116839	6318573	100.00%	11.356%
36	23.839	3537	3545	3557	rVB2	1910887	3802716	60.18%	6.834%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031022\
Data File : BN018897.D
Acq On : 10 Mar 2022 10:41
Operator : CG/JU
Sample : PB142853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK853

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Title : SVOA CALIBRATION

37	24.451	3646	3649	3658	rVB	62263	113790	1.80%	0.205%
38	25.286	3787	3791	3803	rVB3	71668	164644	2.61%	0.296%




Sum of corrected areas: 55640939

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031022\
Data File : BN018897.D
Acq On : 10 Mar 2022 10:41
Operator : CG/JU
Sample : PB142853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK853

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

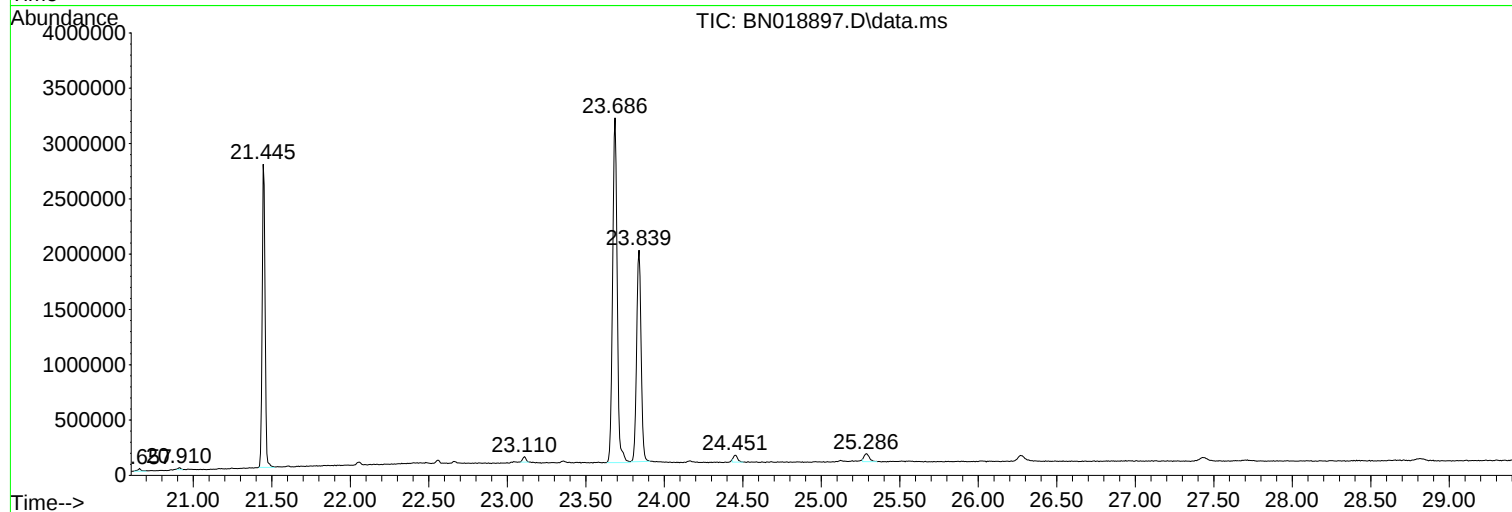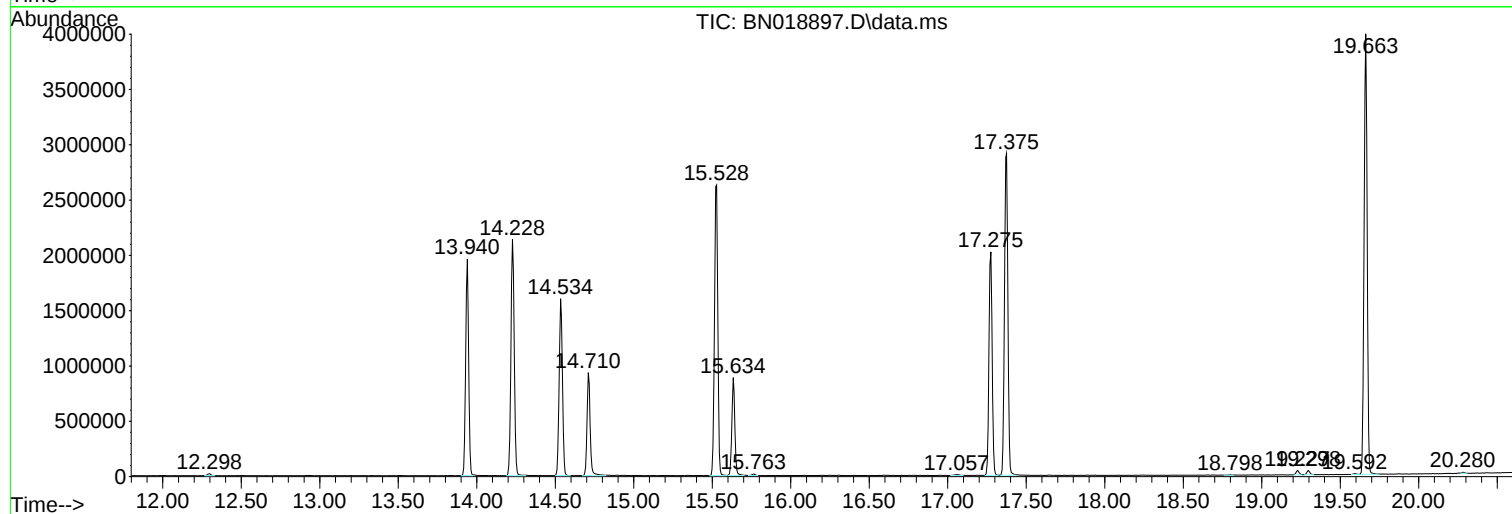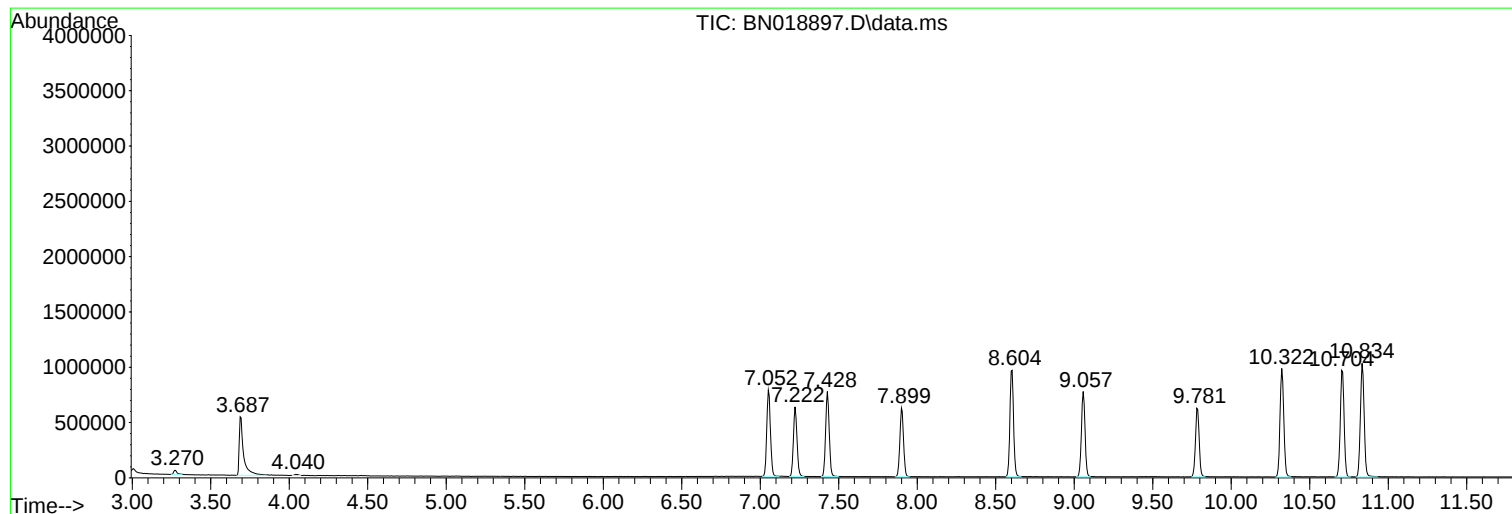

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031022\
Data File : BN018897.D
Acq On : 10 Mar 2022 10:41
Operator : CG/JU
Sample : PB142853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK853

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031022\
Data File : BN018897.D
Acq On : 10 Mar 2022 10:41
Operator : CG/JU
Sample : PB142853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK853

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc