

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031022\
 Data File : BN018899.D
 Acq On : 10 Mar 2022 12:09
 Operator : CG/JU
 Sample : PB142784BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK784

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018899.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	44	48	54	rBV	33055	44095	0.90%	0.101%
2	3.687	115	119	140	rBV	456917	768529	15.63%	1.769%
3	4.040	176	179	184	rVB2	9125	12505	0.25%	0.029%
4	7.051	684	691	704	rBV	616800	943992	19.20%	2.173%
5	7.222	713	720	729	rBV	487123	771306	15.68%	1.775%
6	7.428	748	755	766	rBV	585974	925451	18.82%	2.130%
7	7.899	829	835	845	rBV	471315	758253	15.42%	1.745%
8	8.598	948	954	964	rBV	728365	1182328	24.04%	2.721%
9	9.057	1025	1032	1043	rBV	579533	922100	18.75%	2.122%
10	9.787	1147	1156	1165	rBV	450718	756968	15.39%	1.742%
11	10.322	1240	1247	1262	rBV	724371	1190362	24.21%	2.740%
12	10.710	1305	1313	1321	rBV	726653	1231319	25.04%	2.834%
13	10.834	1327	1334	1351	rBV	770452	1306075	26.56%	3.006%
14	12.298	1577	1583	1591	rVB2	12045	21300	0.43%	0.049%
15	13.510	1785	1789	1792	rBV5	3242	5187	0.11%	0.012%
16	13.939	1856	1862	1874	rBV	1497524	1970564	40.07%	4.536%
17	14.228	1904	1911	1922	rBV	1589394	2314379	47.06%	5.327%
18	14.539	1956	1964	1974	rBV	1238774	1799101	36.58%	4.141%
19	14.716	1987	1994	2015	rBV	659830	942548	19.17%	2.170%
20	15.528	2125	2132	2144	rBV	2016564	3021545	61.44%	6.955%
21	15.633	2144	2150	2165	rVV	604743	866610	17.62%	1.995%
22	15.769	2169	2173	2176	rVB	10537	13799	0.28%	0.032%
23	16.245	2250	2254	2259	rBV5	3555	5549	0.11%	0.013%
24	16.304	2262	2264	2269	rVB4	3995	5195	0.11%	0.012%
25	16.604	2308	2315	2320	rBV8	3450	9407	0.19%	0.022%
26	17.039	2385	2389	2390	rBV4	6086	6540	0.13%	0.015%
27	17.274	2422	2429	2439	rBV	1600915	2247749	45.71%	5.174%
28	17.374	2439	2446	2459	rVV2	2400941	3421659	69.58%	7.876%
29	19.233	2757	2762	2767	rBV	27579	37896	0.77%	0.087%
30	19.304	2769	2774	2777	rVV	28131	35792	0.73%	0.082%
31	19.598	2819	2824	2828	rBV6	6644	11317	0.23%	0.026%
32	19.663	2829	2835	2847	rVV	3069867	4284679	87.13%	9.862%
33	20.663	2999	3005	3009	rBV3	28518	40745	0.83%	0.094%
34	20.921	3046	3049	3054	rVB6	11287	16505	0.34%	0.038%
35	21.457	3134	3140	3145	rBV	2138102	2777424	56.48%	6.393%
36	22.568	3325	3329	3333	rVB2	44491	60549	1.23%	0.139%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031022\
Data File : BN018899.D
Acq On : 10 Mar 2022 12:09
Operator : CG/JU
Sample : PB142784BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK784

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Title : SVOA CALIBRATION

37	23.121	3419	3423	3432	rVB3	88200	141948	2.89%	0.327%
38	23.692	3512	3520	3527	rBV2	2411967	4917671	100.00%	11.319%
39	23.845	3539	3546	3558	rVB2	1495048	2975274	60.50%	6.848%
40	24.462	3646	3651	3658	rVB2	105826	206346	4.20%	0.475%
41	25.303	3788	3794	3802	rVB2	102358	242409	4.93%	0.558%
42	26.286	3956	3961	3973	rVB5	83754	231409	4.71%	0.533%




Sum of corrected areas: 43444379

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031022\
Data File : BN018899.D
Acq On : 10 Mar 2022 12:09
Operator : CG/JU
Sample : PB142784BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK784

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

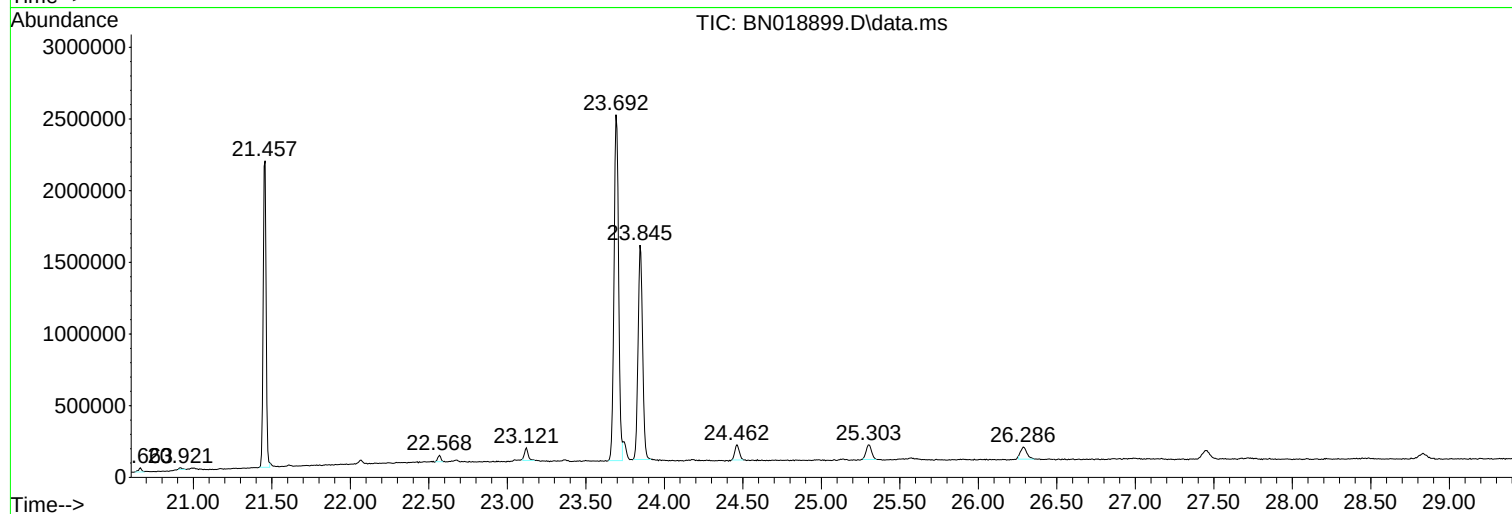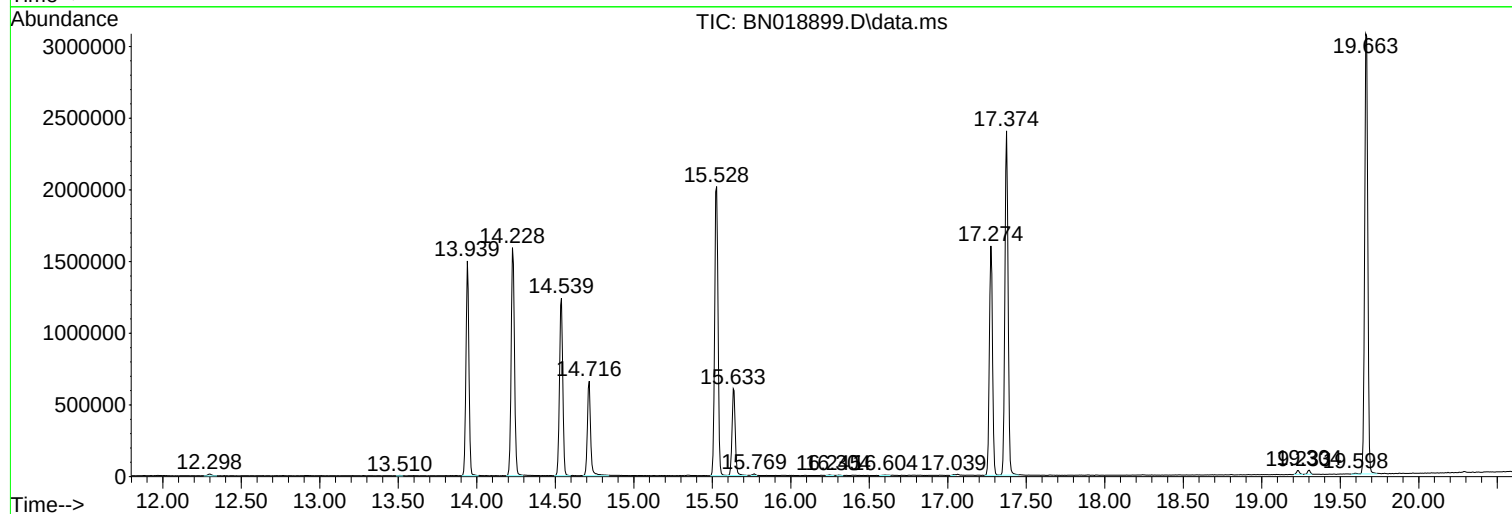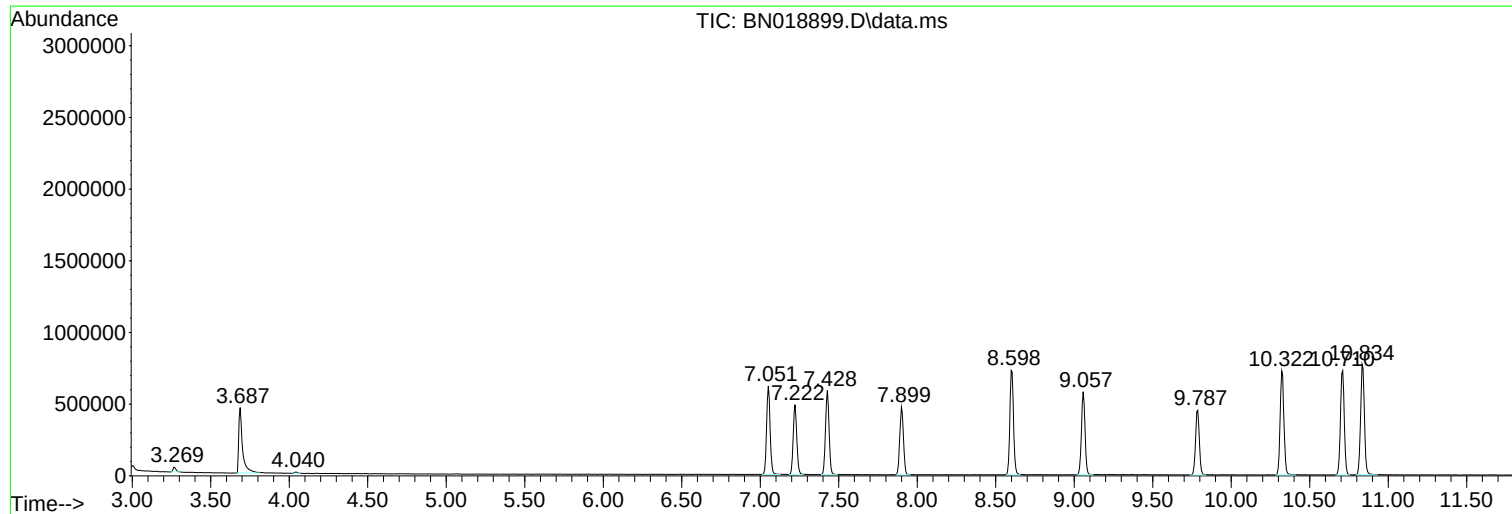

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031022\
Data File : BN018899.D
Acq On : 10 Mar 2022 12:09
Operator : CG/JU
Sample : PB142784BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK784

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031022\
Data File : BN018899.D
Acq On : 10 Mar 2022 12:09
Operator : CG/JU
Sample : PB142784BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK784

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc