


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031025\
Data File : BN036556.D
Acq On : 10 Mar 2025 11:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 16:06:28 2025

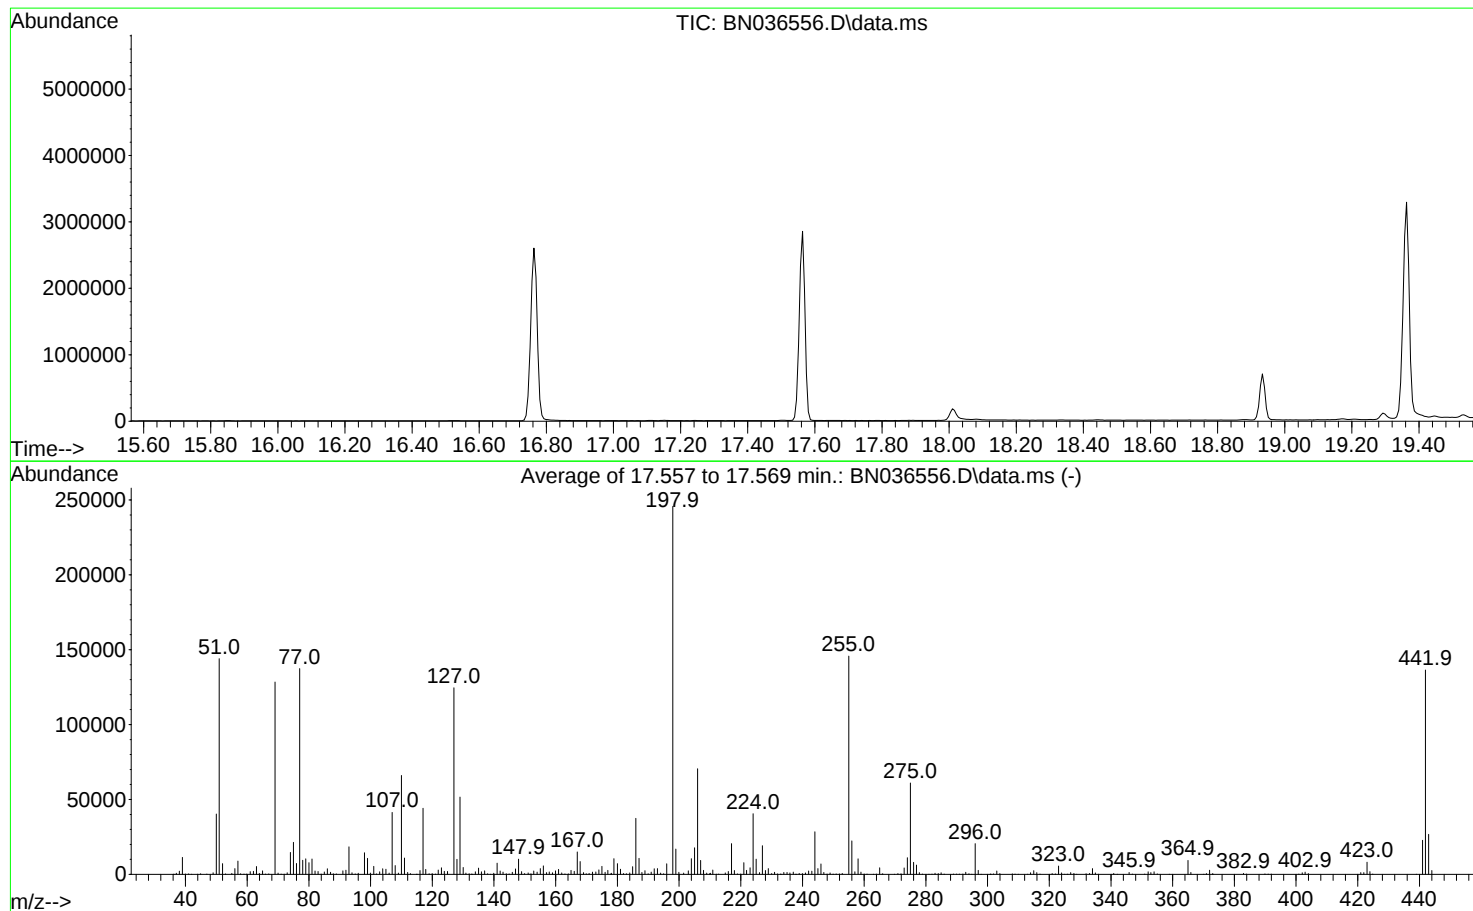

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.6	144050	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	52.3	128410	PASS
70	69	0.00	2	0.7	835	PASS
127	198	10	80	50.7	124576	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	245632	PASS
199	198	5	9	6.9	16887	PASS
275	198	10	60	24.8	60997	PASS
365	198	1	100	3.8	9349	PASS
441	198	0.01	100	9.3	22761	PASS
442	442	50	100	100.0	136488	PASS
443	442	15	24	19.6	26765	PASS

Instrument :
BNA_N
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/10/2025	BNA_N	<u>BN036556.D</u>
Compound Name	Response	Retention Time
DDT	1110406	20.598
DDD	11596	20.21
DDE	530	19.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12126	1122532	1.08

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031025\
Data File : BN036556.D
Acq On : 10 Mar 2025 11:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 10 17:07:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

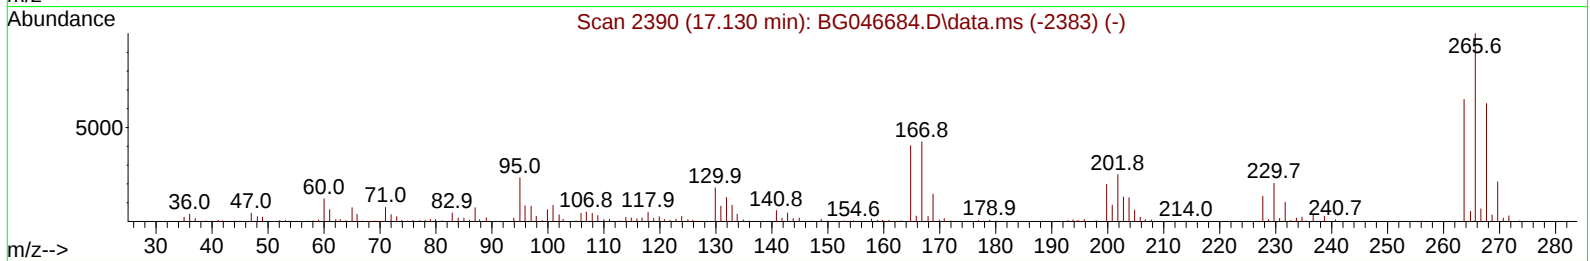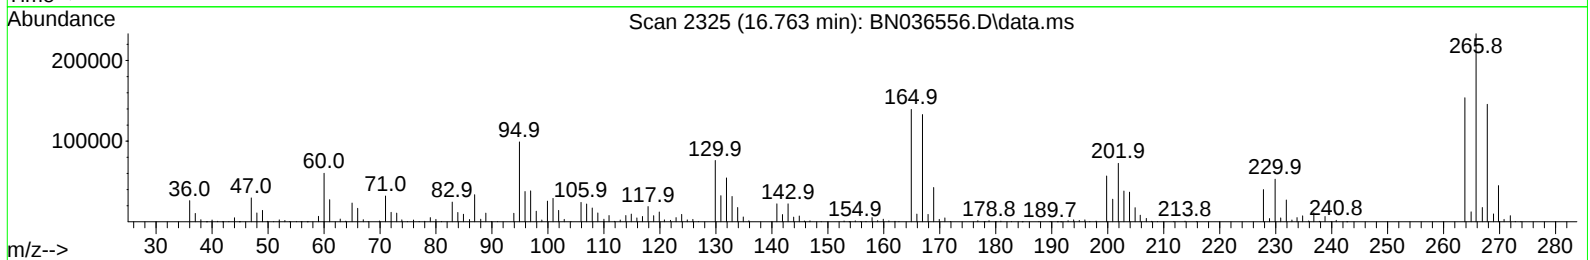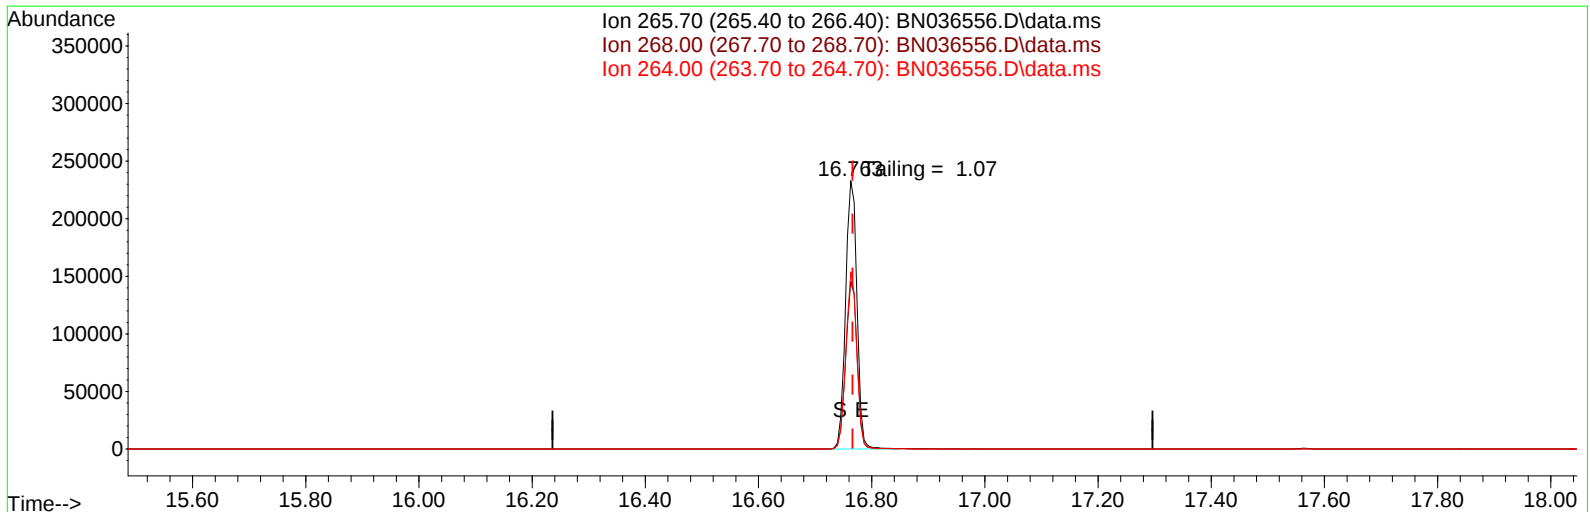

TIC: BN036556.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.003) 23577.14 ng




response 323613

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.52
264.00	61.60	66.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031025\
Data File : BN036556.D
Acq On : 10 Mar 2025 11:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 10 17:07:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

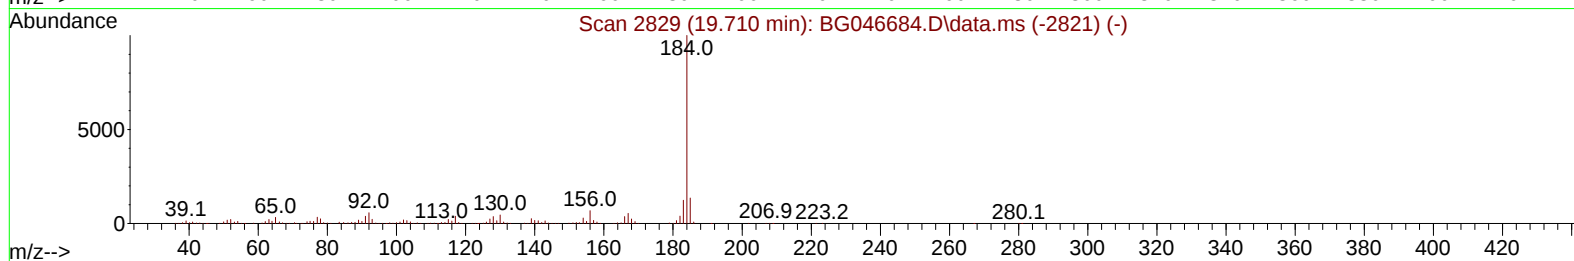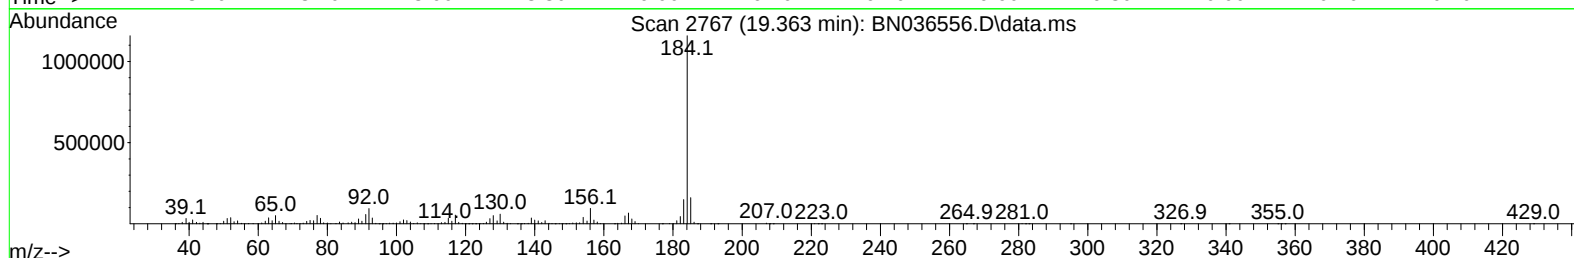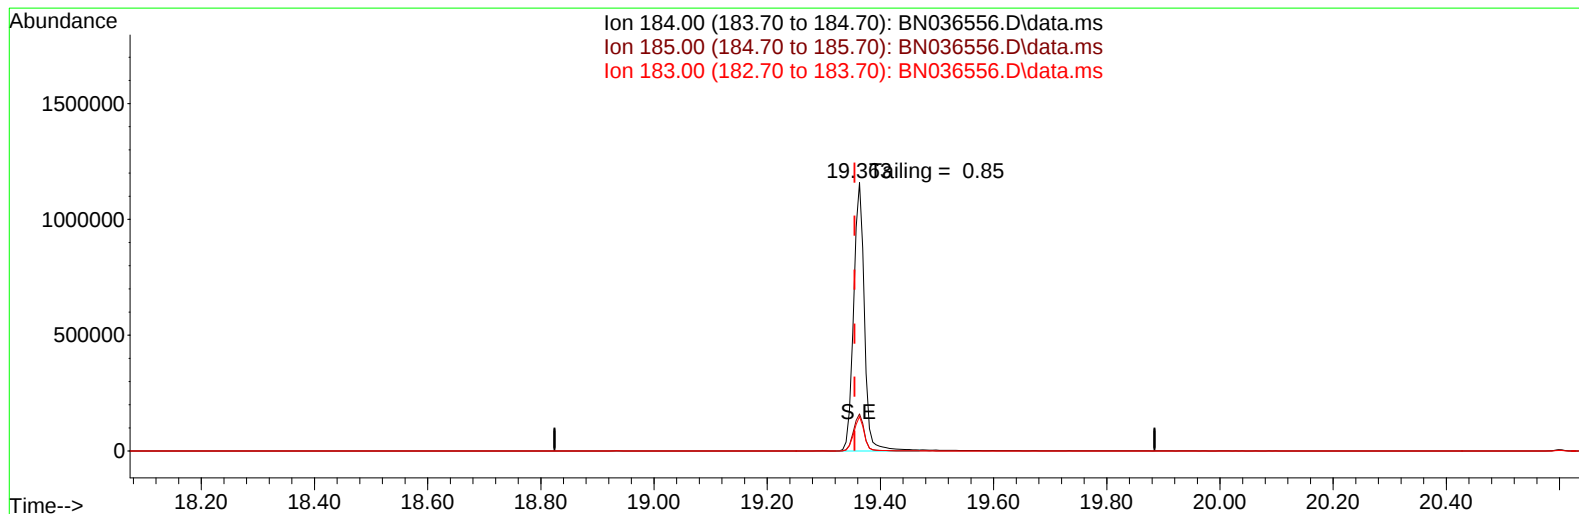

TIC: BN036556.D\data.ms

(77) Benzidine

19.363min (+ 0.009) 0.00 ng

response 1553313

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.86
183.00	13.20	12.85
0.00	0.00	0.00