
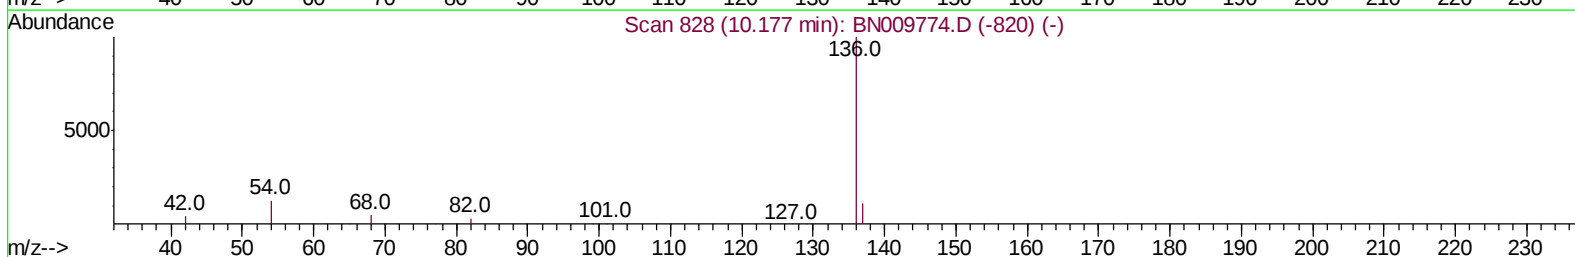
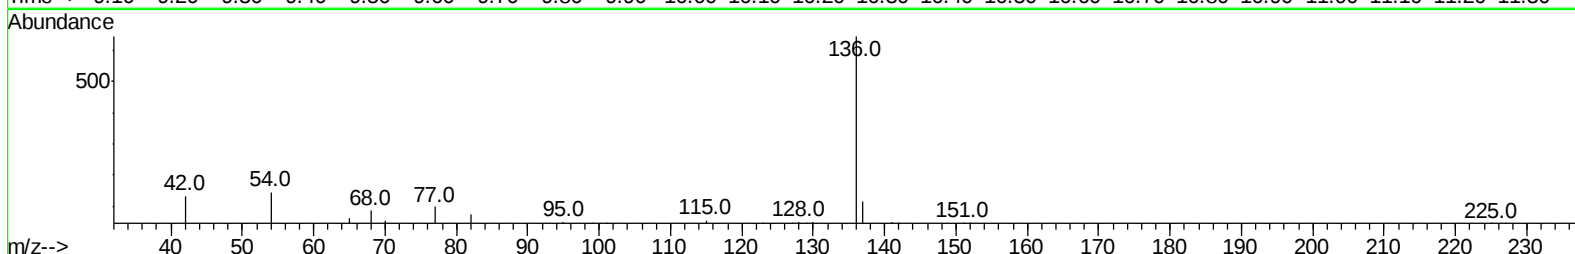


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031120\
 Data File : BN010198.D
 Acq On : 11 Mar 2020 18:47
 Operator : CG/JU
 Sample : L1842-18DL 2X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 12 07:15:43 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN021920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 11 17:37:44 2020
 Response via : Initial Calibration

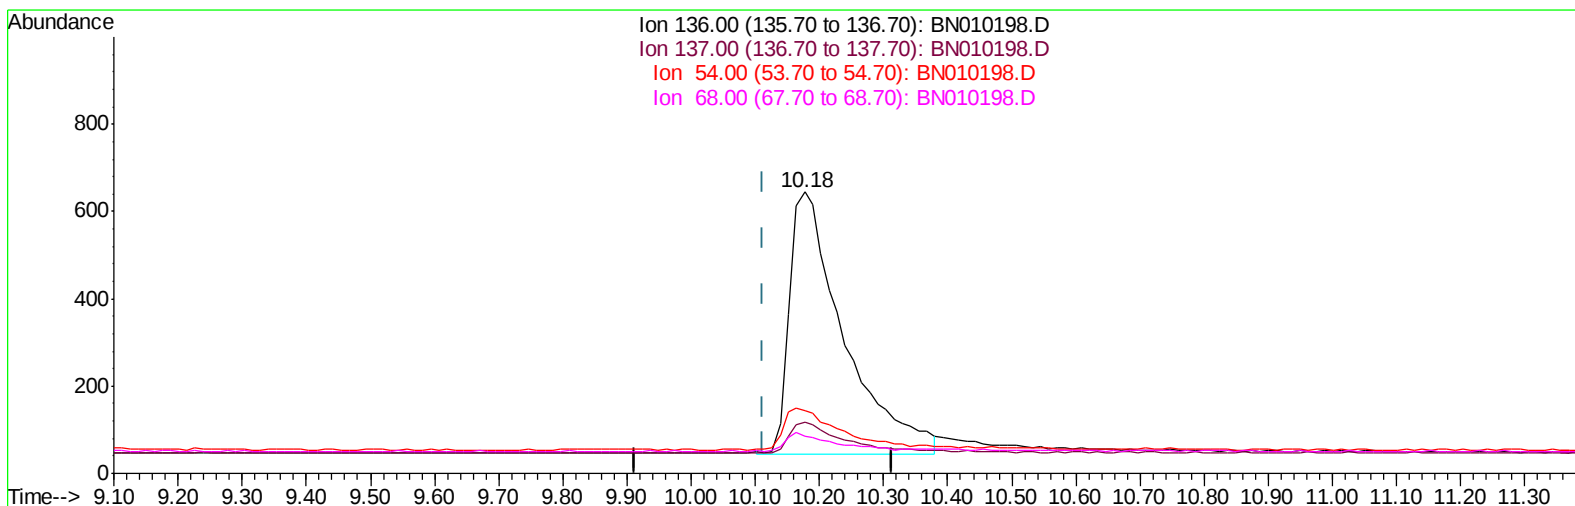

TIC: BN010198.D

(7) Naphthalene-d8 (I)

10.177min (+0.064) 0.40ng m




response 3515

Ion	Exp%	Act%
136.00	100	100
137.00	14.10	17.98#
54.00	16.80	22.33#
68.00	8.70	13.18#

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031120\
Data File : BN010200.D
Acq On : 11 Mar 2020 19:58
Operator : CG/JU
Sample : L1842-21DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 12 07:16:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN021920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 11 17:37:44 2020
Response via : Initial Calibration

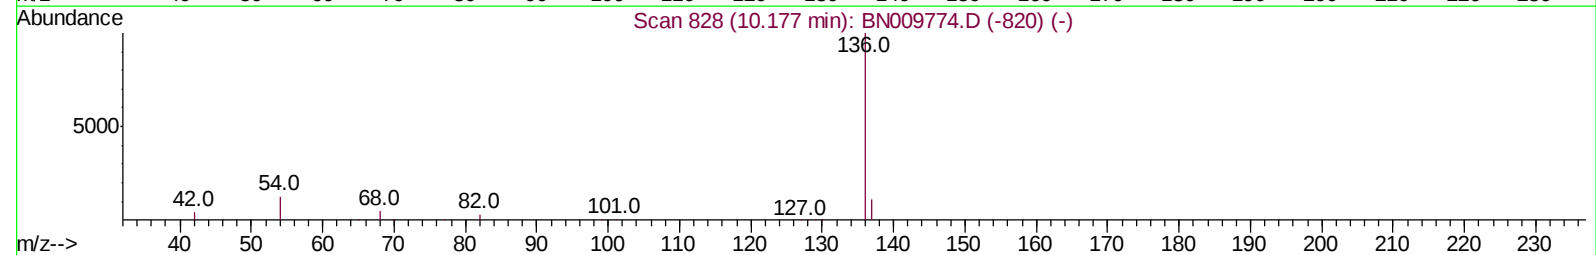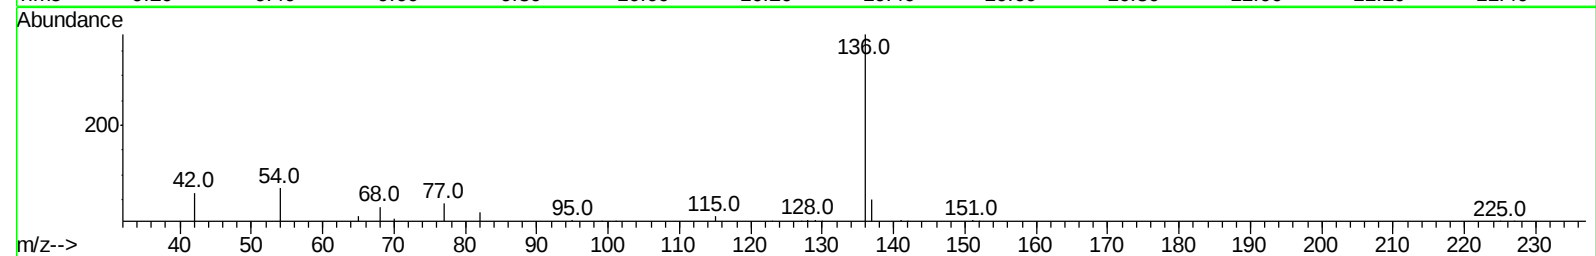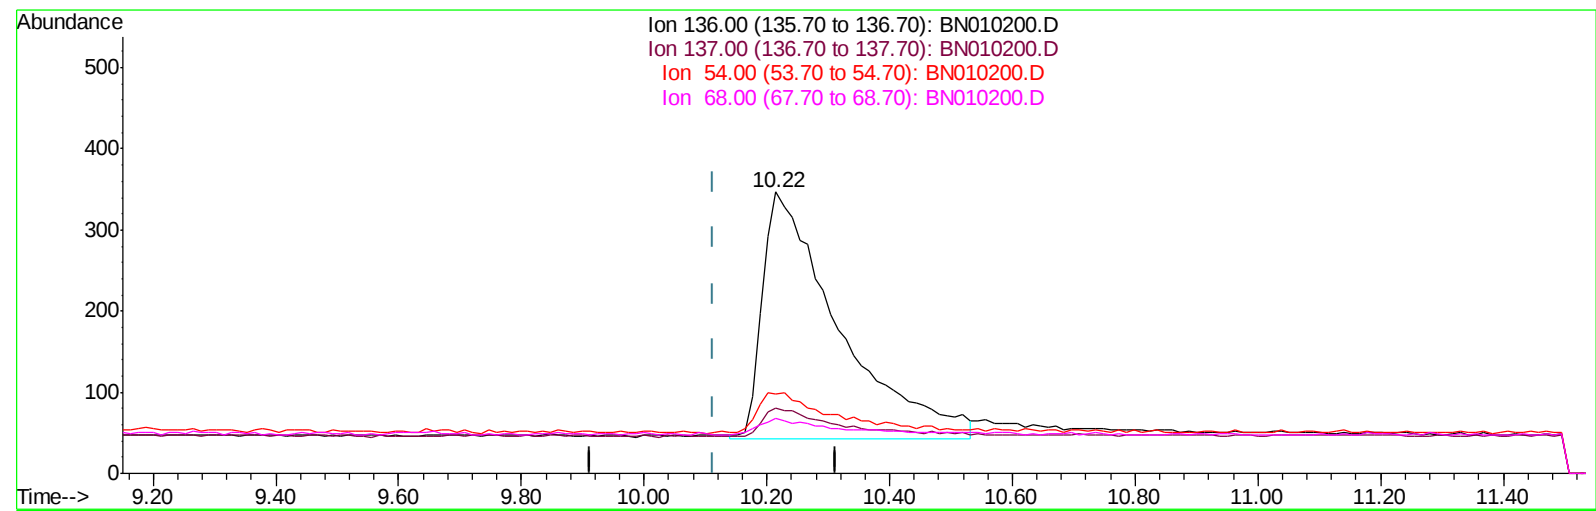

TIC: BN010200.D

(7) Naphthalene-d8 (I)

10.215min (+0.102) 0.40ng m




response 2606

Ion	Exp%	Act%
136.00	100	100
137.00	14.10	23.34#
54.00	16.80	28.24#
68.00	8.70	19.60#

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031120\
Data File : BN010201.D
Acq On : 11 Mar 2020 20:34
Operator : CG/JU
Sample : L1842-23DL 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 12 07:50:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN021920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 11 17:37:44 2020
Response via : Initial Calibration

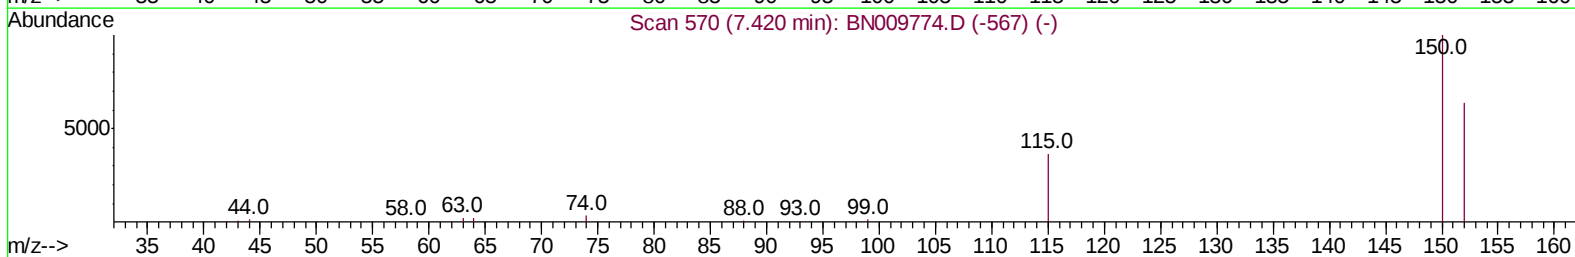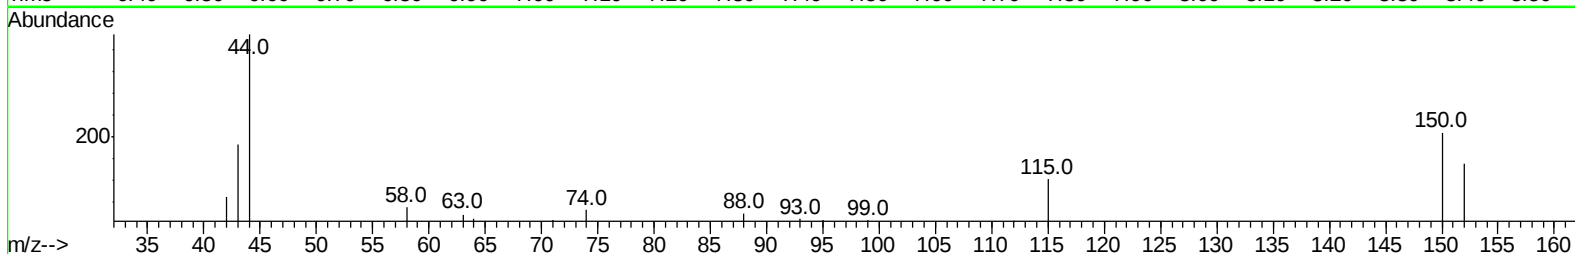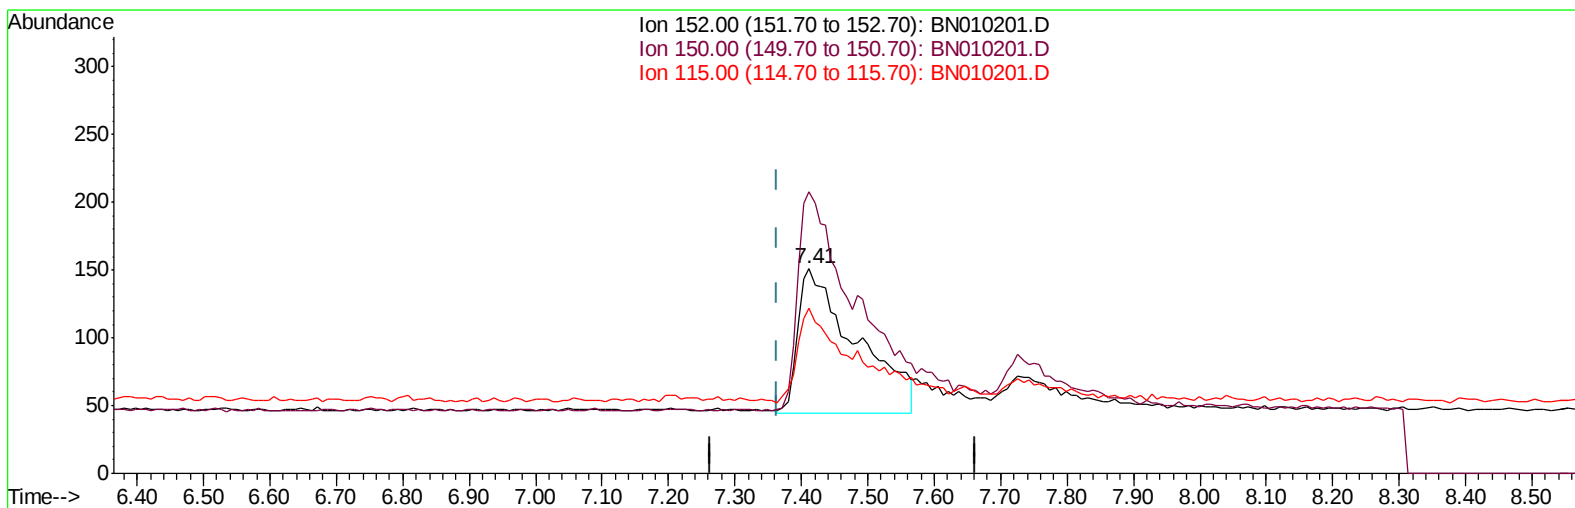

TIC: BN010201.D

(1) 1,4-Dichlorobenzene-d4 (I)

7.412min (+0.048) 0.40ng m




response 652

Ion	Exp%	Act%
152.00	100	100
150.00	150.80	137.75
115.00	64.00	80.79#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031120\
 Data File : BN010192.D
 Acq On : 11 Mar 2020 15:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 12 08:17:15 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN021920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 11 17:37:44 2020
 Response via : Initial Calibration

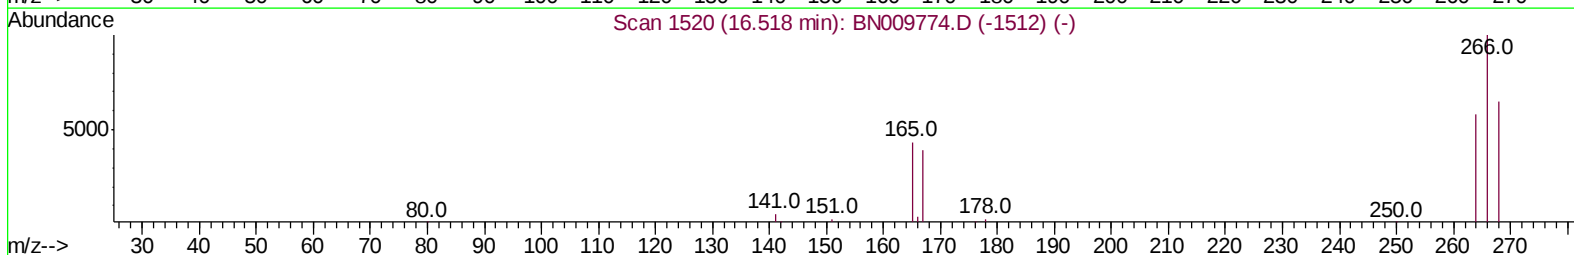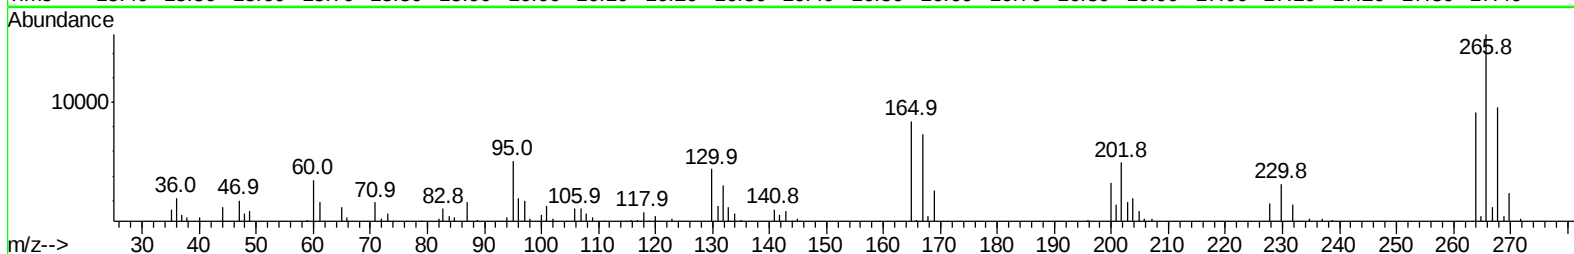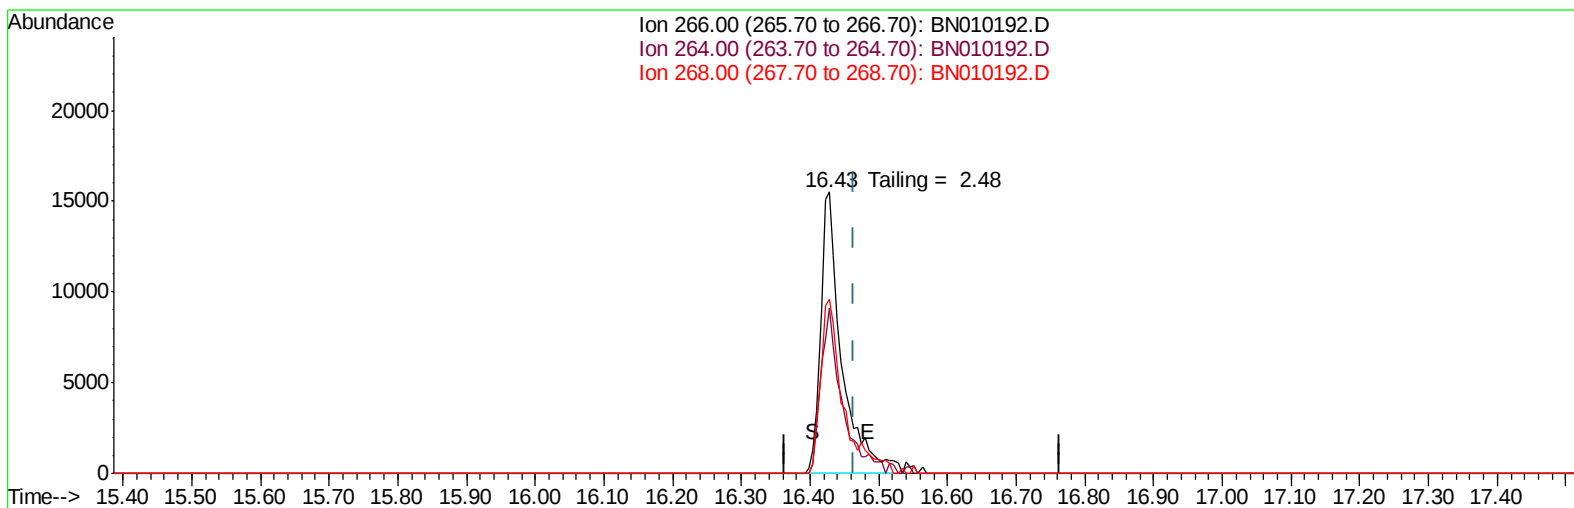

TIC: BN010192.D

(22) Pentachlorophenol

16.428min (-0.037) 0.00ng

response 32285

Ion	Exp%	Act%
266.00	100	100
264.00	72.60	58.74
268.00	82.10	61.82#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031120\
 Data File : BN010192.D
 Acq On : 11 Mar 2020 15:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 12 08:17:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN021920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 11 17:37:44 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ng	-7.36
7) Naphthalene-d8	0.00	136	0	0.00	ng	-10.11
13) Acenaphthene-d10	0.00	164	0	0.00	ng	-14.00
19) Phenanthrene-d10	0.00	188	0	0.00	ng	-16.77
27) Chrysene-d12	0.00	240	0	0.00	ng	-20.99
34) Perylene-d12	0.00	264	0	0.00	ng	-23.10

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units
4) 2-Fluorophenol	0.00	112	0	0.00	ng
5) Phenol-d6	0.00	99	0	0.00	ng
8) Nitrobenzene-d5	0.00	82	0	0.00	ng
11) 2-Methylnaphthalene-d10	0.00	152	0	0.00	ng
14) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng
15) 2-Fluorobiphenyl	0.00	172	0	0.00	ng
25) Fluoranthene-d10	0.00	212	0	0.00	ng
29) Terphenyl-d14	0.00	244	0	0.00	ng

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031120\
Data File : BN010192.D
Acq On : 11 Mar 2020 15:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 12 08:17:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN021920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 11 17:37:44 2020
Response via : Initial Calibration

