


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031120\
 Data File : BN010192.D
 Acq On : 11 Mar 2020 15:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN021920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 11 17:37:44 2020

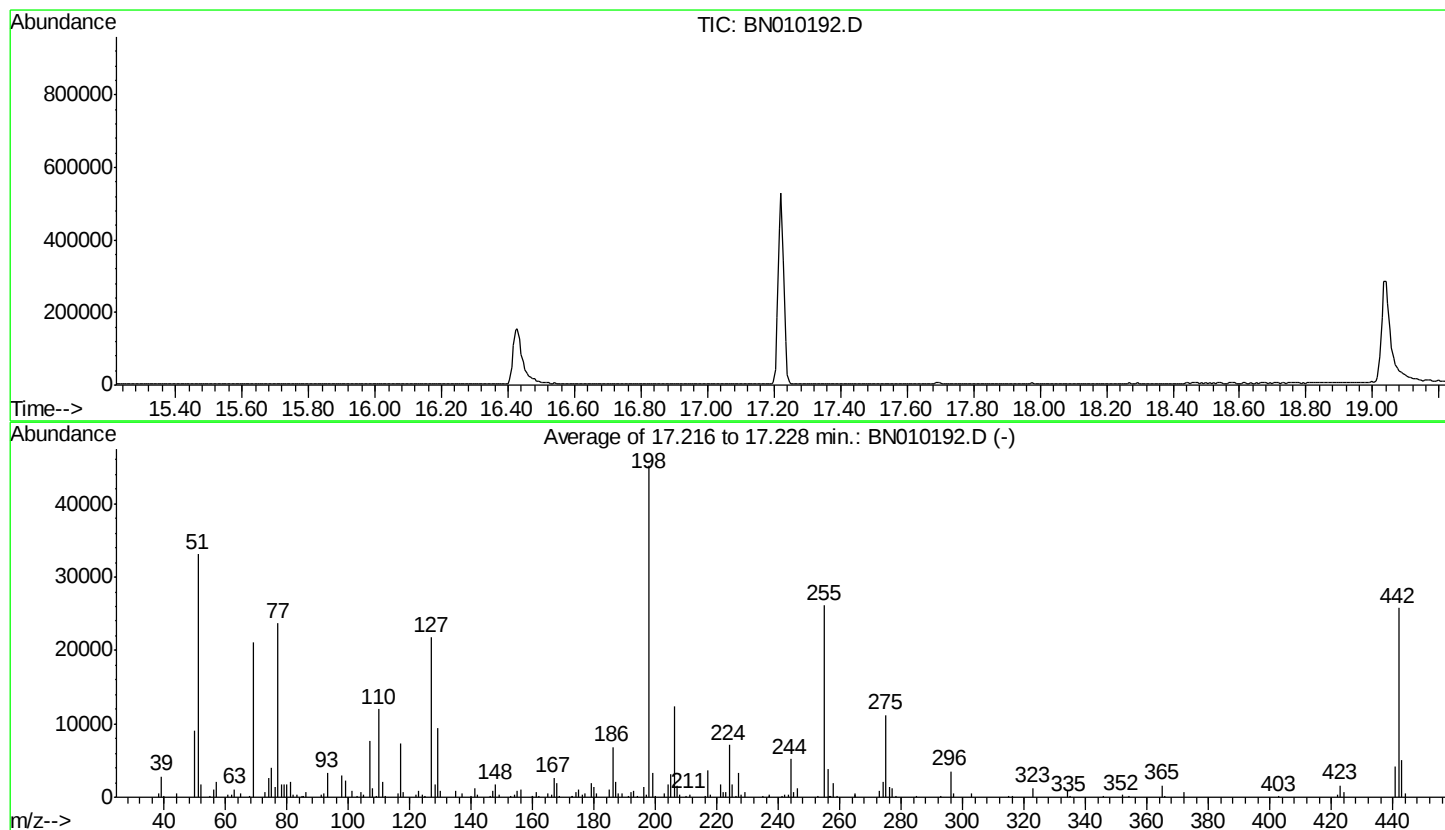

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	73.3	33117	PASS
68	69	0.00	2	1.2	260	PASS
69	198	0.00	100	46.8	21156	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	21729	PASS
197	198	0.00	2	0.8	373	PASS
198	198	100	100	100.0	45194	PASS
199	198	5	9	7.2	3240	PASS
275	198	10	60	24.8	11214	PASS
365	198	1	100	3.6	1637	PASS
441	198	0.01	100	9.2	4167	PASS
442	198	50	100	57.0	25781	PASS
443	442	15	24	19.9	5138	PASS