
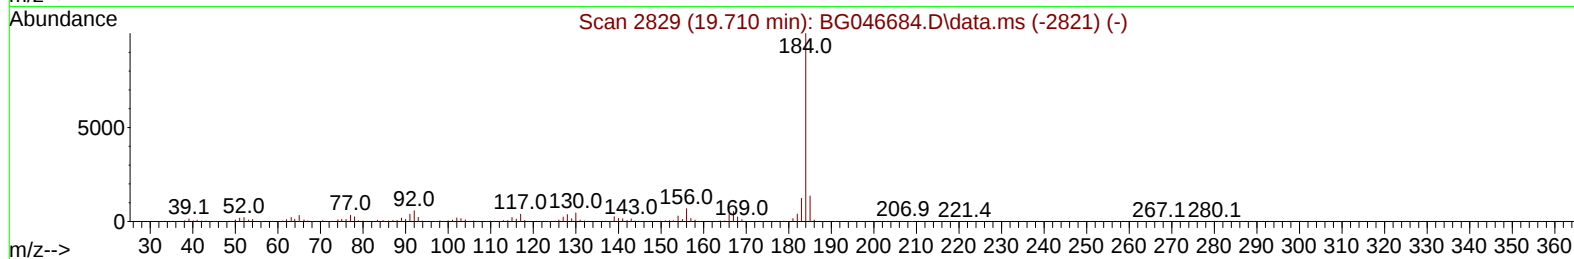
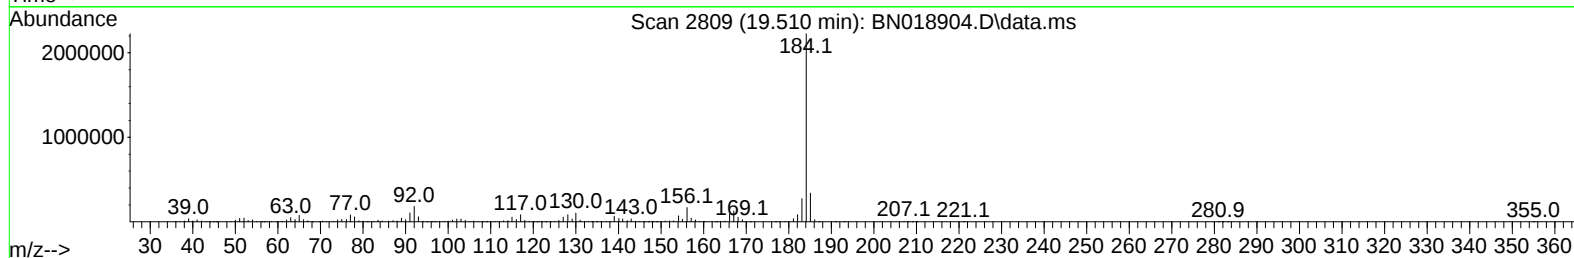


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031122\
Data File : BN018904.D
Acq On : 10 Mar 2022 16:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 06:09:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 11 06:09:36 2022
Response via : Initial Calibration

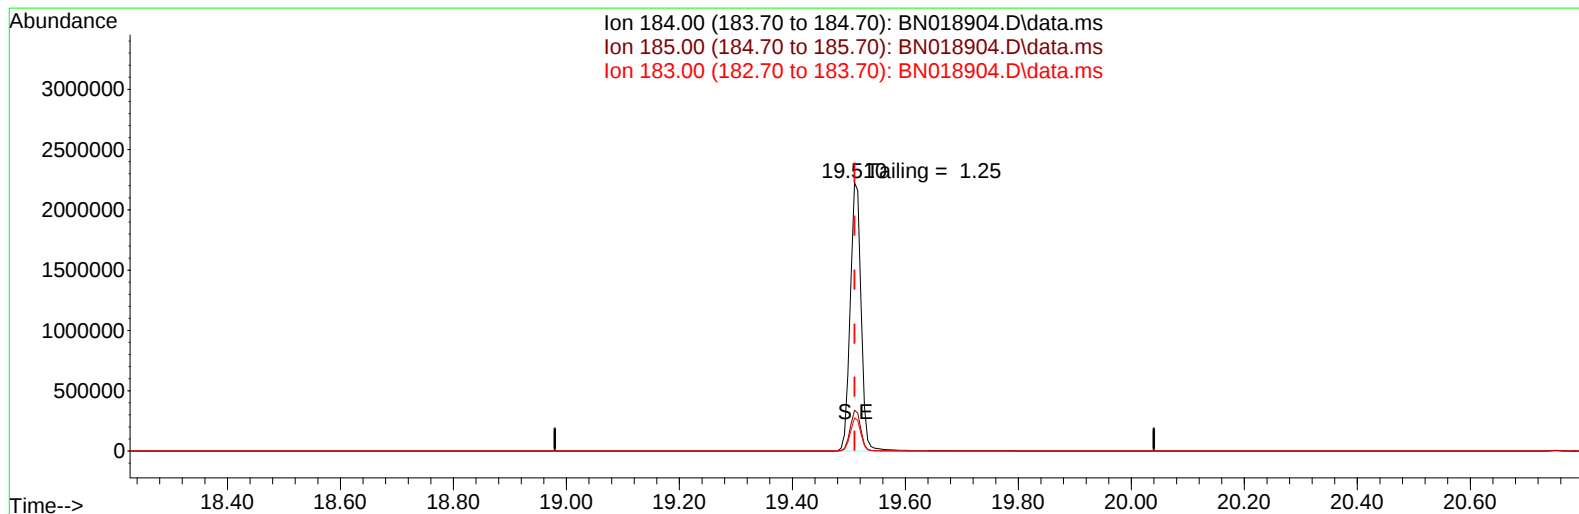

TIC: BN018904.D\data.ms

(77) Benzidine




19.510min (0.000) 0.00 ng

response 2997859

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.22
183.00	13.20	12.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031122\
Data File : BN018904.D
Acq On : 10 Mar 2022 16:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 06:09:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 11 06:09:36 2022
Response via : Initial Calibration

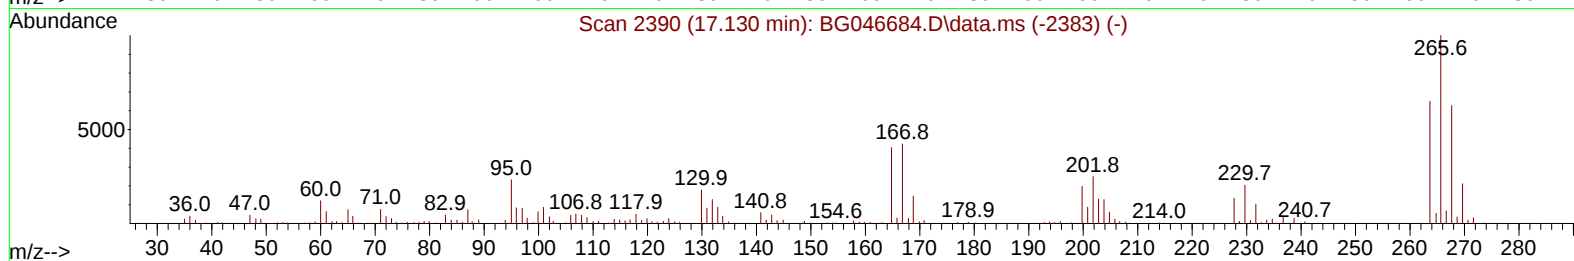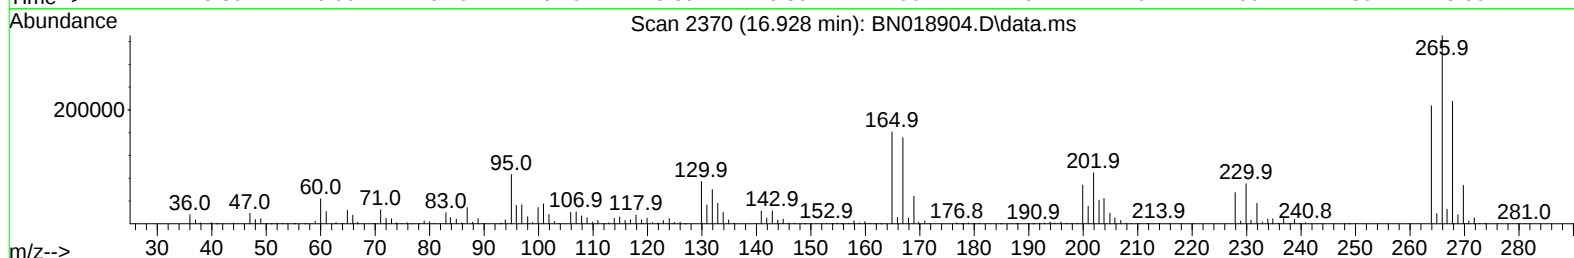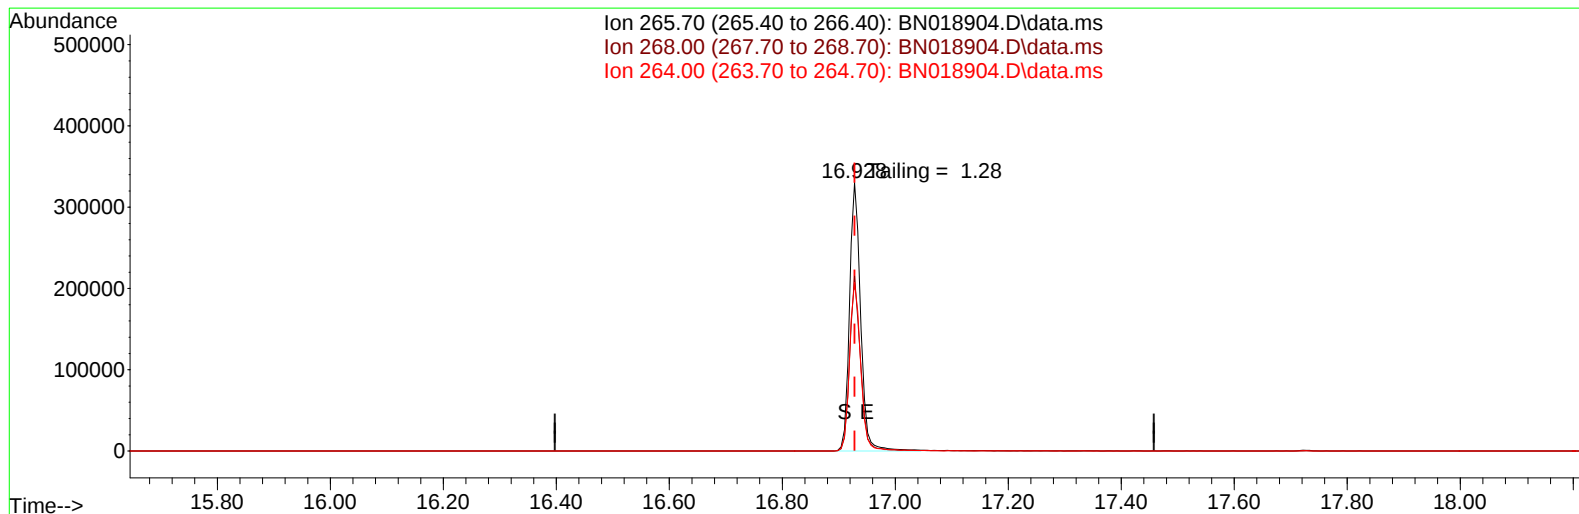

TIC: BN018904.D\data.ms

(70) Pentachlorophenol (C)

16.928min (0.000) 19498.40 ng

response 453853

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.16
264.00	61.60	62.77
0.00	0.00	0.00