
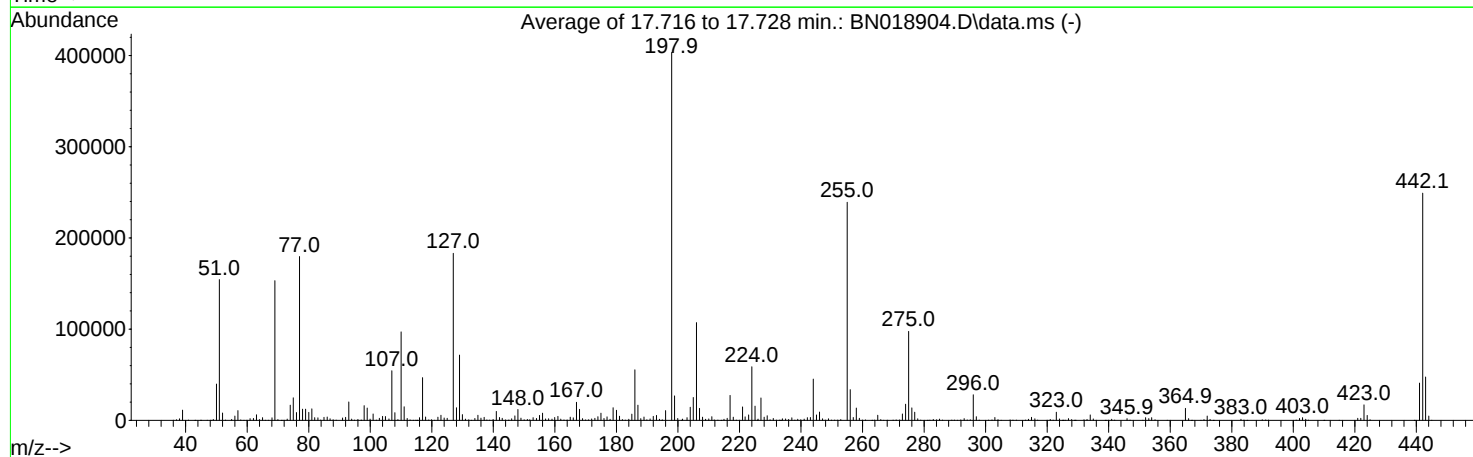


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031122\
 Data File : BN018904.D
 Acq On : 10 Mar 2022 16:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN030322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 11 03:02:57 2022

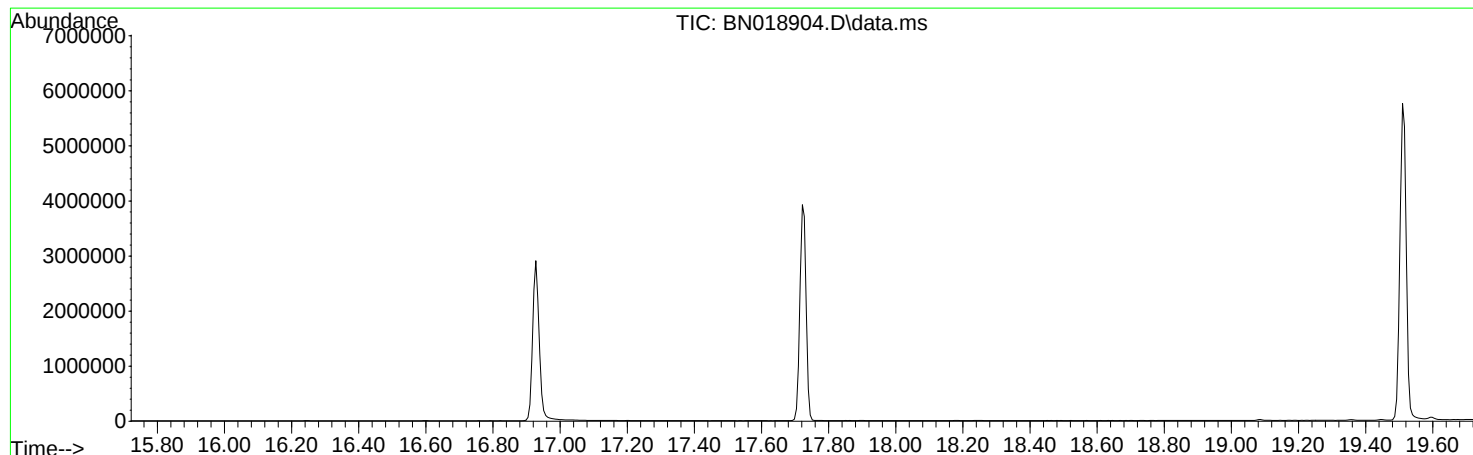

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	154331	PASS
68	69	0.00	2	1.8	2819	PASS
69	198	0.00	100	38.0	153136	PASS
70	69	0.00	2	0.6	880	PASS
127	198	10	80	45.4	183211	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	403371	PASS
199	198	5	9	6.7	26845	PASS
275	198	10	60	24.2	97589	PASS
365	198	1	100	3.3	13187	PASS
441	198	0.01	100	10.1	40904	PASS
442	442	50	100	100.0	249131	PASS
443	442	15	24	19.1	47512	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/11/2022	BNA_N	<u>BN018904.D</u>
Compound Name	Response	Retention Time
DDT	1514338	20.751
DDD	26035	20.31
DDE	1473	19.798
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27508	1541846	1.78

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031122\
Data File : BN018904.D
Acq On : 10 Mar 2022 16:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 11 06:09:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 11 06:09:36 2022
Response via : Initial Calibration

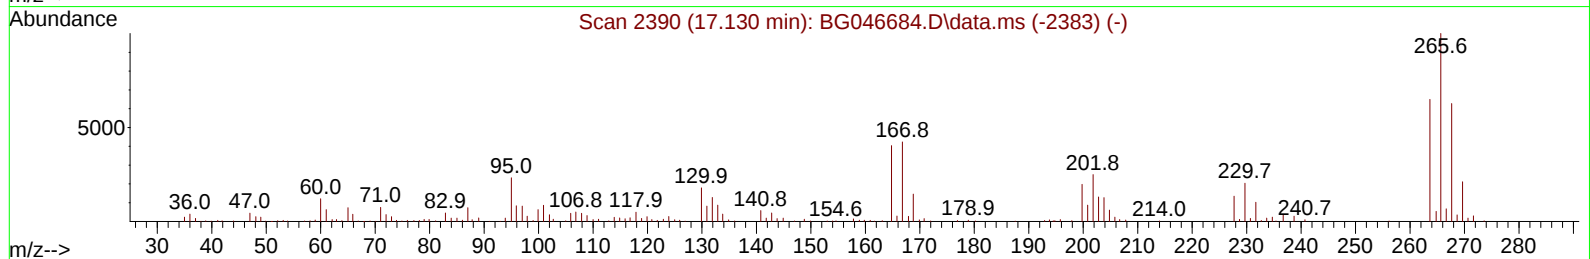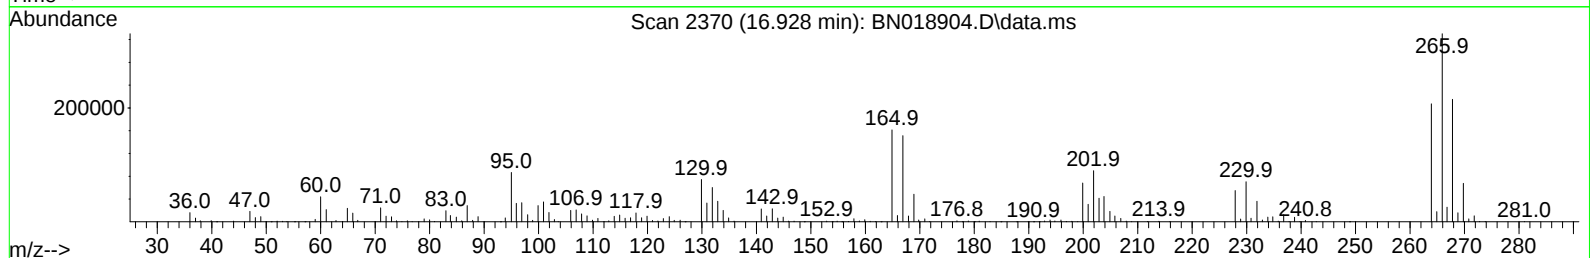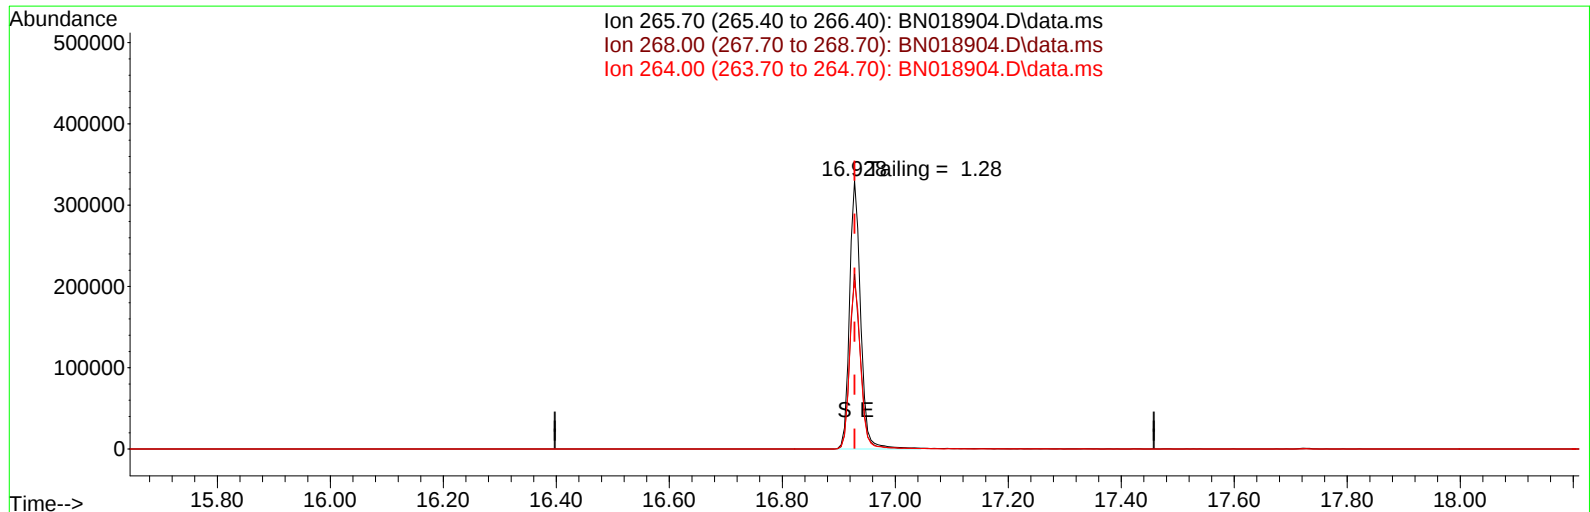

TIC: BN018904.D\data.ms

(70) Pentachlorophenol (C)

16.928min (0.000) 19498.40 ng




response 453853

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.16
264.00	61.60	62.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031122\
Data File : BN018904.D
Acq On : 10 Mar 2022 16:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 11 06:09:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 11 06:09:36 2022
Response via : Initial Calibration

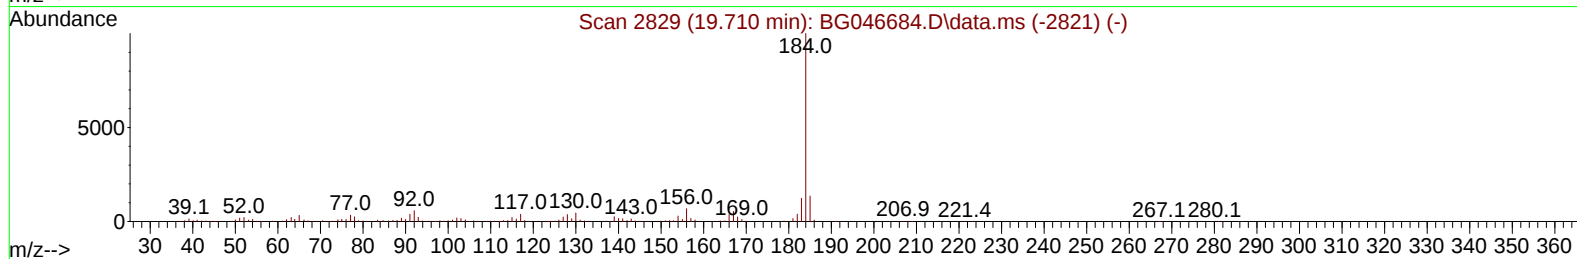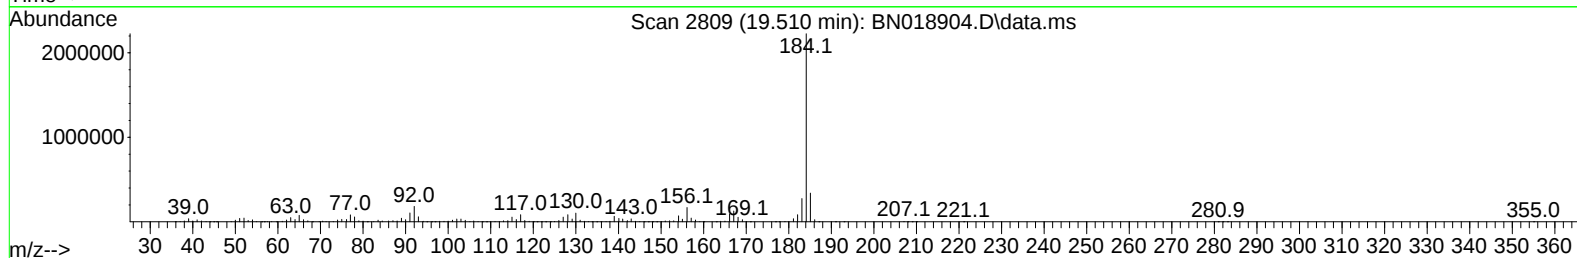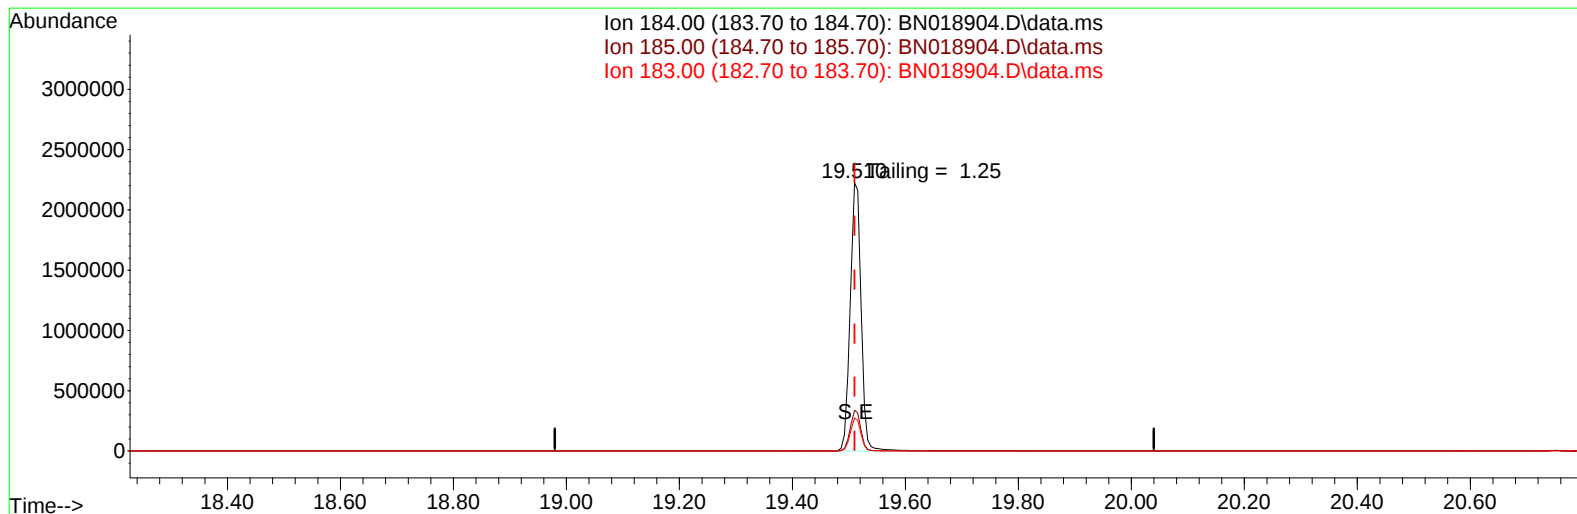

TIC: BN018904.D\data.ms

(77) Benzidine

19.510min (0.000) 0.00 ng

response 2997859

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.22
183.00	13.20	12.34
0.00	0.00	0.00