

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031124\
 Data File : BN030358.D
 Acq On : 11 Mar 2024 12:15
 Operator : MA/JU
 Sample : PB159425BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK425

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030358.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	28	31	38	rVB	32156	43105	2.08%	0.185%
2	3.676	97	100	115	rBV	345935	554847	26.77%	2.375%
3	3.946	144	146	150	rBV5	2213	3674	0.18%	0.016%
4	3.993	151	154	159	rVB3	6869	9317	0.45%	0.040%
5	4.634	261	263	269	rVB4	1713	2221	0.11%	0.010%
6	5.281	371	373	376	rBV3	1879	2249	0.11%	0.010%
7	6.417	560	566	568	rBV5	1518	2170	0.10%	0.009%
8	6.675	606	610	616	rBV5	1407	2212	0.11%	0.009%
9	6.964	653	659	672	rVB	454235	704463	33.99%	3.016%
10	7.140	683	689	697	rBV	317453	504757	24.35%	2.161%
11	7.322	712	720	732	rBV	494276	770586	37.18%	3.299%
12	7.793	793	800	808	rBV	381155	602678	29.08%	2.580%
13	8.505	914	921	932	rBV	544417	865638	41.76%	3.706%
14	8.963	991	999	1011	rBV	428623	702623	33.90%	3.008%
15	9.681	1114	1121	1133	rBV	353965	598260	28.86%	2.561%
16	10.210	1203	1211	1222	rBV	533998	886182	42.75%	3.794%
17	10.587	1268	1275	1283	rBV	460044	766840	37.00%	3.283%
18	10.740	1292	1301	1316	rBV	480008	855660	41.28%	3.663%
19	12.199	1543	1549	1557	rBV3	5233	9305	0.45%	0.040%
20	13.351	1741	1745	1751	rVB4	4437	4809	0.23%	0.021%
21	13.875	1826	1834	1842	rBV	825523	1158087	55.87%	4.958%
22	14.140	1873	1879	1893	rBV	927837	1366561	65.93%	5.850%
23	14.451	1925	1932	1942	rBV	596632	890538	42.96%	3.812%
24	14.657	1961	1967	1981	rBV	295451	503386	24.29%	2.155%
25	15.451	2095	2102	2114	rBV	1152931	1634796	78.87%	6.998%
26	15.581	2118	2124	2135	rVV	361088	516961	24.94%	2.213%
27	15.687	2139	2142	2148	rVB5	4054	6068	0.29%	0.026%
28	16.240	2232	2236	2239	rBV4	3018	4880	0.24%	0.021%
29	16.992	2362	2364	2371	rVB5	2120	4039	0.19%	0.017%
30	17.210	2395	2401	2409	rBV	741962	1023709	49.39%	4.382%
31	17.310	2412	2418	2436	rVB2	1170729	1714046	82.69%	7.338%
32	18.134	2555	2558	2563	rBV5	6286	9228	0.45%	0.040%
33	19.181	2732	2736	2741	rVB4	12238	16330	0.79%	0.070%
34	19.251	2745	2748	2755	rVV	11122	14356	0.69%	0.061%
35	19.428	2774	2778	2781	rBV5	6727	8052	0.39%	0.034%
36	19.622	2804	2811	2818	rBV	1415335	1928563	93.04%	8.256%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031124\
Data File : BN030358.D
Acq On : 11 Mar 2024 12:15
Operator : MA/JU
Sample : PB159425BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK425

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Title : SVOA CALIBRATION

37	20.281	2921	2923	2924	rBV2	3638	2159	0.10%	0.009%
38	21.428	3113	3118	3131	rBV	847102	1136937	54.85%	4.867%
39	23.116	3402	3405	3412	rVB4	41073	66797	3.22%	0.286%
40	23.633	3485	3493	3505	rBV2	1035011	2072797	100.00%	8.873%
41	23.733	3507	3510	3511	rVV2	58671	65598	3.16%	0.281%
42	23.780	3512	3518	3527	rVB	582847	1209813	58.37%	5.179%
43	24.451	3628	3632	3641	rVB4	53859	114147	5.51%	0.489%




Sum of corrected areas: 23359444

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031124\
Data File : BN030358.D
Acq On : 11 Mar 2024 12:15
Operator : MA/JU
Sample : PB159425BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

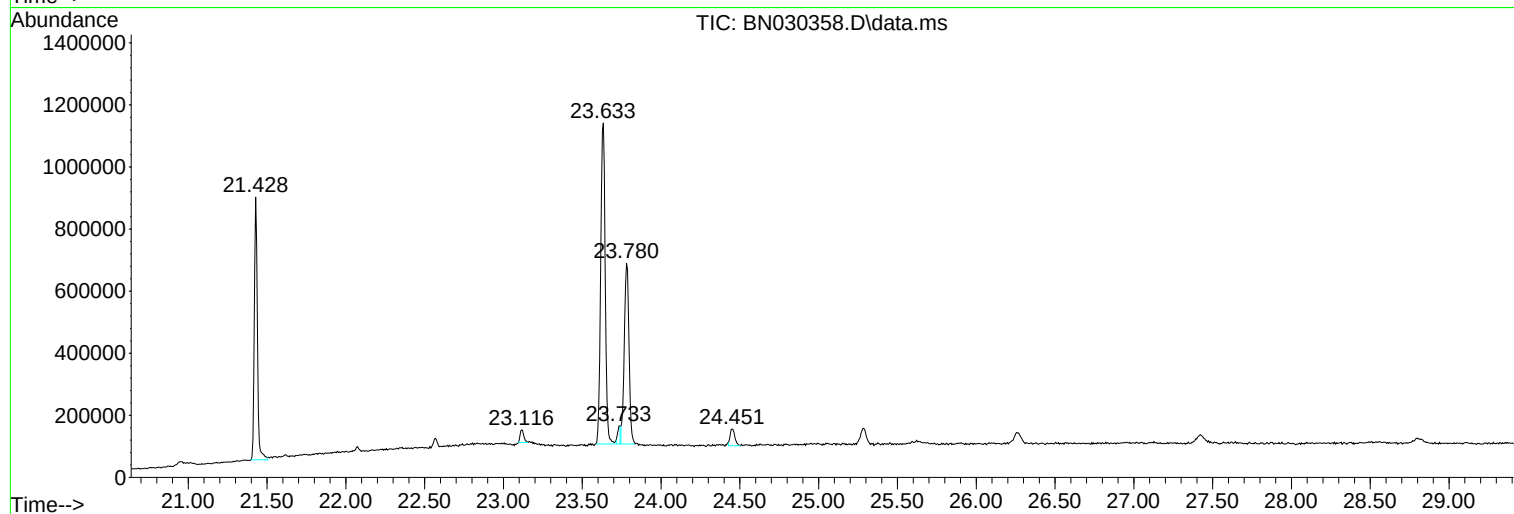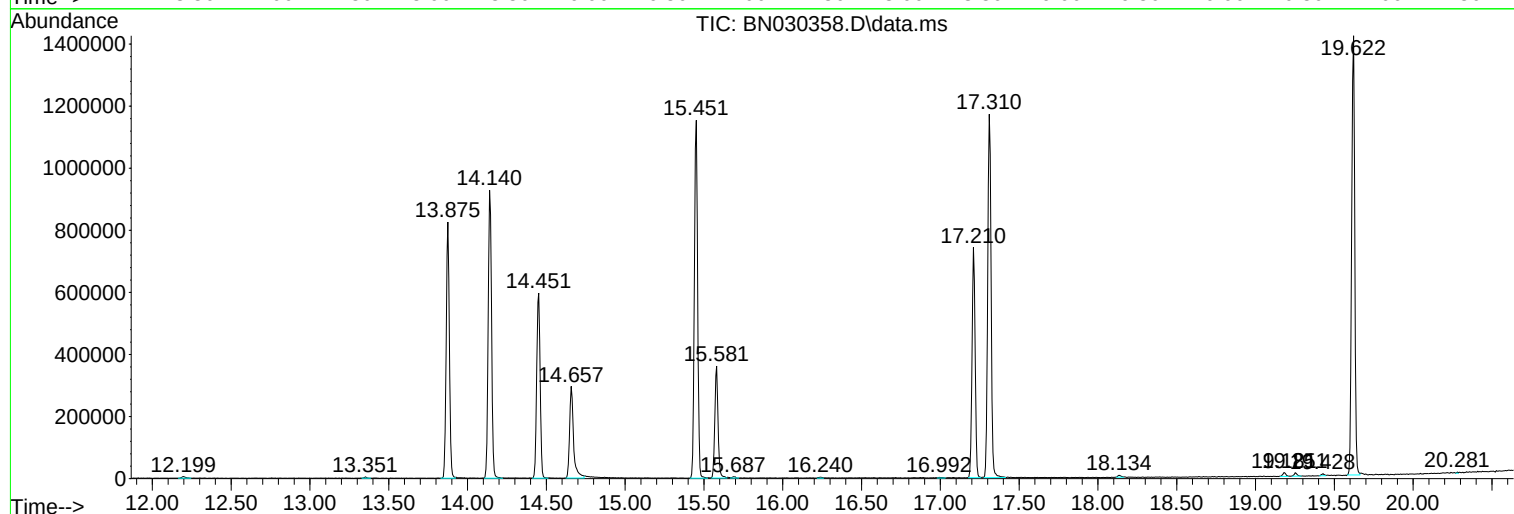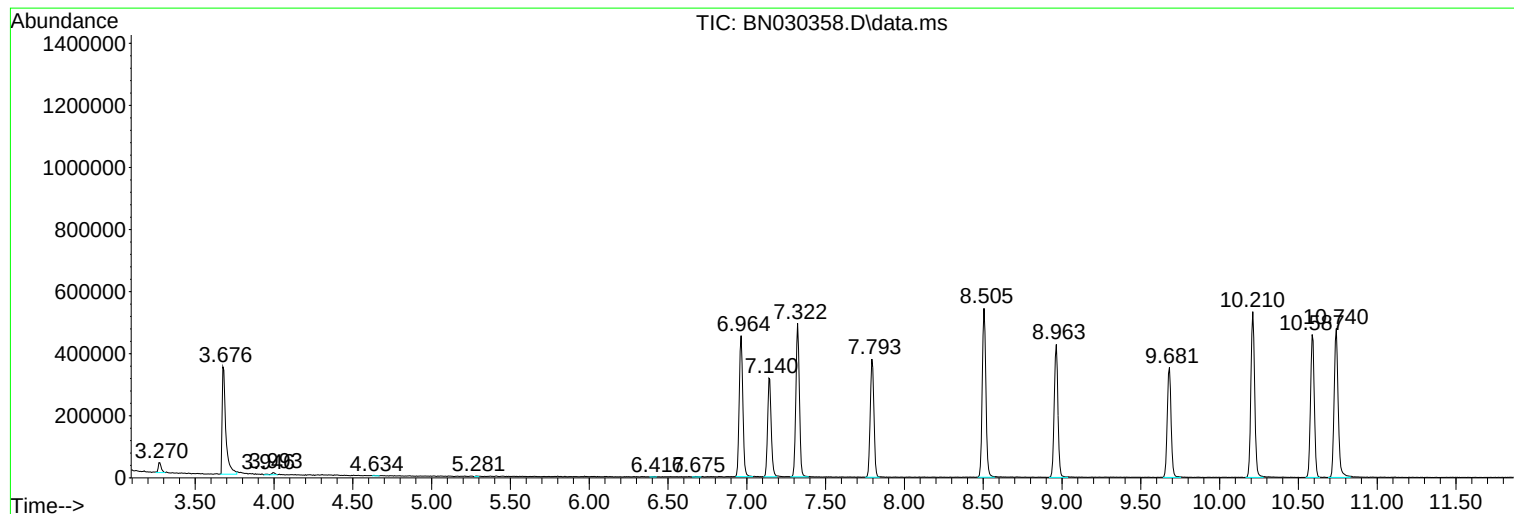

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031124\
Data File : BN030358.D
Acq On : 11 Mar 2024 12:15
Operator : MA/JU
Sample : PB159425BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031124\
Data File : BN030358.D
Acq On : 11 Mar 2024 12:15
Operator : MA/JU
Sample : PB159425BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------