

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031124\
 Data File : BN030362.D
 Acq On : 11 Mar 2024 16:19
 Operator : MA/JU
 Sample : PB159444BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK444

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030362.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	36	rVB	33831	45570	1.59%	0.146%
2	3.670	96	99	118	rBV	392318	638208	22.23%	2.047%
3	3.993	150	154	158	rVB3	5288	7928	0.28%	0.025%
4	6.958	652	658	670	rBV	541057	844509	29.42%	2.709%
5	7.140	682	689	701	rBV	385349	617180	21.50%	1.980%
6	7.317	712	719	732	rBV	578516	901443	31.40%	2.891%
7	7.787	793	799	808	rBV	425995	670475	23.36%	2.150%
8	8.499	912	920	931	rBV	681554	1087268	37.87%	3.487%
9	8.958	991	998	1010	rBV	547731	882080	30.73%	2.829%
10	9.328	1053	1061	1066	rBV7	7562	16957	0.59%	0.054%
11	9.675	1113	1120	1132	rBV	484512	781696	27.23%	2.507%
12	10.205	1203	1210	1227	rBV	671961	1143686	39.84%	3.668%
13	10.587	1267	1275	1284	rBV	568988	944276	32.89%	3.029%
14	10.734	1293	1300	1321	rBV	632506	1152378	40.14%	3.696%
15	12.187	1543	1547	1558	rBV3	7343	17455	0.61%	0.056%
16	13.875	1827	1834	1845	rBV	1307284	1799980	62.70%	5.773%
17	14.146	1872	1880	1889	rBV	1297754	1964872	68.45%	6.302%
18	14.451	1925	1932	1940	rBV	846176	1247035	43.44%	4.000%
19	14.657	1960	1967	1983	rBV	517546	826716	28.80%	2.652%
20	15.451	2095	2102	2115	rBV	1755012	2417440	84.21%	7.754%
21	15.581	2117	2124	2137	rVV	637730	885952	30.86%	2.842%
22	15.693	2138	2143	2148	rVB2	6201	9760	0.34%	0.031%
23	16.240	2232	2236	2242	rVB3	4434	6325	0.22%	0.020%
24	17.210	2395	2401	2409	rBV	1065120	1490648	51.93%	4.781%
25	17.310	2411	2418	2433	rVV	1807370	2636668	91.85%	8.457%
26	18.134	2554	2558	2564	rBV4	10054	16041	0.56%	0.051%
27	18.387	2597	2601	2605	rVB5	1584	3121	0.11%	0.010%
28	19.186	2731	2737	2741	rBV2	19773	27896	0.97%	0.089%
29	19.257	2745	2749	2755	rVB	15553	22978	0.80%	0.074%
30	19.428	2775	2778	2783	rVB6	8359	12669	0.44%	0.041%
31	19.622	2805	2811	2818	rBV	2085557	2870700	100.00%	9.207%
32	21.433	3114	3119	3133	rBV	1017772	1403313	48.88%	4.501%
33	22.575	3311	3313	3320	rVB5	29939	34355	1.20%	0.110%
34	23.127	3403	3407	3412	rBV2	42685	68830	2.40%	0.221%
35	23.639	3487	3494	3504	rBV2	1147815	2255222	78.56%	7.233%
36	23.792	3509	3520	3533	rVB	619836	1324245	46.13%	4.247%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031124\
Data File : BN030362.D
Acq On : 11 Mar 2024 16:19
Operator : MA/JU
Sample : PB159444BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK444

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Title : SVOA CALIBRATION

37	24.463	3630	3634	3643	rVB4	52479	102456	3.57%	0.329%
----	--------	------	------	------	------	-------	--------	-------	--------




Sum of corrected areas: 31178331

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031124\
Data File : BN030362.D
Acq On : 11 Mar 2024 16:19
Operator : MA/JU
Sample : PB159444BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK444

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

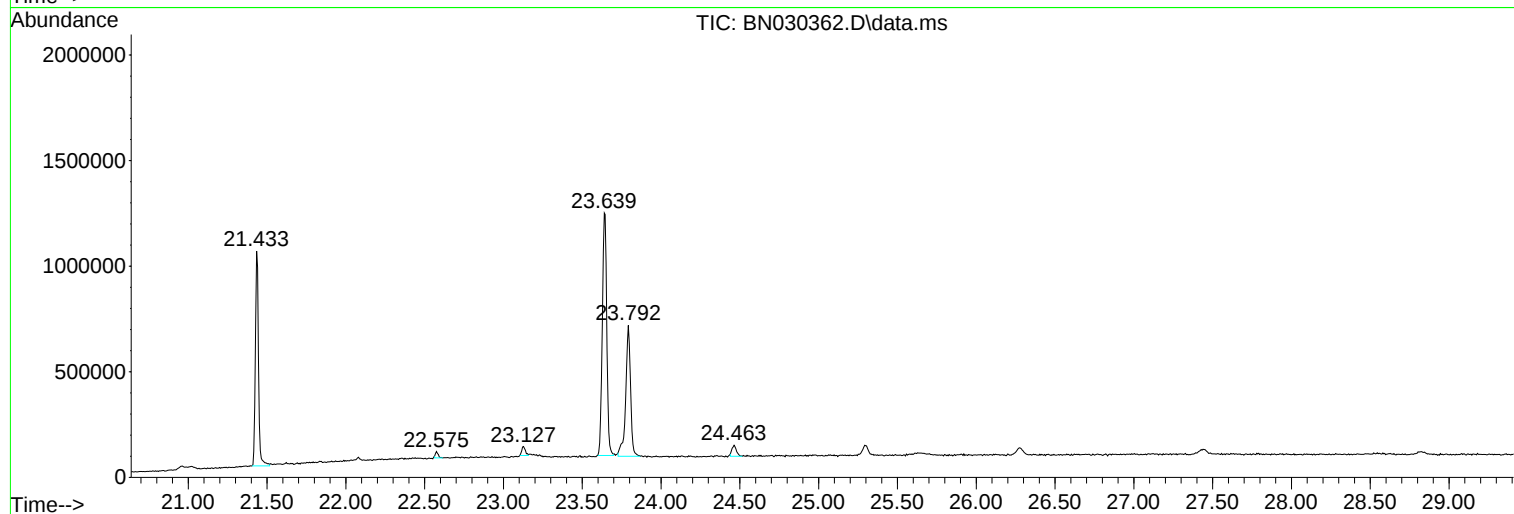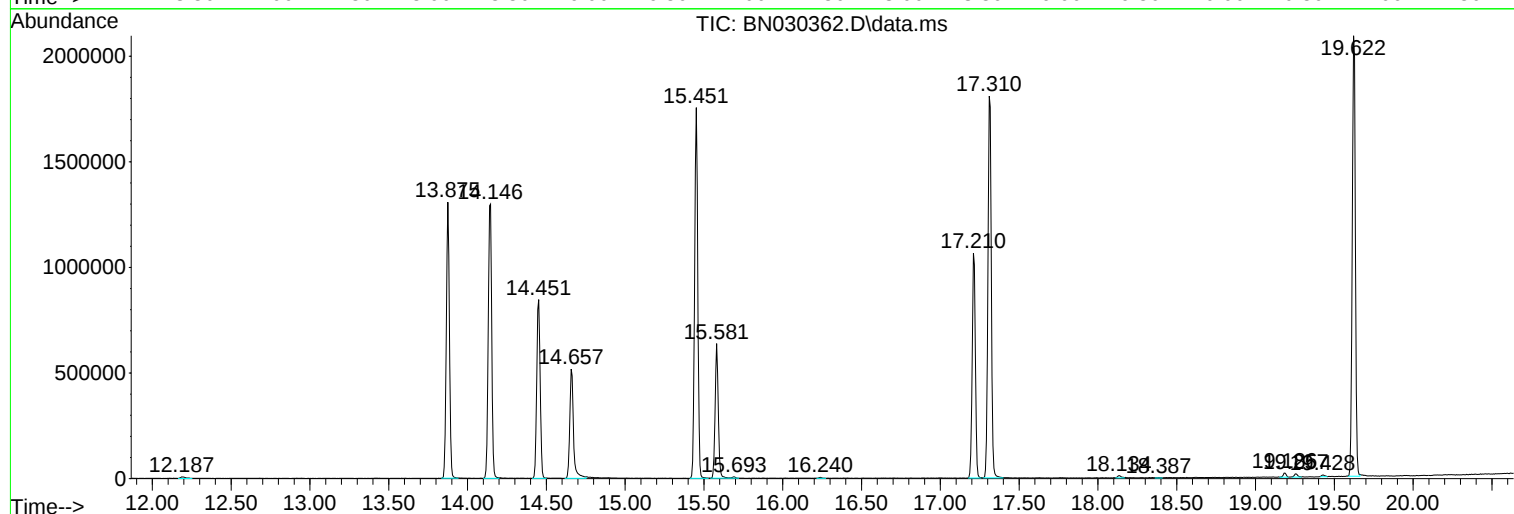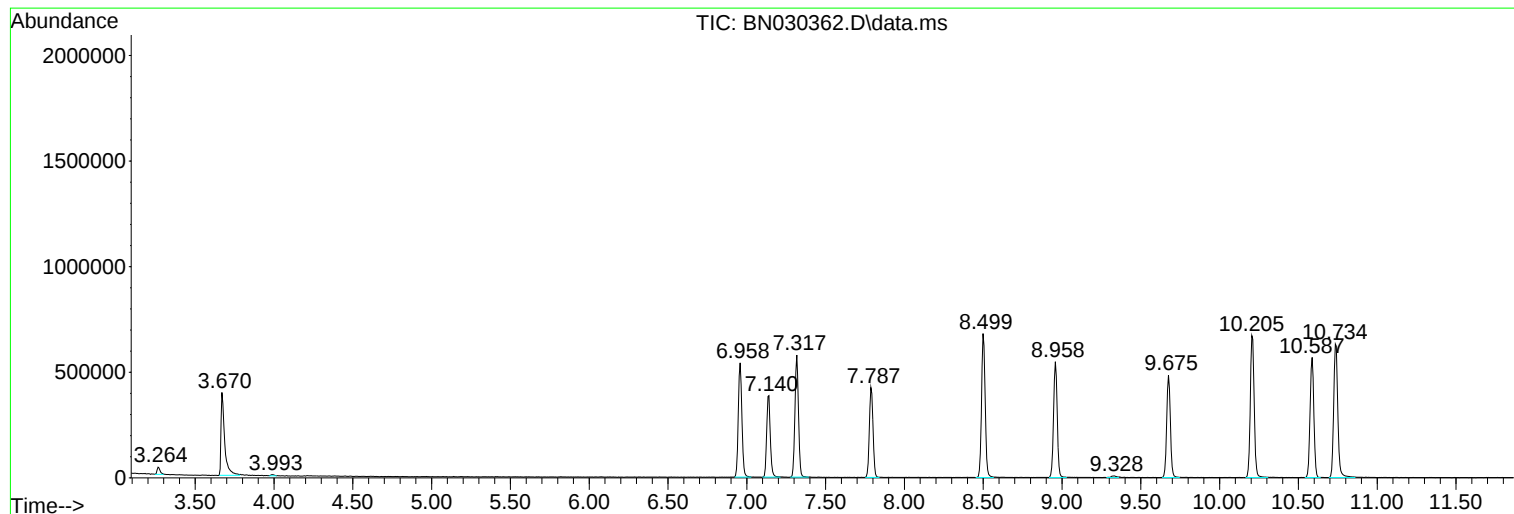

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031124\
Data File : BN030362.D
Acq On : 11 Mar 2024 16:19
Operator : MA/JU
Sample : PB159444BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK444

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031124\
Data File : BN030362.D
Acq On : 11 Mar 2024 16:19
Operator : MA/JU
Sample : PB159444BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK444

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc