

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031124\
 Data File : BN030363.D
 Acq On : 11 Mar 2024 16:56
 Operator : MA/JU
 Sample : PB159446BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK446

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	28	31	40	rVB	36653	52534	1.77%	0.159%
2	3.675	96	100	120	rBV	439521	712590	24.05%	2.163%
3	3.993	151	154	159	rVB3	7189	9314	0.31%	0.028%
4	4.217	190	192	197	rVB5	3855	5602	0.19%	0.017%
5	6.964	652	659	672	rBV	575778	902995	30.48%	2.740%
6	7.140	683	689	701	rBV	419243	655035	22.11%	1.988%
7	7.322	713	720	728	rBV	624484	967714	32.66%	2.937%
8	7.793	793	800	808	rBV	452051	711874	24.03%	2.160%
9	8.505	914	921	936	rBV	733828	1173407	39.60%	3.561%
10	8.963	992	999	1014	rBV	575685	947599	31.98%	2.876%
11	9.681	1113	1121	1138	rBV	501883	841136	28.39%	2.553%
12	10.210	1203	1211	1225	rBV	733271	1220993	41.21%	3.705%
13	10.587	1267	1275	1284	rBV	587481	985303	33.25%	2.990%
14	10.740	1292	1301	1315	rBV	700091	1227899	41.44%	3.726%
15	12.199	1543	1549	1559	rBV3	7516	19136	0.65%	0.058%
16	13.351	1741	1745	1751	rBV2	12798	18933	0.64%	0.057%
17	13.875	1827	1834	1845	rBV	1349002	1881311	63.49%	5.709%
18	14.140	1872	1879	1889	rBV	1403112	2074843	70.02%	6.297%
19	14.451	1925	1932	1939	rBV	877817	1286697	43.42%	3.905%
20	14.657	1960	1967	1989	rBV	559780	890898	30.07%	2.704%
21	15.451	2095	2102	2114	rBV	1801005	2521727	85.11%	7.653%
22	15.581	2117	2124	2137	rVV	657040	913099	30.82%	2.771%
23	15.687	2139	2142	2146	rVB2	7807	8754	0.30%	0.027%
24	16.234	2232	2235	2240	rBV3	4111	5177	0.17%	0.016%
25	17.210	2395	2401	2412	rBV	1102949	1525273	51.48%	4.629%
26	17.310	2412	2418	2431	rVV2	1863973	2693515	90.90%	8.174%
27	18.134	2554	2558	2564	rBV4	5764	9059	0.31%	0.027%
28	19.181	2731	2736	2741	rVB2	18273	25670	0.87%	0.078%
29	19.251	2741	2748	2754	rBV2	17292	26971	0.91%	0.082%
30	19.428	2774	2778	2783	rBV8	6317	10340	0.35%	0.031%
31	19.622	2805	2811	2825	rBV	2206082	2963053	100.00%	8.992%
32	21.433	3113	3119	3131	rBV	1029603	1436863	48.49%	4.360%
33	22.569	3309	3312	3318	rVB4	32005	43338	1.46%	0.132%
34	23.116	3402	3405	3412	rVB2	40995	62656	2.11%	0.190%
35	23.633	3485	3493	3504	rBV	1254404	2487172	83.94%	7.548%
36	23.739	3507	3511	3512	rVV2	62060	84850	2.86%	0.257%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031124\
Data File : BN030363.D
Acq On : 11 Mar 2024 16:56
Operator : MA/JU
Sample : PB159446BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK446

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Title : SVOA CALIBRATION

37	23.780	3512	3518	3530	rVB	641133	1329263	44.86%	4.034%
38	24.451	3628	3632	3642	rVB4	55846	113760	3.84%	0.345%
39	25.280	3771	3773	3785	rVB4	53687	105576	3.56%	0.320%




Sum of corrected areas: 32951929

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031124\
Data File : BN030363.D
Acq On : 11 Mar 2024 16:56
Operator : MA/JU
Sample : PB159446BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

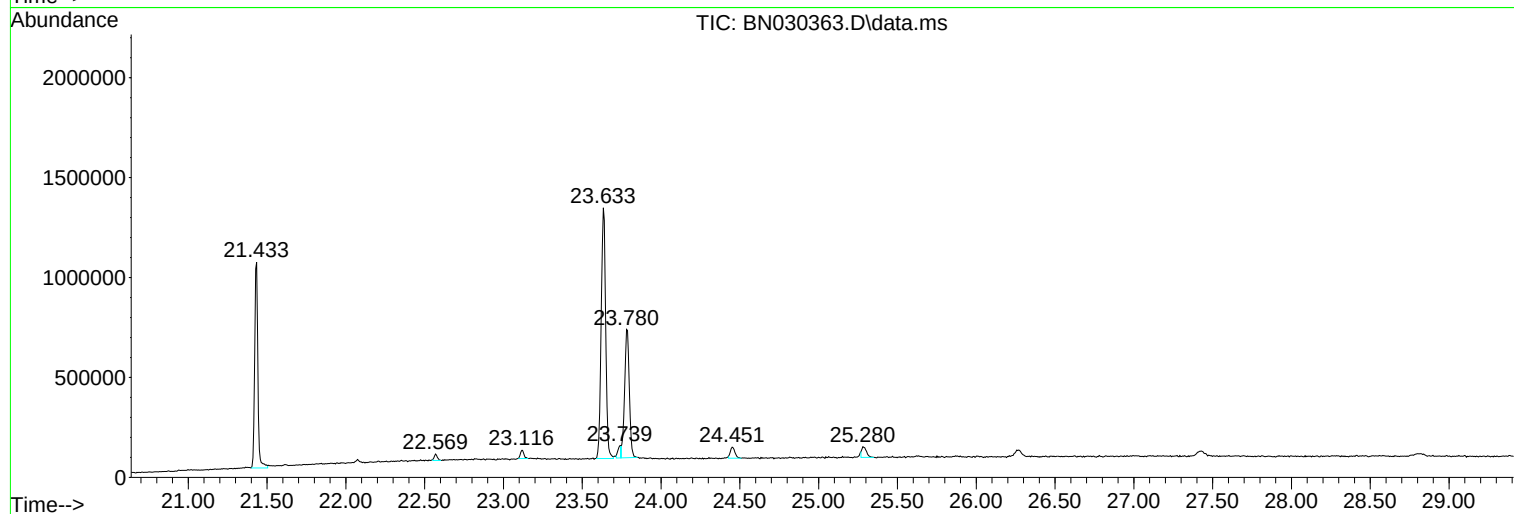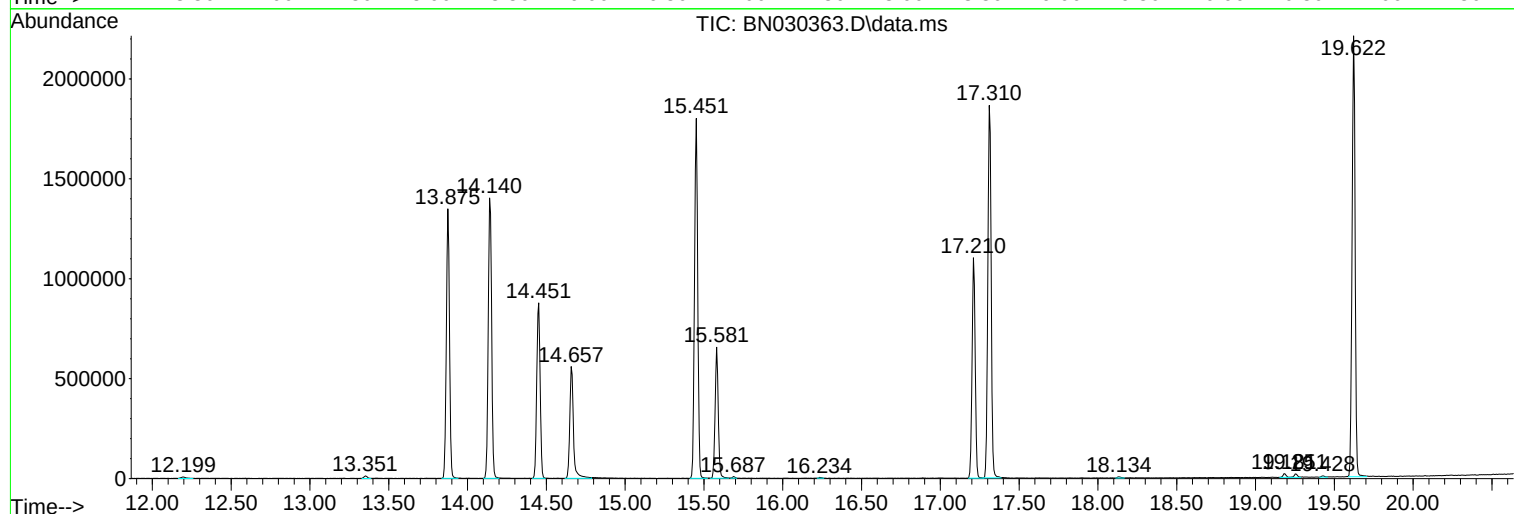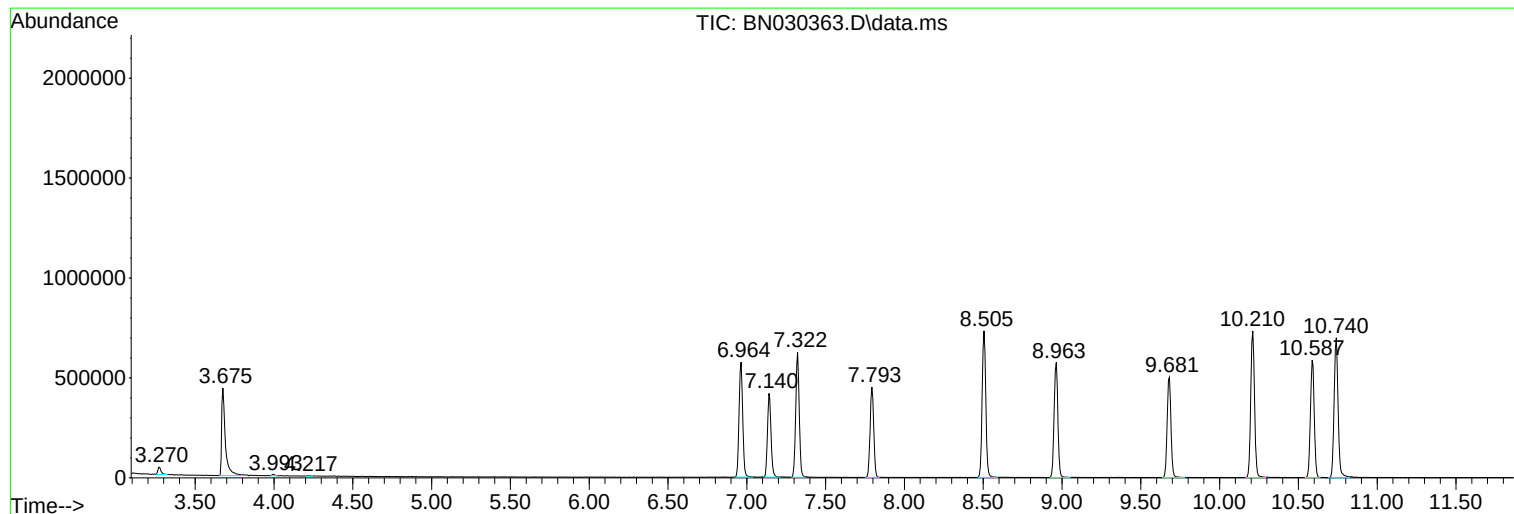

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031124\
Data File : BN030363.D
Acq On : 11 Mar 2024 16:56
Operator : MA/JU
Sample : PB159446BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031124\
Data File : BN030363.D
Acq On : 11 Mar 2024 16:56
Operator : MA/JU
Sample : PB159446BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc