


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031125\
Data File : BN036573.D
Acq On : 11 Mar 2025 08:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 16:06:28 2025

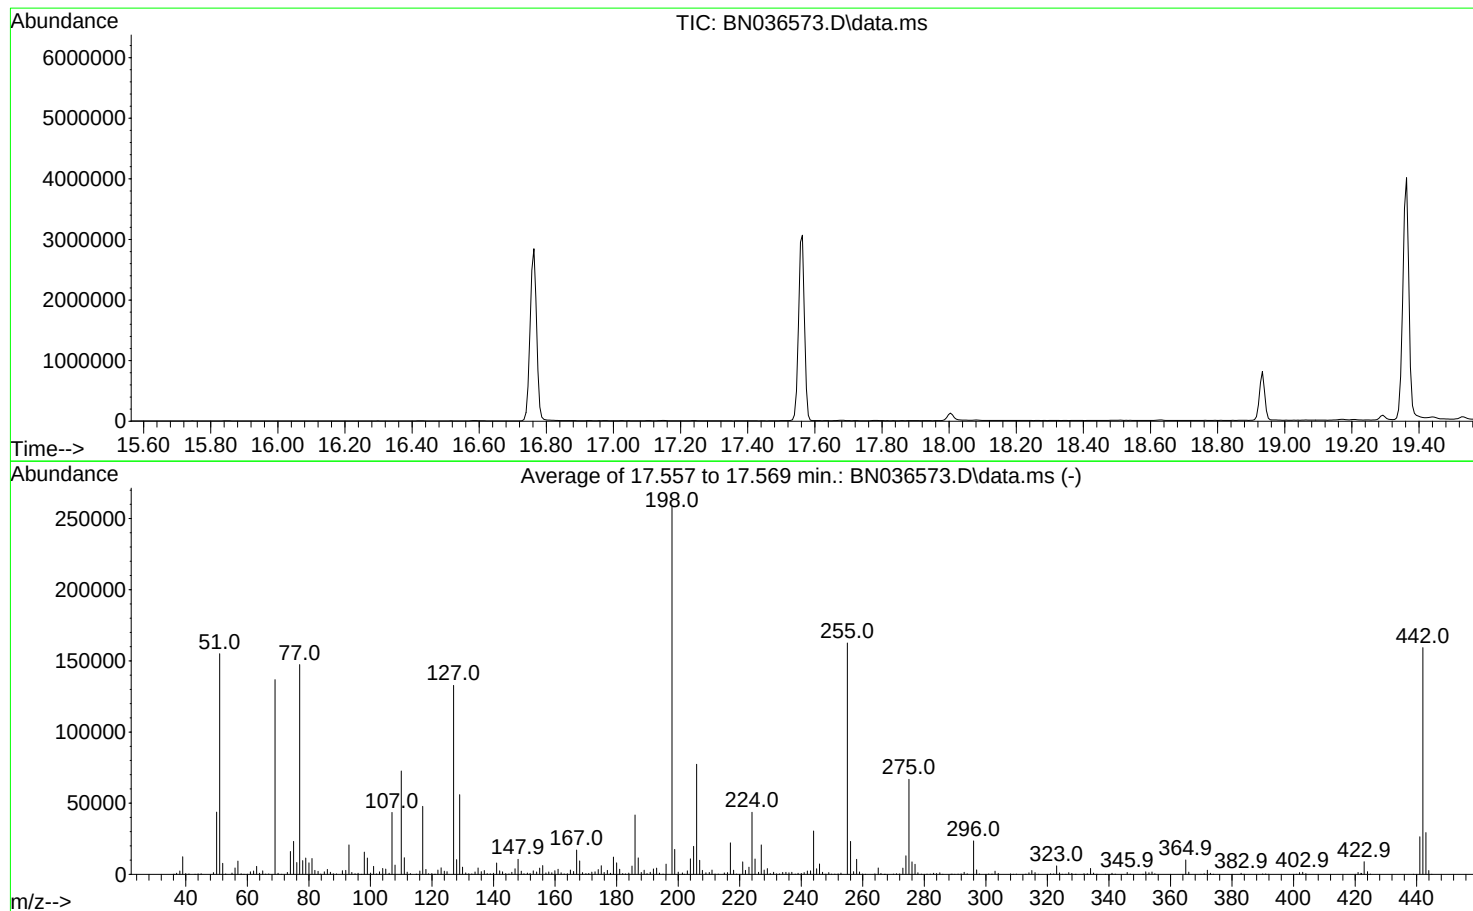

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.0	155027	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	53.0	136882	PASS
70	69	0.00	2	0.6	784	PASS
127	198	10	80	51.4	132840	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	258496	PASS
199	198	5	9	6.8	17565	PASS
275	198	10	60	25.8	66808	PASS
365	198	1	100	3.9	10081	PASS
441	198	0.01	100	10.2	26384	PASS
442	442	50	100	100.0	159296	PASS
443	442	15	24	18.4	29344	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/11/2025	BNA_N	<u>BN036573.D</u>
Compound Name	Response	Retention Time
DDT	1170989	20.598
DDD	12216	20.21
DDE	544	19.651
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12760	1183749	1.08

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031125\
Data File : BN036573.D
Acq On : 11 Mar 2025 08:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 11 17:55:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

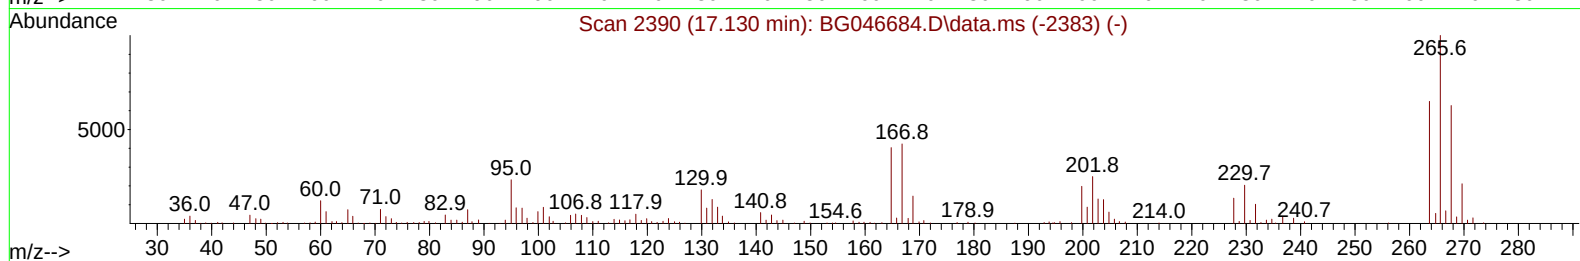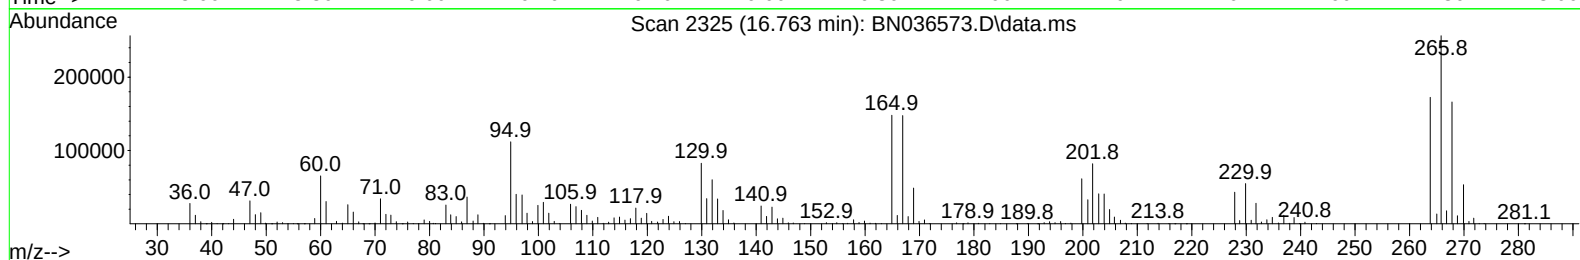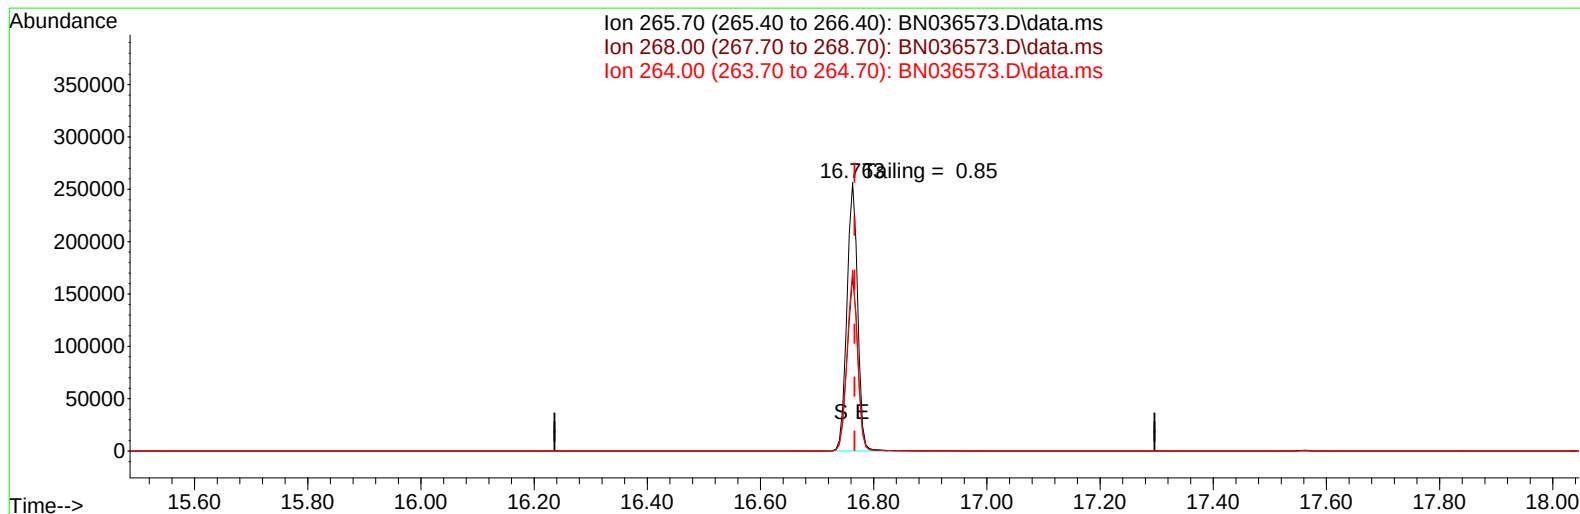

TIC: BN036573.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.003) 22415.21 ng




response 337921

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.83
264.00	61.60	67.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031125\
Data File : BN036573.D
Acq On : 11 Mar 2025 08:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 11 17:55:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

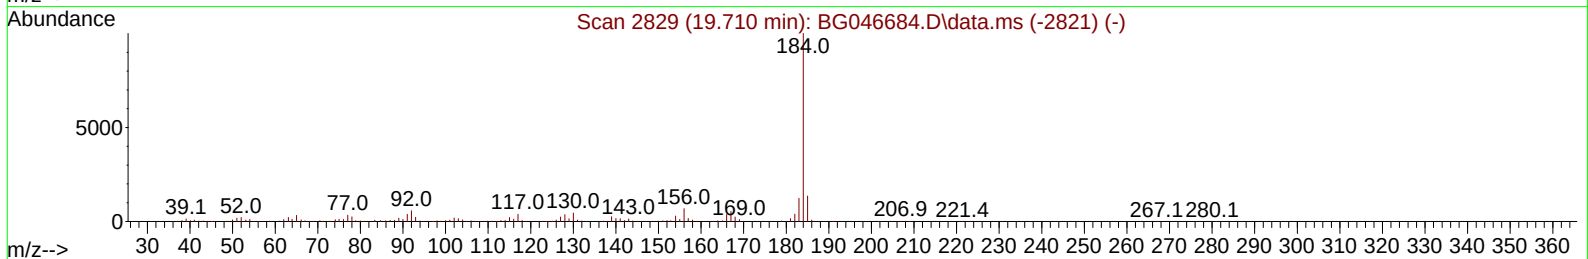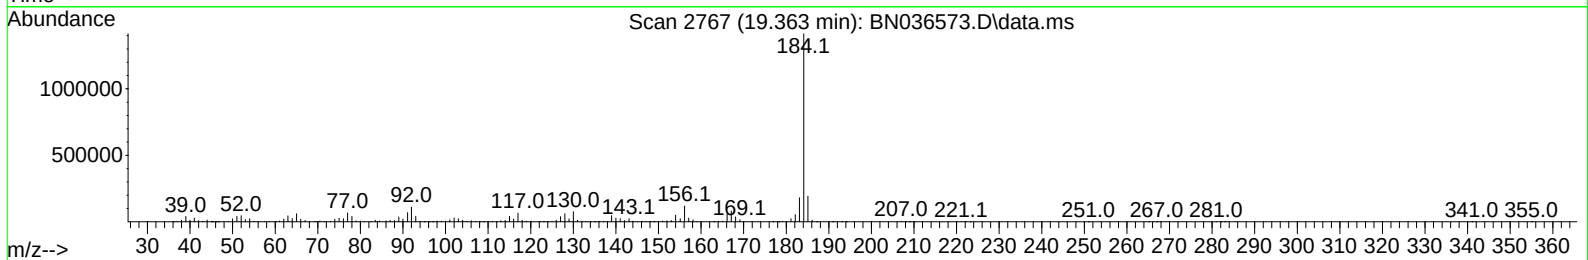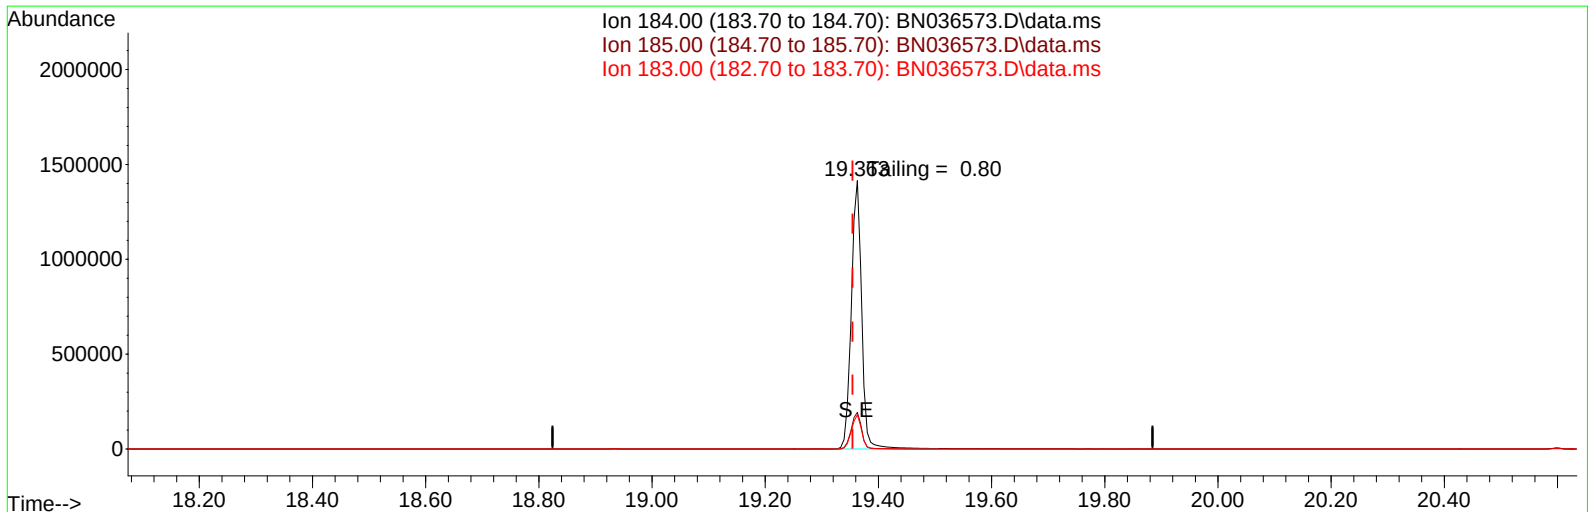

TIC: BN036573.D\data.ms

(77) Benzidine

19.363min (+ 0.009) 0.00 ng

response 1813573

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.66
183.00	13.20	12.80
0.00	0.00	0.00