

Data Path : Z:\HPCHEM1\BNA_N\DATA\BN031218\
 Data File : BN000309.D
 Acq On : 12 Mar 2018 14:19
 Operator : JU/SJ
 Sample : J1843-10MSD
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAM67MSD

Manual Integrations
 APPROVED

Sohil
 3/13/2018 5:32:45 PM

Quant Time: Mar 12 15:13:57 2018
 Quant Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 12 15:04:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.45	152	284326	20.00	ng/ul	0.00
2) Naphthalene-d8	11.29	136	1367605	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.06	164	761167	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.78	188	1587601	20.00	ng/ul	0.00
17) Chrysene-d12	21.90	240	1617981	20.00	ng/ul	0.00
22) Perylene-d12	24.37	264	1532301	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	14.76	160	2970954	39.33	ng/ul	0.00
10) Fluorene-d10	16.04	176	1930495	37.74	ng/ul	0.00
14) Anthracene-d10	17.88	188	2867753	38.66	ng/ul	0.00
18) Pyrene-d10	20.13	212	3120952	39.43	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.22	264	2796054	39.96	ng/ul	0.01
Target Compounds						
9) Acenaphthene	15.12	153	2117073	40.067	ng/ul	96
13) Phenanthrene	17.82	178	289288	3.177	ng/ul	100
16) Fluoranthene	19.80	202	596542	6.064	ng/ul	96
19) Pyrene	20.16	202	4661253	45.631	ng/ul#	87
20) Benzo(a)anthracene	21.88	228	326019	3.241	ng/ul	98
21) Chrysene	21.93	228	310795	3.256	ng/ul	97
23) Benzo(b)fluoranthene	23.62	252	445889m	4.880	ng/ul	
24) Benzo(k)fluoranthene	23.66	252	141332m	1.652	ng/ul	
26) Benzo(a)pyrene	24.27	252	279681	3.216	ng/ul#	93
27) Indeno(1,2,3-cd)pyrene	26.93	276	178064	1.899	ng/ul#	84
29) Benzo(g,h,i)perylene	27.71	276	164827	2.105	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_N\DATA\BN031218\
Data File : BN000309.D
Acq On : 12 Mar 2018 14:19
Operator : JU/SJ
Sample : J1843-10MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DAM67MSD

Manual Integrations
APPROVED

Sohil
3/13/2018 5:32:45 PM

Quant Time: Mar 12 15:13:57 2018
Quant Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 12 15:04:53 2018
Response via : Initial Calibration

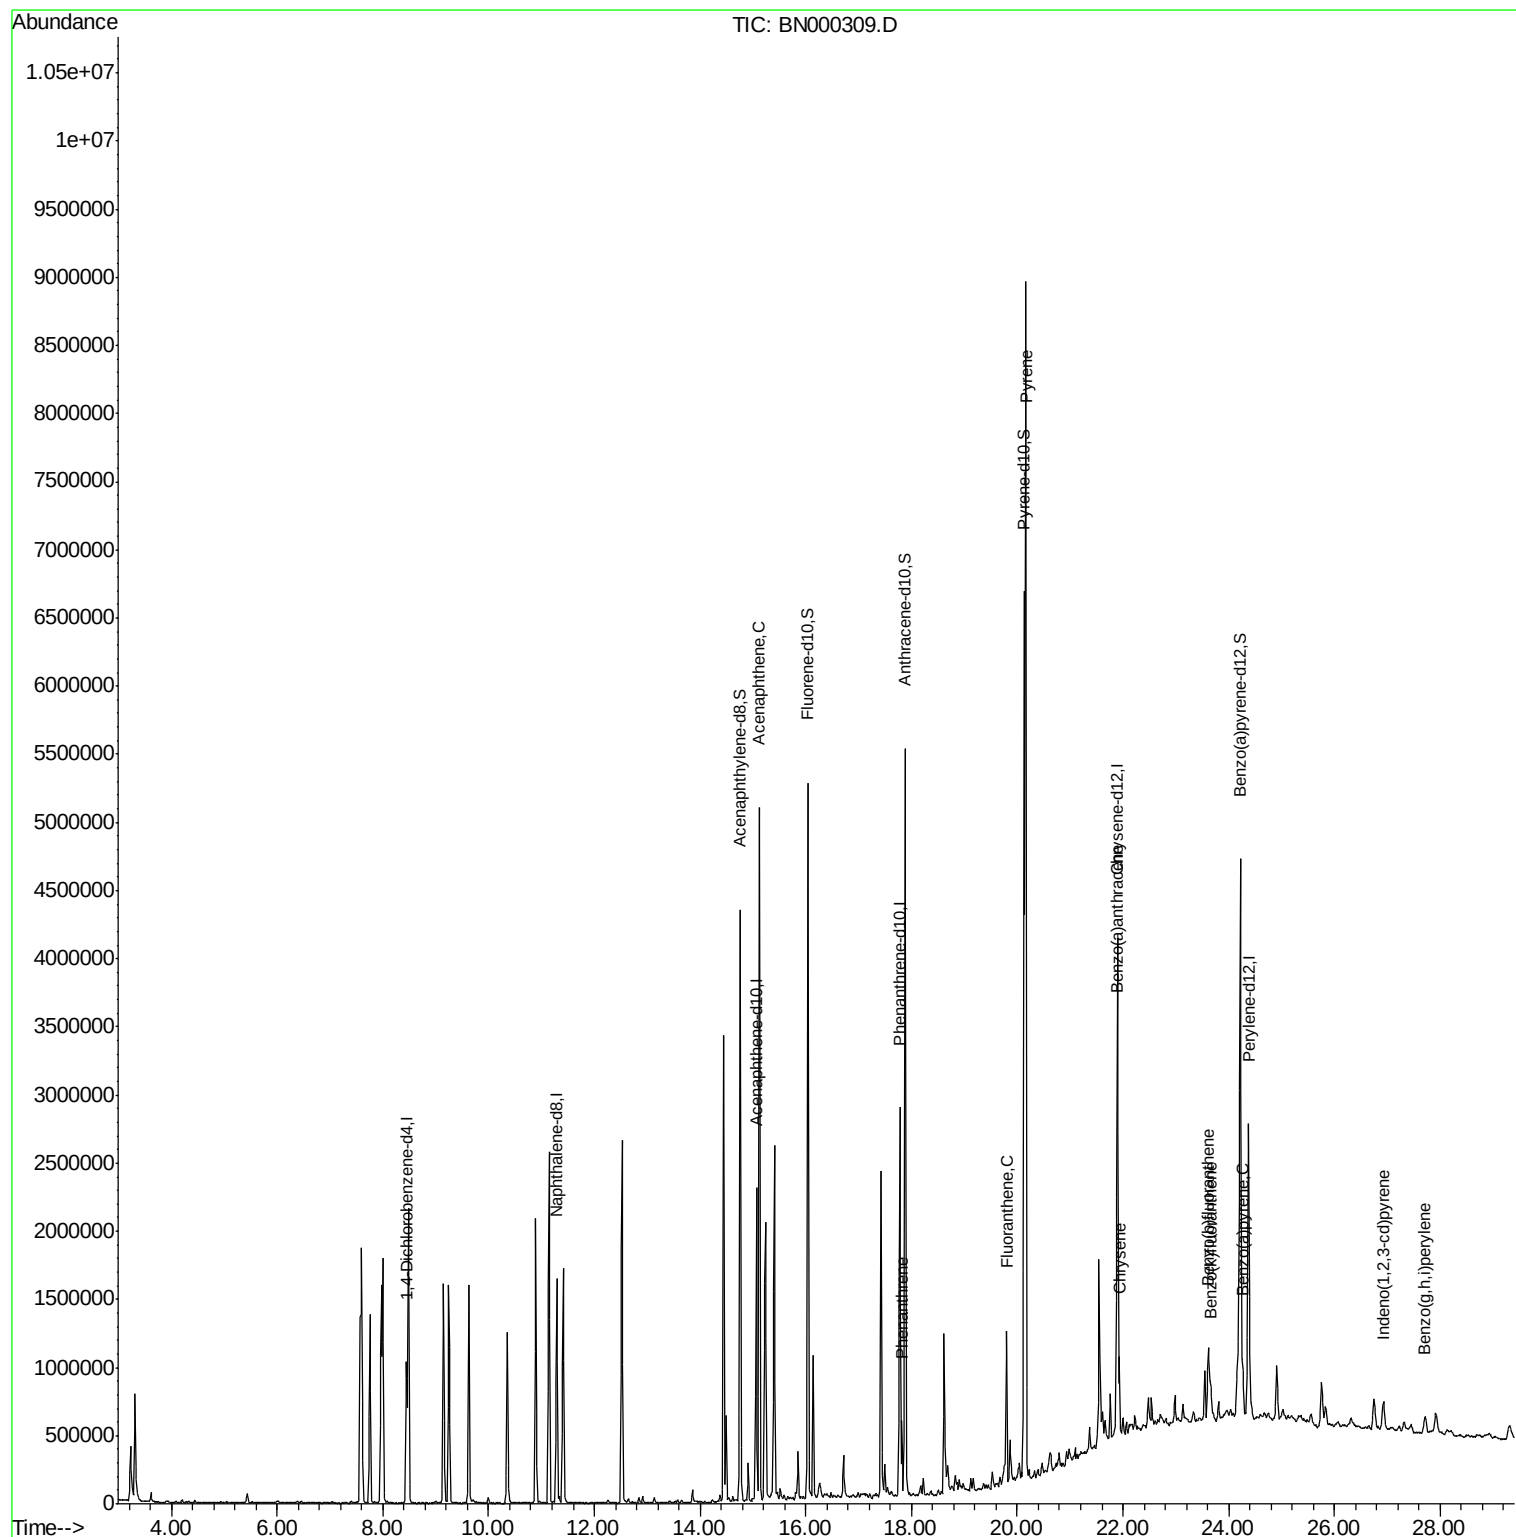



#9

Acenaphthene

Concen: 40.067 ng/ul

RT: 15.12 min Scan# 2063

Delta R.T. -0.00 min

Lab File: BN000309.D

Acq: 12 Mar 2018 14:19

Instrument :

BNA_N

ClientSampleId :

DAM67MSD

Tgt Ion:153 Resp: 2117073

Ion Ratio Lower Upper

153 100

152 47.2 39.0 58.6


154 87.6 66.8 100.2

Manual Integrations

APPROVED

Sohil




3/13/2018 5:32:45 PM

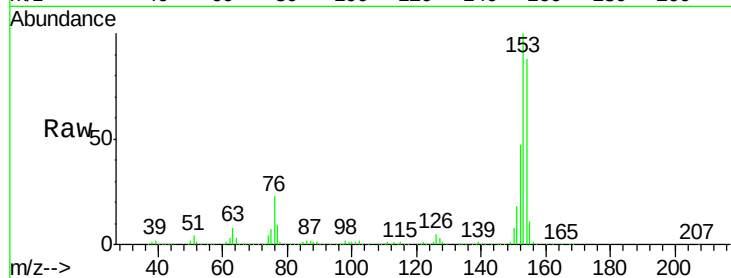

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

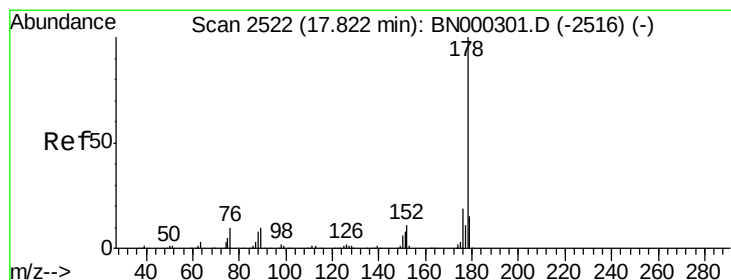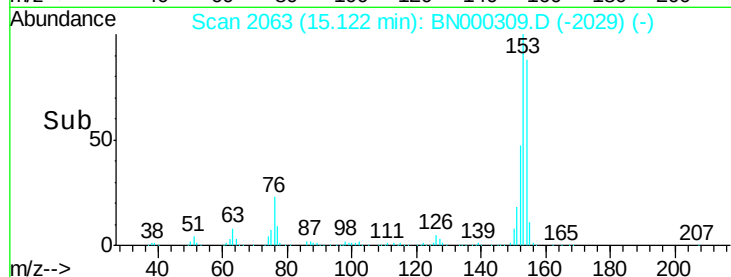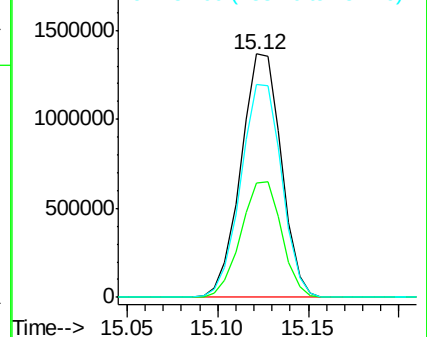

#13

Phenanthrene

Concen: 3.177 ng/ul

RT: 17.82 min Scan# 2522

Delta R.T. -0.00 min

Lab File: BN000309.D

Acq: 12 Mar 2018 14:19


Tgt Ion:178 Resp: 289288

Ion Ratio Lower Upper

178 100

179 15.1 12.3 18.5



176 18.8 15.1 22.7

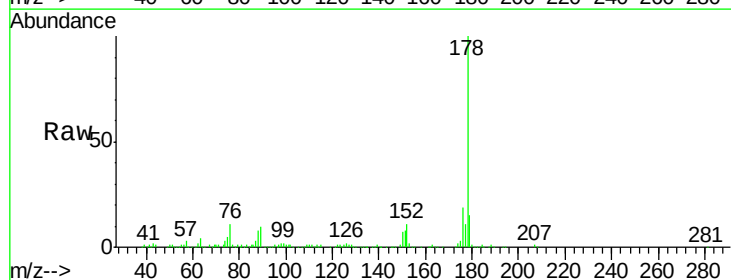


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

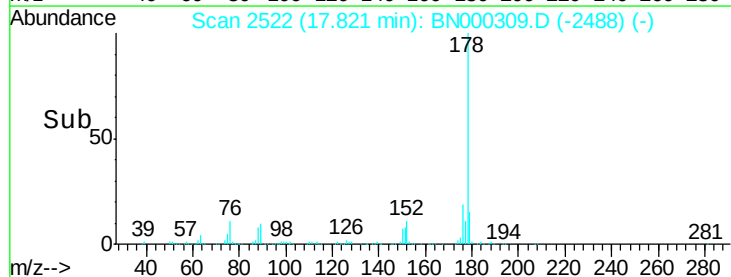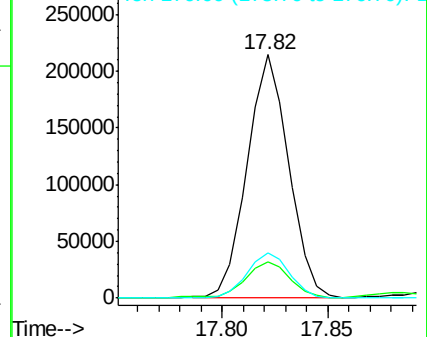



#16

Fluoranthene

Concen: 6.064 ng/ul

RT: 19.80 min Scan# 2858

Delta R.T. -0.00 min

Lab File: BN000309.D

Acq: 12 Mar 2018 14:19

Instrument :

BNA_N


ClientSampleId :

DAM67MSD




Tgt	Ion	202	Resp	596542
Ion	Ratio	Lower	Upper	
202	100			
101	14.4	9.9	14.9	
100	10.5	7.4	11.0	

Manual Integrations
APPROVED

Sohil
3/13/2018 5:32:45 PM

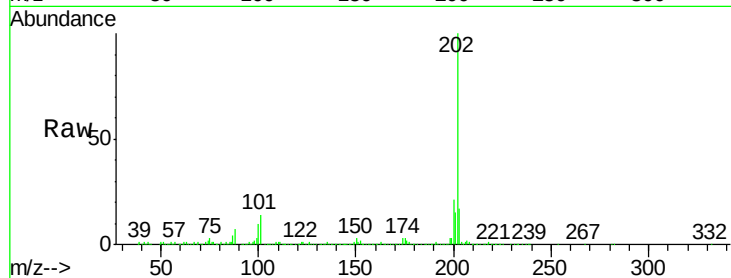

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

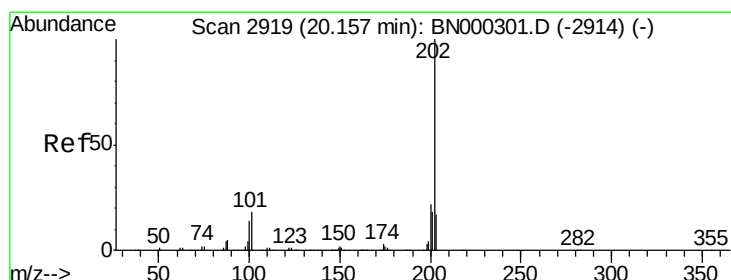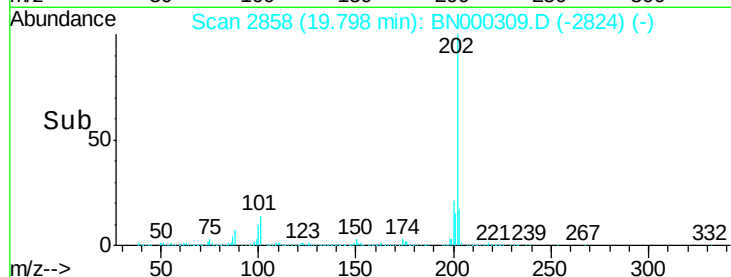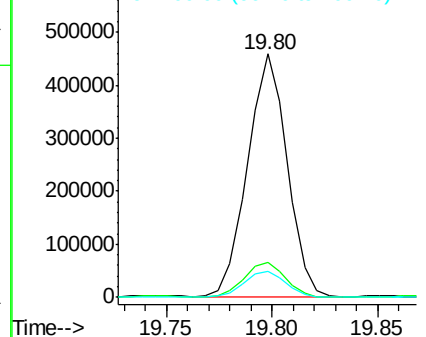

#19

Pyrene

Concen: 45.631 ng/ul

RT: 20.16 min Scan# 2920




Delta R.T. 0.01 min


Lab File: BN000309.D

Acq: 12 Mar 2018 14:19

Tgt	Ion	202	Resp	4661253
Ion	Ratio	Lower	Upper	
202	100			
101	18.4	11.0	16.4#	
100	15.3	8.1	12.1#	

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

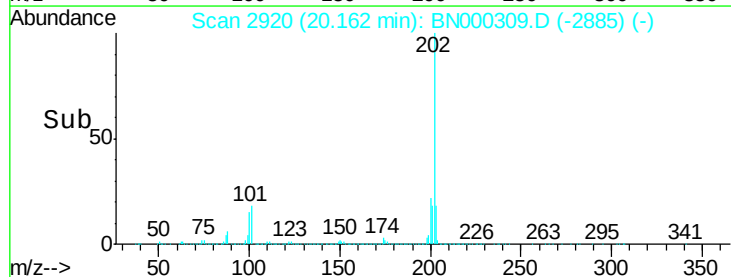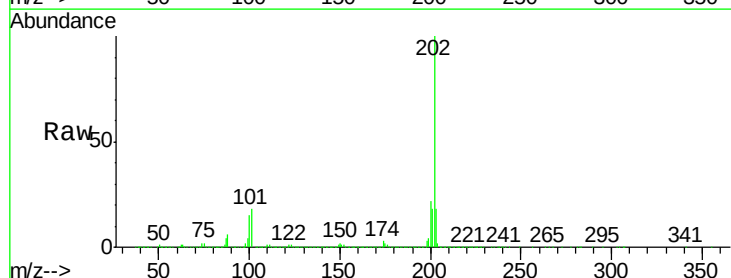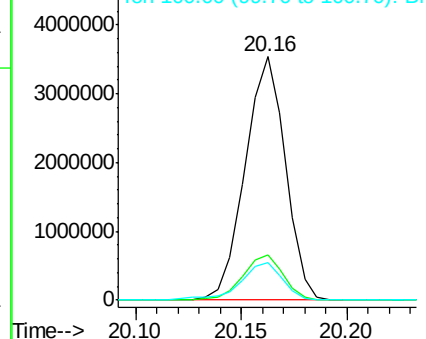







#20
Benzo(a)anthracene
Concen: 3.241 ng/ul
RT: 21.88 min Scan# 3212
Delta R.T. 0.01 min
Lab File: BN000309.D
Acq: 12 Mar 2018 14:19

Instrument :
BNA_N
ClientSampleId :
DAM67MSD

Tgt Ion	Ratio	Lower	Upper
228	100		
229	20.3	15.7	23.5
226	27.4	21.1	31.7




Manual Integrations
APPROVED


Sohil
3/13/2018 5:32:45 PM

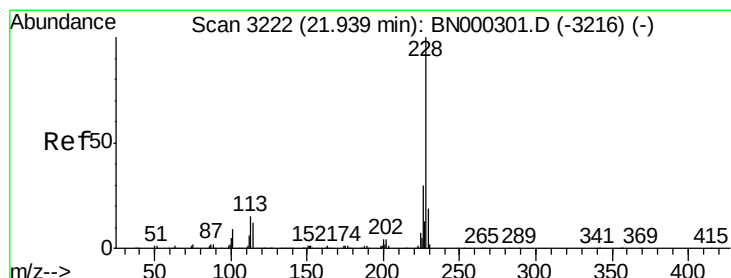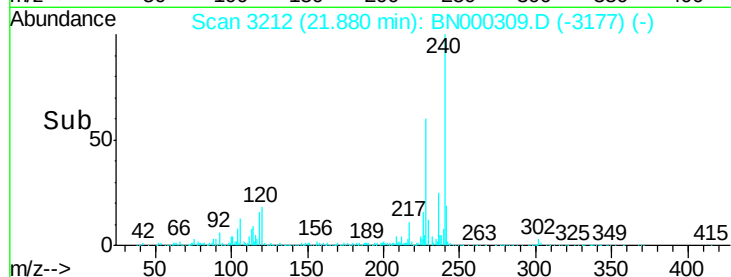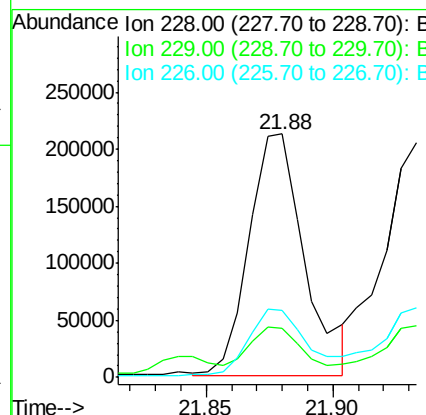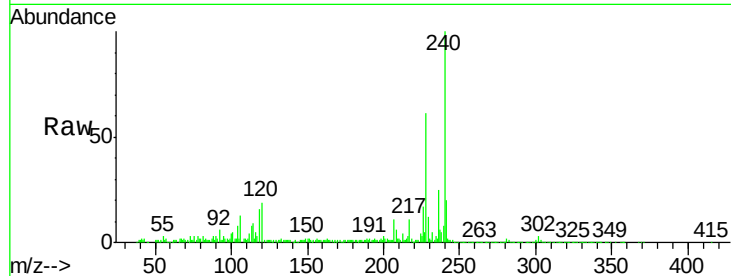

#21
Chrysene
Concen: 3.256 ng/ul
RT: 21.93 min Scan# 3221
Delta R.T. -0.00 min
Lab File: BN000309.D
Acq: 12 Mar 2018 14:19

Tgt Ion	Ratio	Lower	Upper
228	100		
226	29.9	24.5	36.7
229	22.0	15.8	23.8

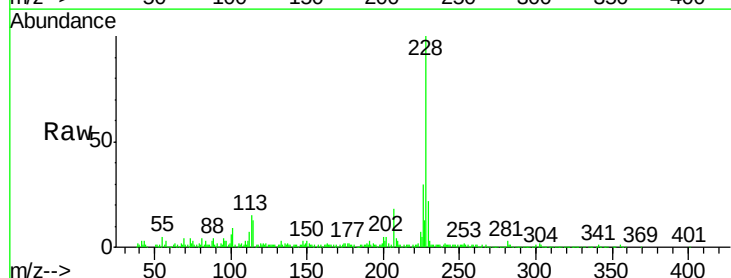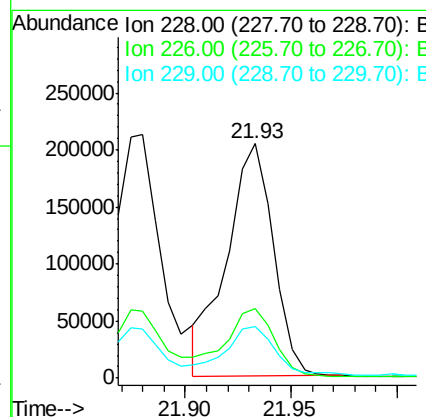







#23
Benzo(b)fluoranthene
Concen: 4.880 ng/ul m
RT: 23.62 min Scan# 3507
Delta R.T. -0.00 min
Lab File: BN000309.D
Acq: 12 Mar 2018 14:19

Instrument :
BNA_N
ClientSampleId :
DAM67MSD

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.3	18.0	27.0
125	16.3	8.0	12.0




Manual Integrations
APPROVED


Sohil
3/13/2018 5:32:45 PM

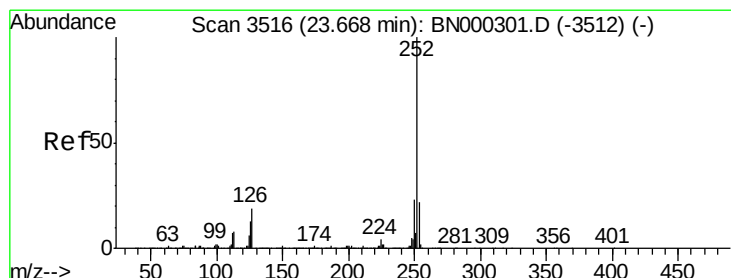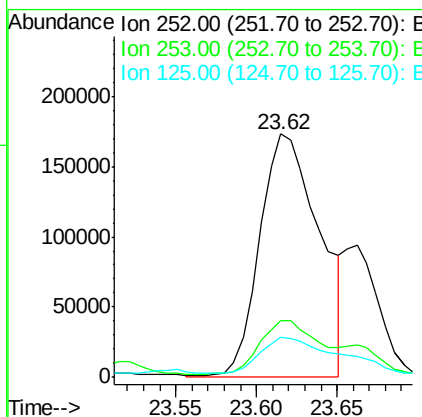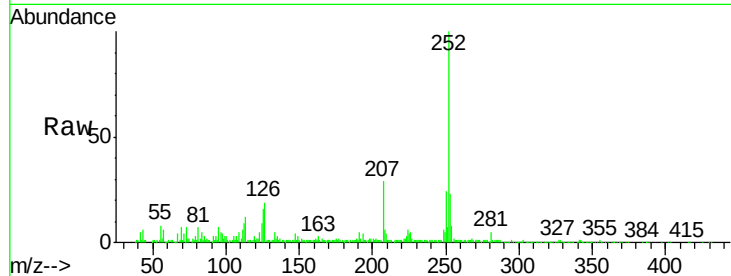

#24
Benzo(k)fluoranthene
Concen: 1.652 ng/ul m
RT: 23.66 min Scan# 3515
Delta R.T. -0.00 min
Lab File: BN000309.D
Acq: 12 Mar 2018 14:19

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.5	18.0	27.0
125	16.0	8.1	12.1

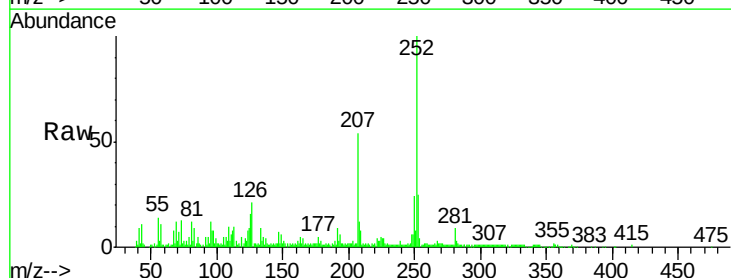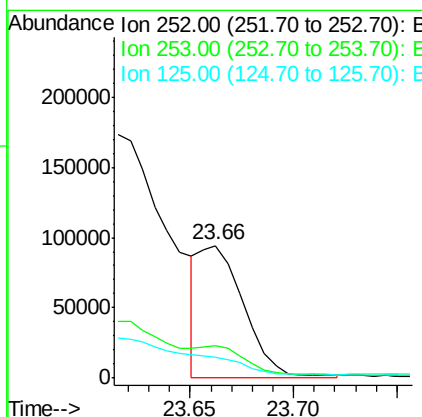







#26
Benzo(a)pyrene
Concen: 3.216 ng/ul
RT: 24.27 min Scan# 3618
Delta R.T. 0.01 min
Lab File: BN000309.D
Acq: 12 Mar 2018 14:19

Instrument :
BNA_N
ClientSampleId :
DAM67MSD

Tgt Ion	Ratio	Resp Lower	Resp Upper
252	100		
253	22.9	17.2	25.8
125	16.4	8.2	12.4




Manual Integrations
APPROVED


Sohil
3/13/2018 5:32:45 PM

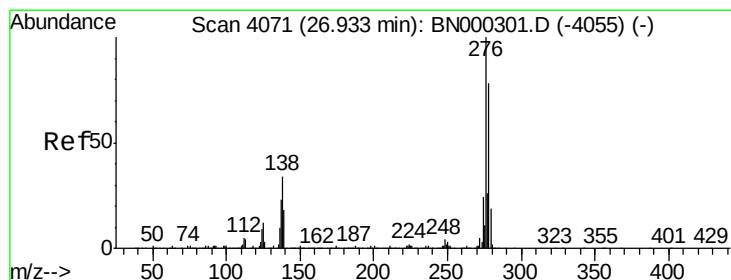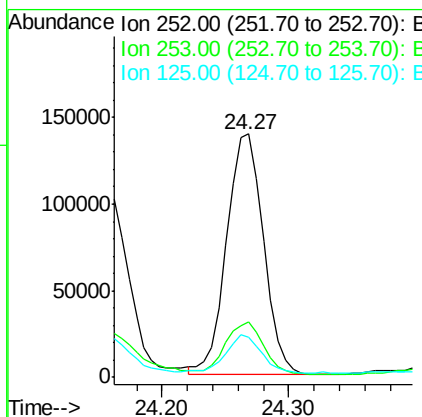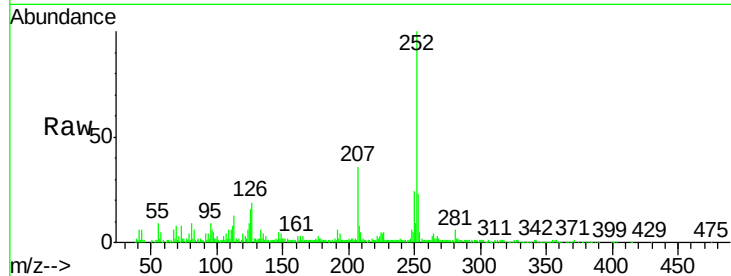

#27
Indeno(1,2,3-cd)pyrene
Concen: 1.899 ng/ul
RT: 26.93 min Scan# 4070
Delta R.T. -0.00 min
Lab File: BN000309.D
Acq: 12 Mar 2018 14:19

Tgt Ion	Ratio	Resp Lower	Resp Upper
276	100		
138	30.3	14.4	21.6
277	25.9	18.0	27.0

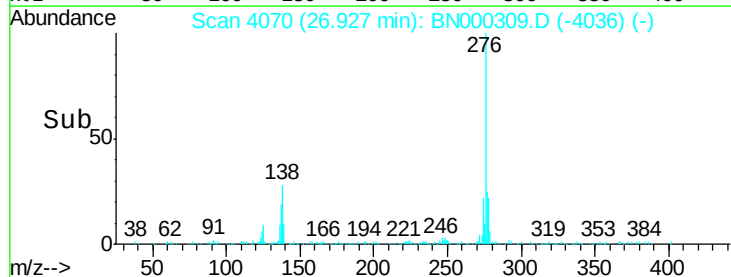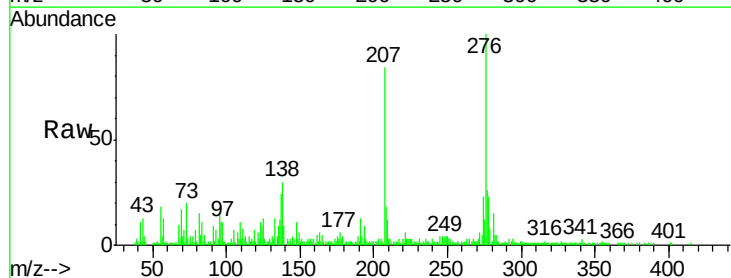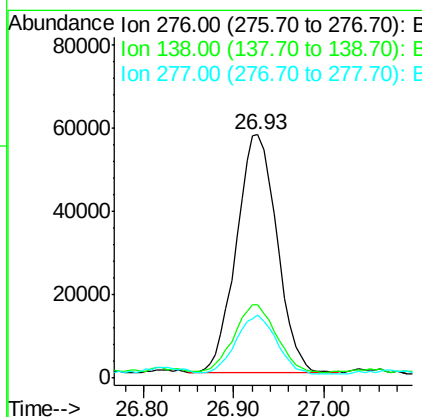



#29

Benzo(g,h,i)perylene

Concen: 2.105 ng/ul

RT: 27.71 min Scan# 4204

Delta R.T. -0.00 min

Lab File: BN000309.D

Acq: 12 Mar 2018 14:19

Instrument :

BNA_N

ClientSampleId :

DAM67MSD

Tgt Ion:	276	Resp:	164827
Ion Ratio	Lower	Upper	
276	100		
138	32.9	15.3	22.9#
277	24.8	19.0	28.4

Manual Integrations
APPROVED

Sohil
3/13/2018 5:32:45 PM

