

Data Path : Z:\HPCHEM1\BNA_N\DATA\BN031218\
 Data File : BN000320.D
 Acq On : 12 Mar 2018 20:40
 Operator : JU/SJ
 Sample : J1864-17
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAMH3

Quant Time: Mar 13 11:59:50 2018
 Quant Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 09 23:47:40 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.45	152	262171	20.00	ng/ul	0.00
2) Naphthalene-d8	11.29	136	1273478	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.06	164	711128	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.78	188	1493351	20.00	ng/ul	0.00
17) Chrysene-d12	21.89	240	1547457	20.00	ng/ul	0.00
22) Perylene-d12	24.37	264	1465460	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	14.76	160	2299697	32.58	ng/ul	0.00
10) Fluorene-d10	16.04	176	1495628	31.29	ng/ul	0.00
14) Anthracene-d10	17.88	188	2268464	32.51	ng/ul	0.00
18) Pyrene-d10	20.13	212	2452222	32.39	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.22	264	2207278	32.98	ng/ul	0.00
Target Compounds						
16) Fluoranthene	19.80	202	114580	1.238	ng/ul#	94
19) Pyrene	20.16	202	101394	1.038	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_N\DATA\BN031218\
Data File : BN000320.D
Acq On : 12 Mar 2018 20:40
Operator : JU/SJ
Sample : J1864-17
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DAMH3

Quant Time: Mar 13 11:59:50 2018
Quant Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 09 23:47:40 2018
Response via : Initial Calibration




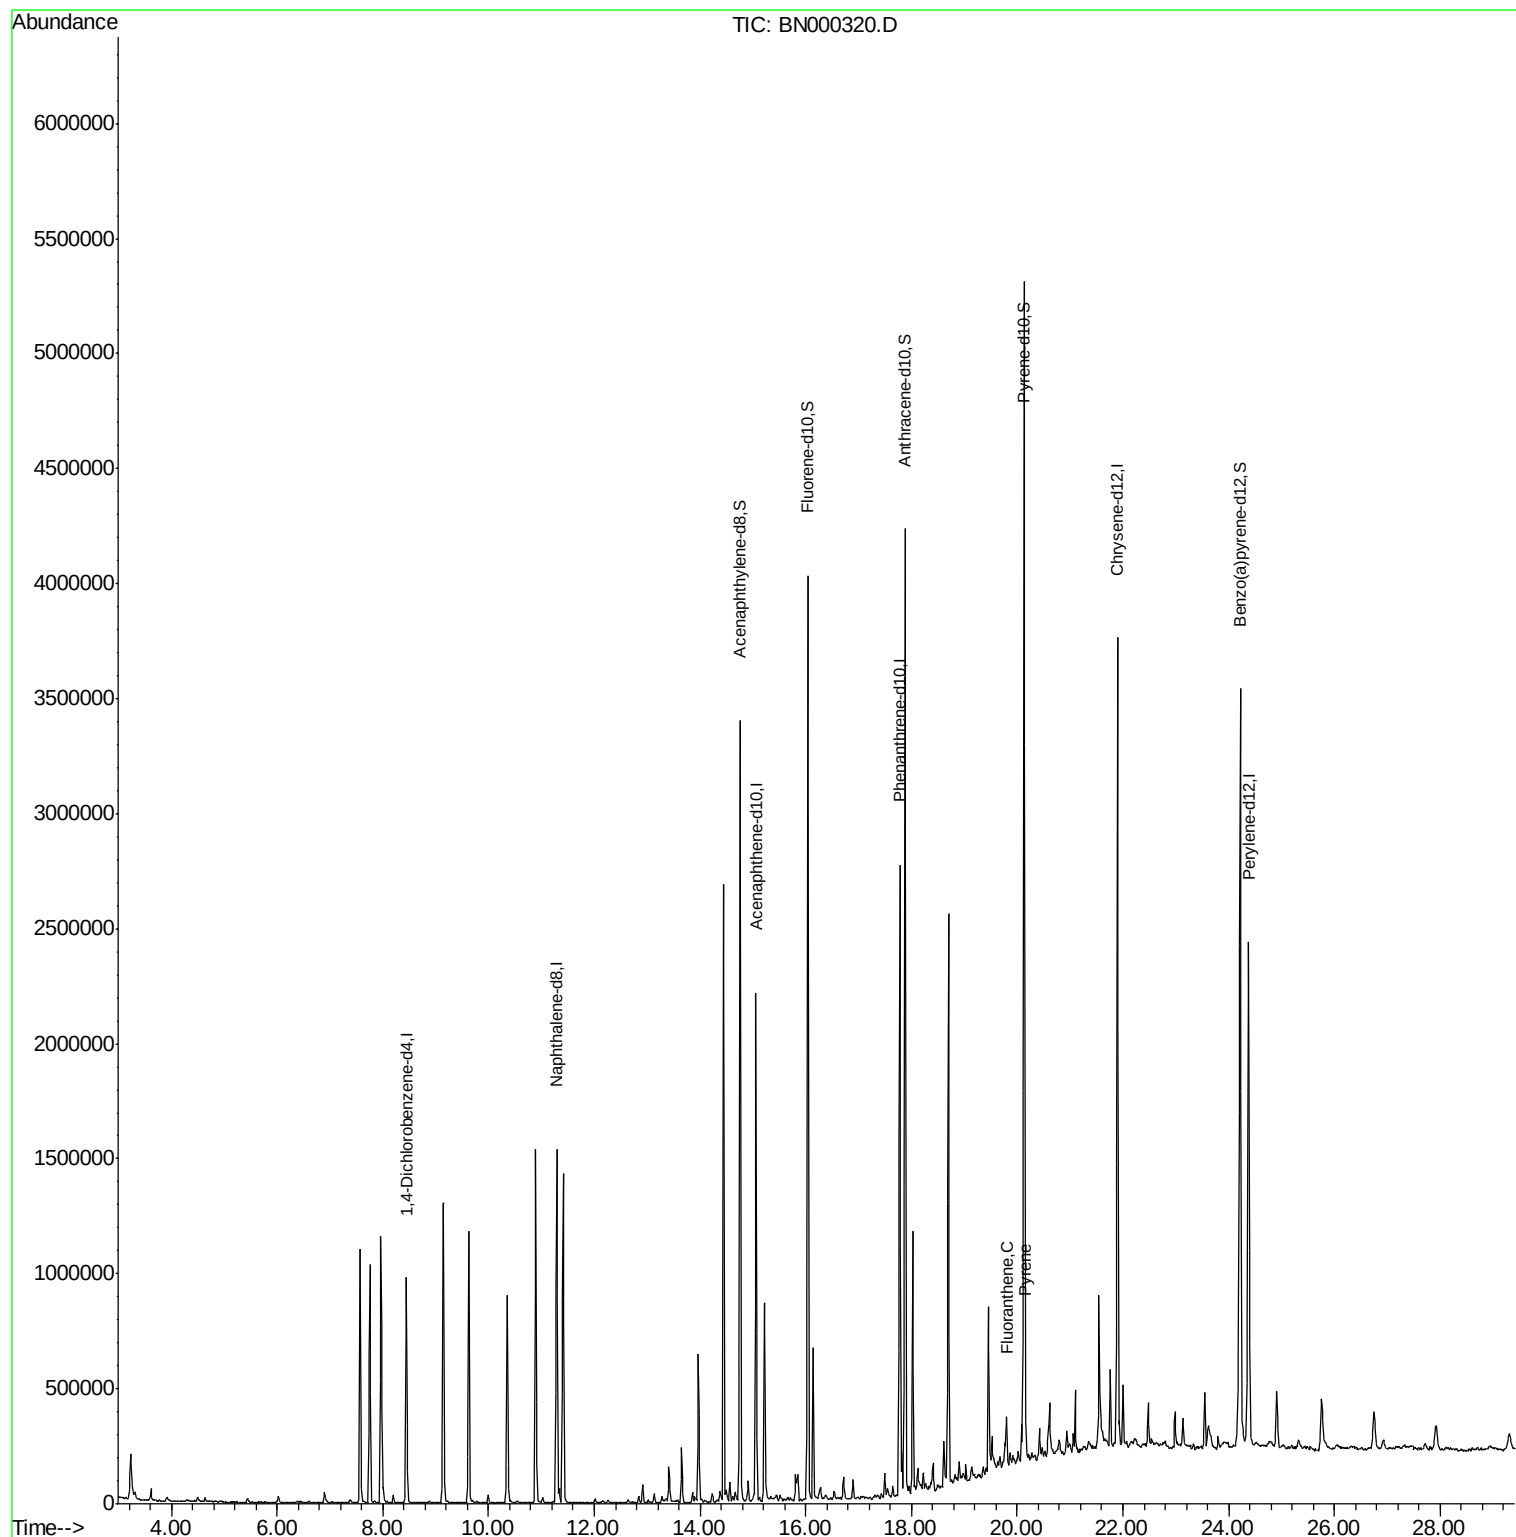


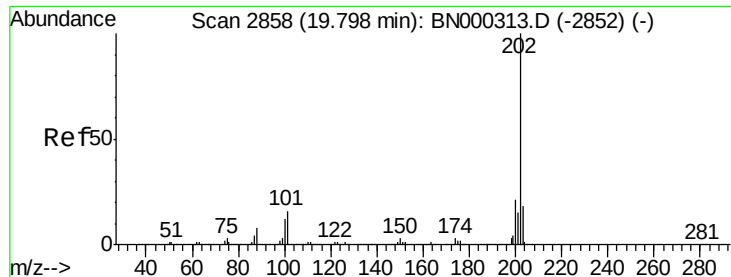

#16
Fluoranthene
Concen: 1.238 ng/ul
RT: 19.80 min Scan# 2858
Delta R.T. -0.00 min
Lab File: BN000320.D
Acq: 12 Mar 2018 20:40

Instrument :
BNA_N
ClientSampleId :
DAMH3

Tgt Ion	Ratio	Lower	Upper
202	100		
101	14.8	9.9	14.9
100	11.2	7.4	11.0#

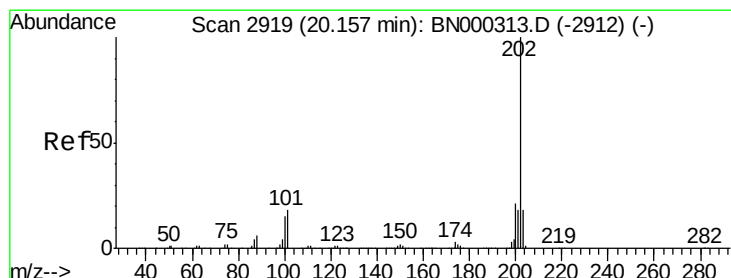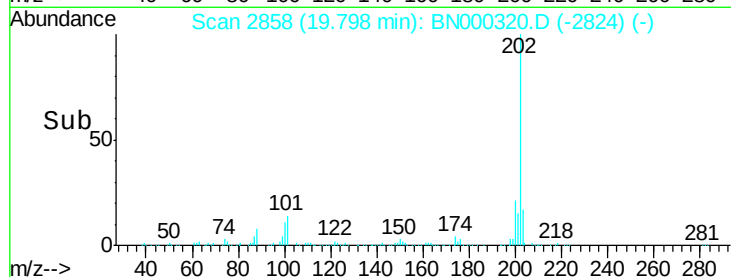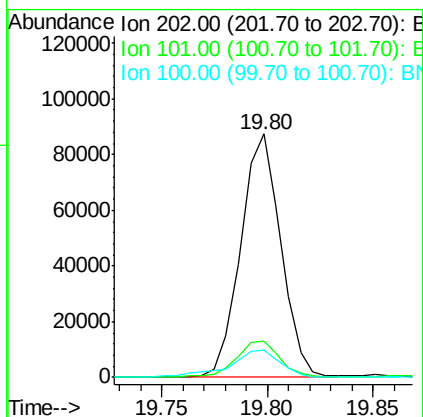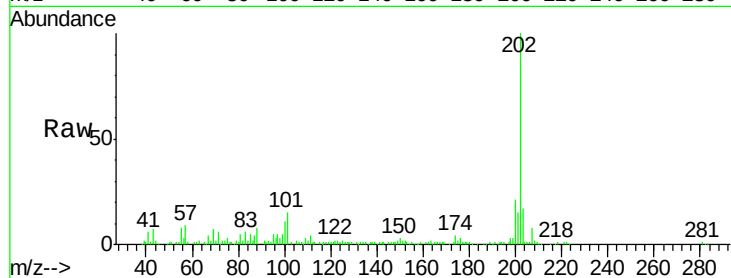

#19
Pyrene
Concen: 1.038 ng/ul
RT: 20.16 min Scan# 2919
Delta R.T. -0.00 min
Lab File: BN000320.D
Acq: 12 Mar 2018 20:40

Tgt Ion	Ratio	Lower	Upper
202	100		
101	17.6	11.0	16.4#
100	13.9	8.1	12.1#

