
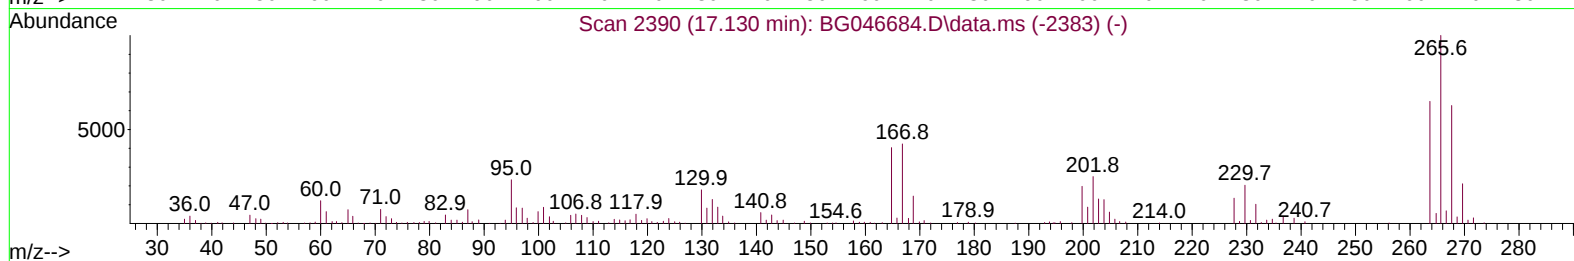
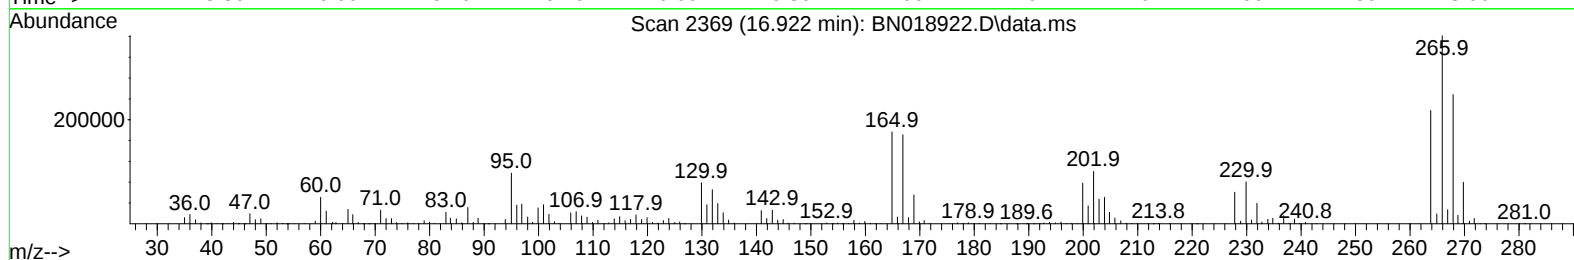


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031222\
Data File : BN018922.D
Acq On : 11 Mar 2022 13:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 15:03:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 11 15:03:53 2022
Response via : Initial Calibration

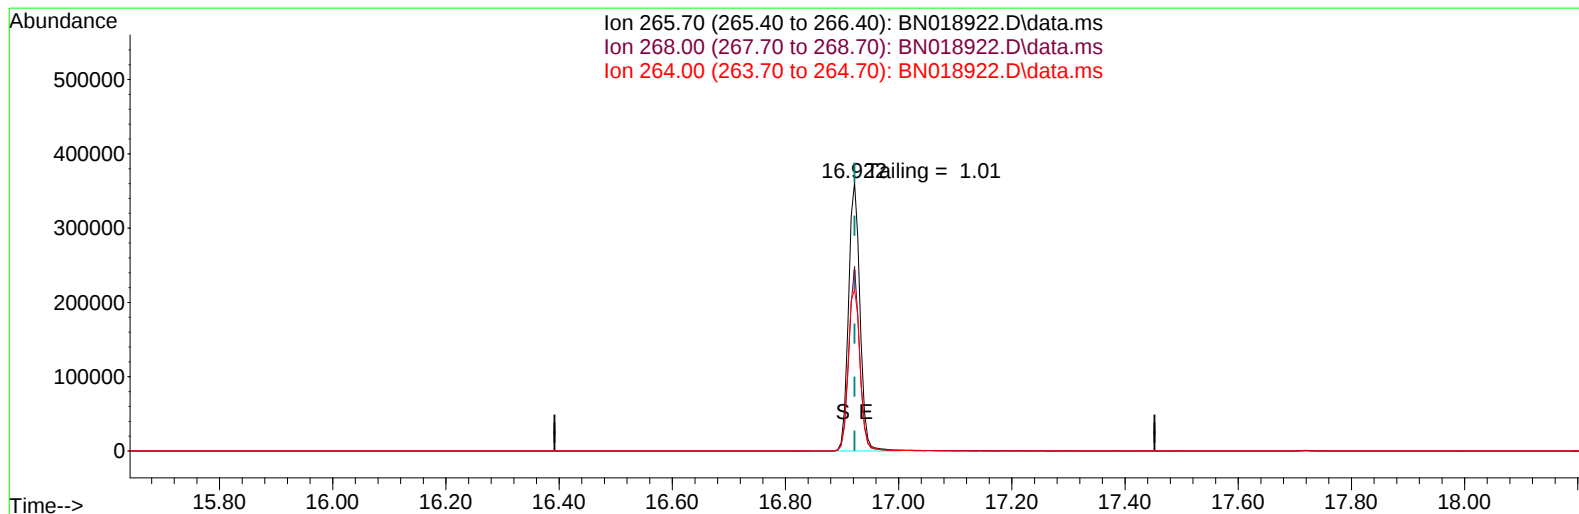

TIC: BN018922.D\data.ms

(70) Pentachlorophenol (C)

16.922min (0.000) 21379.49 ng

response 513745

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.66
264.00	61.60	60.27
0.00	0.00	0.00