
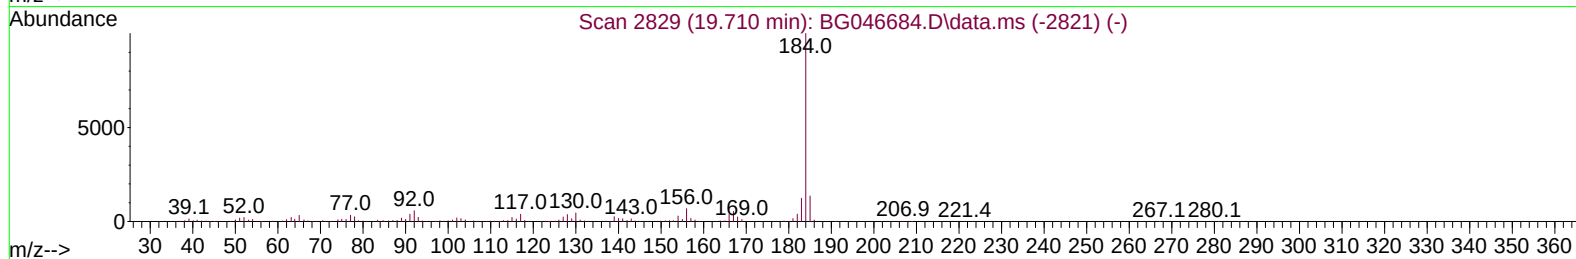
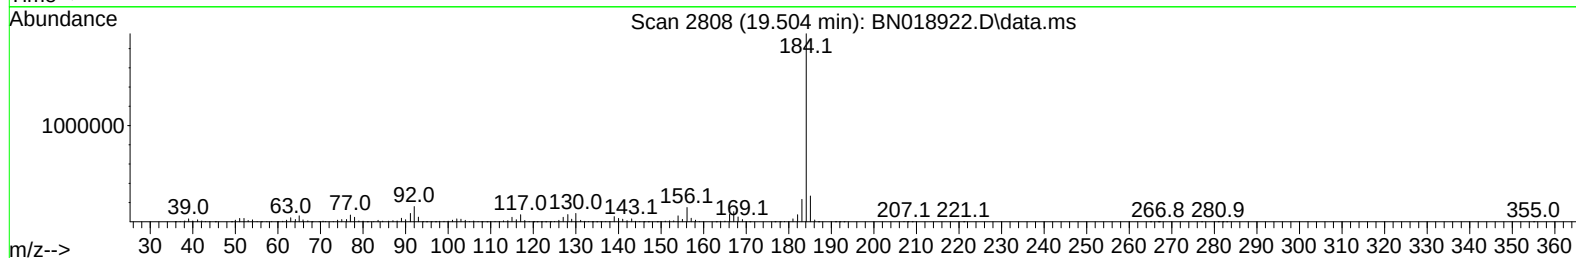


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031222\
Data File : BN018922.D
Acq On : 11 Mar 2022 13:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 15:03:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 11 15:03:53 2022
Response via : Initial Calibration

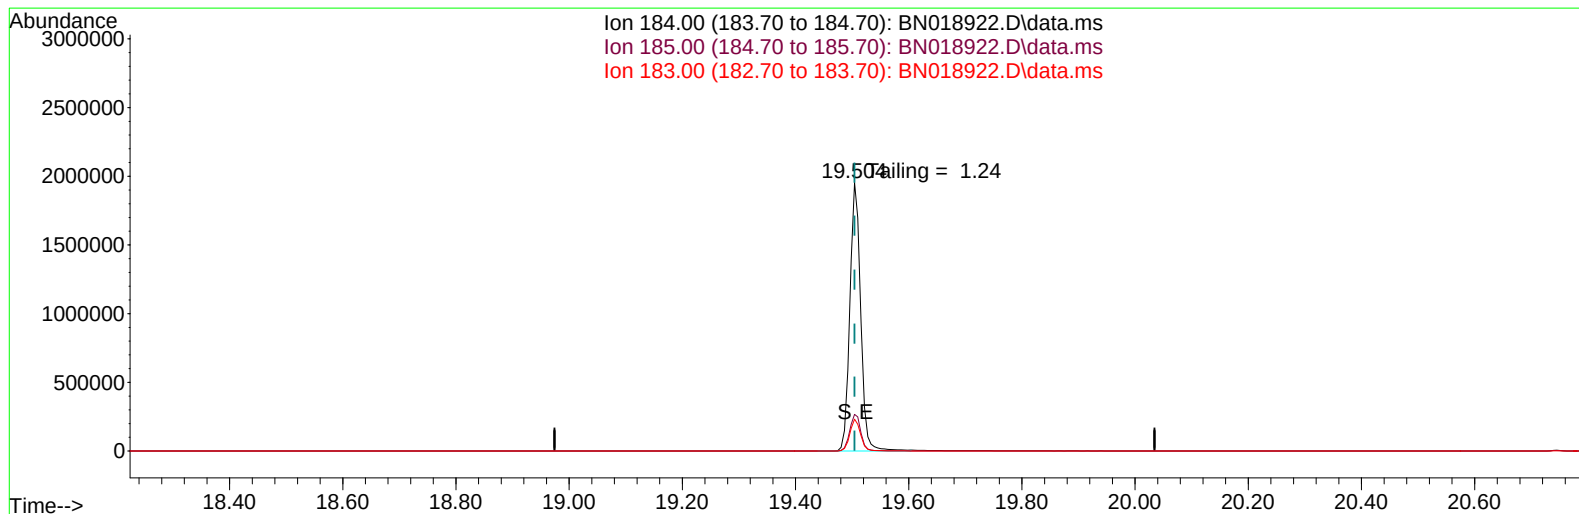

TIC: BN018922.D\data.ms

(77) Benzidine

19.504min (0.000) 0.00 ng

response 2611474

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.68
183.00	13.20	11.88
0.00	0.00	0.00