
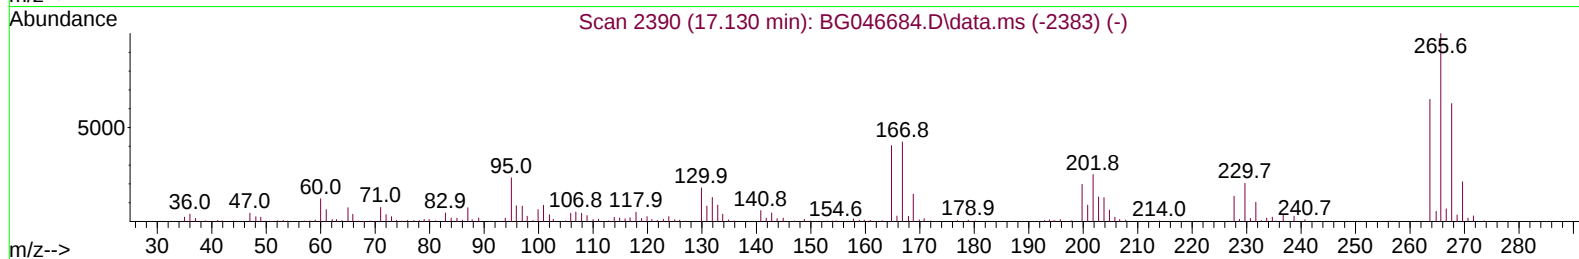
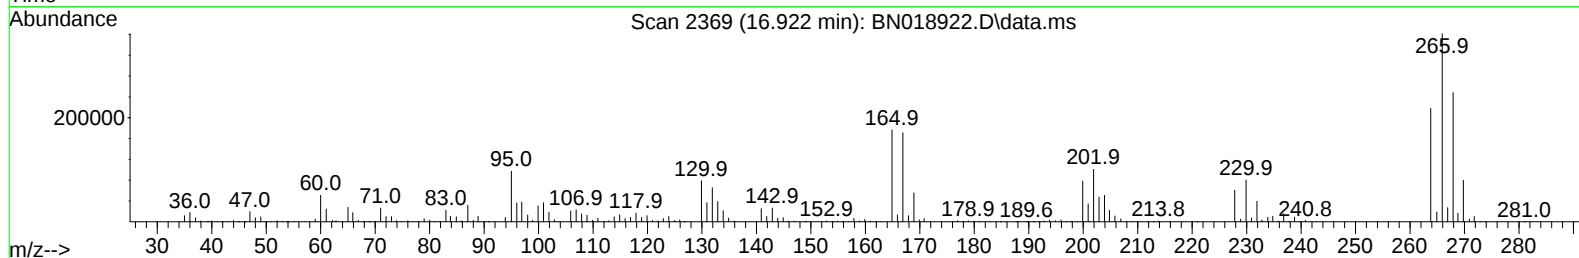


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN031222\  
Data File : BN018922.D  
Acq On : 11 Mar 2022 13:18  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 15:03:59 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 11 15:03:53 2022  
Response via : Initial Calibration

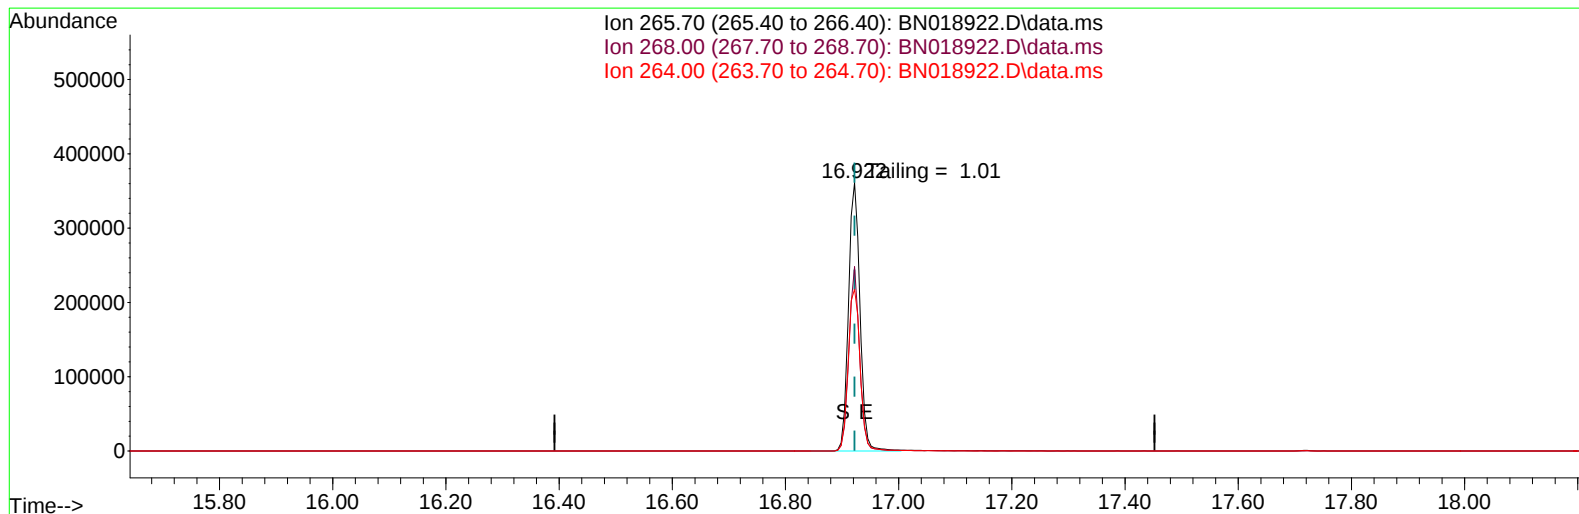

TIC: BN018922.D\data.ms

**(70) Pentachlorophenol (C)**




**16.922min ( 0.000) 21379.49 ng**

**response 513745**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 68.66  |
| 264.00 | 61.60  | 60.27  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN031222\  
Data File : BN018922.D  
Acq On : 11 Mar 2022 13:18  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 15:03:59 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 11 15:03:53 2022  
Response via : Initial Calibration

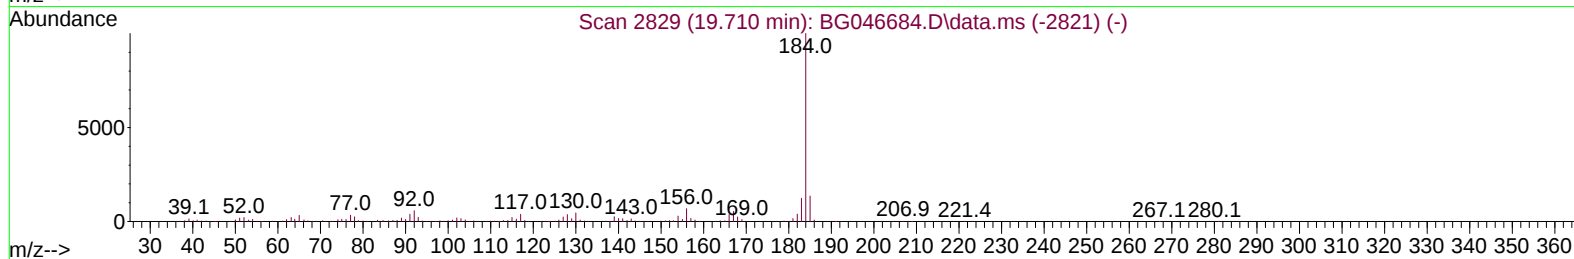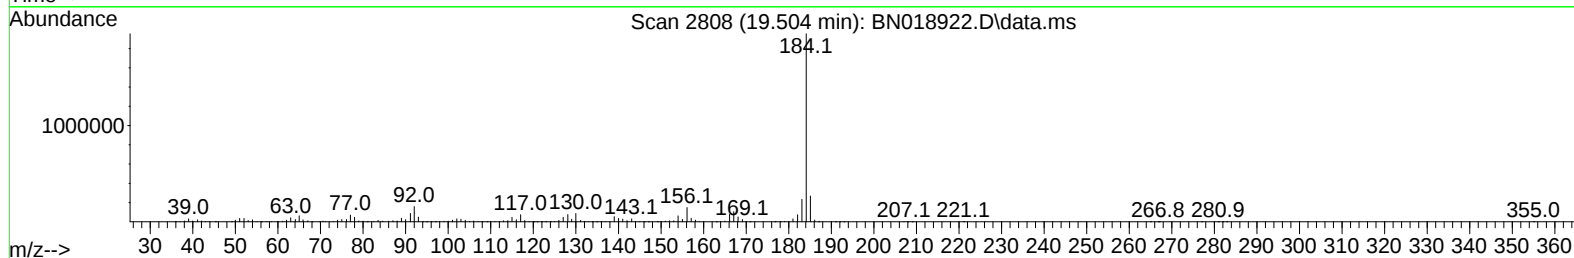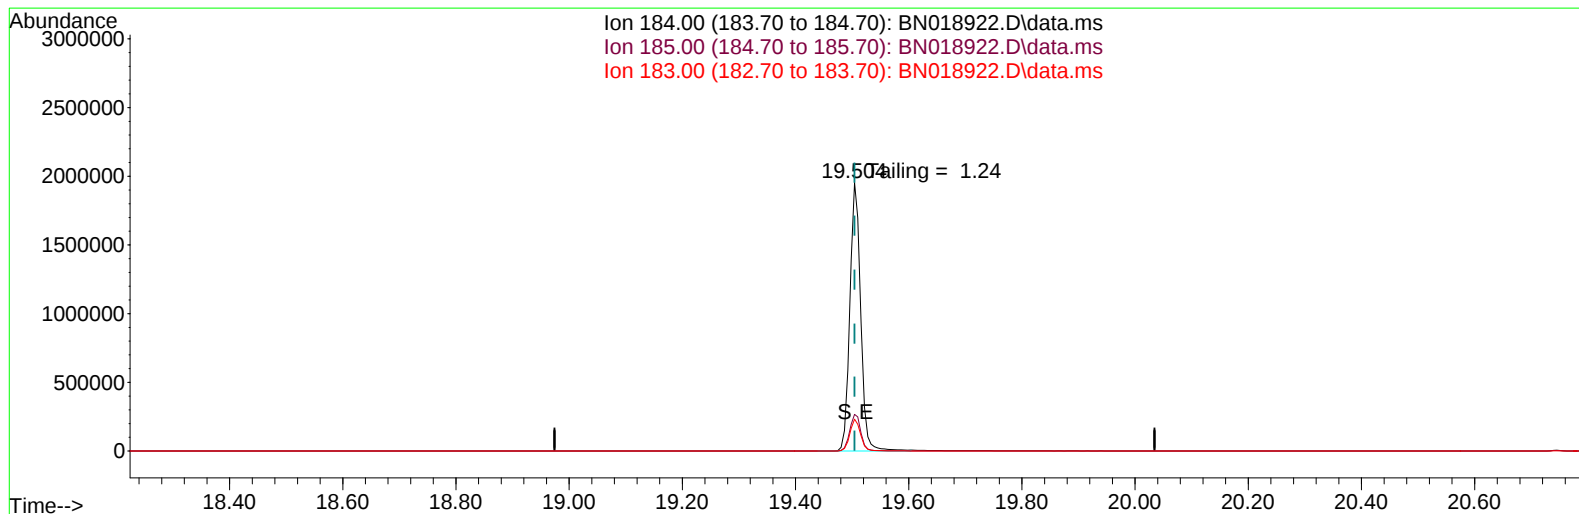

TIC: BN018922.D\data.ms

**(77) Benzidine**

19.504min ( 0.000) 0.00 ng

response 2611474

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.68  |
| 183.00 | 13.20  | 11.88  |
| 0.00   | 0.00   | 0.00   |