


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031222\
 Data File : BN018922.D
 Acq On : 11 Mar 2022 13:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 11 23:19:11 2022

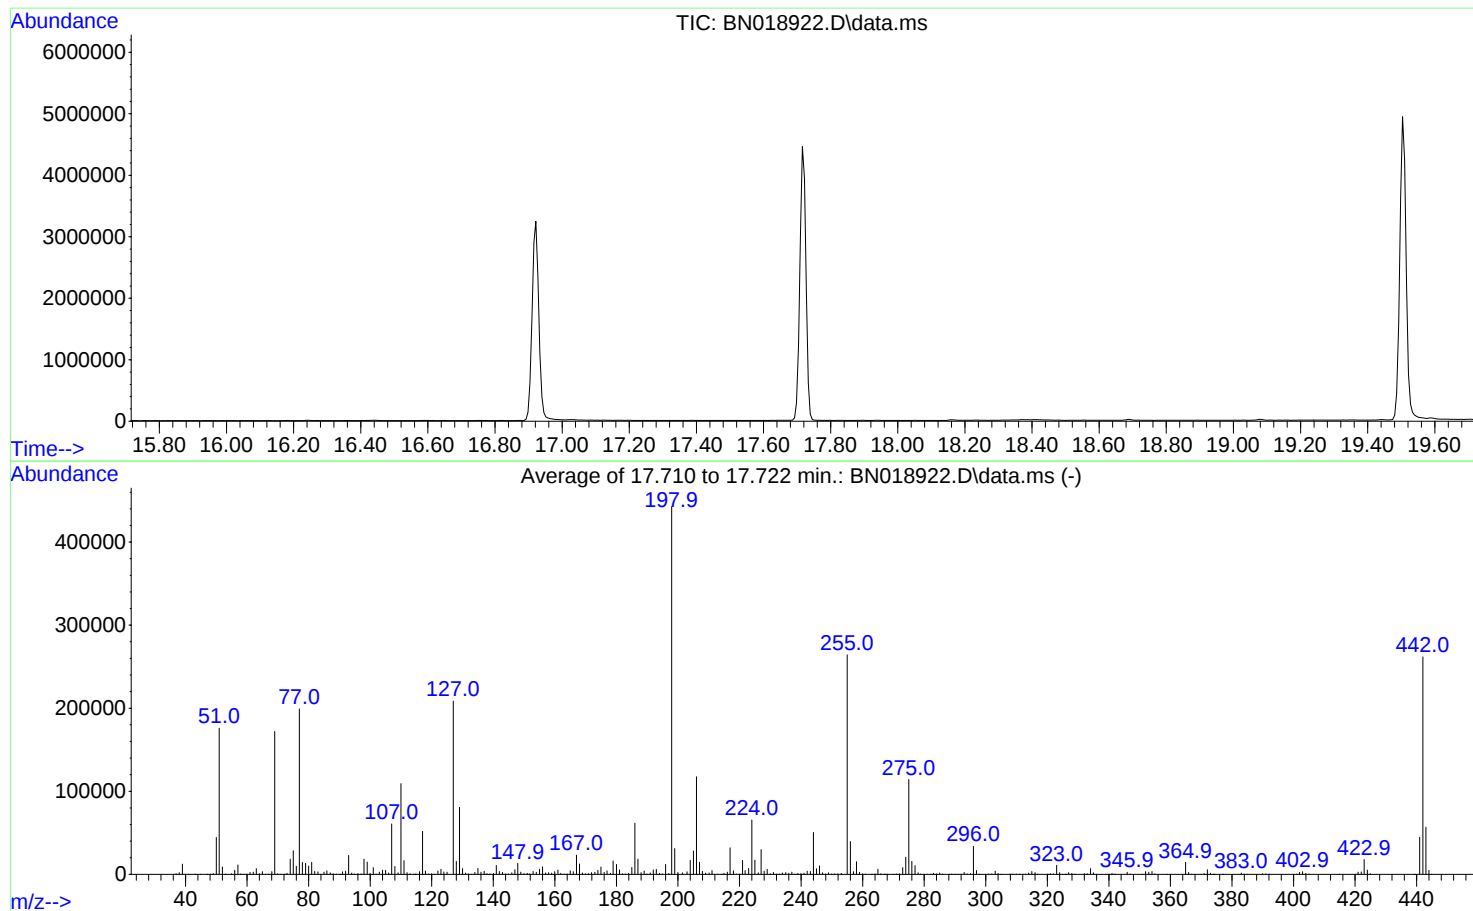




AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	175849	PASS
68	69	0.00	2	1.9	3331	PASS
69	198	0.00	100	38.8	171962	PASS
70	69	0.00	2	0.5	796	PASS
127	198	10	80	47.1	208683	PASS
197	198	0.00	2	0.2	995	PASS
198	198	100	100	100.0	442816	PASS
199	198	5	9	7.0	30965	PASS
275	198	10	60	25.8	114157	PASS
365	198	1	100	3.3	14435	PASS
441	198	0.01	100	10.0	44496	PASS
442	442	50	100	100.0	261781	PASS
443	442	15	24	21.7	56781	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031222\
Data File : BN018922.D
Acq On : 11 Mar 2022 13:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 11 15:03:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 11 15:03:53 2022
Response via : Initial Calibration

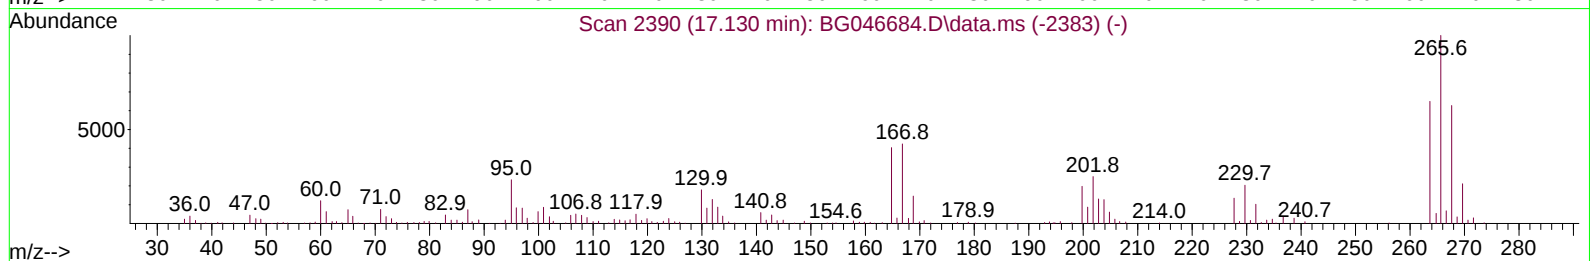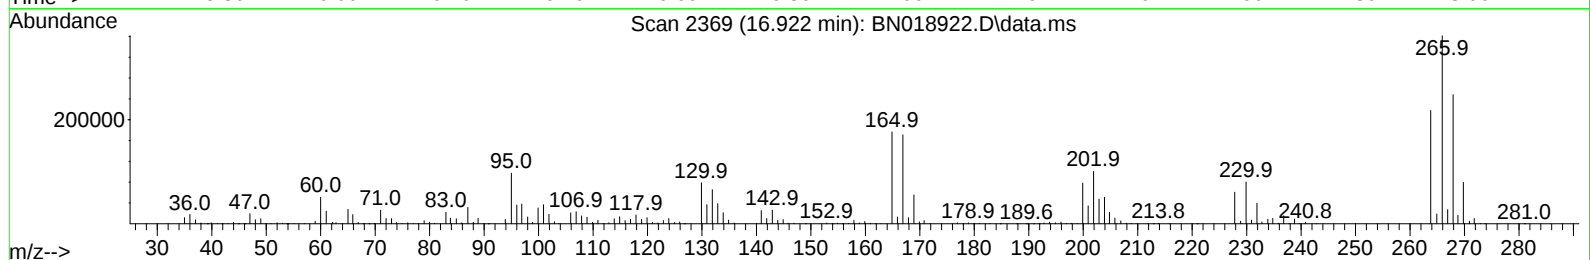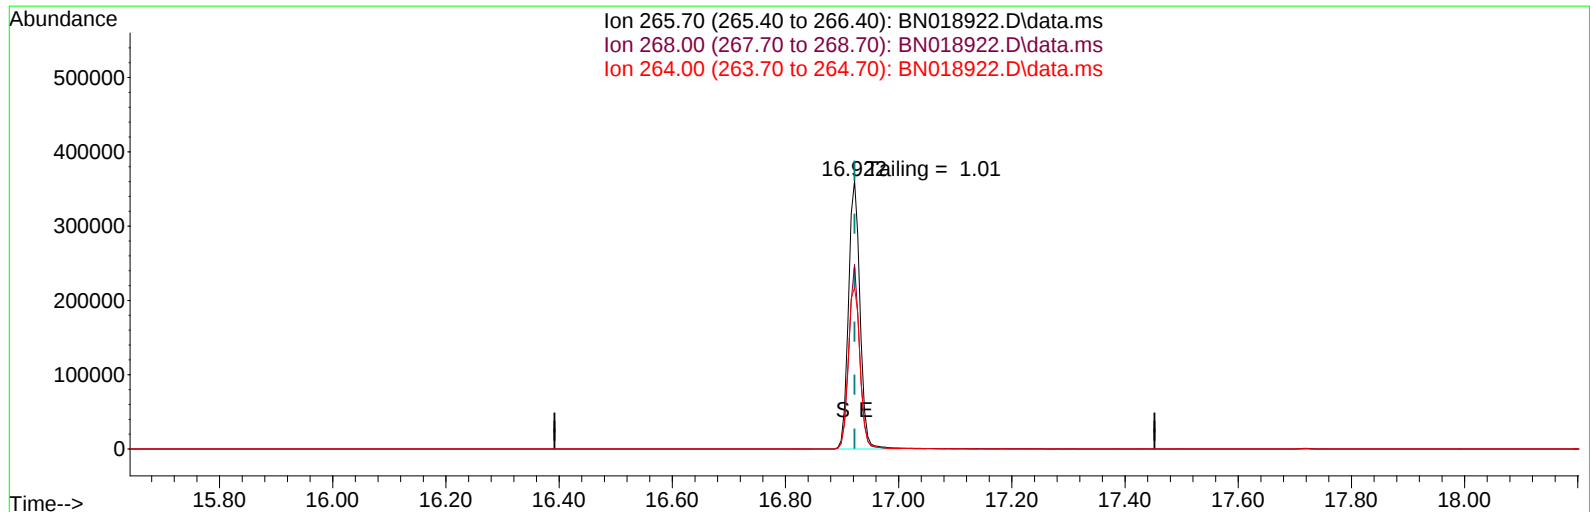

TIC: BN018922.D\data.ms

(70) Pentachlorophenol (C)

16.922min (0.000) 21379.49 ng




response 513745

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.66
264.00	61.60	60.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031222\
Data File : BN018922.D
Acq On : 11 Mar 2022 13:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 11 15:03:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 11 15:03:53 2022
Response via : Initial Calibration

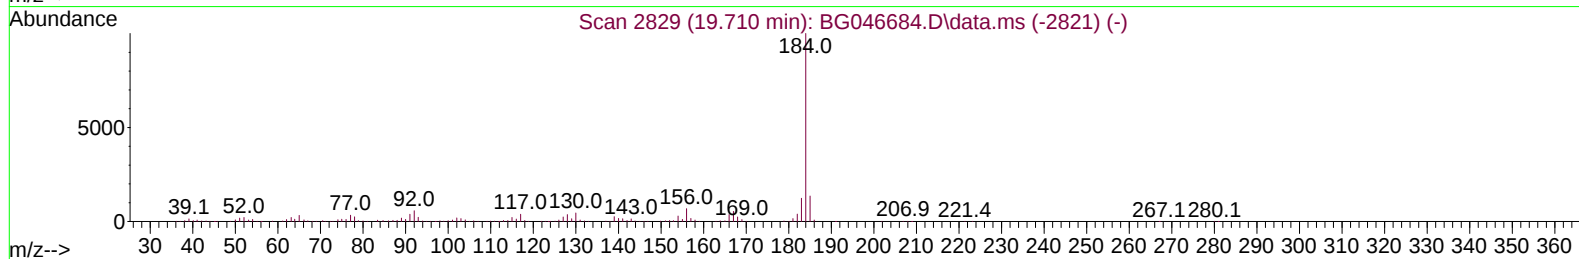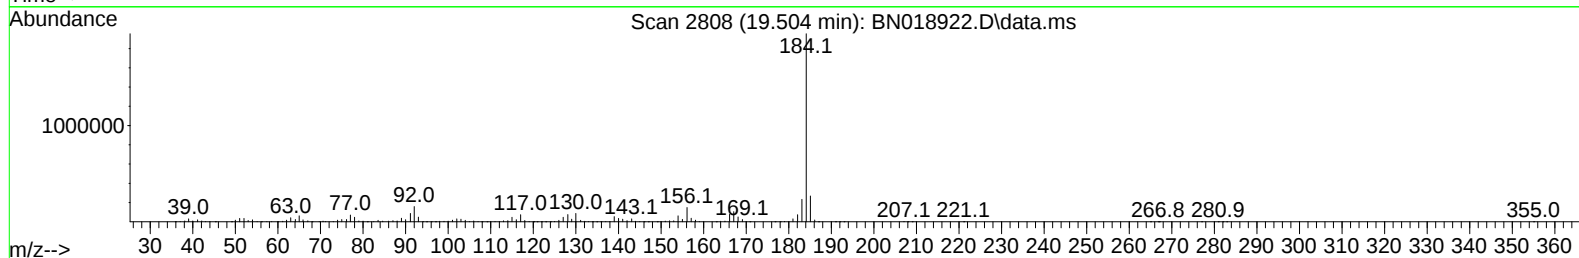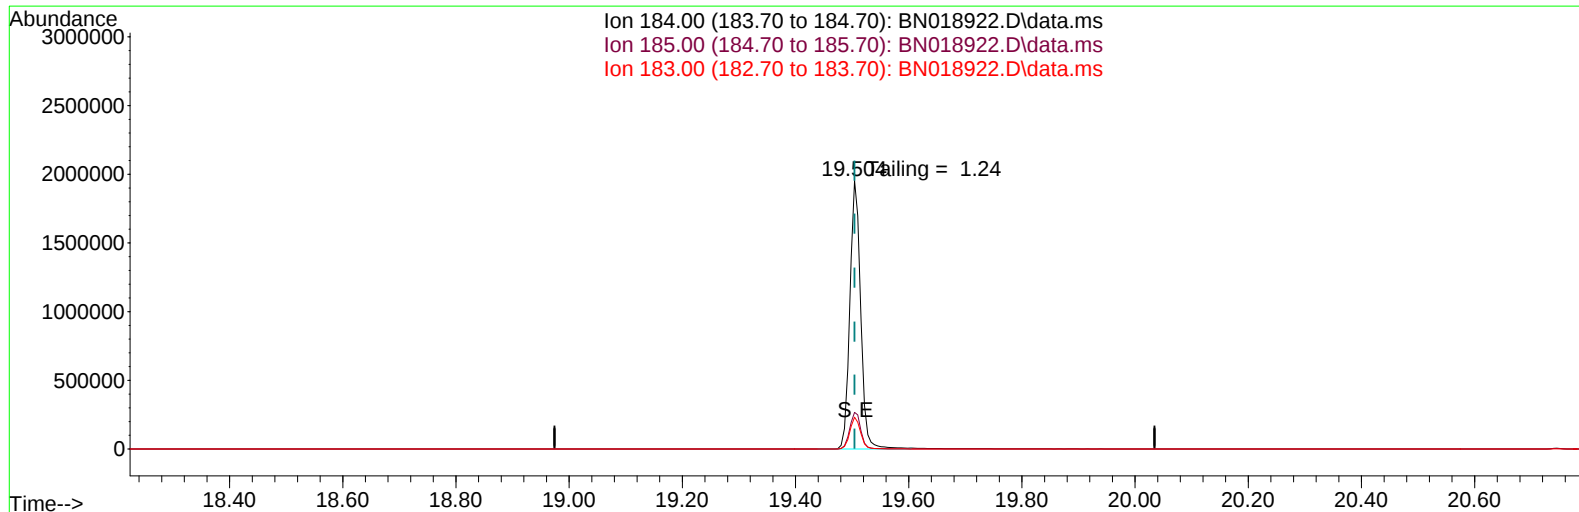

TIC: BN018922.D\data.ms

(77) Benzidine

19.504min (0.000) 0.00 ng

response 2611474

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.68
183.00	13.20	11.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/12/2022	BNA_N	<u>BN018922.D</u>
Compound Name	Response	Retention Time
DDT	1392060	20.74
DDD	5410	20.35
DDE	0	19.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5410	1397470	0.39

Instrument :
BNA_N
ClientSampleId :
DFTPP