

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
 Data File : BN030367.D
 Acq On : 12 Mar 2024 10:08
 Operator : MA/JU
 Sample : PB159439BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK439

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030367.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	28	31	38	rVB	40516	52028	2.56%	0.203%
2	3.676	97	100	115	rBV	424470	642552	31.57%	2.501%
3	3.993	151	154	159	rVB5	7096	9629	0.47%	0.037%
4	4.128	174	177	180	rVB4	2030	2414	0.12%	0.009%
5	4.223	190	193	196	rBV5	6125	7117	0.35%	0.028%
6	4.611	256	259	260	rBV3	3234	2511	0.12%	0.010%
7	6.964	652	659	671	rBV	510275	814648	40.02%	3.171%
8	7.140	683	689	702	rVV	383883	593479	29.16%	2.310%
9	7.322	713	720	733	rVB	556384	882762	43.37%	3.436%
10	7.793	793	800	812	rVB	436348	690685	33.93%	2.689%
11	8.505	914	921	934	rBV	626186	1014252	49.83%	3.948%
12	8.963	991	999	1009	rBV	486436	810210	39.81%	3.154%
13	9.681	1114	1121	1130	rBV	420511	702069	34.49%	2.733%
14	10.210	1203	1211	1225	rBV	614055	1037502	50.97%	4.039%
15	10.587	1267	1275	1284	rBV	548775	907094	44.57%	3.531%
16	10.740	1293	1301	1319	rBV	554864	1020079	50.12%	3.971%
17	12.199	1542	1549	1557	rVB3	5871	13543	0.67%	0.053%
18	13.351	1741	1745	1750	rVV4	7519	9469	0.47%	0.037%
19	13.428	1752	1758	1765	rBV5	1524	2844	0.14%	0.011%
20	13.875	1827	1834	1845	rBV	988870	1414999	69.52%	5.508%
21	14.140	1872	1879	1889	rBV	1123163	1629142	80.04%	6.342%
22	14.446	1925	1931	1940	rBV	729467	1078871	53.00%	4.200%
23	14.657	1960	1967	1982	rBV	334001	567362	27.87%	2.209%
24	15.451	2095	2102	2113	rBV	1322621	1923827	94.52%	7.489%
25	15.575	2118	2123	2133	rBV	401887	595715	29.27%	2.319%
26	15.693	2139	2143	2147	rBV3	4110	5941	0.29%	0.023%
27	16.240	2233	2236	2239	rVB4	3934	4816	0.24%	0.019%
28	16.998	2363	2365	2370	rVB3	2197	2093	0.10%	0.008%
29	17.210	2395	2401	2410	rBV	816883	1164480	57.21%	4.533%
30	17.310	2411	2418	2436	rVB2	1327060	1906303	93.66%	7.421%
31	18.139	2552	2559	2561	rBV6	5468	7960	0.39%	0.031%
32	19.181	2732	2736	2742	rVB4	12297	19459	0.96%	0.076%
33	19.257	2744	2749	2755	rVB2	10801	16804	0.83%	0.065%
34	19.428	2775	2778	2782	rBV6	4127	6874	0.34%	0.027%
35	19.616	2804	2810	2824	rBV	1430736	2035440	100.00%	7.924%
36	20.239	2914	2916	2920	rBV4	3013	4513	0.22%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
Data File : BN030367.D
Acq On : 12 Mar 2024 10:08
Operator : MA/JU
Sample : PB159439BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK439

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Title : SVOA CALIBRATION

37	21.433	3114	3119	3129	rBV	800824	1075353	52.83%	4.186%
38	23.122	3403	3406	3412	rBV3	32135	50294	2.47%	0.196%
39	23.633	3486	3493	3506	rBV2	946959	1879013	92.31%	7.315%
40	23.786	3513	3519	3528	rVB	535059	1083706	53.24%	4.219%




Sum of corrected areas: 25687852

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
Data File : BN030367.D
Acq On : 12 Mar 2024 10:08
Operator : MA/JU
Sample : PB159439BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK439

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

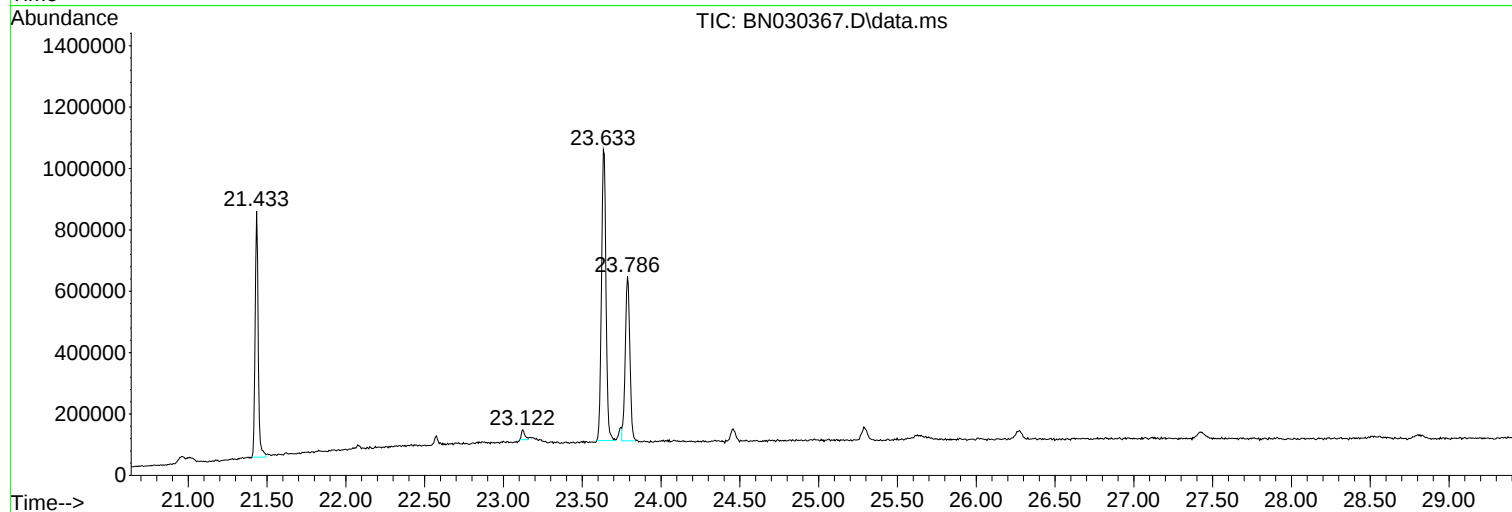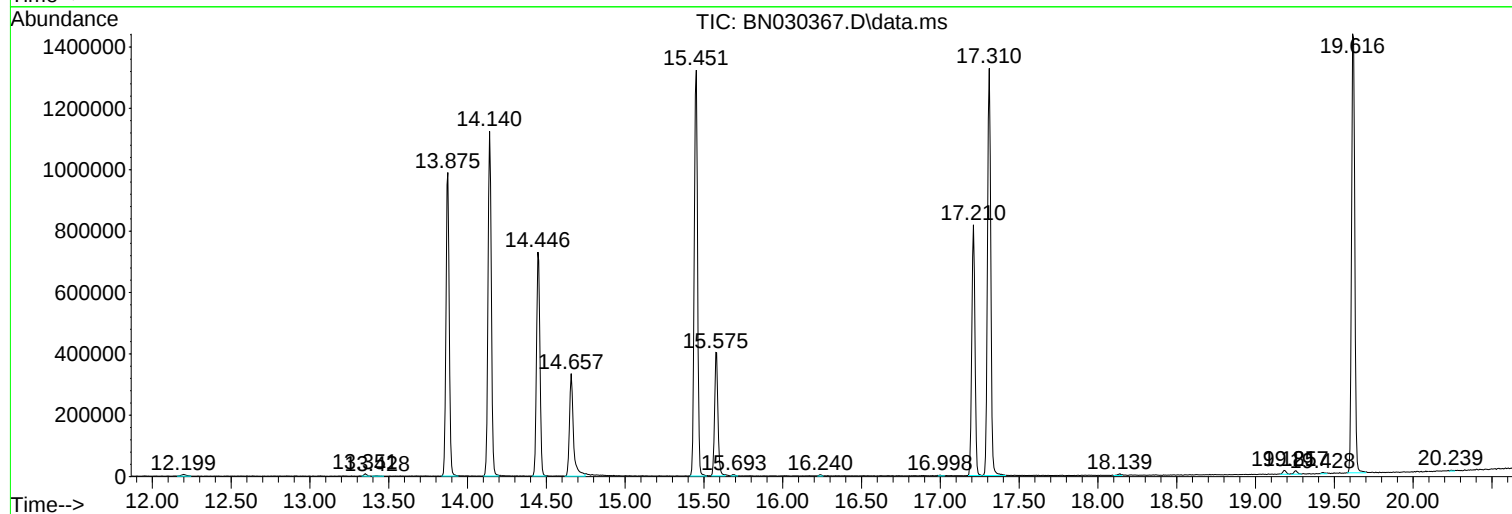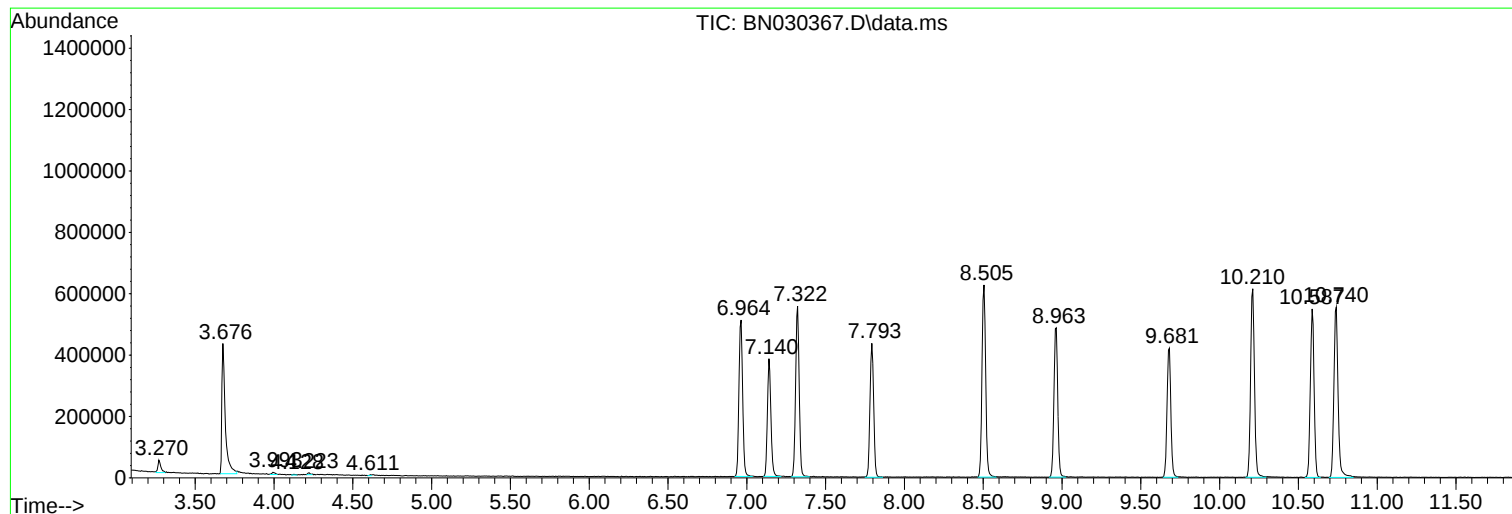

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
Data File : BN030367.D
Acq On : 12 Mar 2024 10:08
Operator : MA/JU
Sample : PB159439BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK439

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
Data File : BN030367.D
Acq On : 12 Mar 2024 10:08
Operator : MA/JU
Sample : PB159439BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK439

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc