

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
 Data File : BN030371.D
 Acq On : 12 Mar 2024 12:38
 Operator : MA/JU
 Sample : PB159472BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK472

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030371.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	39	rVB	32893	45576	2.07%	0.175%
2	3.675	96	100	115	rBV	355420	564350	25.65%	2.167%
3	3.993	151	154	158	rVB3	7262	8002	0.36%	0.031%
4	4.222	189	193	196	rBV5	6027	8773	0.40%	0.034%
5	4.452	228	232	234	rBV4	1920	2211	0.10%	0.008%
6	4.628	259	262	264	rBV3	2607	2585	0.12%	0.010%
7	5.328	378	381	383	rBV3	2237	2464	0.11%	0.009%
8	6.675	607	610	614	rVB3	2011	2482	0.11%	0.010%
9	6.957	652	658	670	rBV	454057	736701	33.48%	2.829%
10	7.140	683	689	704	rBV	336909	522267	23.74%	2.005%
11	7.316	713	719	729	rBV	483347	778556	35.38%	2.990%
12	7.793	793	800	807	rBV	395784	614942	27.95%	2.361%
13	8.504	914	921	933	rBV	588065	943855	42.89%	3.624%
14	8.963	990	999	1008	rBV	455764	763926	34.72%	2.933%
15	9.675	1112	1120	1135	rBV	403180	679086	30.86%	2.608%
16	10.210	1200	1211	1223	rBV	596546	999538	45.43%	3.838%
17	10.587	1268	1275	1286	rVB	527726	866467	39.38%	3.327%
18	10.740	1293	1301	1315	rBV	557142	998392	45.37%	3.834%
19	12.192	1543	1548	1557	rVB3	6400	13145	0.60%	0.050%
20	13.351	1740	1745	1752	rBV4	5220	8463	0.38%	0.032%
21	13.875	1826	1834	1845	rBV	1138214	1545032	70.22%	5.933%
22	14.139	1872	1879	1893	rBV	1132638	1706234	77.54%	6.552%
23	14.451	1925	1932	1943	rBV	771277	1134098	51.54%	4.355%
24	14.657	1961	1967	1992	rBV	387320	658541	29.93%	2.529%
25	15.451	2095	2102	2111	rBV	1462918	2051319	93.23%	7.877%
26	15.581	2118	2124	2138	rBV	485359	678513	30.84%	2.605%
27	15.692	2140	2143	2149	rVB4	5321	8082	0.37%	0.031%
28	16.233	2232	2235	2240	rBV3	3236	5302	0.24%	0.020%
29	16.692	2309	2313	2316	rVB3	1525	2525	0.11%	0.010%
30	16.992	2362	2364	2370	rBV4	1827	2451	0.11%	0.009%
31	17.210	2395	2401	2409	rBV	912046	1276617	58.02%	4.902%
32	17.310	2412	2418	2433	rVV2	1486150	2093150	95.13%	8.038%
33	18.139	2555	2559	2564	rVB6	5930	10021	0.46%	0.038%
34	19.039	2710	2712	2717	rVB5	1870	2772	0.13%	0.011%
35	19.186	2732	2737	2742	rBV2	14624	22197	1.01%	0.085%
36	19.257	2744	2749	2755	rVB3	12665	19481	0.89%	0.075%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
Data File : BN030371.D
Acq On : 12 Mar 2024 12:38
Operator : MA/JU
Sample : PB159472BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK472

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Title : SVOA CALIBRATION

37	19.421	2775	2777	2781	rBV5	5292	7315	0.33%	0.028%
38	19.621	2805	2811	2819	rBV	1660235	2200392	100.00%	8.449%
39	21.433	3114	3119	3133	rBV	818793	1145204	52.05%	4.398%
40	23.639	3486	3494	3506	rBV2	941963	1837935	83.53%	7.058%
41	23.792	3513	3520	3535	rVB	508194	1072909	48.76%	4.120%




Sum of corrected areas: 26041871

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
Data File : BN030371.D
Acq On : 12 Mar 2024 12:38
Operator : MA/JU
Sample : PB159472BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK472

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

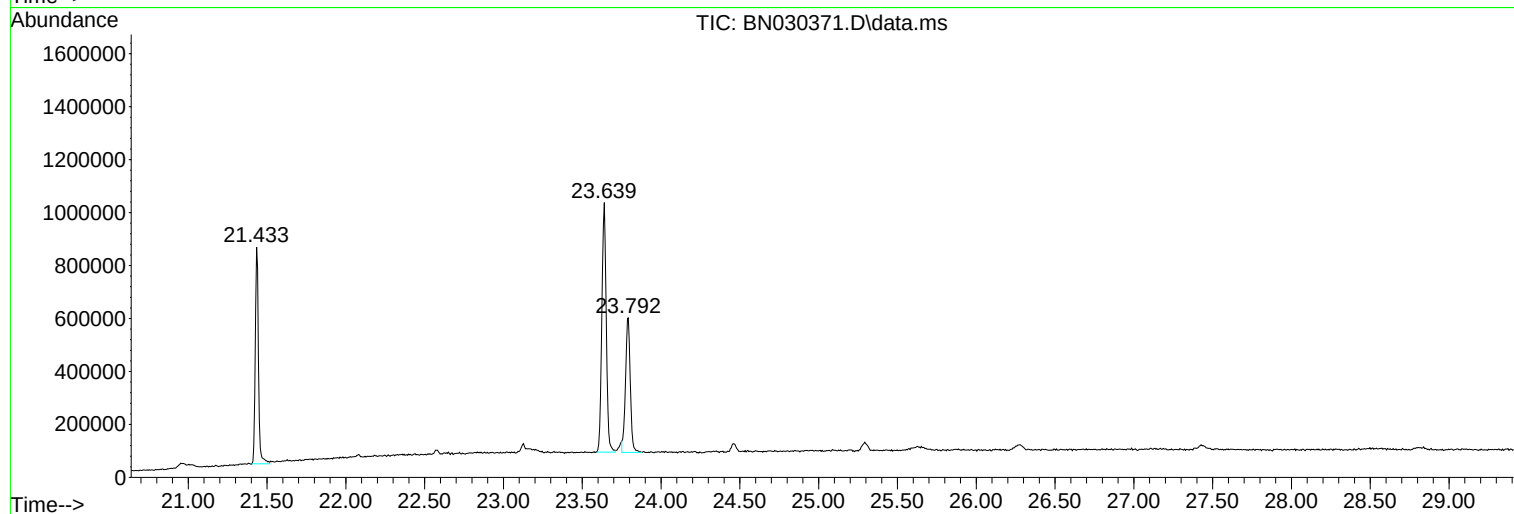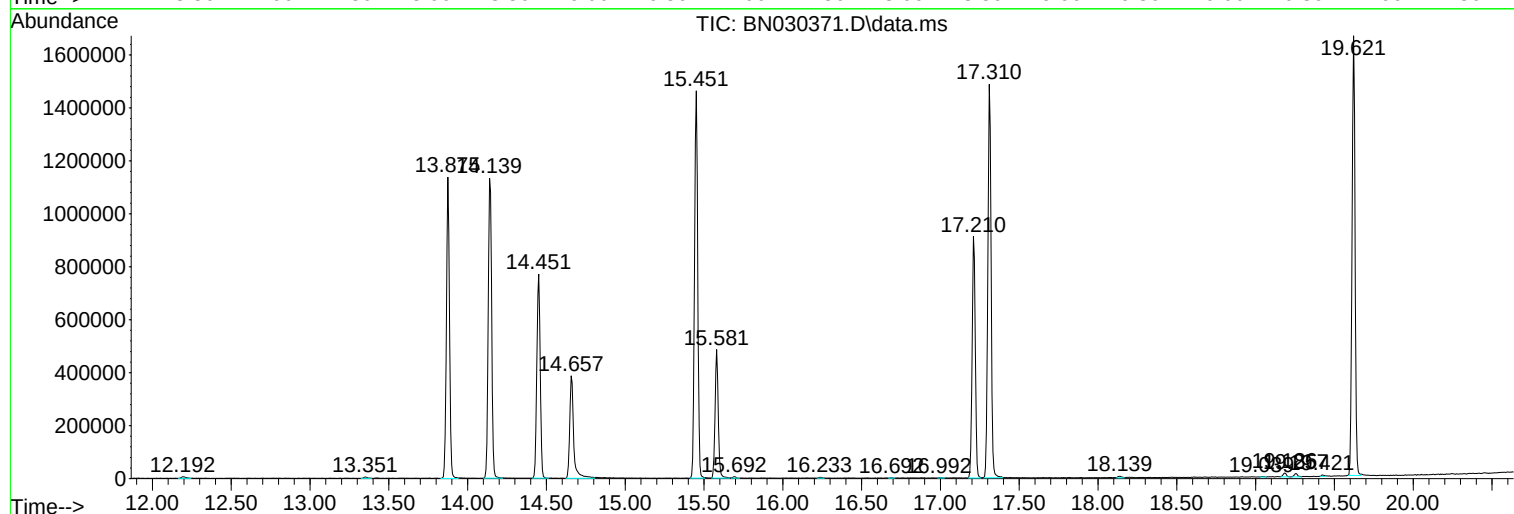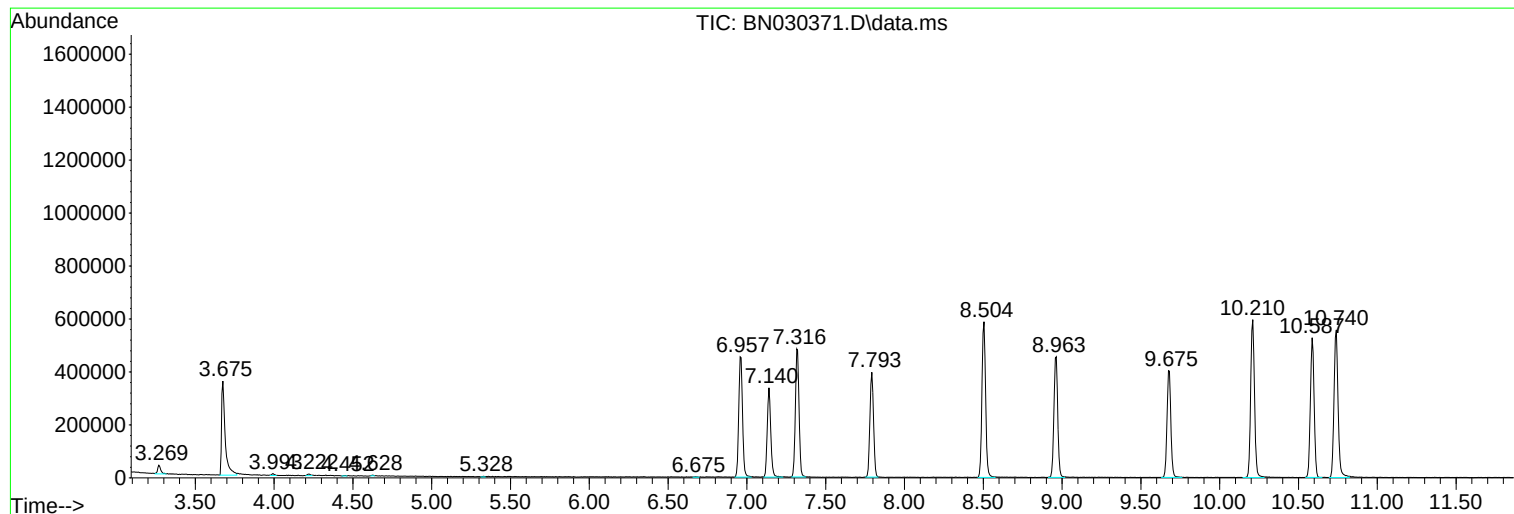

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
Data File : BN030371.D
Acq On : 12 Mar 2024 12:38
Operator : MA/JU
Sample : PB159472BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK472

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
Data File : BN030371.D
Acq On : 12 Mar 2024 12:38
Operator : MA/JU
Sample : PB159472BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK472

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------