

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
 Data File : BN030372.D
 Acq On : 12 Mar 2024 13:13
 Operator : MA/JU
 Sample : PB159474BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK474

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030372.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	38	rBV	28347	38695	1.63%	0.152%
2	3.675	96	100	114	rBV	330739	532579	22.50%	2.091%
3	3.993	152	154	159	rVB2	5416	6822	0.29%	0.027%
4	4.222	189	193	198	rBV6	4899	8059	0.34%	0.032%
5	4.628	258	262	266	rBV5	3201	5362	0.23%	0.021%
6	6.963	652	659	669	rBV	440308	683376	28.87%	2.683%
7	7.140	683	689	702	rBV	308523	493668	20.85%	1.938%
8	7.322	713	720	729	rBV	473098	734556	31.03%	2.883%
9	7.793	794	800	808	rVV	359859	562512	23.76%	2.208%
10	8.504	914	921	934	rBV	552053	872814	36.87%	3.426%
11	8.963	991	999	1011	rBV	434459	717309	30.30%	2.816%
12	9.681	1114	1121	1130	rBV	379872	626494	26.47%	2.459%
13	10.210	1204	1211	1222	rBV	559655	922008	38.95%	3.619%
14	10.587	1268	1275	1284	rVB	467509	776686	32.81%	3.049%
15	10.739	1294	1301	1320	rBV	528258	941456	39.77%	3.696%
16	12.192	1543	1548	1555	rBV	6014	10779	0.46%	0.042%
17	13.351	1739	1745	1750	rBV3	7887	11828	0.50%	0.046%
18	13.875	1827	1834	1846	rBV	1045786	1451941	61.34%	5.699%
19	14.139	1872	1879	1892	rBV	1091229	1608277	67.94%	6.313%
20	14.451	1925	1932	1945	rVB	698970	1024227	43.27%	4.021%
21	14.657	1960	1967	1982	rBV	405501	650614	27.48%	2.554%
22	15.451	2095	2102	2115	rBV	1390716	1988677	84.01%	7.806%
23	15.580	2118	2124	2133	rVV	493011	678041	28.64%	2.662%
24	15.645	2133	2135	2139	rVV4	2647	4011	0.17%	0.016%
25	15.698	2139	2144	2149	rVB5	4530	6907	0.29%	0.027%
26	16.239	2232	2236	2243	rVB4	4060	5404	0.23%	0.021%
27	17.210	2395	2401	2411	rBV	886096	1236540	52.24%	4.854%
28	17.310	2411	2418	2436	rVV	1531462	2103190	88.85%	8.256%
29	18.133	2554	2558	2566	rBV6	3399	7262	0.31%	0.029%
30	19.180	2732	2736	2741	rBV3	15567	20365	0.86%	0.080%
31	19.257	2745	2749	2754	rVB	12850	19029	0.80%	0.075%
32	19.427	2774	2778	2783	rBV6	3481	5978	0.25%	0.023%
33	19.621	2805	2811	2828	rBV	1811796	2367180	100.00%	9.292%
34	21.433	3114	3119	3129	rBV	912346	1209137	51.08%	4.746%
35	23.633	3486	3493	3505	rBV2	1021985	1949934	82.37%	7.654%
36	23.786	3507	3519	3532	rVB	556898	1193292	50.41%	4.684%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
Data File : BN030372.D
Acq On : 12 Mar 2024 13:13
Operator : MA/JU
Sample : PB159474BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK474

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 25475009

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
Data File : BN030372.D
Acq On : 12 Mar 2024 13:13
Operator : MA/JU
Sample : PB159474BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK474

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

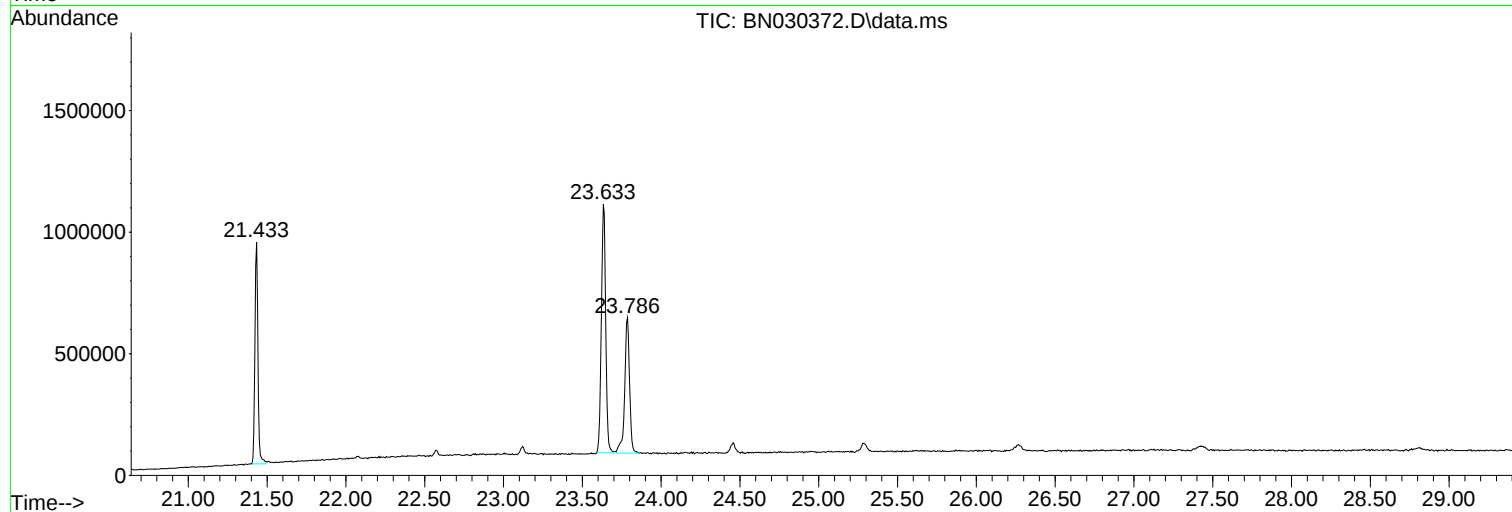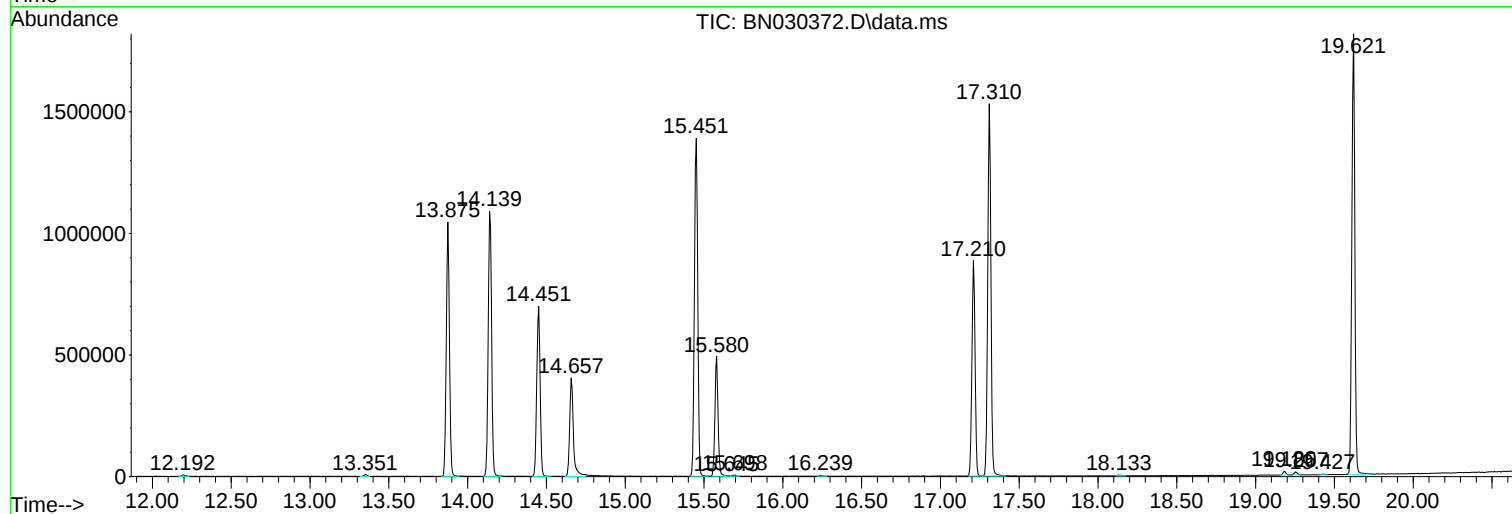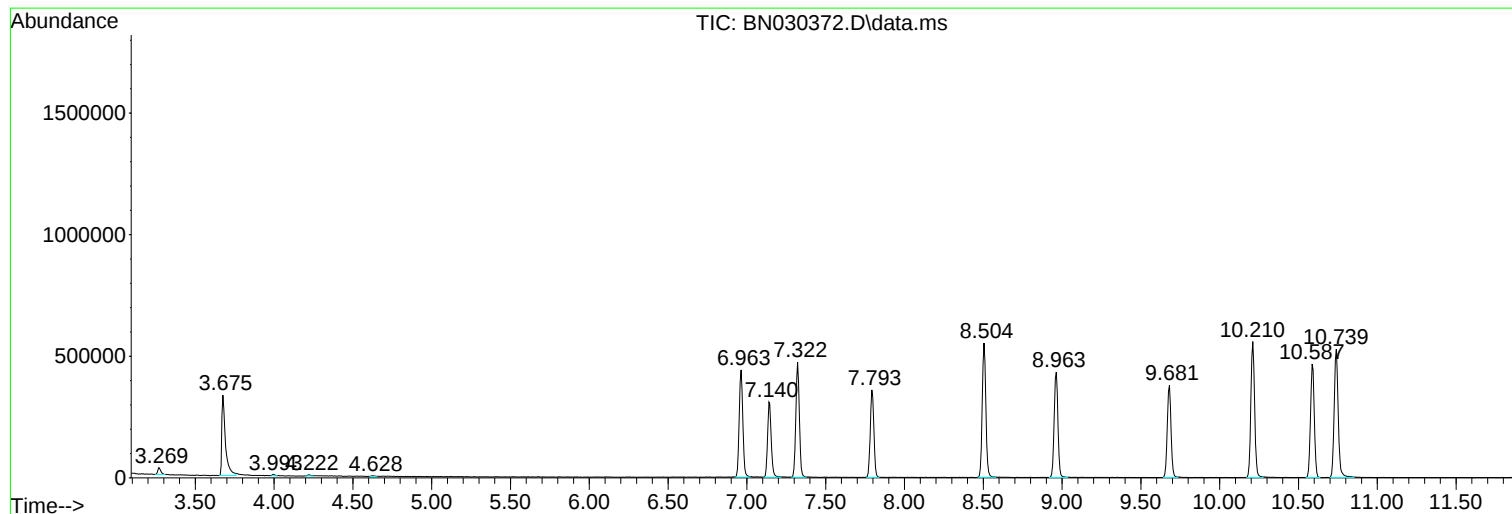

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
Data File : BN030372.D
Acq On : 12 Mar 2024 13:13
Operator : MA/JU
Sample : PB159474BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK474

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
Data File : BN030372.D
Acq On : 12 Mar 2024 13:13
Operator : MA/JU
Sample : PB159474BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK474

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------