

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
 Data File : BN030375.D
 Acq On : 12 Mar 2024 17:32
 Operator : MA/JU
 Sample : PB159553BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK553

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030375.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	28	31	37	rBV	22116	28867	1.35%	0.124%
2	3.675	97	100	118	rBV	267583	437692	20.49%	1.874%
3	3.899	137	138	146	rBV7	1918	3140	0.15%	0.013%
4	3.993	151	154	158	rVB2	4203	5260	0.25%	0.023%
5	6.963	653	659	668	rBV	361372	572169	26.79%	2.449%
6	7.140	683	689	701	rBV	258796	403262	18.88%	1.726%
7	7.322	713	720	730	rBV	391071	613482	28.72%	2.626%
8	7.793	793	800	808	rBV	373925	588406	27.55%	2.519%
9	8.505	914	921	938	rBV2	463096	742896	34.78%	3.180%
10	8.963	991	999	1011	rBV	363050	600012	28.09%	2.569%
11	9.681	1114	1121	1134	rBV	319025	533596	24.98%	2.284%
12	10.210	1204	1211	1222	rBV	476495	779166	36.48%	3.336%
13	10.587	1267	1275	1284	rBV	497768	827917	38.76%	3.544%
14	10.740	1293	1301	1313	rBV	444362	787306	36.86%	3.370%
15	12.193	1542	1548	1557	rVB	4752	9247	0.43%	0.040%
16	13.351	1741	1745	1750	rBV3	8468	12312	0.58%	0.053%
17	13.875	1827	1834	1844	rBV	943776	1290002	60.39%	5.522%
18	14.140	1871	1879	1891	rBV2	953429	1392148	65.17%	5.960%
19	14.451	1924	1932	1940	rBV	730960	1115752	52.23%	4.776%
20	14.657	1960	1967	1983	rBV	353741	573253	26.84%	2.454%
21	15.451	2095	2102	2113	rBV	1194378	1713311	80.21%	7.335%
22	15.581	2117	2124	2133	rVV	397186	573248	26.84%	2.454%
23	15.687	2137	2142	2147	rVB2	4552	5502	0.26%	0.024%
24	16.239	2233	2236	2242	rVB4	2990	4596	0.22%	0.020%
25	16.992	2363	2364	2371	rVB4	2053	3173	0.15%	0.014%
26	17.210	2394	2401	2408	rBV	975050	1353831	63.38%	5.796%
27	17.310	2411	2418	2431	rBV	1373483	1924014	90.07%	8.237%
28	18.139	2555	2559	2565	rVB6	2959	5789	0.27%	0.025%
29	19.180	2732	2736	2743	rVB	13904	17534	0.82%	0.075%
30	19.251	2744	2748	2753	rBV2	10468	15146	0.71%	0.065%
31	19.422	2775	2777	2781	rBV5	2361	2202	0.10%	0.009%
32	19.622	2805	2811	2822	rBV	1586664	2136078	100.00%	9.144%
33	19.898	2856	2858	2861	rVB4	2785	2421	0.11%	0.010%
34	19.928	2861	2863	2866	rBV4	2494	3084	0.14%	0.013%
35	21.433	3114	3119	3130	rBV	1048410	1327400	62.14%	5.683%
36	23.121	3403	3406	3413	rVB4	35693	53238	2.49%	0.228%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
Data File : BN030375.D
Acq On : 12 Mar 2024 17:32
Operator : MA/JU
Sample : PB159553BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK553

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Title : SVOA CALIBRATION

37	23.639	3486	3494	3503	rBV	864225	1694412	79.32%	7.254%
38	23.786	3513	3519	3529	rVB	569717	1136669	53.21%	4.866%
39	24.457	3630	3633	3640	rVB5	40532	71827	3.36%	0.307%




Sum of corrected areas: 23359360

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
Data File : BN030375.D
Acq On : 12 Mar 2024 17:32
Operator : MA/JU
Sample : PB159553BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK553

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

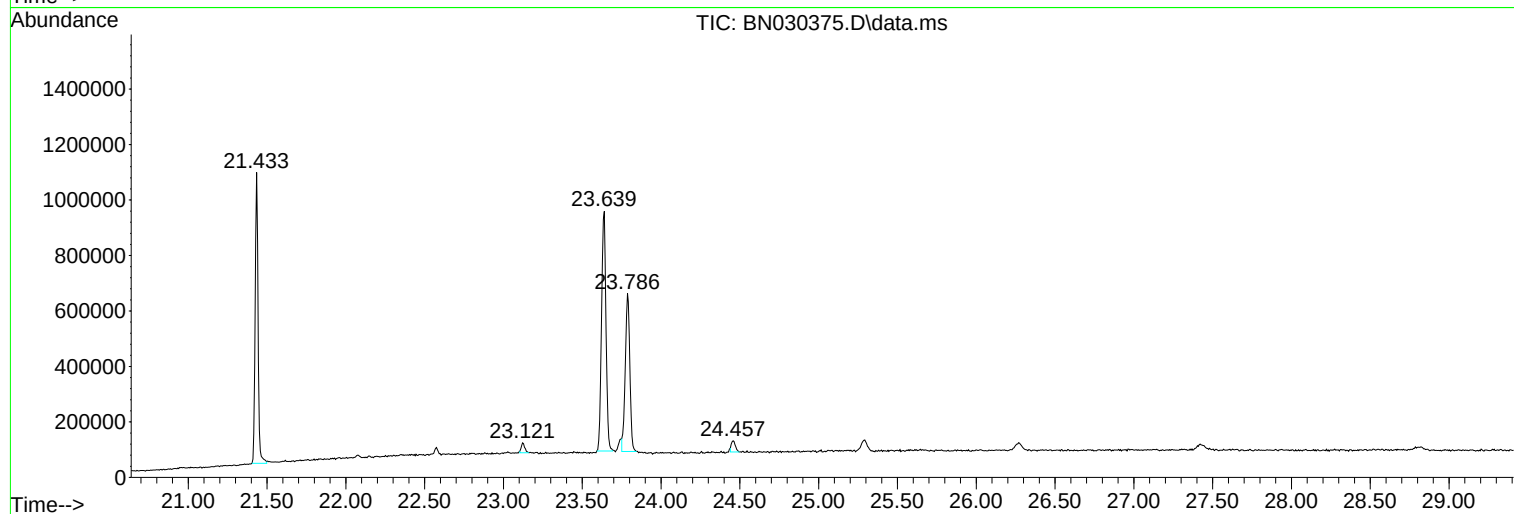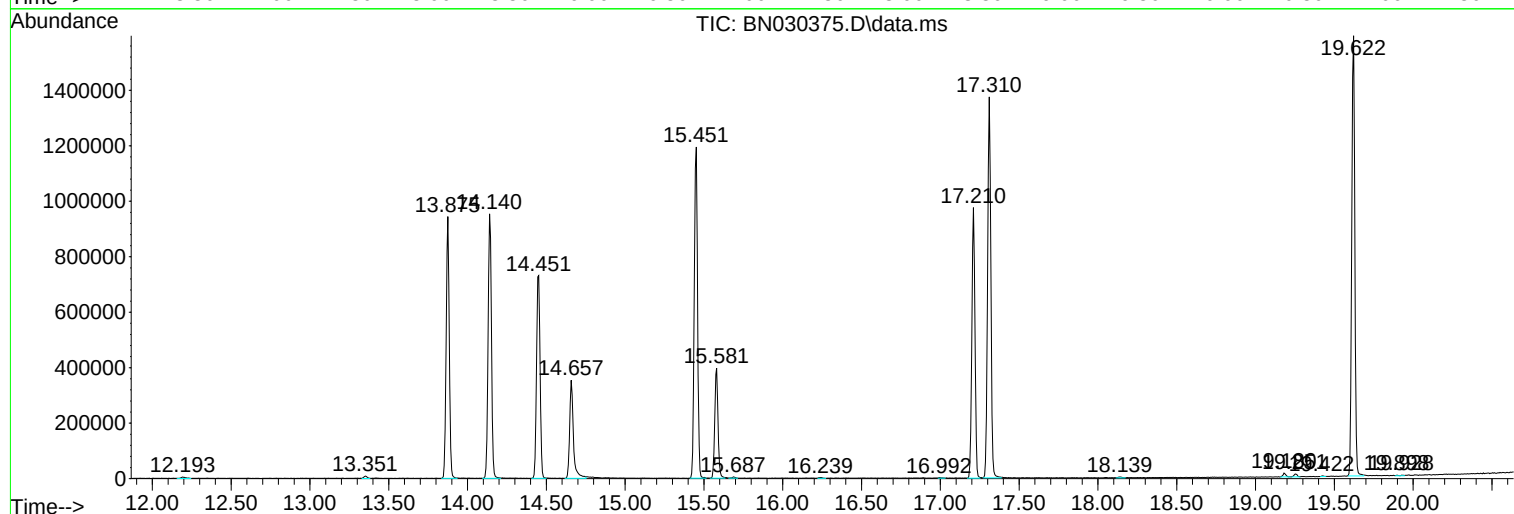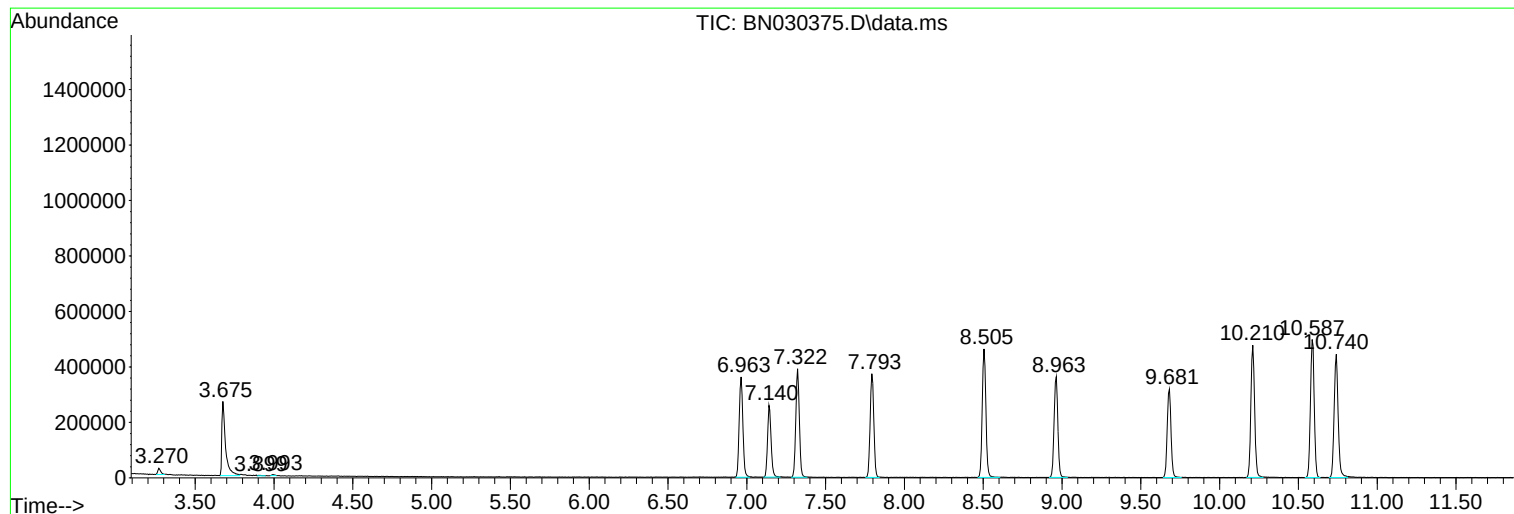

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
Data File : BN030375.D
Acq On : 12 Mar 2024 17:32
Operator : MA/JU
Sample : PB159553BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK553

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031224\
Data File : BN030375.D
Acq On : 12 Mar 2024 17:32
Operator : MA/JU
Sample : PB159553BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK553

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------