
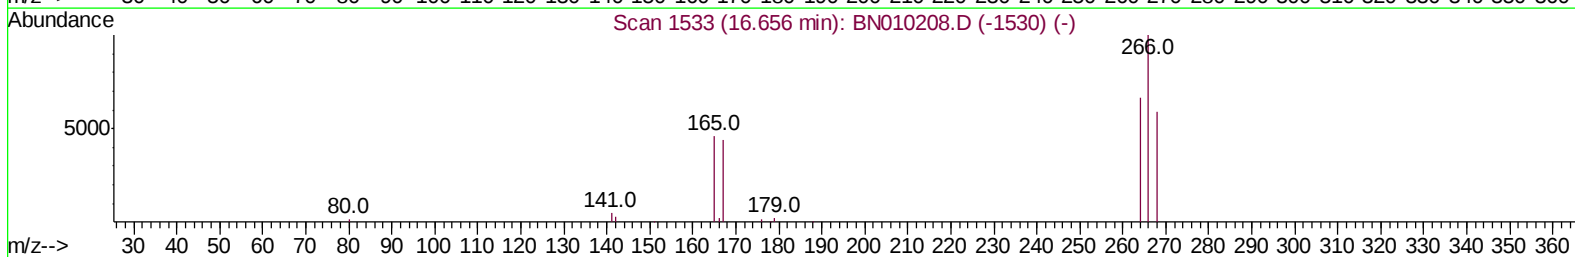
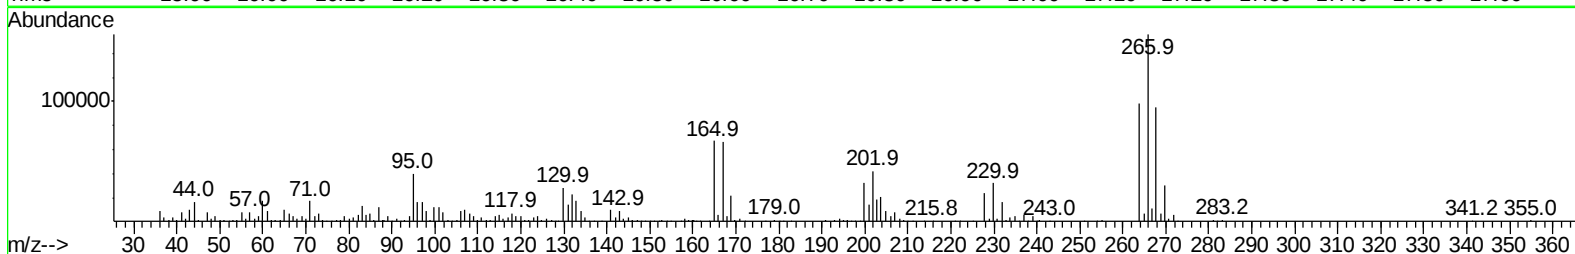


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN031320\
Data File : BN010205.D
Acq On : 13 Mar 2020 17:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 02:24:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN031320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 02:17:23 2020
Response via : Initial Calibration

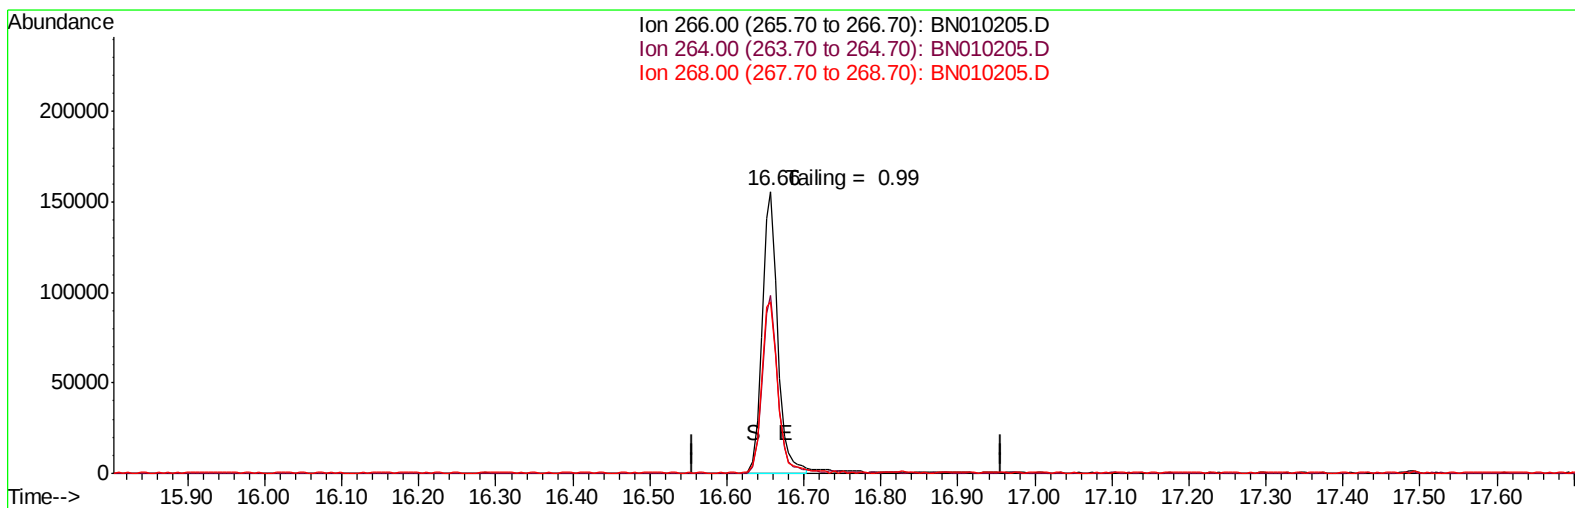

TIC: BN010205.D

(22) Pentachlorophenol

16.656min (-16.656) 0.00ng

response 0

Ion	Exp%	Act%
266.00	100	0.00
264.00	70.20	0.00#
268.00	76.80	0.00#
0.00	0.00	0.00