


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031320\
 Data File : BN010205.D
 Acq On : 13 Mar 2020 17:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 16 02:17:23 2020

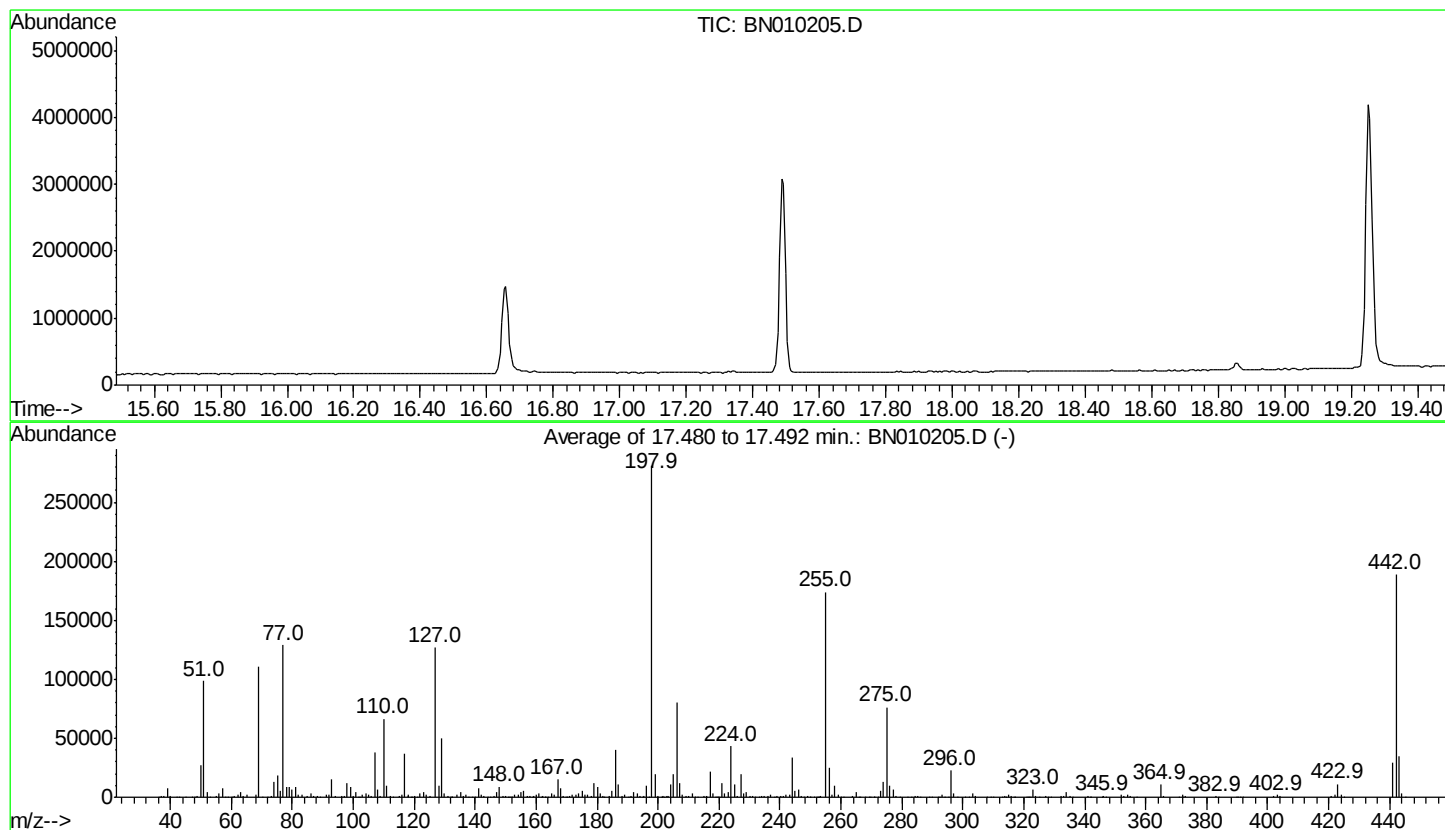

AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	98335	PASS
68	69	0.00	2	1.9	2123	PASS
69	198	0.00	100	39.6	111189	PASS
70	69	0.00	2	0.1	117	PASS
127	198	10	80	45.1	126764	PASS
197	198	0.00	2	0.2	529	PASS
198	198	100	100	100.0	281109	PASS
199	198	5	9	7.1	19987	PASS
275	198	10	60	27.2	76328	PASS
365	198	1	100	3.7	10369	PASS
441	198	0.01	100	10.3	28816	PASS
442	198	50	100	67.0	188448	PASS
443	442	15	24	18.3	34472	PASS