

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031323\
 Data File : BN024246.D
 Acq On : 13 Mar 2023 15:02
 Operator : CG/JU
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Quant Time: Mar 14 02:40:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 14 02:35:29 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.047	152	8721	0.400	ng	0.00
7) Naphthalene-d8	10.866	136	25014	0.400	ng	0.00
13) Acenaphthene-d10	14.675	164	13792	0.400	ng	0.00
19) Phenanthrene-d10	17.425	188	28635	0.400	ng	0.00
29) Chrysene-d12	21.610	240	22247	0.400	ng	# 0.00
35) Perylene-d12	24.129	264	17210	0.400	ng	0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.584	112	14680	0.810	ng	0.00
5) Phenol-d6	7.195	99	18758	0.878	ng	0.00
8) Nitrobenzene-d5	9.211	82	12385	0.617	ng	0.00
11) 2-Methylnaphthalene-d10	12.444	152	23420	0.674	ng	0.00
14) 2,4,6-Tribromophenol	16.172	330	5060	0.712	ng	0.01
15) 2-Fluorobiphenyl	13.307	172	39413	0.722	ng	0.00
27) Fluoranthene-d10	19.450	212	45124	0.649	ng	0.00
31) Terphenyl-d14	20.042	244	27060	0.652	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.439	88	7501	0.907	ng	100
3) n-Nitrosodimethylamine	3.764	42	11102	1.198	ng	97
6) bis(2-Chloroethyl)ether	7.462	93	19336	0.905	ng	100
9) Naphthalene	10.919	128	48832	0.783	ng	100
10) Hexachlorobutadiene	11.208	225	9263	0.566	ng	# 100
12) 2-Methylnaphthalene	12.520	142	32804	0.790	ng	98
16) Acenaphthylene	14.397	152	48891	0.910	ng	100
17) Acenaphthene	14.739	154	31214	0.854	ng	99
18) Fluorene	15.725	166	37800	0.763	ng	97
20) 4,6-Dinitro-2-methylph...	15.787	198	2539	0.542	ng	92
21) 4-Bromophenyl-phenylether	16.618	248	12717	0.683	ng	98
22) Hexachlorobenzene	16.730	284	15817	0.707	ng	100
23) Atrazine	16.879	200	7530	0.618	ng	99
24) Pentachlorophenol	17.065	266	6904	0.871	ng	100
25) Phenanthrene	17.462	178	64274	0.814	ng	100
26) Anthracene	17.549	178	57913	0.891	ng	100
28) Fluoranthene	19.480	202	70107	0.774	ng	100
30) Pyrene	19.842	202	69093	0.895	ng	100
32) Benzo(a)anthracene	21.601	228	56636	0.796	ng	99
33) Chrysene	21.655	228	60102	0.782	ng	100
34) Bis(2-ethylhexyl)phtha...	21.511	149	24325	0.748	ng	99
36) Indeno(1,2,3-cd)pyrene	26.760	276	47879	0.612	ng	100
37) Benzo(b)fluoranthene	23.357	252	50873	0.730	ng	97
38) Benzo(k)fluoranthene	23.413	252	52170	0.758	ng	97
39) Benzo(a)pyrene	24.012	252	46749	0.885	ng	96
40) Dibenzo(a,h)anthracene	26.781	278	37133	0.593	ng	99
41) Benzo(g,h,i)perylene	27.570	276	44031	0.663	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031323\
Data File : BN024246.D
Acq On : 13 Mar 2023 15:02
Operator : CG/JU
Sample : SSTDICC0.8
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Quant Time: Mar 14 02:40:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 14 02:35:29 2023
Response via : Initial Calibration

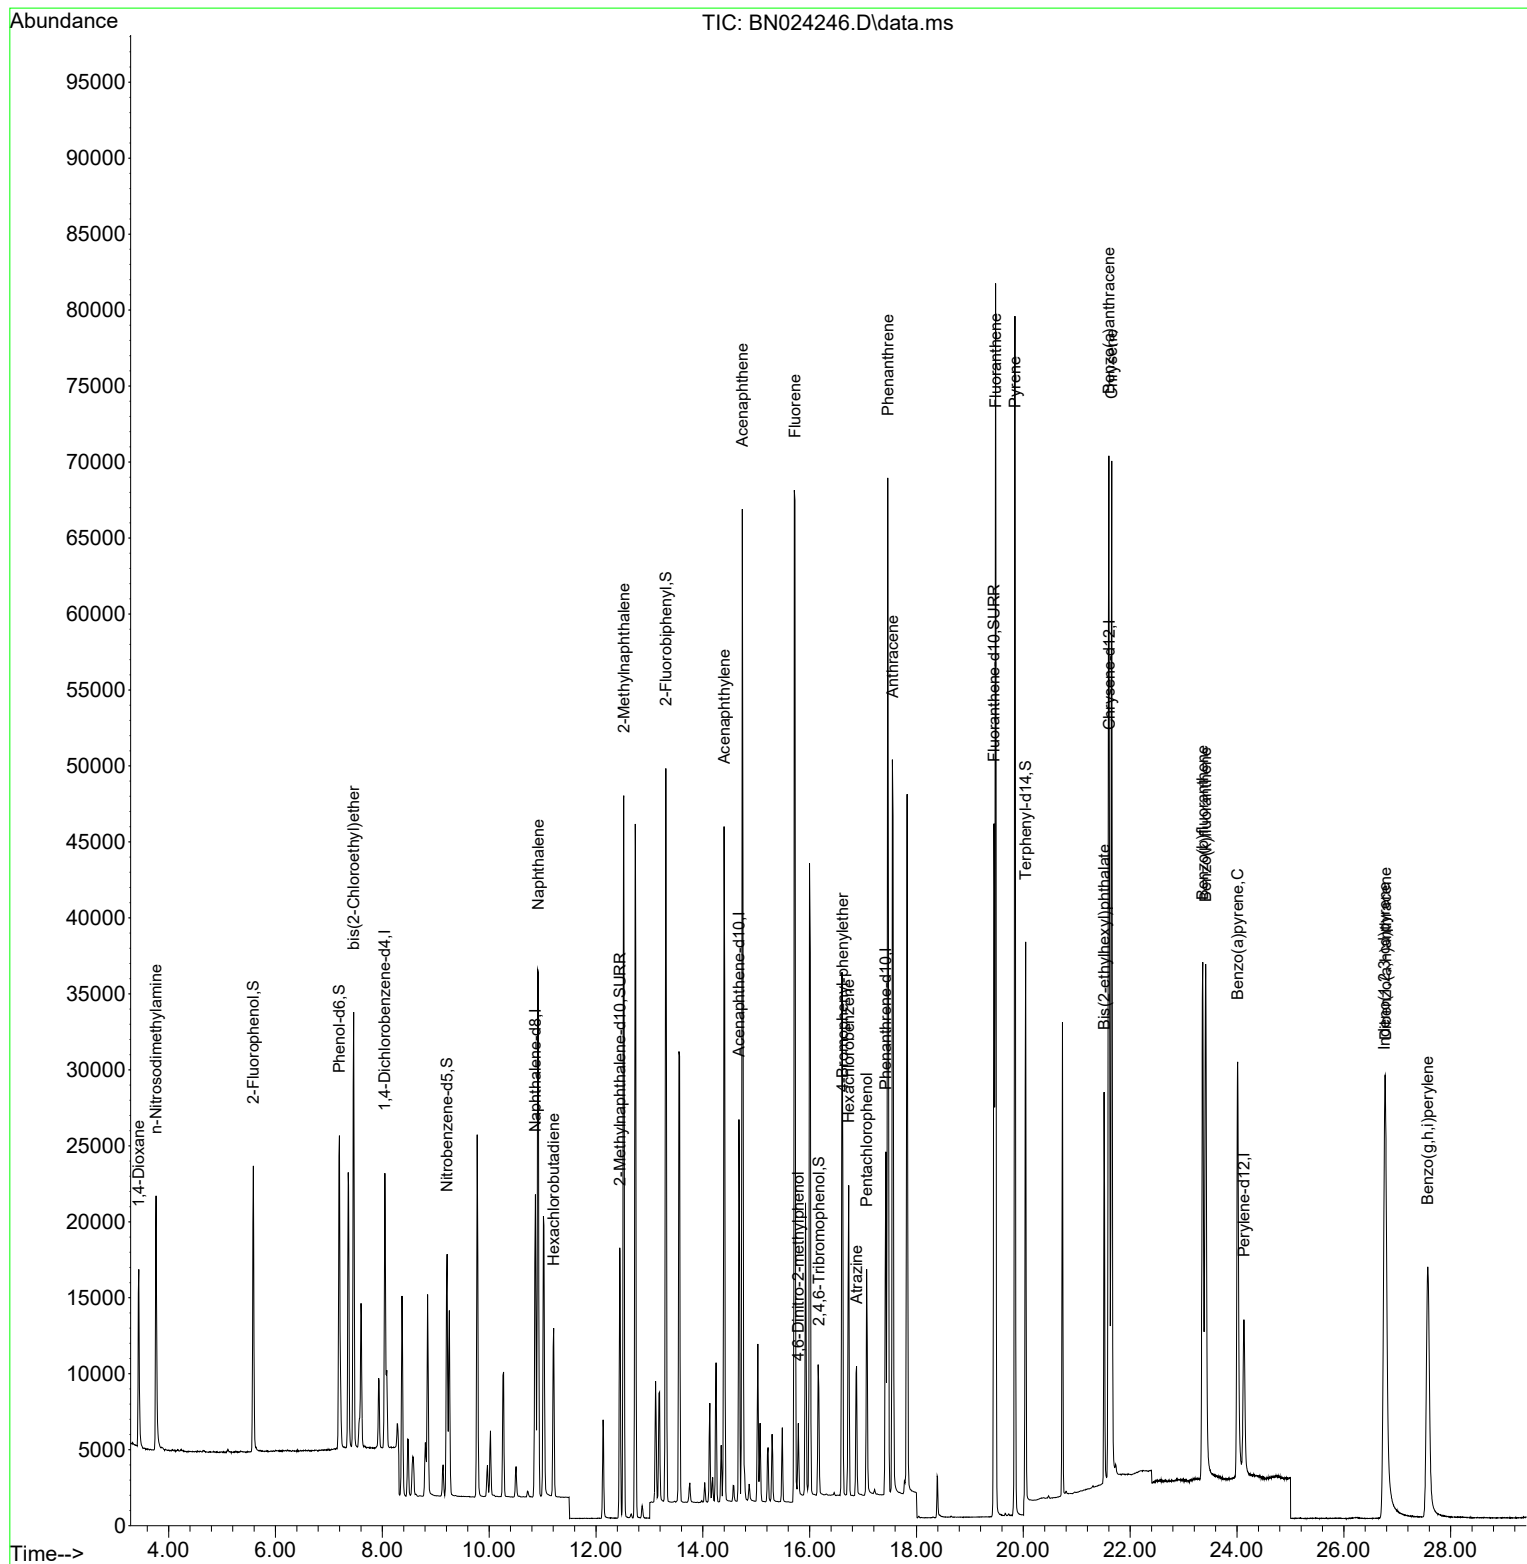





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.047 min Scan# 660
 Delta R.T. 0.000 min
 Lab File: BN024246.D
 Acq: 13 Mar 2023 15:02


Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

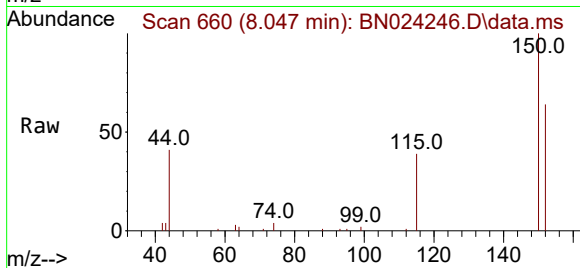



Tgt Ion:152 Resp: 8721
 Ion Ratio Lower Upper
 152 100
 150 156.4 124.7 187.1
 115 60.5 49.1 73.7

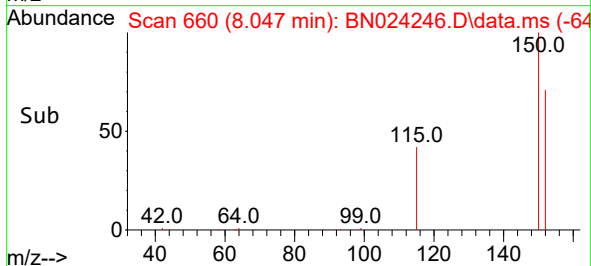


#2
 1,4-Dioxane
 Concen: 0.907 ng
 RT: 3.439 min Scan# 22
 Delta R.T. 0.000 min
 Lab File: BN024246.D
 Acq: 13 Mar 2023 15:02

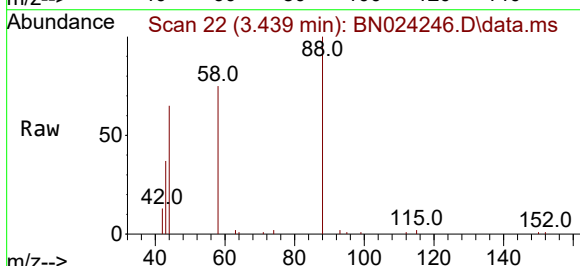

Tgt Ion: 88 Resp: 7501
 Ion Ratio Lower Upper
 88 100
 43 36.0 29.0 43.4
 58 84.3 67.3 100.9




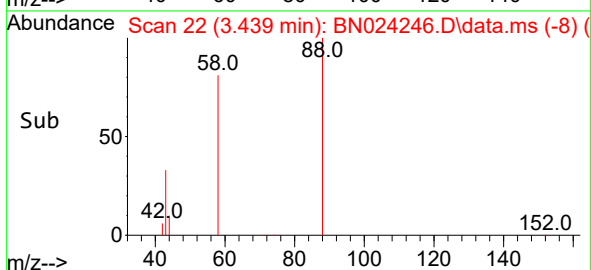


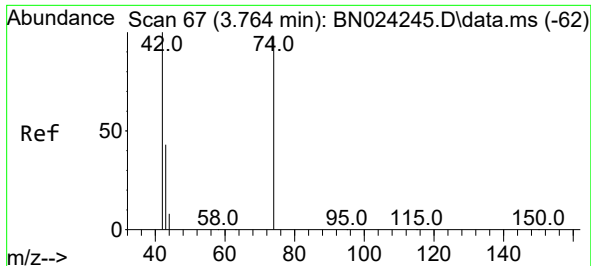

#3
n-Nitrosodimethylamine
Concen: 1.198 ng
RT: 3.764 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion: 42 Resp: 11102
Ion Ratio Lower Upper
42 100
74 99.5 81.6 122.4
44 8.1 7.3 10.9

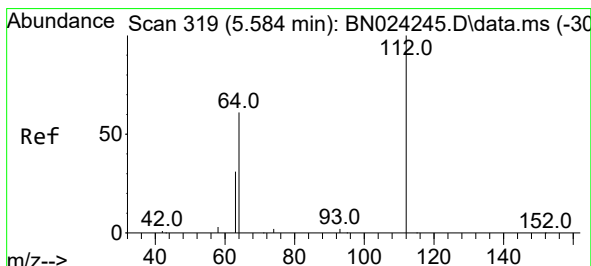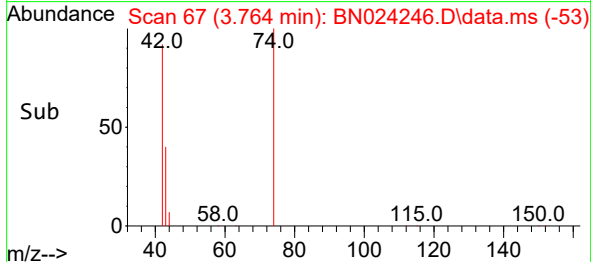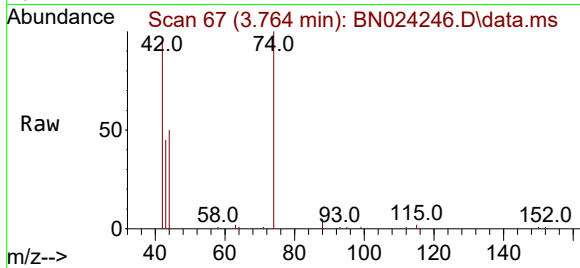

#4
2-Fluorophenol
Concen: 0.810 ng
RT: 5.584 min Scan# 319
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02

Tgt Ion: 112 Resp: 14680
Ion Ratio Lower Upper
112 100
64 61.9 49.0 73.6
63 32.6 25.7 38.5



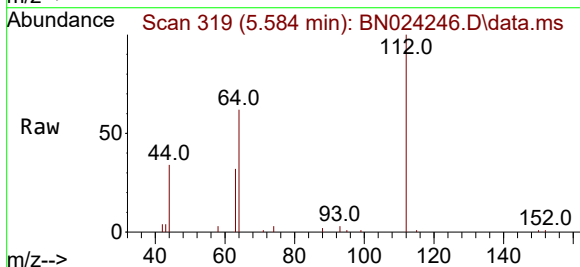




#5
Phenol-d6
Concen: 0.878 ng
RT: 7.195 min Scan# 542
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion: 99 Resp: 18758
Ion Ratio Lower Upper
99 100
42 25.0 20.1 30.1
71 32.8 25.8 38.8

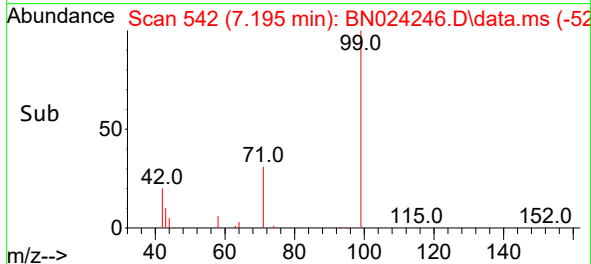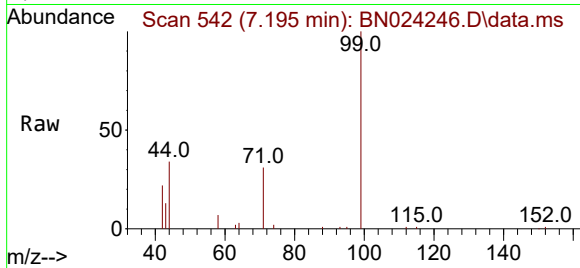

#6
bis(2-Chloroethyl)ether
Concen: 0.905 ng
RT: 7.462 min Scan# 579
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02

Tgt Ion: 93 Resp: 19336
Ion Ratio Lower Upper
93 100
63 82.2 65.4 98.2
95 32.2 25.8 38.8


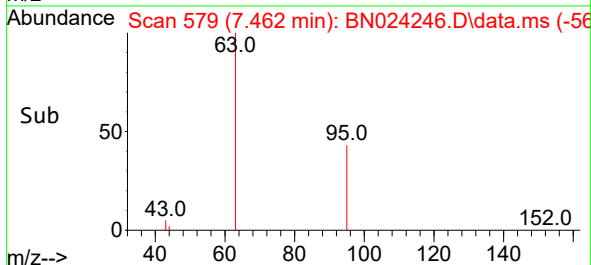
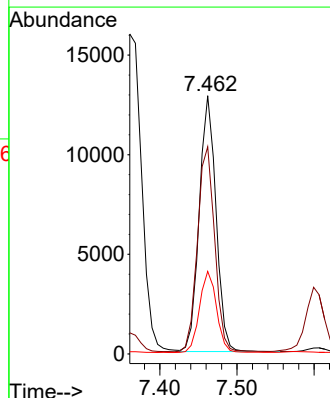
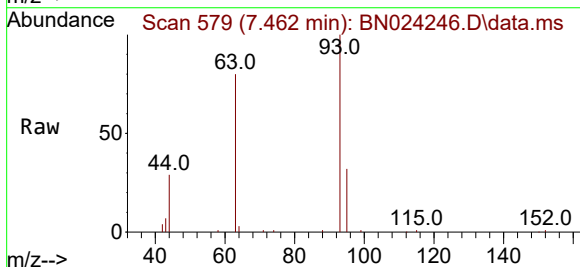




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.866 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion:	136	Resp:	25014
Ion Ratio	Lower	Upper	
136	100		
137	11.2	8.9	13.3
54	9.3	7.1	10.7
68	6.9	5.3	7.9

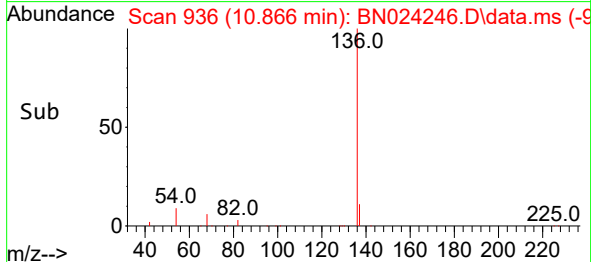

#8
Nitrobenzene-d5
Concen: 0.617 ng
RT: 9.211 min Scan# 781
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02

Tgt Ion:	82	Resp:	12385
Ion Ratio	Lower	Upper	
82	100		
128	40.6	32.4	48.6
54	56.1	45.2	67.8




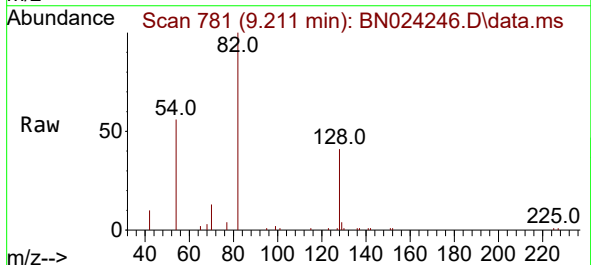




#9
Naphthalene
Concen: 0.783 ng
RT: 10.919 min Scan# 941
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion:128 Resp: 48832
Ion Ratio Lower Upper
128 100
129 11.1 9.0 13.6
127 12.8 10.2 15.4

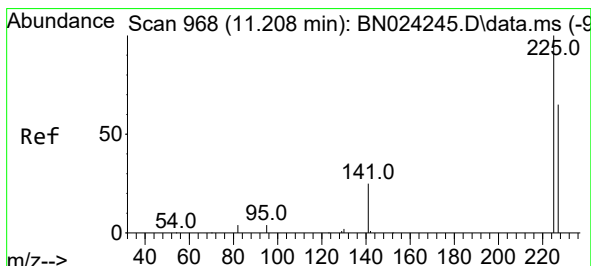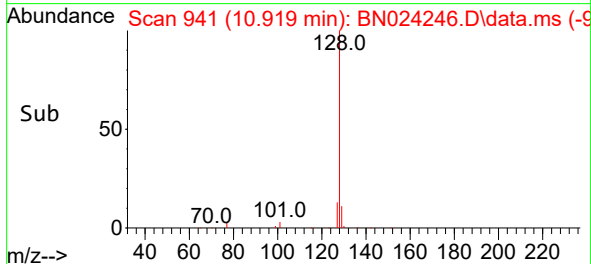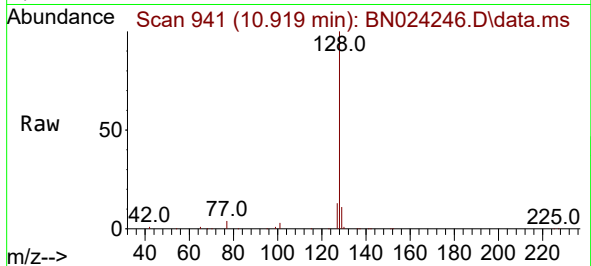

#10
Hexachlorobutadiene
Concen: 0.566 ng
RT: 11.208 min Scan# 968
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02

Tgt Ion:225 Resp: 9263
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.9 51.0 76.4


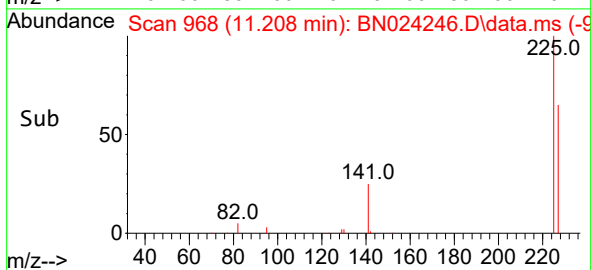

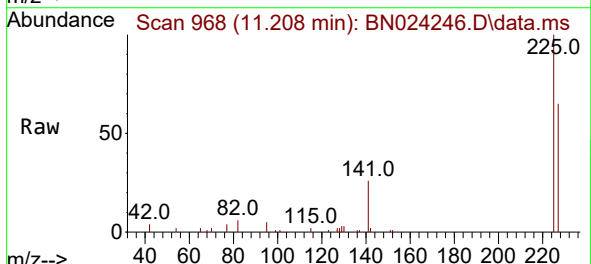




#11
2-Methylnaphthalene-d10
Concen: 0.674 ng
RT: 12.444 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:152 Resp: 23420
Ion Ratio Lower Upper
152 100
151 20.8 16.8 25.2

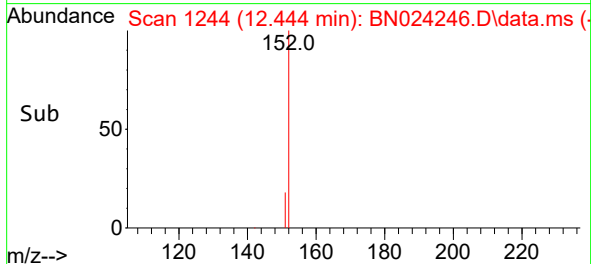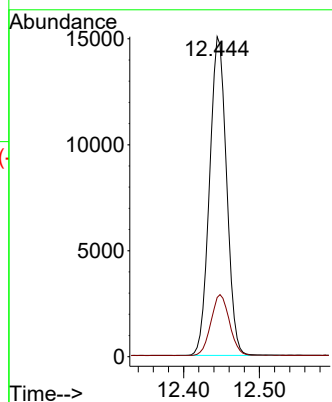

#12
2-Methylnaphthalene
Concen: 0.790 ng
RT: 12.520 min Scan# 1264
Delta R.T. 0.004 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02

Tgt Ion:142 Resp: 32804
Ion Ratio Lower Upper
142 100
141 87.9 71.8 107.6
115 35.6 30.0 45.0


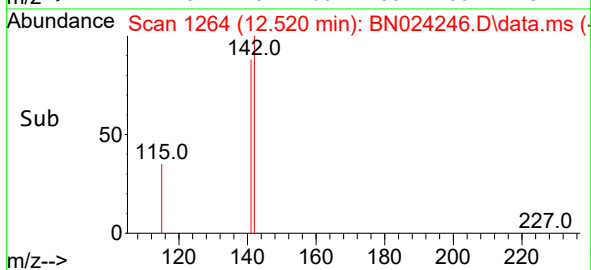
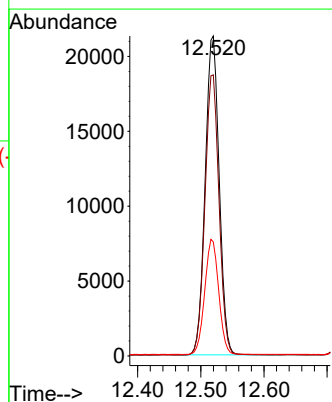



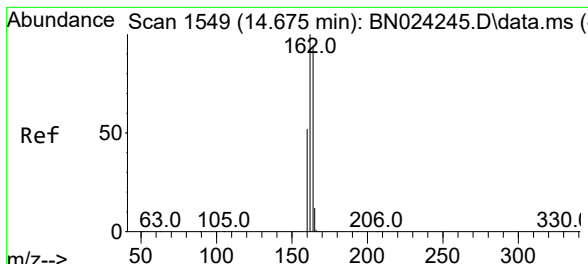

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.675 min Scan# 1549
 Delta R.T. 0.000 min
 Lab File: BN024246.D
 Acq: 13 Mar 2023 15:02




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Tgt Ion:164	Resp:	13792
Ion Ratio	Lower	Upper
164	100	
162	104.4	84.7 127.1
160	55.8	44.6 66.8

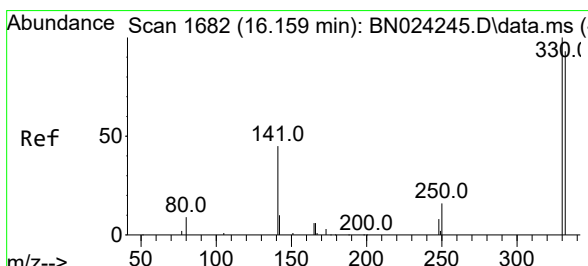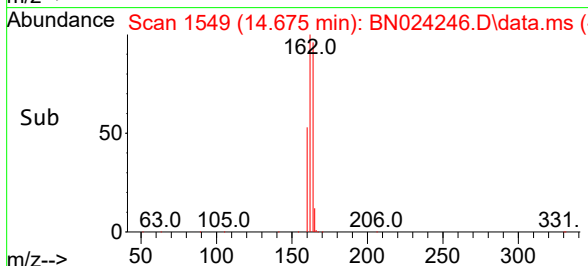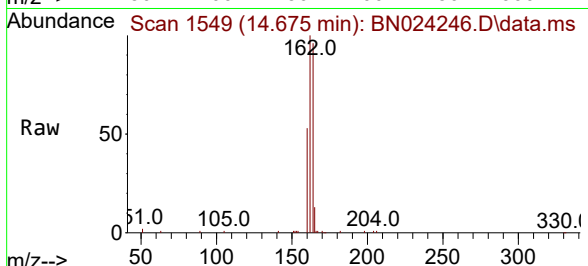

#14
 2,4,6-Tribromophenol
 Concen: 0.712 ng
 RT: 16.172 min Scan# 1683
 Delta R.T. 0.013 min
 Lab File: BN024246.D
 Acq: 13 Mar 2023 15:02

Tgt Ion:330	Resp:	5060
Ion Ratio	Lower	Upper
330	100	
332	96.8	78.0 117.0
141	40.2	30.8 46.2

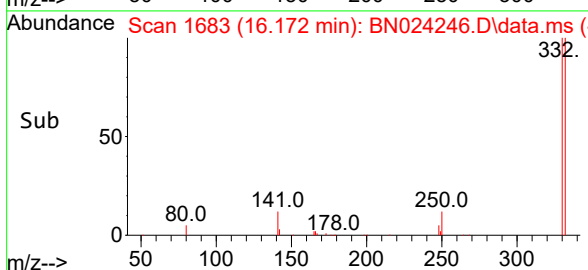

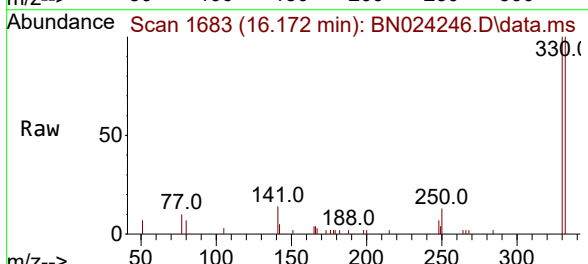




#15
2-Fluorobiphenyl
Concen: 0.722 ng
RT: 13.307 min Scan# 1421
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion:172 Resp: 39413
Ion Ratio Lower Upper
172 100
171 35.1 27.8 41.8
170 24.1 19.0 28.6

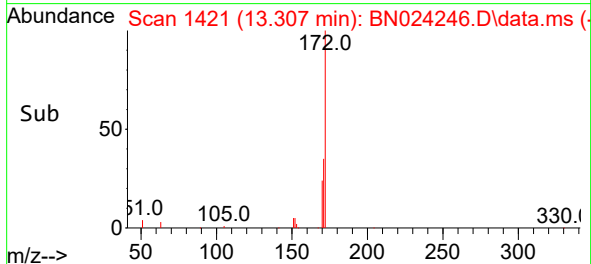

#16
Acenaphthylene
Concen: 0.910 ng
RT: 14.397 min Scan# 1523
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02

Tgt Ion:152 Resp: 48891
Ion Ratio Lower Upper
152 100
151 19.2 15.4 23.0
153 12.9 10.4 15.6

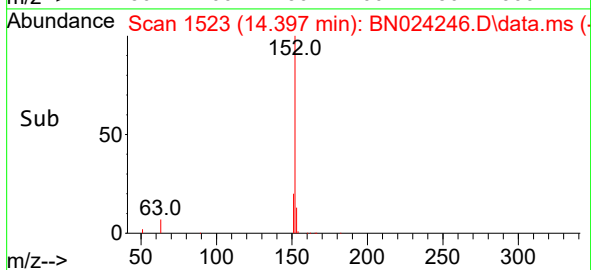






#17
Acenaphthene
Concen: 0.854 ng
RT: 14.739 min Scan# 1555
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion:154 Resp: 31214
Ion Ratio Lower Upper
154 100
153 111.3 88.4 132.6
152 60.5 48.7 73.1

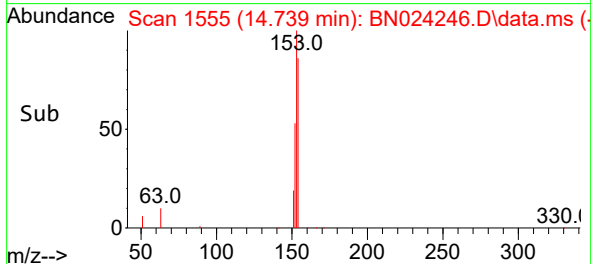

#18
Fluorene
Concen: 0.763 ng
RT: 15.725 min Scan# 1647
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02

Tgt Ion:166 Resp: 37800
Ion Ratio Lower Upper
166 100
165 97.4 80.2 120.2
167 13.2 10.8 16.2

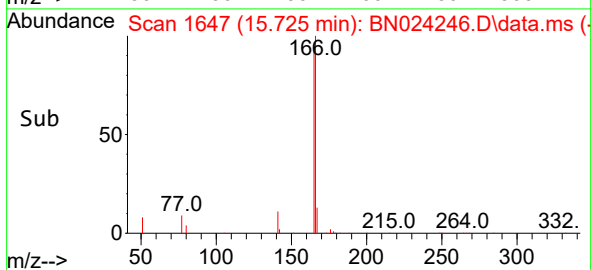



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.425 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN024246.D

Acq: 13 Mar 2023 15:02

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:188 Resp: 28635

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 11.1 8.9 13.3

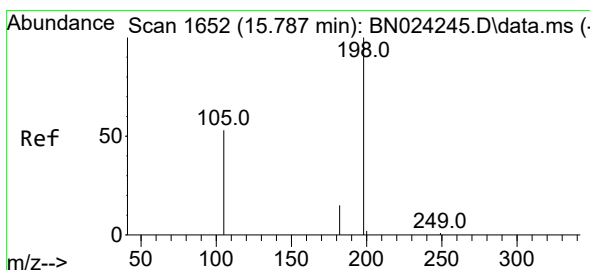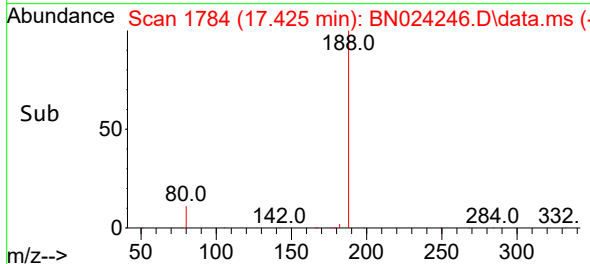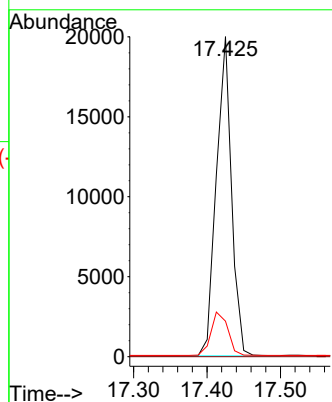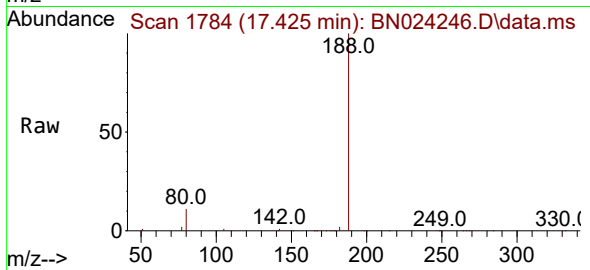

#20

4,6-Dinitro-2-methylphenol

Concen: 0.542 ng

RT: 15.787 min Scan# 1652

Delta R.T. 0.000 min

Lab File: BN024246.D

Acq: 13 Mar 2023 15:02




Tgt Ion:198 Resp: 2539


Ion Ratio Lower Upper

198 100

51 74.8 68.2 102.2

105 61.2 51.6 77.4


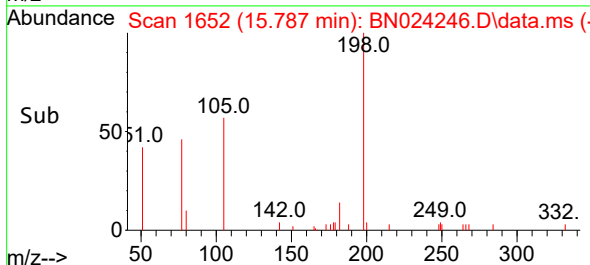

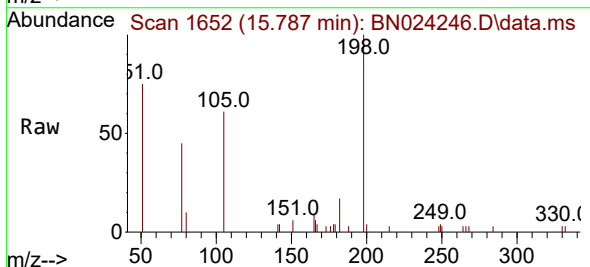




#21
4-Bromophenyl-phenylether
Concen: 0.683 ng
RT: 16.618 min Scan# 1719
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:248 Resp: 12717
Ion Ratio Lower Upper
248 100
250 103.3 81.9 122.9
141 31.4 28.2 42.2

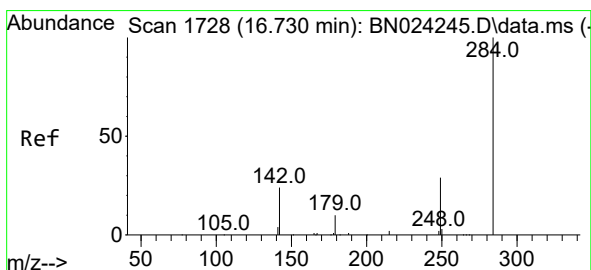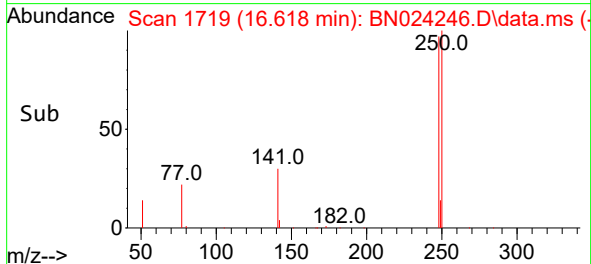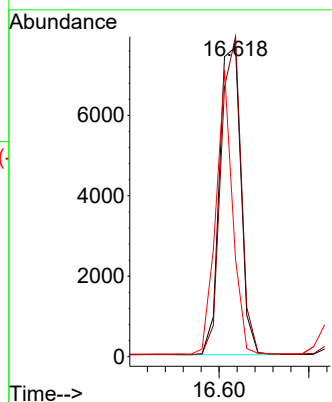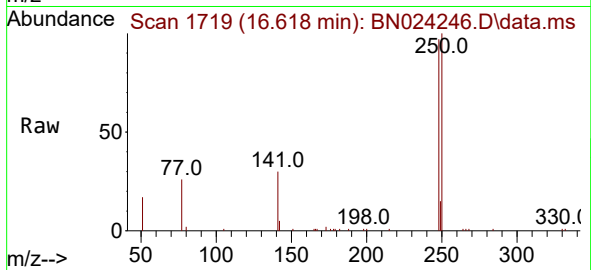

#22
Hexachlorobenzene
Concen: 0.707 ng
RT: 16.730 min Scan# 1728
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02

Tgt Ion:284 Resp: 15817
Ion Ratio Lower Upper
284 100
142 37.4 30.2 45.4
249 30.5 24.5 36.7

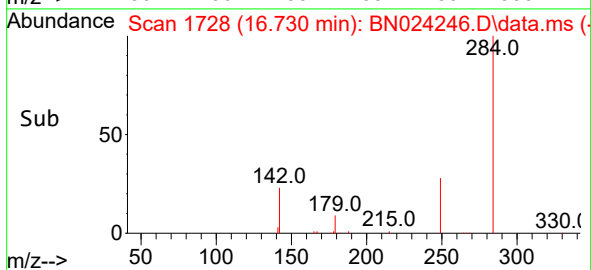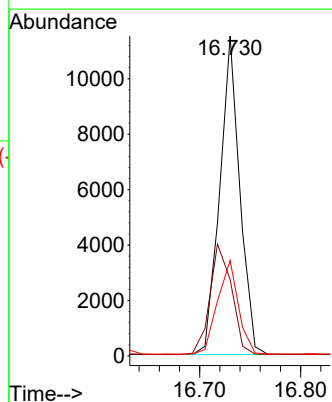

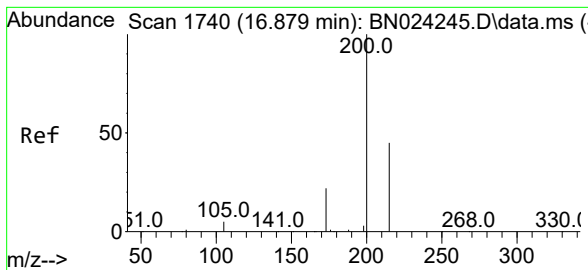

#23

Atrazine

Concen: 0.618 ng

RT: 16.879 min Scan# 1740

Delta R.T. 0.000 min

Lab File: BN024246.D

Acq: 13 Mar 2023 15:02

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:200 Resp: 7530

Ion Ratio Lower Upper

200 100

173 22.5 18.9 28.3

215 46.2 36.7 55.1

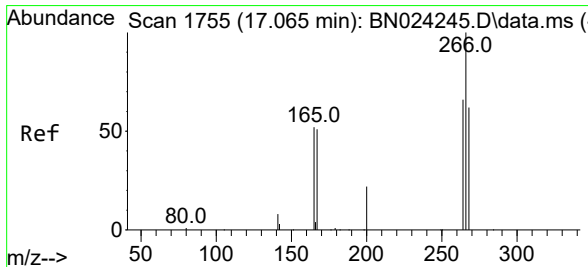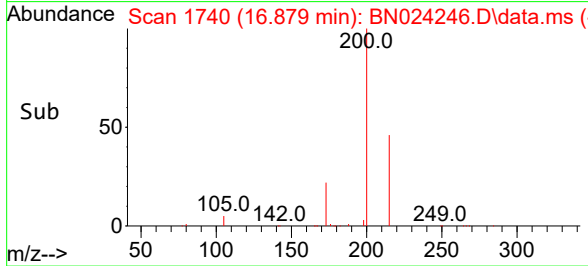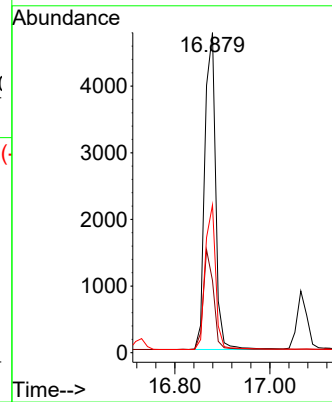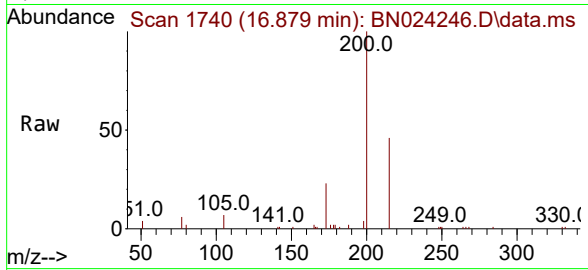

#24

Pentachlorophenol

Concen: 0.871 ng

RT: 17.065 min Scan# 1755

Delta R.T. 0.000 min

Lab File: BN024246.D

Acq: 13 Mar 2023 15:02




Tgt Ion:266 Resp: 6904


Ion Ratio Lower Upper

266 100

264 63.4 51.1 76.7

268 65.5 52.2 78.4


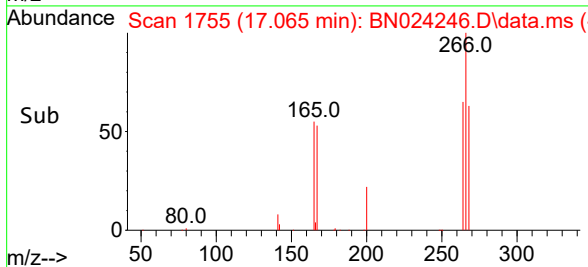

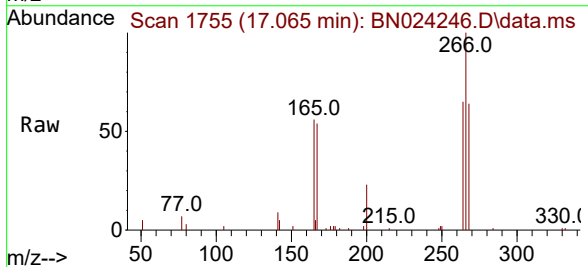


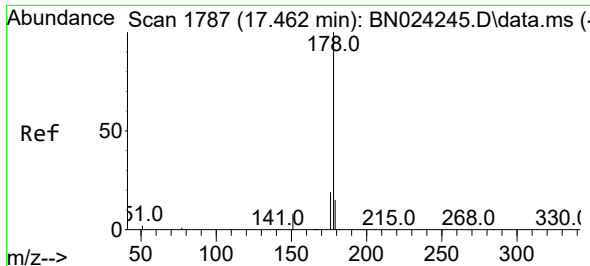

#25
Phenanthrene
Concen: 0.814 ng
RT: 17.462 min Scan# 1787
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion:178 Resp: 64274
Ion Ratio Lower Upper
178 100
176 19.3 15.4 23.0
179 15.1 12.2 18.2

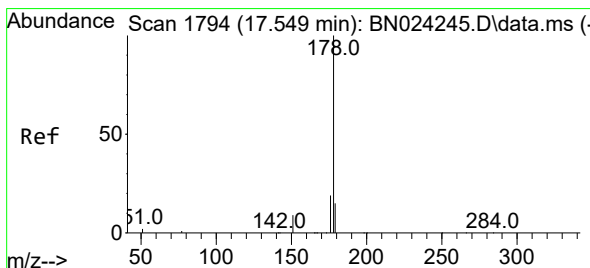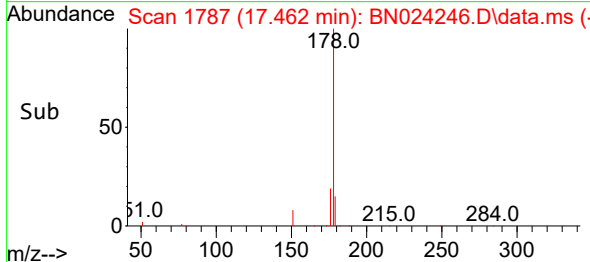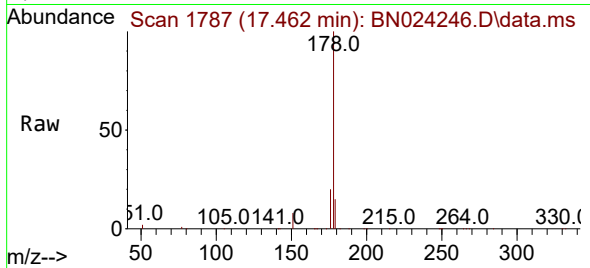

#26
Anthracene
Concen: 0.891 ng
RT: 17.549 min Scan# 1794
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02

Tgt Ion:178 Resp: 57913
Ion Ratio Lower Upper
178 100
176 18.8 15.1 22.7
179 15.1 12.1 18.1

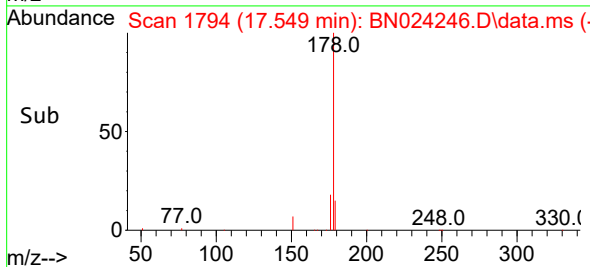

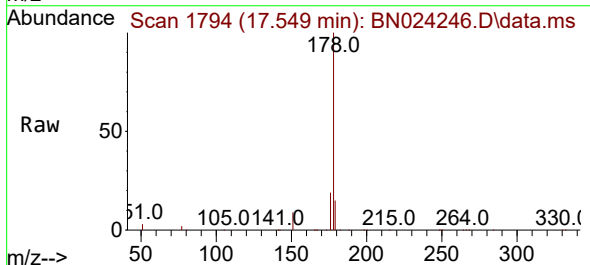




#27
Fluoranthene-d10
Concen: 0.649 ng
RT: 19.450 min Scan# 2173
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:212 Resp: 45124
Ion Ratio Lower Upper
212 100
106 19.4 15.4 23.2
104 10.9 8.6 13.0

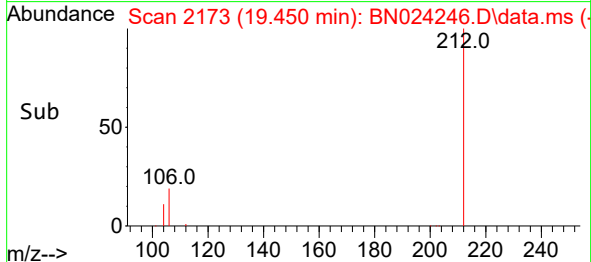

#28
Fluoranthene
Concen: 0.774 ng
RT: 19.480 min Scan# 2180
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02

Tgt Ion:202 Resp: 70107
Ion Ratio Lower Upper
202 100
101 13.9 11.3 16.9
203 17.1 13.6 20.4




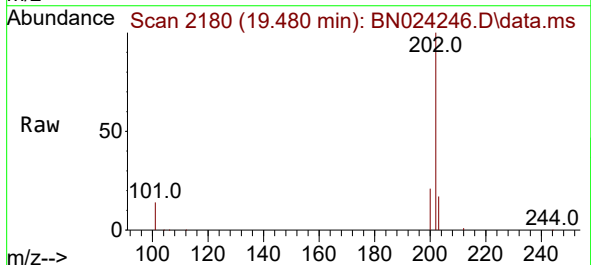


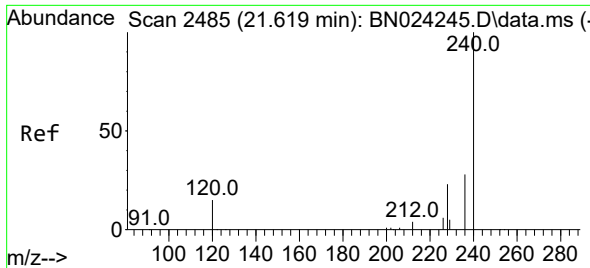

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.610 min Scan# 2484
Delta R.T. -0.009 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:240 Resp: 22247
Ion Ratio Lower Upper
240 100
120 22.1 12.8 19.2#
236 29.0 22.5 33.7

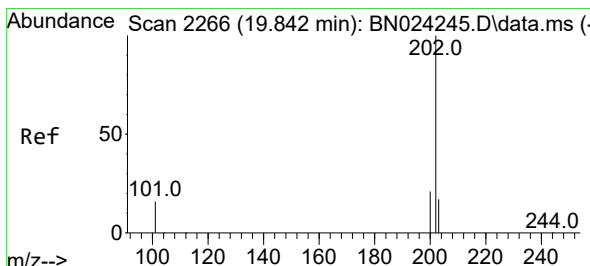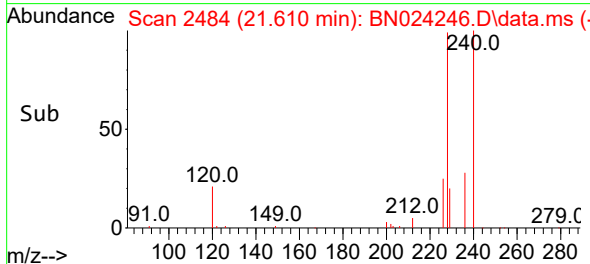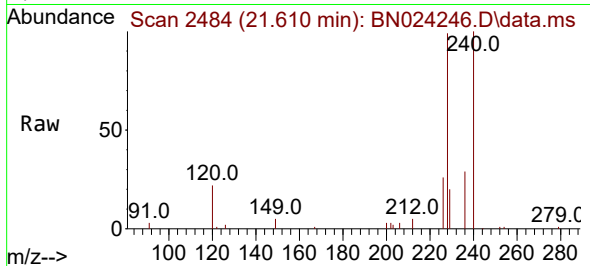

#30
Pyrene
Concen: 0.895 ng
RT: 19.842 min Scan# 2266
Delta R.T. 0.000 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02

Tgt Ion:202 Resp: 69093
Ion Ratio Lower Upper
202 100
200 21.1 17.0 25.4
203 17.7 14.2 21.2

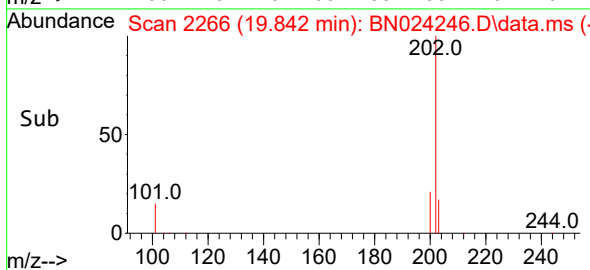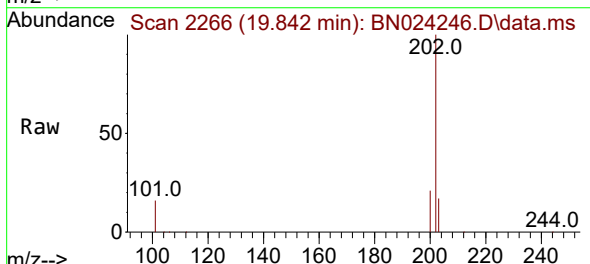

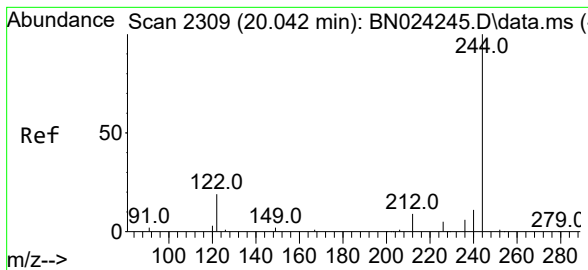

#31

Terphenyl-d14

Concen: 0.652 ng

RT: 20.042 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN024246.D

Acq: 13 Mar 2023 15:02

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8




Tgt Ion:244 Resp: 27060

Ion Ratio Lower Upper

244 100

212 8.4 7.6 11.4

122 14.6 15.1 22.7#

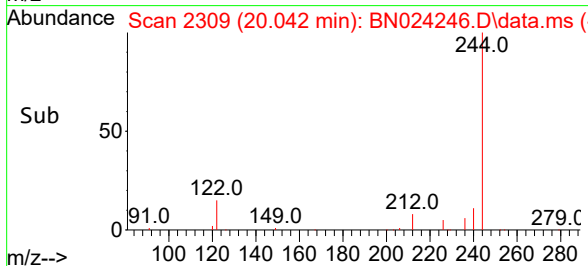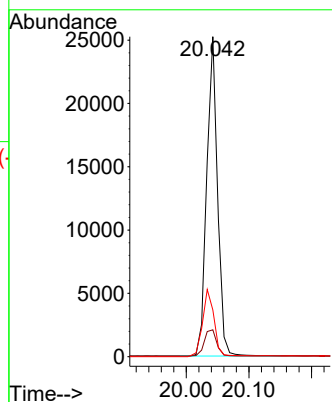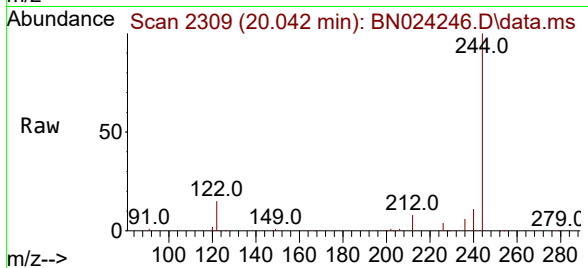

#32

Benzo(a)anthracene

Concen: 0.796 ng

RT: 21.601 min Scan# 2483

Delta R.T. 0.000 min

Lab File: BN024246.D

Acq: 13 Mar 2023 15:02




Tgt Ion:228 Resp: 56636

Ion Ratio Lower Upper

228 100

226 27.2 22.2 33.2

229 19.8 15.9 23.9

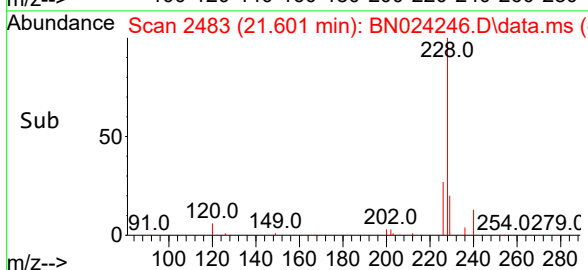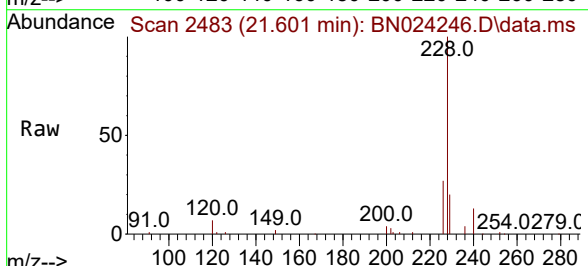



#33

Chrysene

Concen: 0.782 ng

RT: 21.655 min Scan# 2489

Delta R.T. 0.000 min

Lab File: BN024246.D

Acq: 13 Mar 2023 15:02

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:228 Resp: 60102

Ion Ratio Lower Upper

228 100

226 30.8 24.5 36.7

229 19.6 15.5 23.3

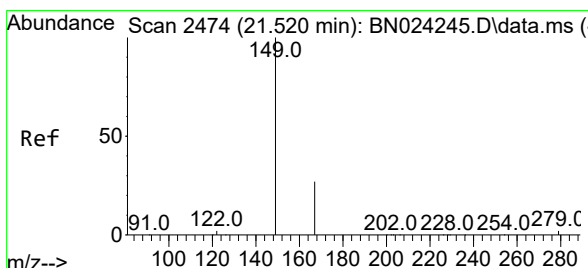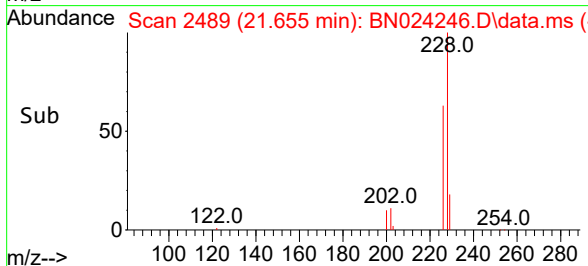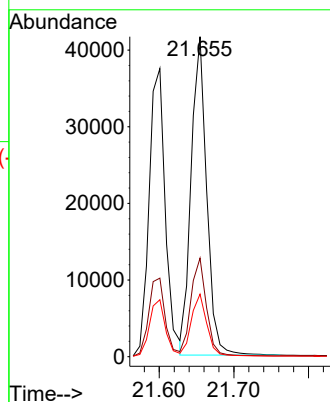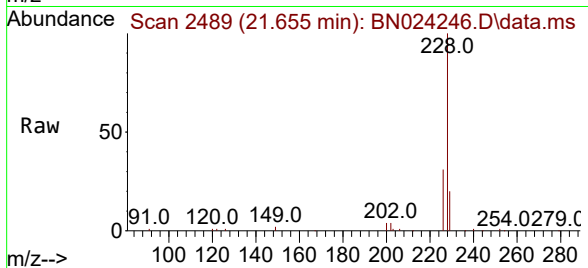

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.748 ng

RT: 21.511 min Scan# 2473

Delta R.T. -0.009 min

Lab File: BN024246.D

Acq: 13 Mar 2023 15:02




Tgt Ion:149 Resp: 24325


Ion Ratio Lower Upper

149 100

167 26.0 21.2 31.8

279 2.2 1.8 2.8


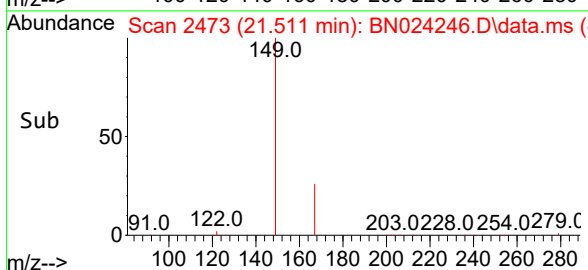

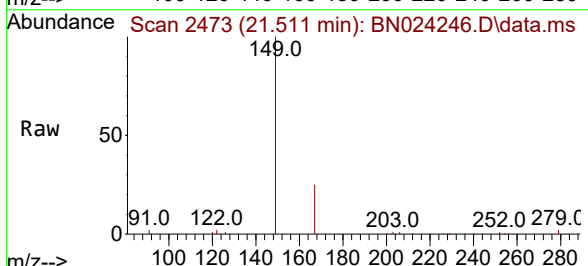


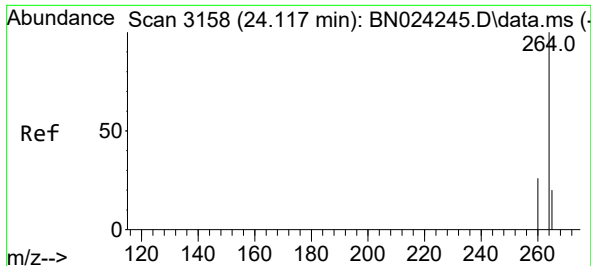

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.129 min Scan# 3158
 Delta R.T. 0.012 min
 Lab File: BN024246.D
 Acq: 13 Mar 2023 15:02




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Tgt Ion:264 Resp: 17210
 Ion Ratio Lower Upper
 264 100
 260 27.2 21.4 32.2
 265 47.5 35.7 53.5

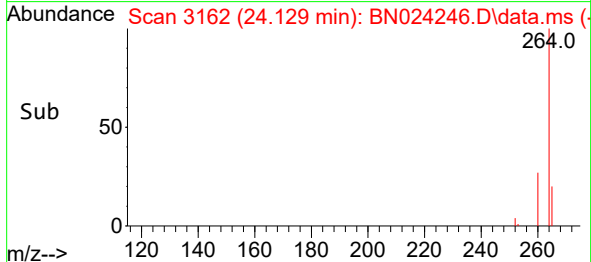

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.612 ng
 RT: 26.760 min Scan# 4062
 Delta R.T. 0.035 min
 Lab File: BN024246.D
 Acq: 13 Mar 2023 15:02

Tgt Ion:276 Resp: 47879
 Ion Ratio Lower Upper
 276 100
 138 34.4 27.4 41.2
 277 24.8 19.8 29.6



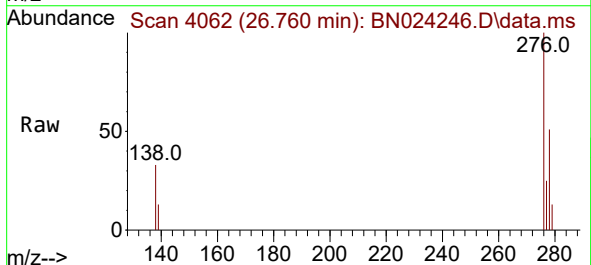




#37
Benzo(b)fluoranthene
Concen: 0.730 ng
RT: 23.357 min Scan# 21
Delta R.T. 0.006 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion:252 Resp: 50873
Ion Ratio Lower Upper
252 100
253 22.8 18.9 28.3
125 15.2 13.8 20.6

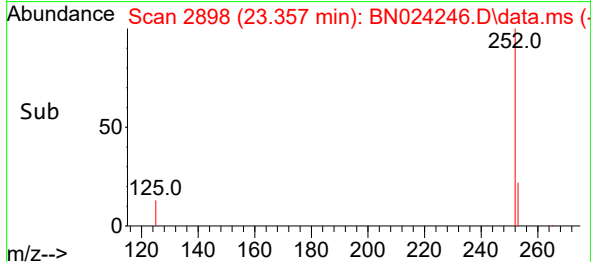

#38
Benzo(k)fluoranthene
Concen: 0.758 ng
RT: 23.413 min Scan# 2917
Delta R.T. 0.012 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02

Tgt Ion:252 Resp: 52170
Ion Ratio Lower Upper
252 100
253 22.2 19.0 28.6
125 15.3 13.5 20.3


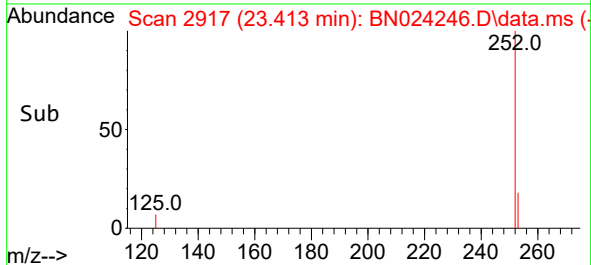






#39
Benzo(a)pyrene
Concen: 0.885 ng
RT: 24.012 min Scan# 3119
Delta R.T. 0.009 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion:252 Resp: 46749
Ion Ratio Lower Upper
252 100
253 22.9 19.5 29.3
125 17.5 16.2 24.4

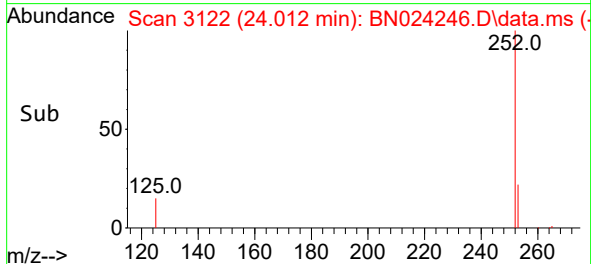

#40
Dibenzo(a,h)anthracene
Concen: 0.593 ng
RT: 26.781 min Scan# 4069
Delta R.T. 0.035 min
Lab File: BN024246.D
Acq: 13 Mar 2023 15:02


Tgt Ion:278 Resp: 37133
Ion Ratio Lower Upper
278 100
139 24.3 19.4 29.0
279 24.6 20.7 31.1

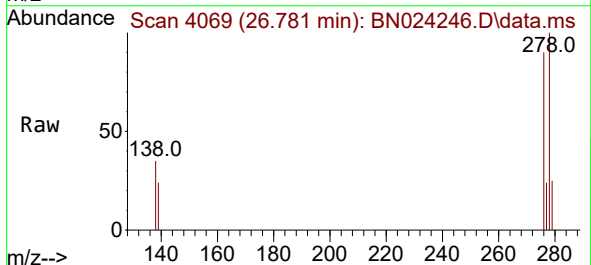



#41
 Benzo(g,h,i)perylene
 Concen: 0.663 ng
 RT: 27.570 min Scan# 41
 Delta R.T. 0.041 min
 Lab File: BN024246.D
 Acq: 13 Mar 2023 15:02

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

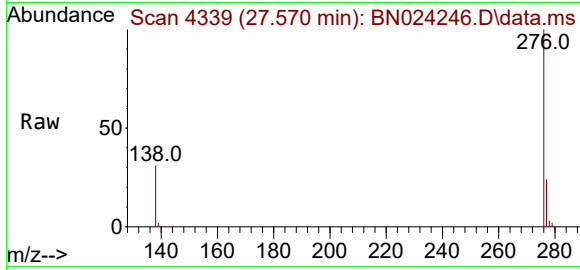

Tgt Ion:	276	Resp:	44031
Ion	Ratio	Lower	Upper
276	100		
277	24.1	19.9	29.9
138	30.8	24.5	36.7

